
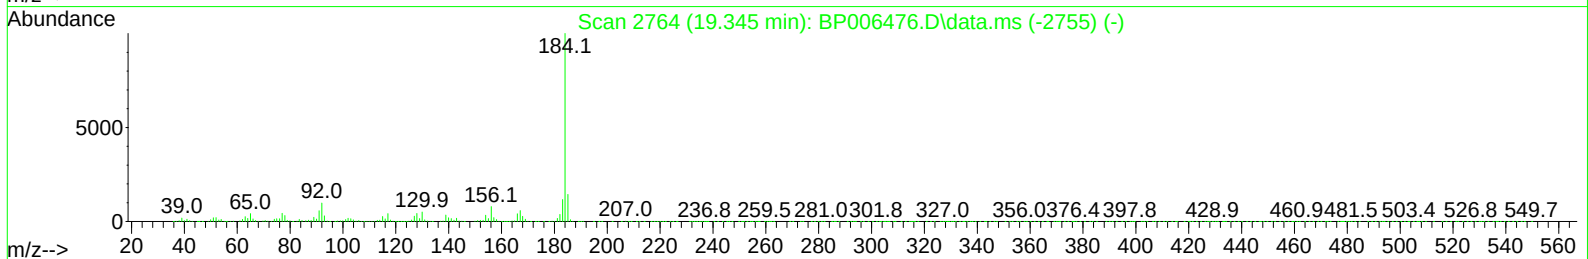
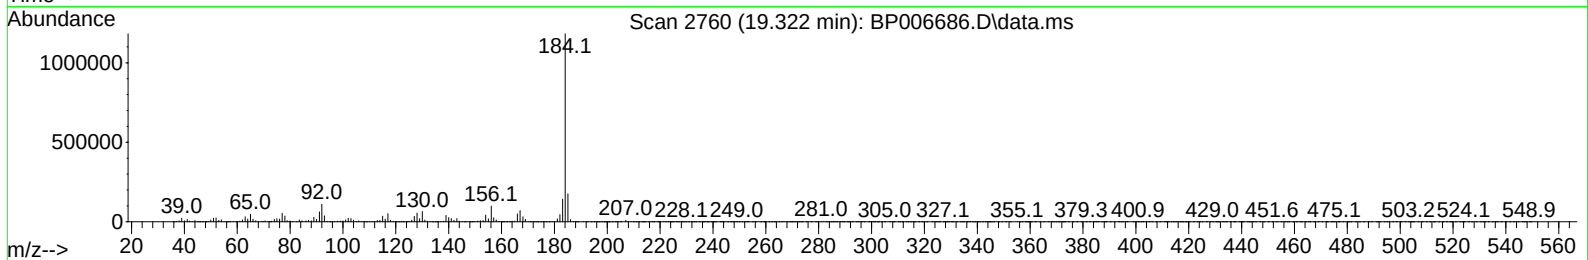


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081721\
 Data File : BP006686.D
 Acq On : 16 Aug 2021 16:53
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 16 18:13:16 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP080321.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Aug 03 15:41:30 2021
 Response via : Initial Calibration

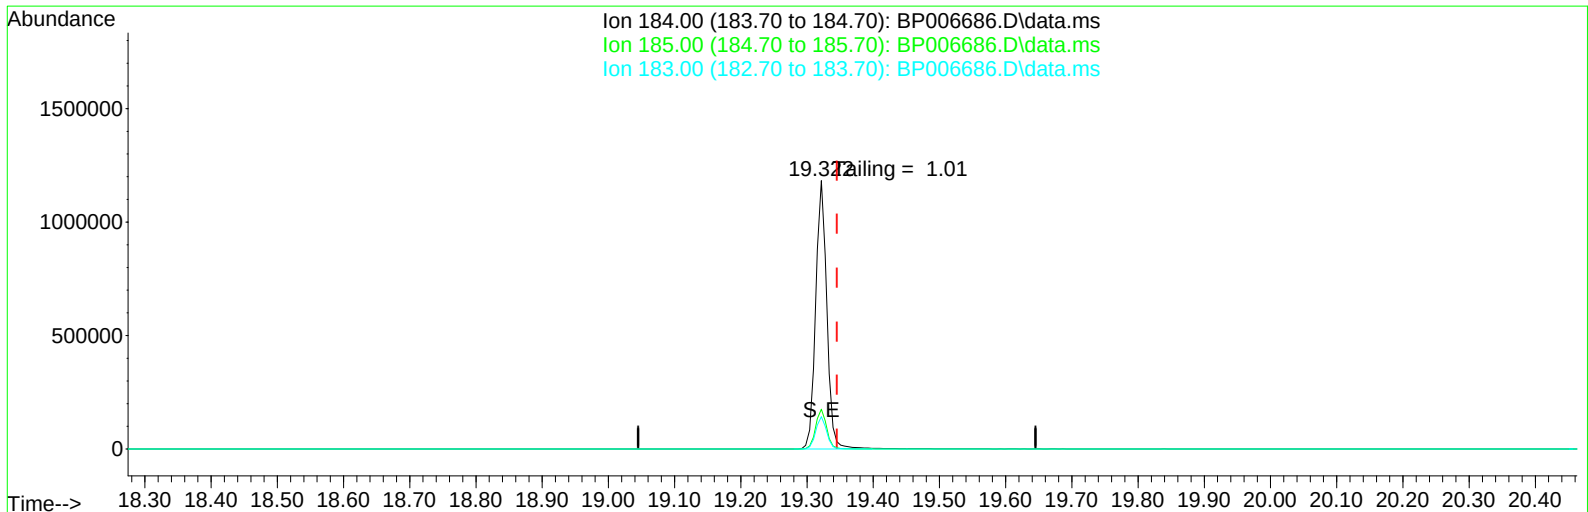

TIC: BP006686.D\data.ms

(77) Benzidine




19.322min (-0.024) 781004.84 ng

response 1387577

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.70	14.86
183.00	11.90	12.03
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081721\
Data File : BP006686.D
Acq On : 16 Aug 2021 16:53
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 16 18:13:16 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP080321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Aug 03 15:41:30 2021
Response via : Initial Calibration

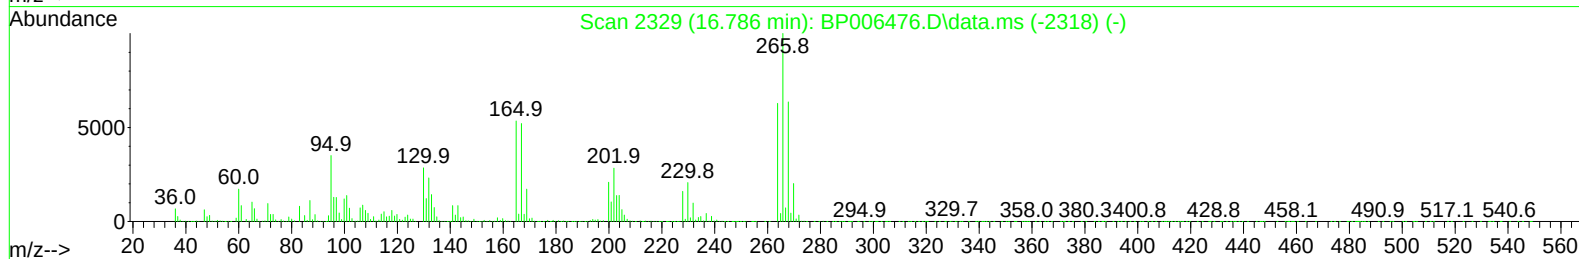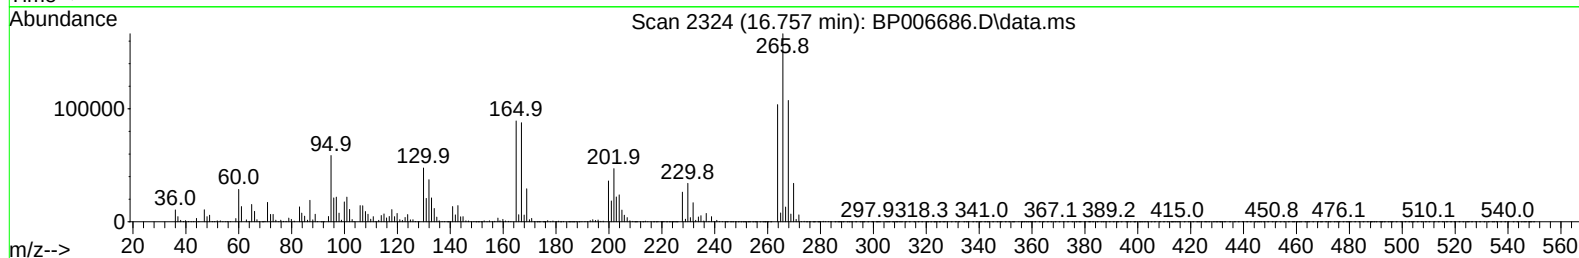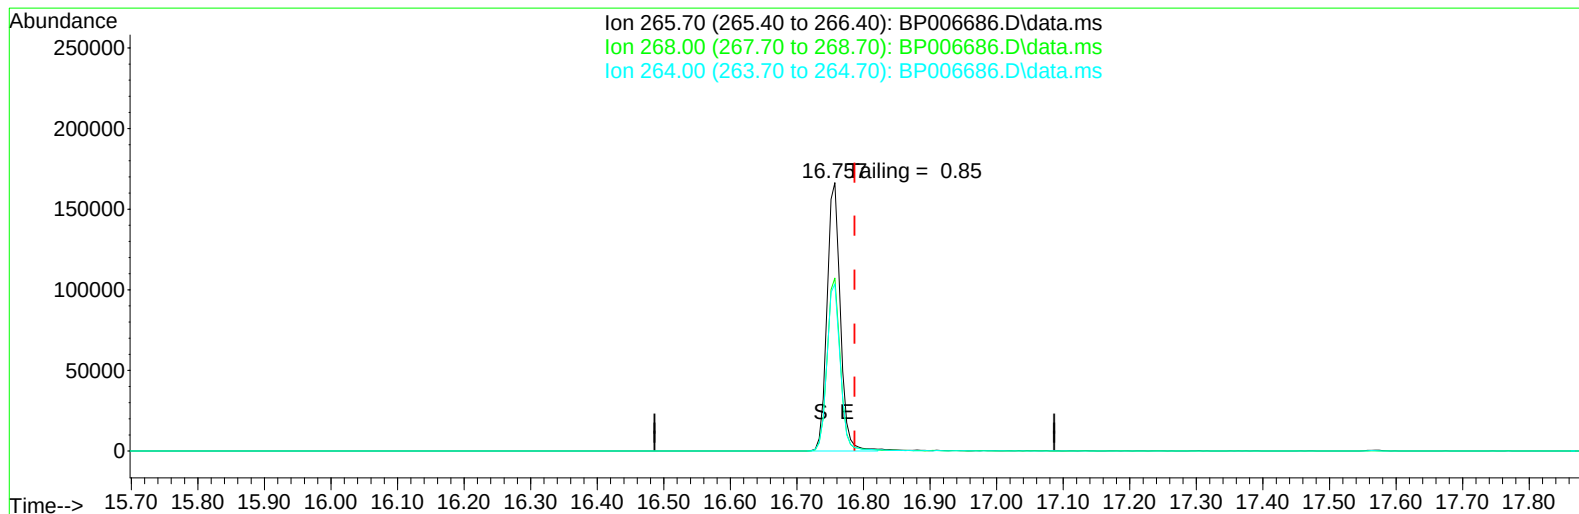

TIC: BP006686.D\data.ms

(70) Pentachlorophenol (C)

16.757min (-0.029) 1053627.50 ng

response 233577

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.50	64.49
264.00	62.90	62.26
0.00	0.00	0.00