
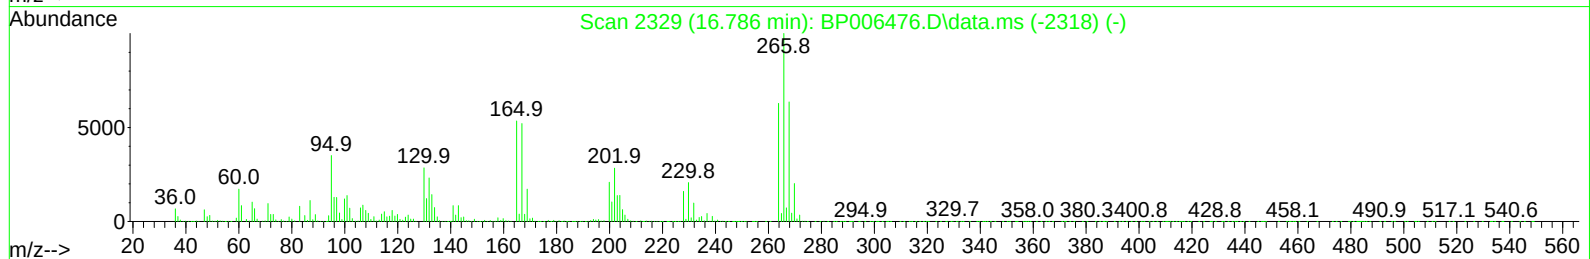
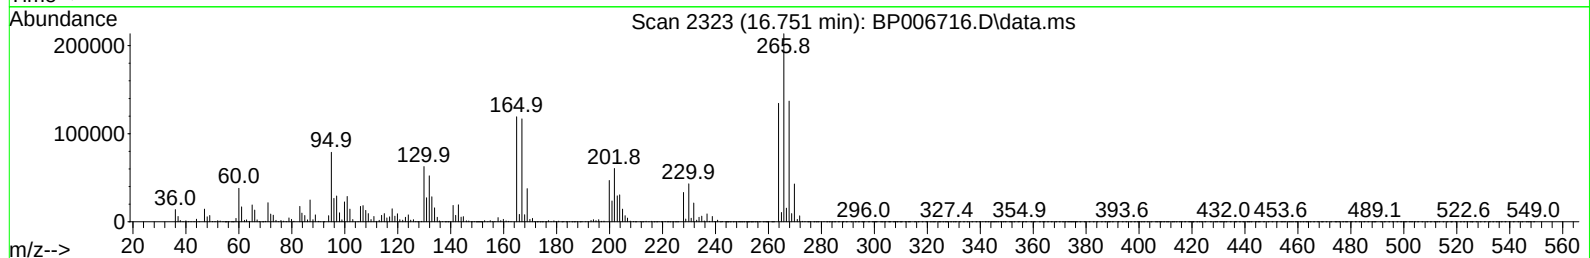


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081721\
Data File : BP006716.D
Acq On : 17 Aug 2021 14:00
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 17 14:36:48 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP080321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Aug 16 18:17:59 2021
Response via : Initial Calibration

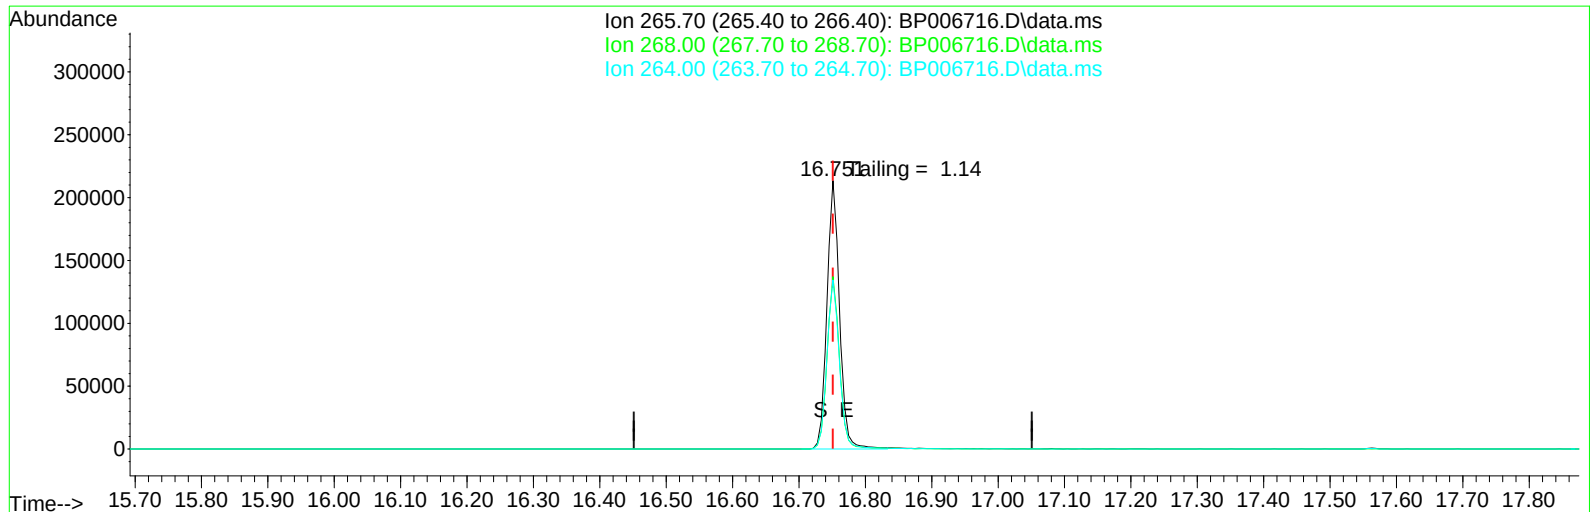

TIC: BP006716.D\data.ms

(70) Pentachlorophenol (C)




16.751min (+ 0.000) 2143062.96 ng

response 282086

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.50	64.21
264.00	62.90	62.95
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081721\
Data File : BP006716.D
Acq On : 17 Aug 2021 14:00
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 17 14:36:48 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP080321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Aug 16 18:17:59 2021
Response via : Initial Calibration

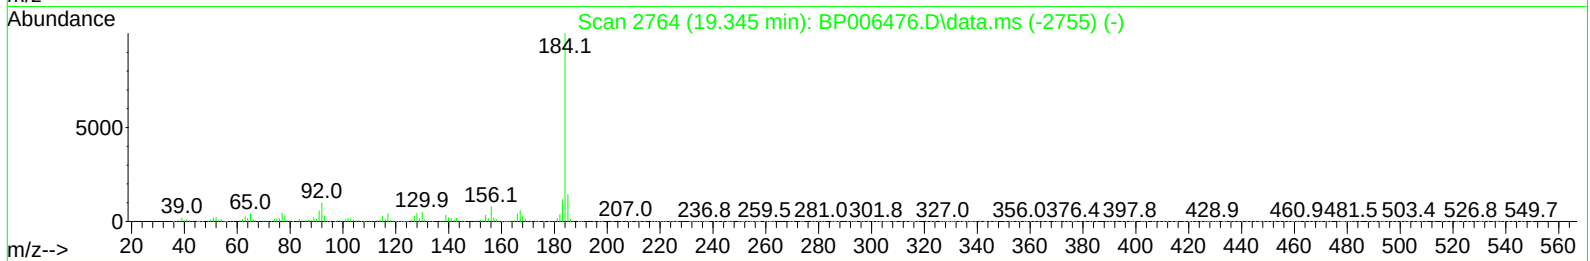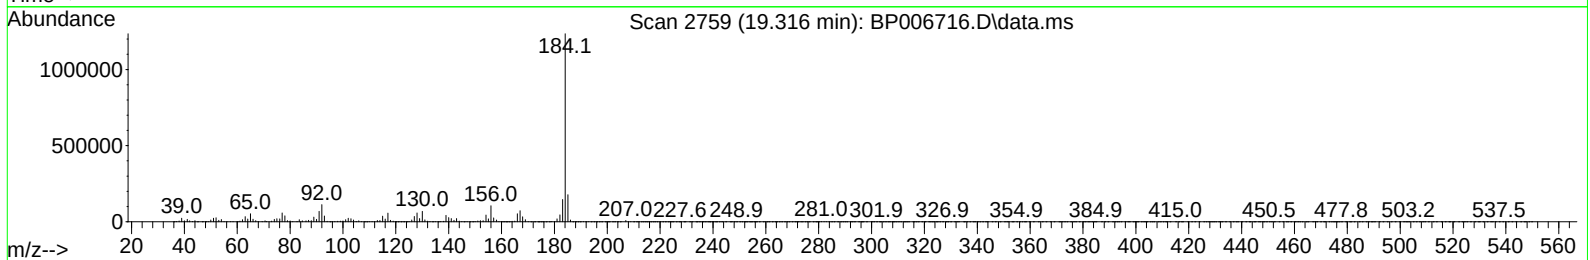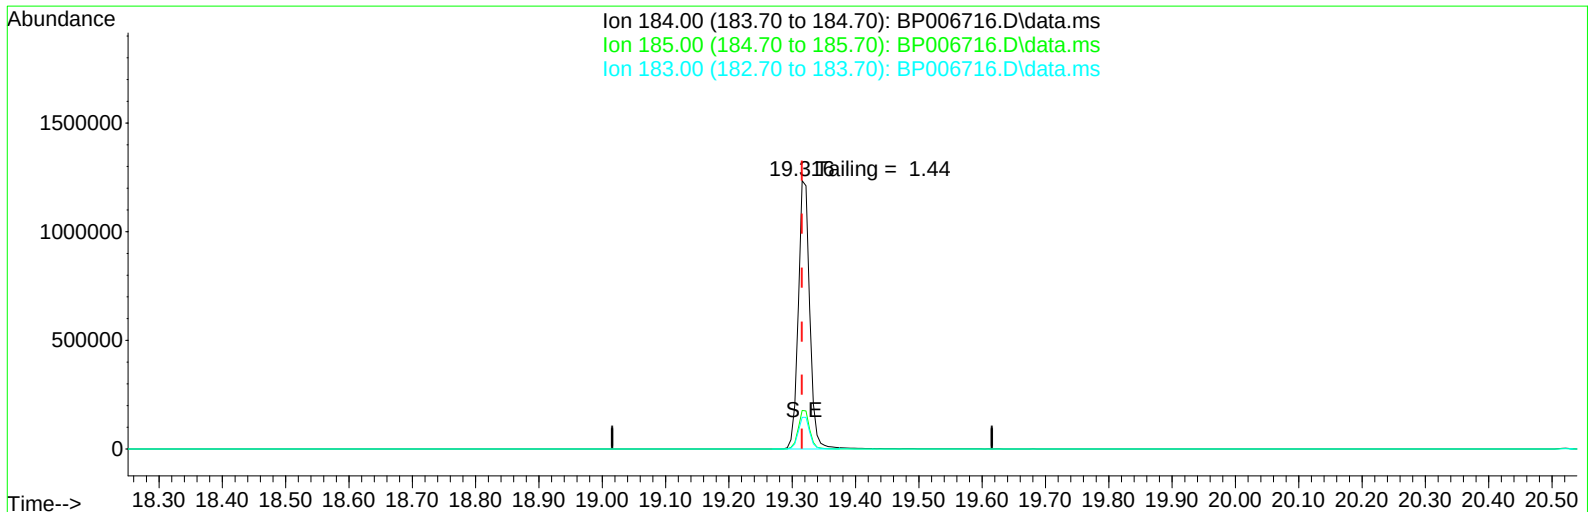

TIC: BP006716.D\data.ms

(77) Benzidine

19.316min (+ 0.000) 23909.43 ng

response 1559751

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.70	14.40
183.00	11.90	11.85
0.00	0.00	0.00