

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081721\
Data File : BP006688.D
Acq On : 16 Aug 2021 18:04
Operator : CG/JU
Sample : PB138482TB
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB138482TB

Integration Parameters: rteint.p
Integrator: RTE
Smoothing : ON Filtering: 5
Sampling : 1 Min Area: 3 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP080321.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BP006688.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.304	371	377	387	rBV	4523792	6323749	47.98%	11.207%
2	6.893	639	647	663	rVB	4229696	6580648	49.93%	11.662%
3	7.704	779	785	794	rVB	683142	1040001	7.89%	1.843%
4	8.863	974	982	994	rBV	2658387	4304344	32.66%	7.628%
5	10.487	1251	1258	1270	rVB	877692	1464745	11.11%	2.596%
6	12.969	1673	1680	1690	rBV	5866616	8576919	65.07%	15.199%
7	14.345	1907	1914	1924	rBV	1244005	1807917	13.72%	3.204%
8	15.845	2162	2169	2189	rBV	4598040	6348577	48.17%	11.251%
9	17.104	2376	2383	2393	rBV	1577763	2119762	16.08%	3.757%
10	19.692	2817	2823	2828	rBV	11149323	13180462	100.00%	23.358%
11	21.209	3076	3081	3088	rBV	1978027	2344007	17.78%	4.154%
12	23.527	3468	3475	3483	rVB2	1197401	2337854	17.74%	4.143%




Sum of corrected areas: 56428985

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081721\
Data File : BP006688.D
Acq On : 16 Aug 2021 18:04
Operator : CG/JU
Sample : PB138482TB
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB138482TB

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP080321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

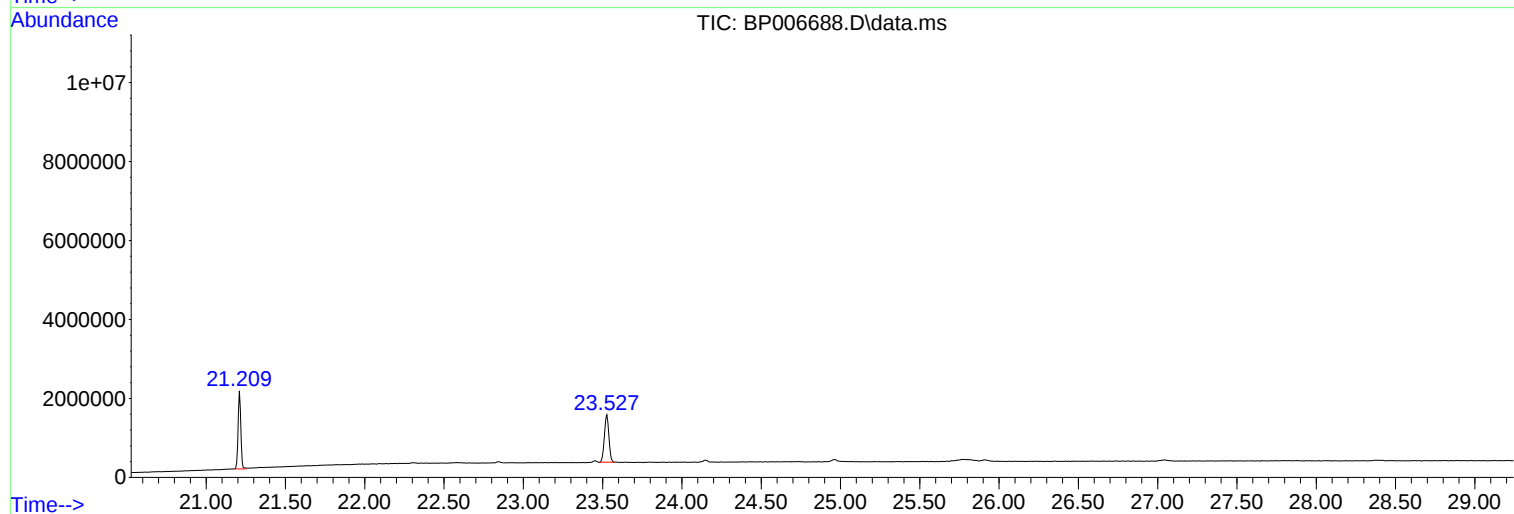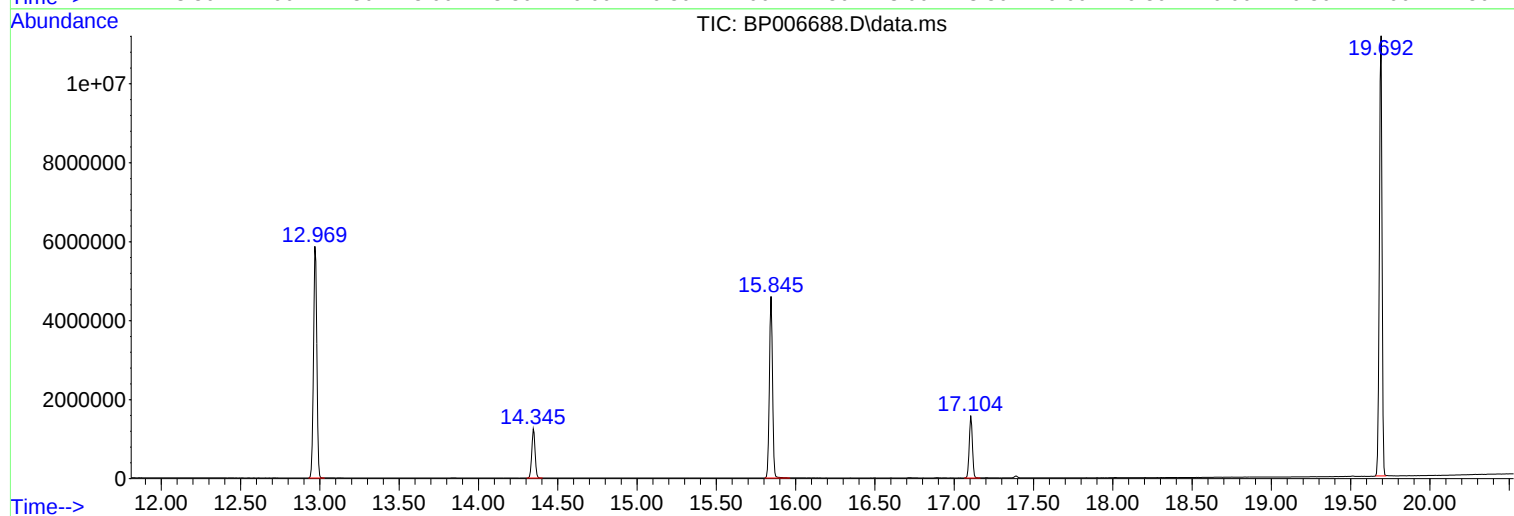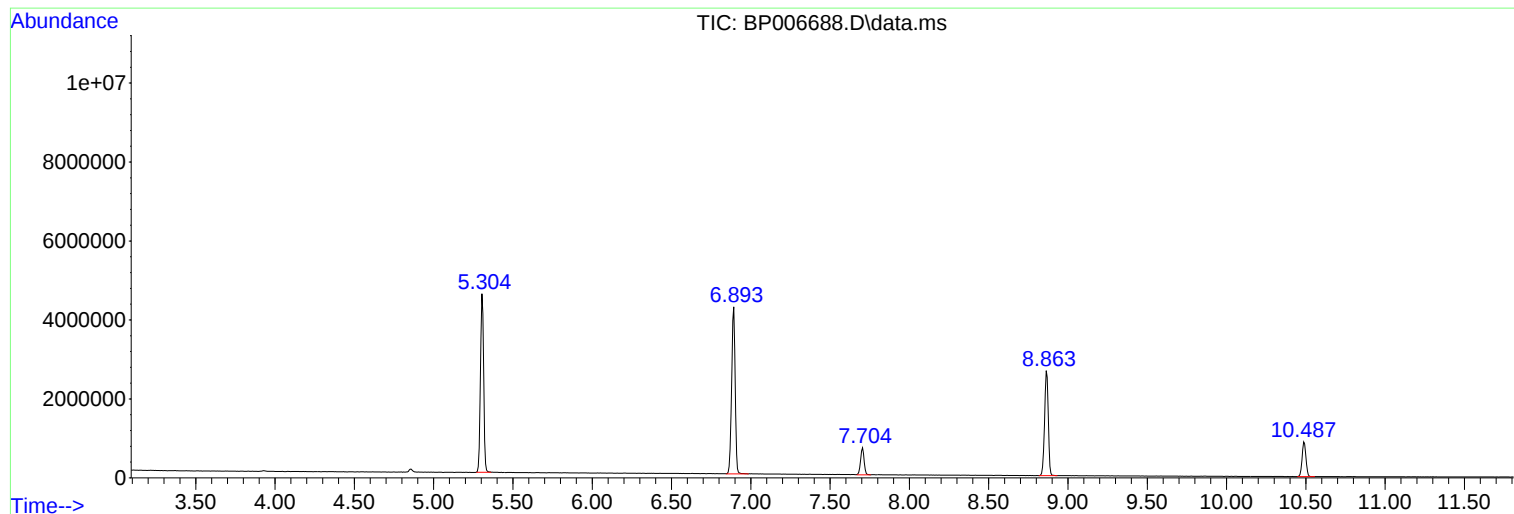

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081721\
Data File : BP006688.D
Acq On : 16 Aug 2021 18:04
Operator : CG/JU
Sample : PB138482TB
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB138482TB

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP080321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081721\
Data File : BP006688.D
Acq On : 16 Aug 2021 18:04
Operator : CG/JU
Sample : PB138482TB
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB138482TB

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP080321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------