

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081721\
 Data File : BP006700.D
 Acq On : 17 Aug 2021 00:54
 Operator : CG/JU
 Sample : M3389-01
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 CRT-21

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP080321.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BP006700.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.934	141	144	148	rVB	46937	59300	1.08%	0.176%
2	4.858	297	301	308	rVB	110898	164771	3.00%	0.488%
3	5.305	371	377	384	rBV	2007554	2777867	50.66%	8.222%
4	6.887	639	646	656	rBV	1949366	2953766	53.86%	8.743%
5	7.705	779	785	795	rVB	736865	1168330	21.31%	3.458%
6	8.864	975	982	990	rVB	1194526	1937990	35.34%	5.736%
7	10.293	1220	1225	1235	rVB2	31559	65169	1.19%	0.193%
8	10.487	1251	1258	1269	rVB	1034438	1684091	30.71%	4.985%
9	12.963	1671	1679	1691	rBV	2754479	3963938	72.29%	11.733%
10	14.346	1906	1914	1921	rBV	1436825	2065569	37.67%	6.114%
11	15.840	2159	2168	2180	rBV	2091036	2896365	52.82%	8.573%
12	17.098	2375	2382	2388	rBV	1645527	2359428	43.03%	6.984%
13	17.145	2388	2390	2395	rVB	54338	59812	1.09%	0.177%
14	18.010	2533	2537	2547	rBV2	133142	186140	3.39%	0.551%
15	19.122	2721	2726	2733	rBV	114509	155161	2.83%	0.459%
16	19.251	2744	2748	2754	rBV	81779	107711	1.96%	0.319%
17	19.475	2782	2786	2789	rBV	96473	108216	1.97%	0.320%
18	19.681	2816	2821	2830	rBV	4665462	5483671	100.00%	16.231%
19	20.939	3031	3035	3040	rBV2	197773	287092	5.24%	0.850%
20	21.204	3075	3080	3085	rBV	2133196	2607841	47.56%	7.719%
21	23.516	3467	3473	3488	rVB2	1374808	2693139	49.11%	7.971%

Sum of corrected areas: 33785367

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081721\
Data File : BP006700.D
Acq On : 17 Aug 2021 00:54
Operator : CG/JU
Sample : M3389-01
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
CRT-21










Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP080321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 2-Pentanone, 4-hydroxy-4-me... Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
4.858	2.82 ng	164771	1,4-Dichlorobenzene-d4	7.705

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1	2-Pentanone, 4-hydroxy-4-methyl-	116	C6H12O2	000123-42-2	72		
2	Propane, 1-ethoxy-2-methyl-	102	C6H14O	000627-02-1	38		
3	2-Hexanol, 2-methyl-	116	C7H16O	000625-23-0	38		
4	Acetic acid, cyano-, 1,1-dimethy...	141	C7H11NO2	001116-98-9	35		
5	Succinic acid, heptyl 2-methoxye...	274	C14H26O5	1000325-80-7	33		

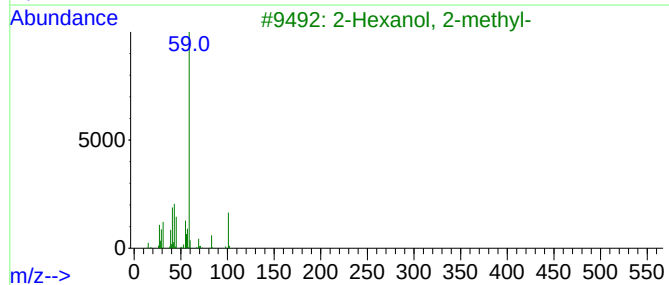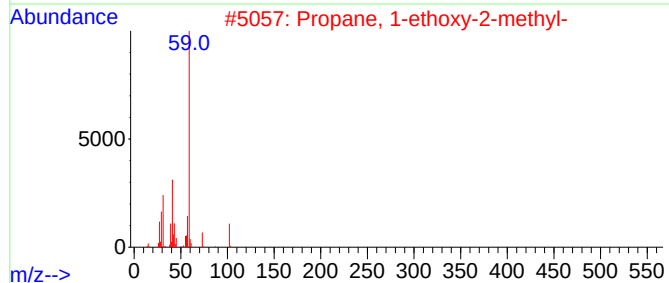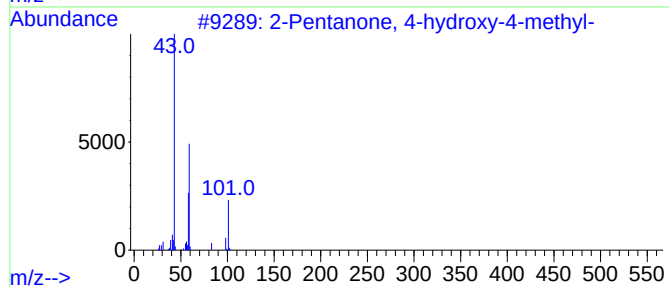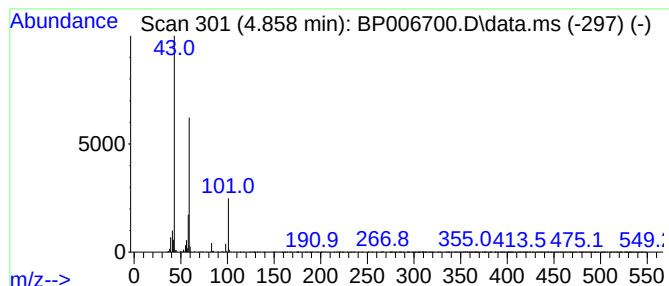

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081721\
Data File : BP006700.D
Acq On : 17 Aug 2021 00:54
Operator : CG/JU
Sample : M3389-01
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
CRT-21










Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP080321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 2 Ethanol, 2-(tetradecyloxy)- Concentration Rank 2

R.T.	EstConc	Area	Relative to ISTD	R.T.
20.939	2.20 ng	287092	Chrysene-d12	21.204

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Ethanol, 2-(tetradecyloxy)-	258	C16H34O2	002136-70-1	90
2			Pentadecafluorooctanoic acid, oc...	666	C26H37F15O2	1000406-04-8	87
3			Hexadecane	226	C16H34	000544-76-3	86
4			Triacontyl acetate	480	C32H64O2	041755-58-2	86
5			Cyclopropane, 1-(1,2-dimethylpro...	252	C18H36	041977-42-8	86

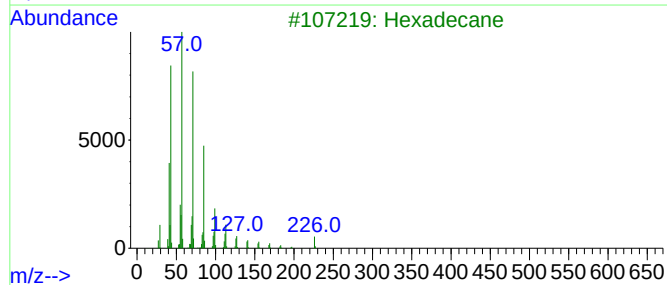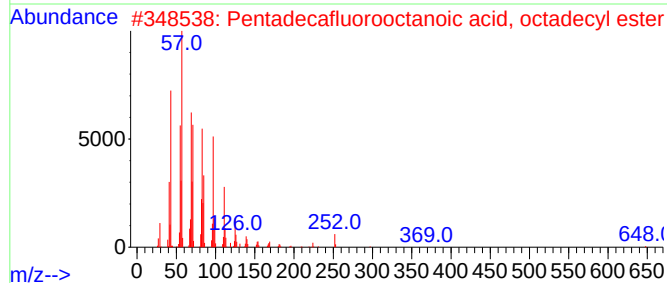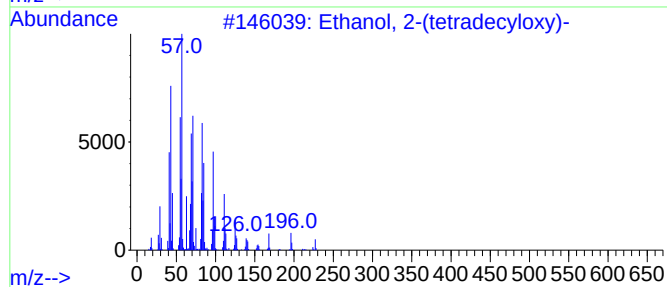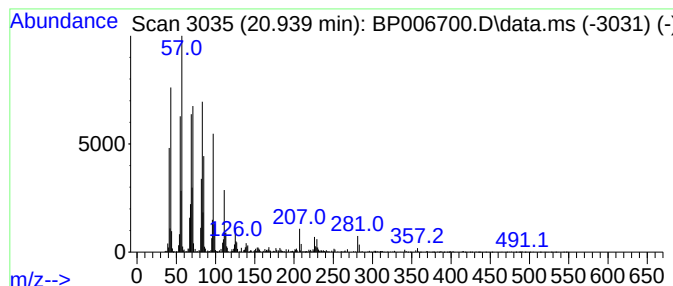

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081721\
Data File : BP006700.D
Acq On : 17 Aug 2021 00:54
Operator : CG/JU
Sample : M3389-01
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
CRT-21

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP080321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
2-Pentanone, 4-...	4.858	2.8	ng	164771	1	7.705	1168330	20.0
Ethanol, 2-(tet...	20.939	2.2	ng	287092	5	21.204	2607840	20.0