

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081721\
 Data File : BP006736.D
 Acq On : 18 Aug 2021 01:28
 Operator : CG/JU
 Sample : M3439-01 2X
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 HD-SOIL-COMP

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP080321.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BP006736.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.299	371	376	388	rVB	1230635	1799581	52.28%	5.847%
2	6.881	639	645	661	rVB	1254426	2017958	58.63%	6.557%
3	7.699	778	784	792	rVB	892350	1374855	39.94%	4.467%
4	8.857	975	981	990	rVB	834012	1322210	38.41%	4.296%
5	10.287	1220	1224	1232	rVB2	21202	38953	1.13%	0.127%
6	10.487	1250	1258	1271	rVB	1210187	2020538	58.70%	6.565%
7	12.963	1672	1679	1692	rBV	1872315	2734430	79.44%	8.885%
8	14.339	1903	1913	1920	rBV	1670776	2367754	68.79%	7.693%
9	14.404	1920	1924	1931	rVB	24922	40393	1.17%	0.131%
10	15.839	2159	2168	2186	rBV	1241344	1870826	54.35%	6.079%
11	17.098	2375	2382	2386	rBV	1887986	2566300	74.56%	8.339%
12	17.139	2386	2389	2394	rVB	225544	304007	8.83%	0.988%
13	17.233	2401	2405	2410	rVB	58534	82049	2.38%	0.267%
14	17.510	2442	2452	2461	rBV2	18673	50753	1.47%	0.165%
15	17.792	2496	2500	2503	rBV	37827	42084	1.22%	0.137%
16	18.010	2533	2537	2546	rVB3	138769	207810	6.04%	0.675%
17	18.163	2558	2563	2567	rBV3	60317	95820	2.78%	0.311%
18	18.463	2610	2614	2617	rBV2	28042	35690	1.04%	0.116%
19	18.904	2686	2689	2691	rBV2	35439	44665	1.30%	0.145%
20	18.927	2691	2693	2701	rVB4	69980	96148	2.79%	0.312%
21	19.122	2720	2726	2733	rBV	579374	790795	22.98%	2.570%
22	19.251	2744	2748	2754	rBV3	76037	107853	3.13%	0.350%
23	19.474	2777	2786	2795	rBV	519120	857300	24.91%	2.786%
24	19.680	2816	2821	2833	rVB	2901204	3441973	100.00%	11.184%
25	19.957	2865	2868	2872	rVB	70043	89668	2.61%	0.291%
26	20.057	2882	2885	2888	rBV2	72416	76977	2.24%	0.250%
27	20.939	3031	3035	3040	rBV3	181059	277263	8.06%	0.901%
28	21.204	3074	3080	3084	rBV	2286688	3111080	90.39%	10.109%
29	21.239	3084	3086	3093	rVB	264298	296457	8.61%	0.963%
30	23.515	3467	3473	3480	rBV2	1371499	2613920	75.94%	8.493%




Sum of corrected areas: 30776110

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081721\
Data File : BP006736.D
Acq On : 18 Aug 2021 01:28
Operator : CG/JU
Sample : M3439-01 2X
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
HD-SOIL-COMP

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP080321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

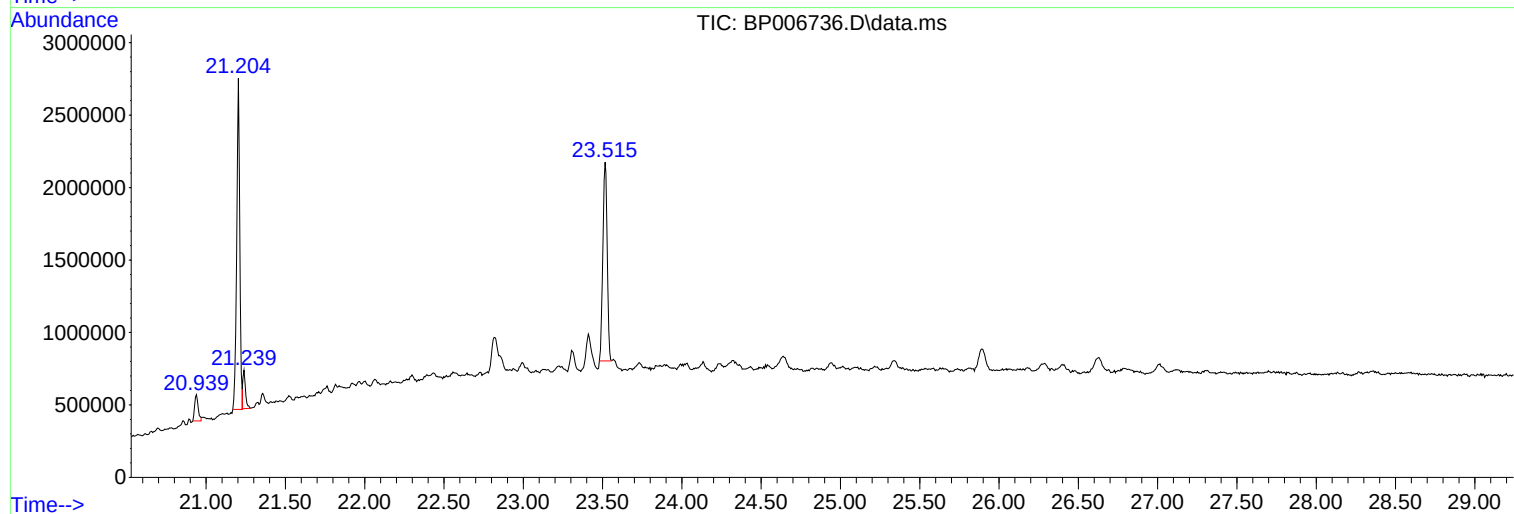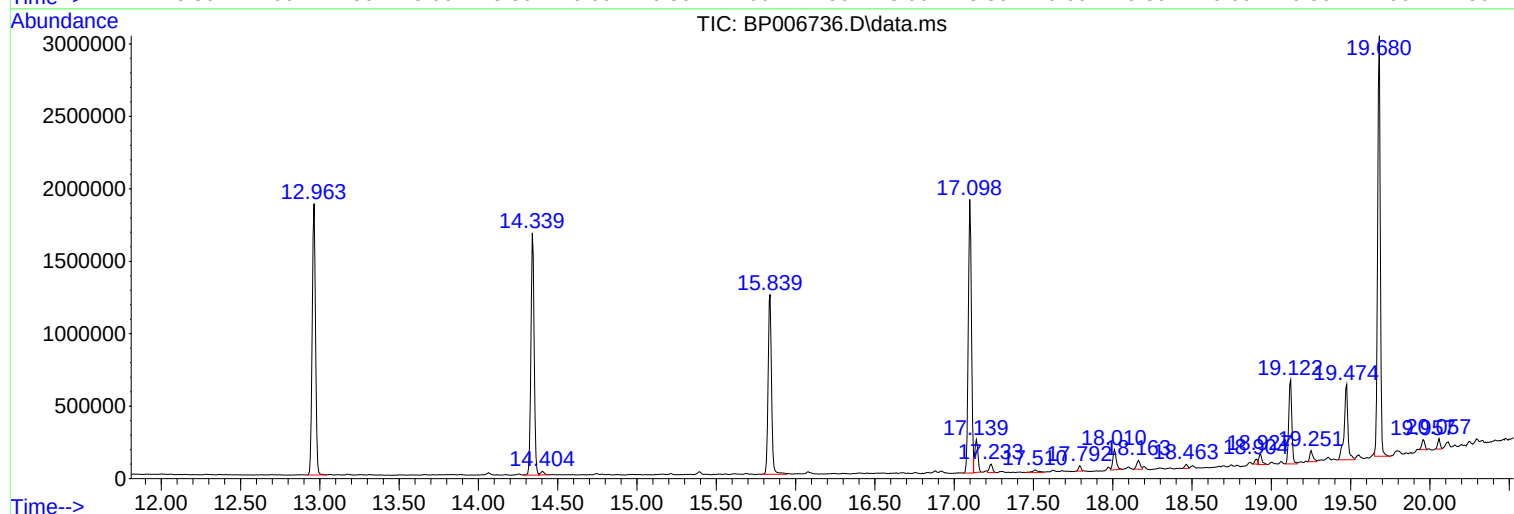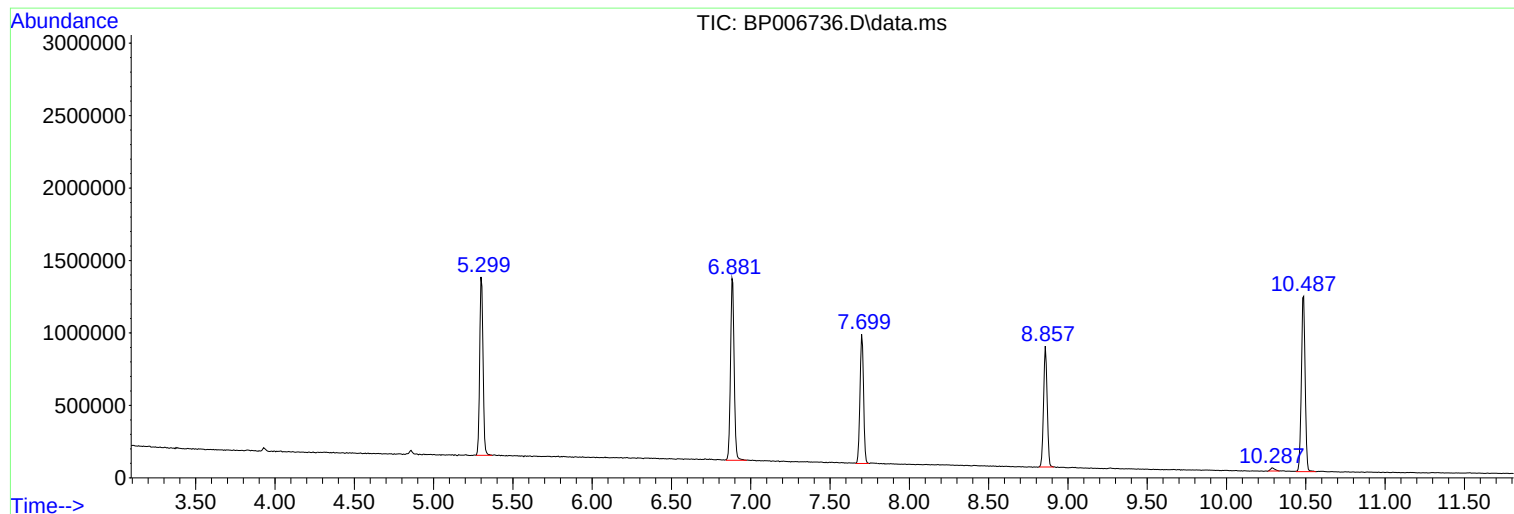

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081721\
Data File : BP006736.D
Acq On : 18 Aug 2021 01:28
Operator : CG/JU
Sample : M3439-01 2X
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
HD-SOIL-COMP

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP080321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081721\
Data File : BP006736.D
Acq On : 18 Aug 2021 01:28
Operator : CG/JU
Sample : M3439-01 2X
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
HD-SOIL-COMP

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP080321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------