
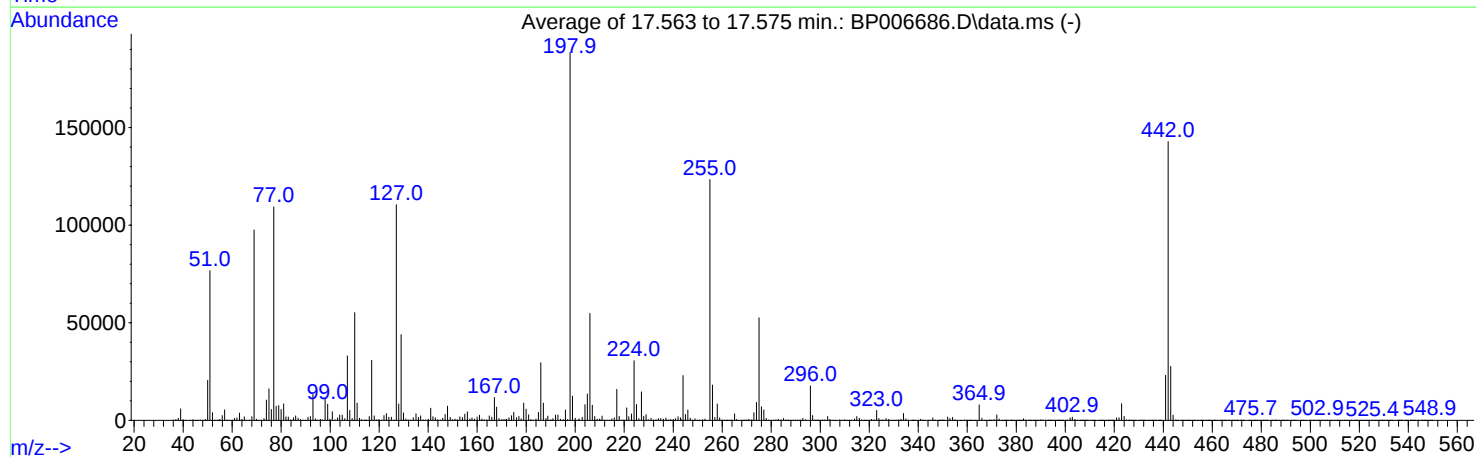


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081721\
 Data File : BP006686.D
 Acq On : 16 Aug 2021 16:53
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP080321.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Aug 16 18:17:59 2021

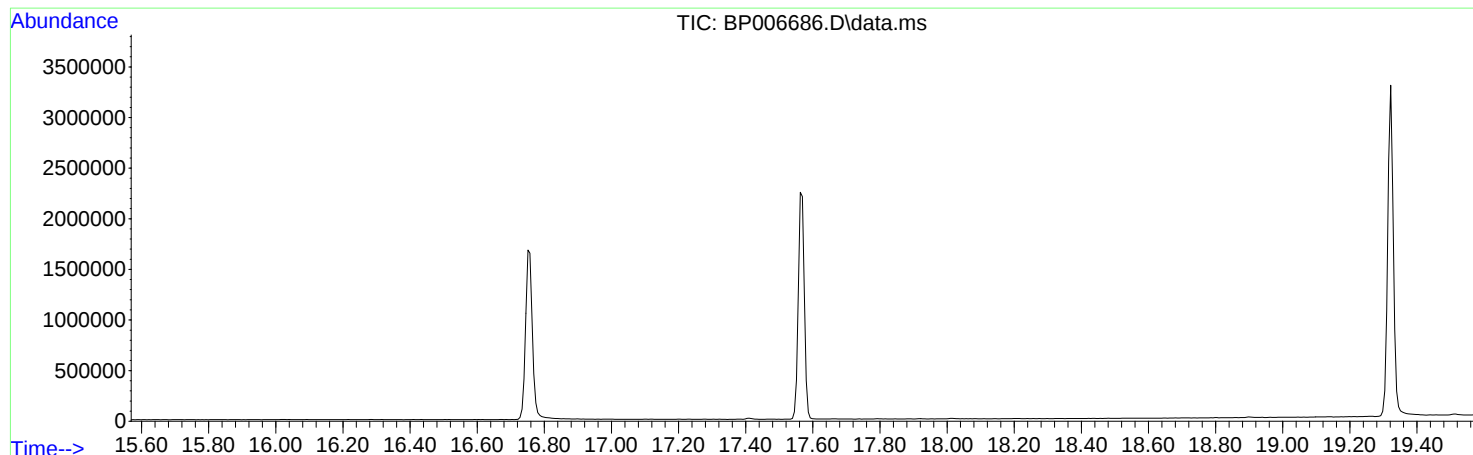




AutoFind: Scans 2461, 2462, 2463; Background Corrected with Scan 2452

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	40.7	76691	PASS
68	69	0.00	2	1.9	1865	PASS
69	198	0.00	100	51.8	97539	PASS
70	69	0.00	2	0.6	588	PASS
127	198	10	80	58.6	110453	PASS
197	198	0.00	2	0.2	425	PASS
198	198	100	100	100.0	188429	PASS
199	198	5	9	6.6	12435	PASS
275	198	10	60	27.9	52574	PASS
365	198	1	100	4.2	7985	PASS
441	198	0.01	100	12.3	23131	PASS
442	442	100	100	100.0	142797	PASS
443	442	15	24	19.3	27617	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081721\
 Data File : BP006686.D
 Acq On : 16 Aug 2021 16:53
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Quant Time: Aug 16 18:13:16 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP080321.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Aug 03 15:41:30 2021
 Response via : Initial Calibration

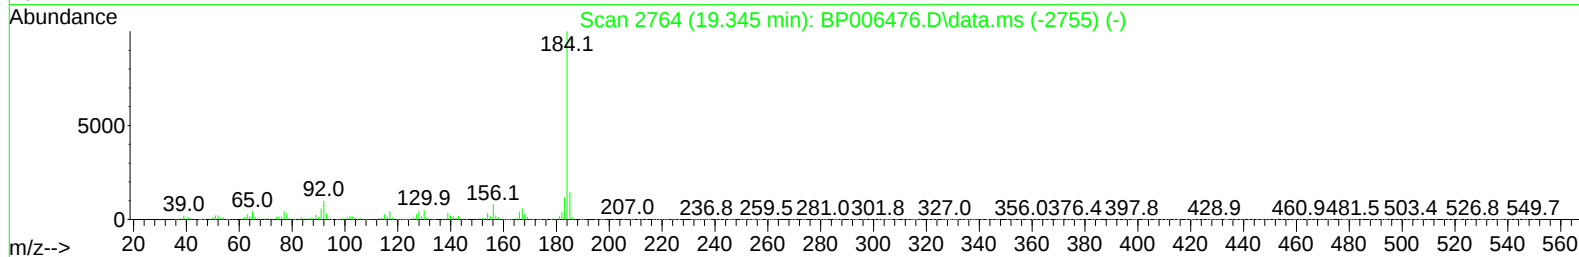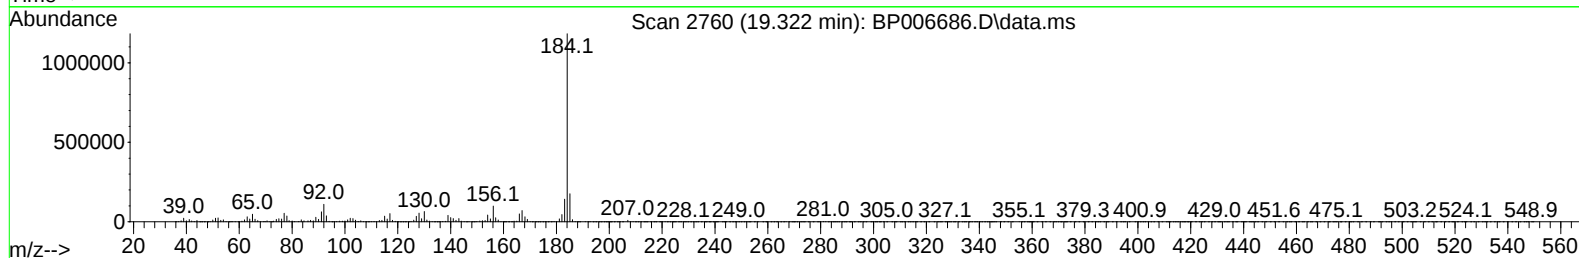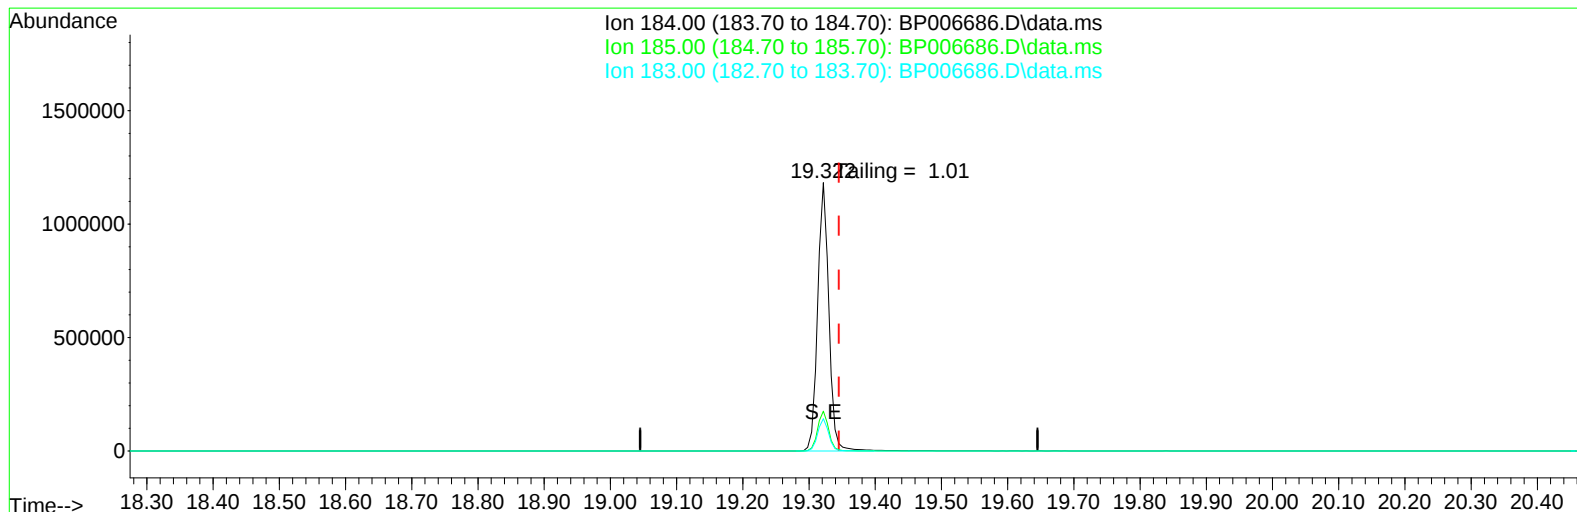

TIC: BP006686.D\data.ms

(77) Benzidine

19.322min (-0.024) 781004.84 ng




response 1387577

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.70	14.86
183.00	11.90	12.03
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081721\
 Data File : BP006686.D
 Acq On : 16 Aug 2021 16:53
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Quant Time: Aug 16 18:13:16 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP080321.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Aug 03 15:41:30 2021
 Response via : Initial Calibration

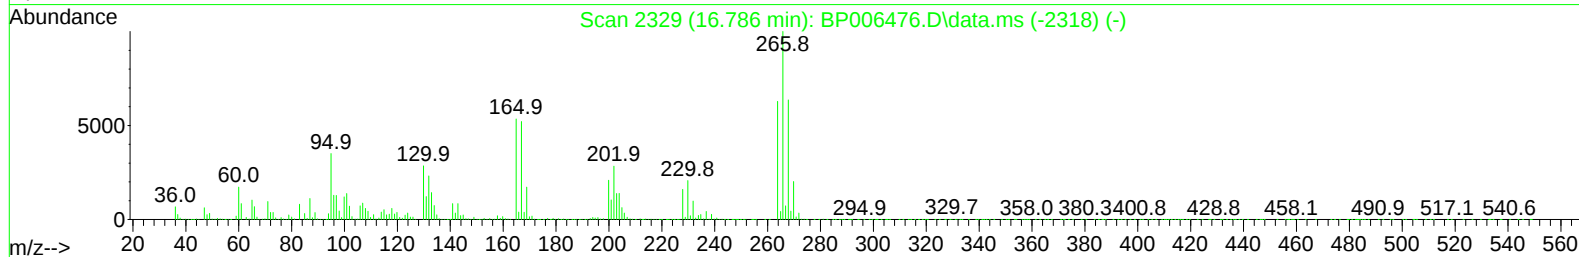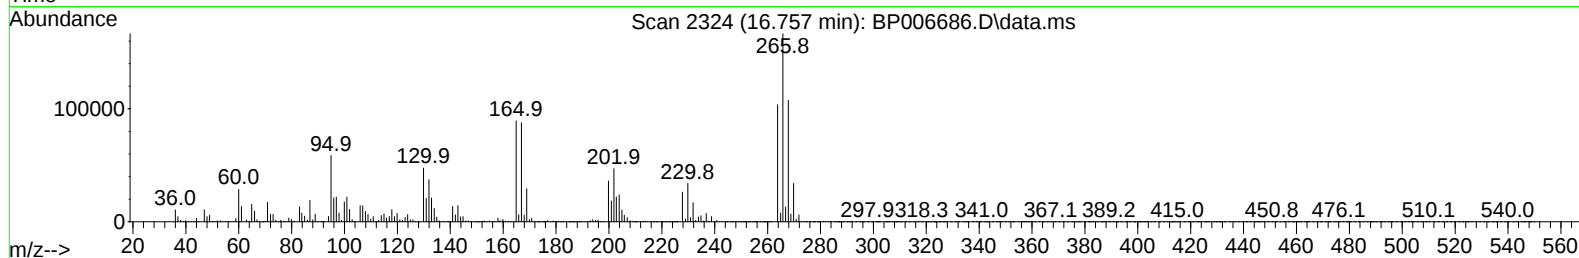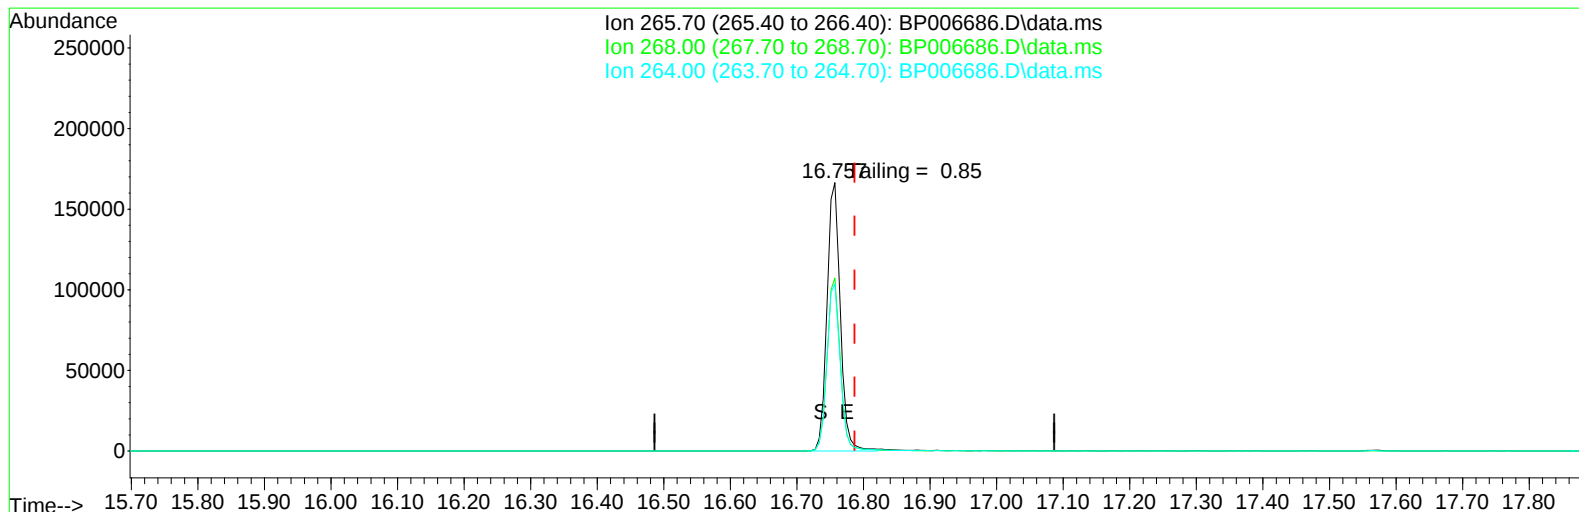

TIC: BP006686.D\data.ms

(70) Pentachlorophenol (C)

16.757min (-0.029) 1053627.50 ng

response 233577

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.50	64.49
264.00	62.90	62.26
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
8/17/2021	BNA_P	<u>BP006686.D</u>
Compound Name	Response	Retention Time
DDT	683960	20.52
DDD	7051	20.09
DDE	1149	19.59
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
8200	692160	1.18

Instrument :
BNA_P
ClientSampleId :
DFTPP