
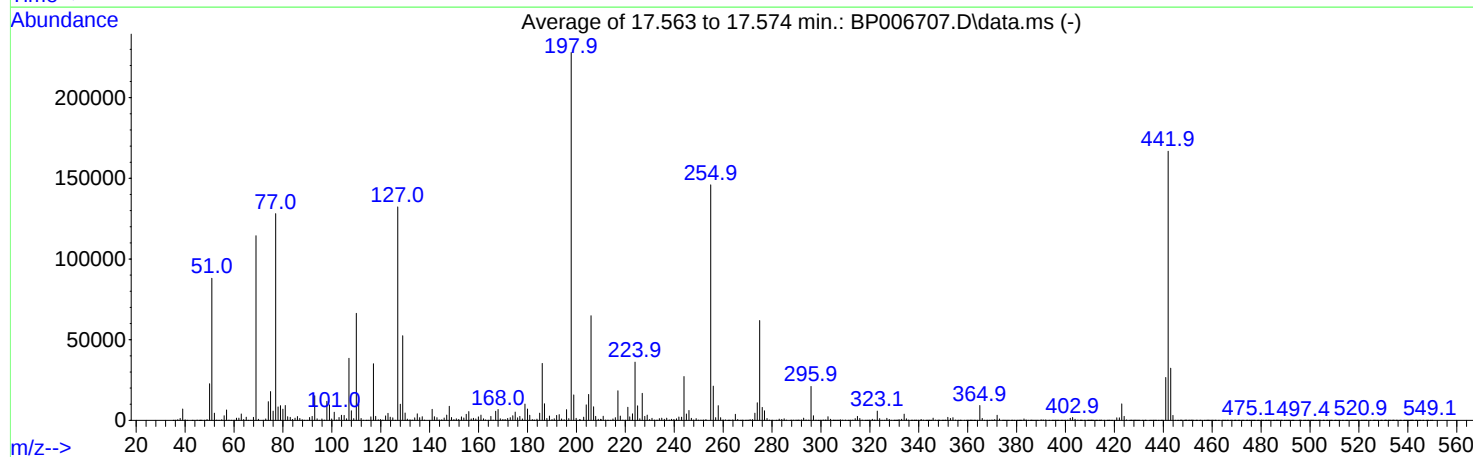


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081721\
 Data File : BP006707.D
 Acq On : 17 Aug 2021 08:40
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP080321.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Aug 16 18:17:59 2021

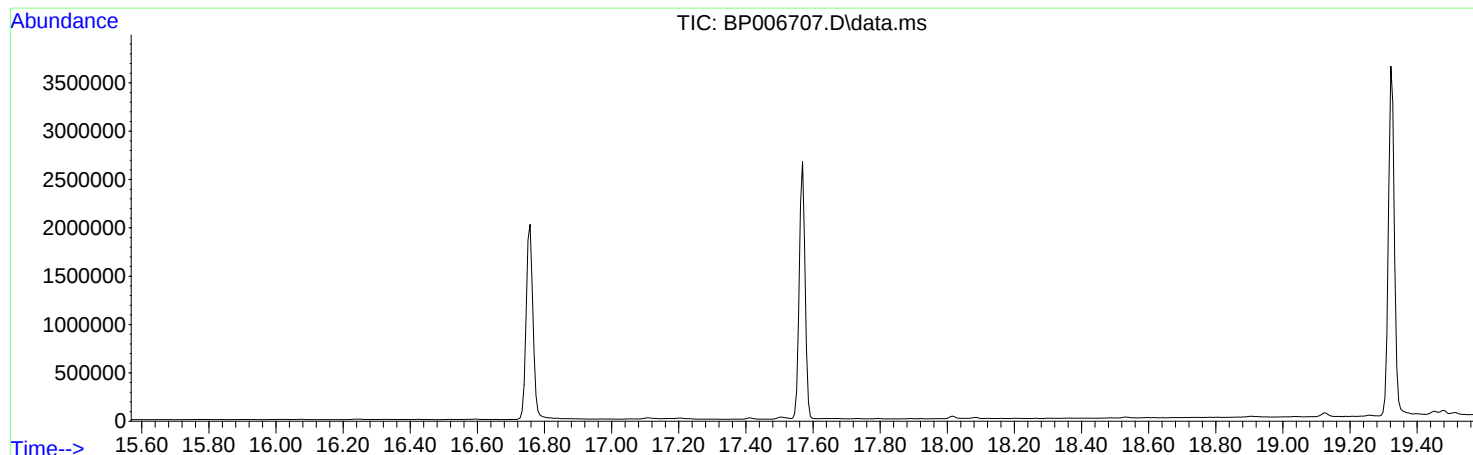




AutoFind: Scans 2461, 2462, 2463; Background Corrected with Scan 2451

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	38.6	88069	PASS
68	69	0.00	2	1.7	1943	PASS
69	198	0.00	100	50.2	114441	PASS
70	69	0.00	2	0.6	712	PASS
127	198	10	80	58.0	132300	PASS
197	198	0.00	2	0.5	1068	PASS
198	198	100	100	100.0	227994	PASS
199	198	5	9	6.9	15786	PASS
275	198	10	60	27.1	61875	PASS
365	198	1	100	4.0	9214	PASS
441	198	0.01	100	11.7	26592	PASS
442	442	100	100	100.0	166799	PASS
443	442	15	24	19.4	32351	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081721\
Data File : BP006707.D
Acq On : 17 Aug 2021 08:40
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: Aug 17 11:27:24 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP080321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Aug 16 18:17:59 2021
Response via : Initial Calibration

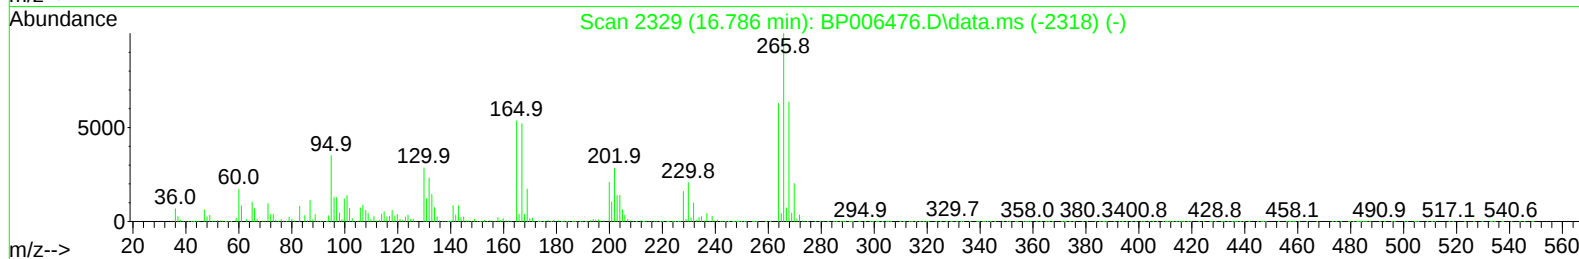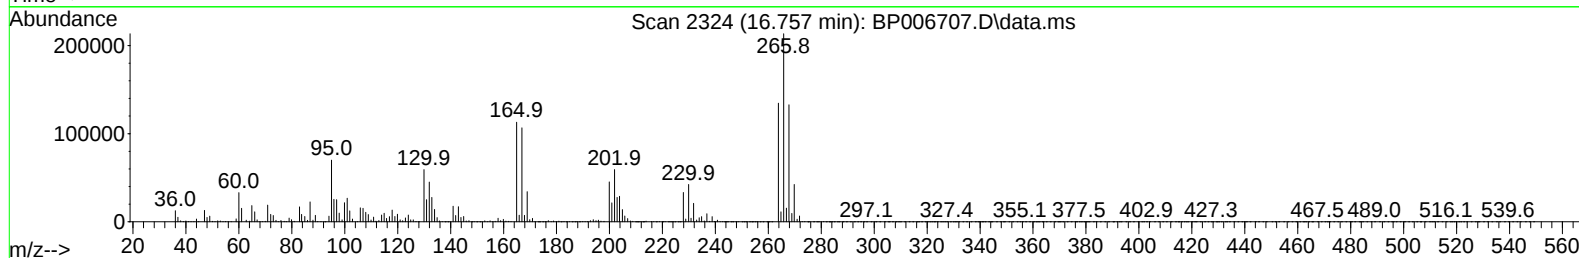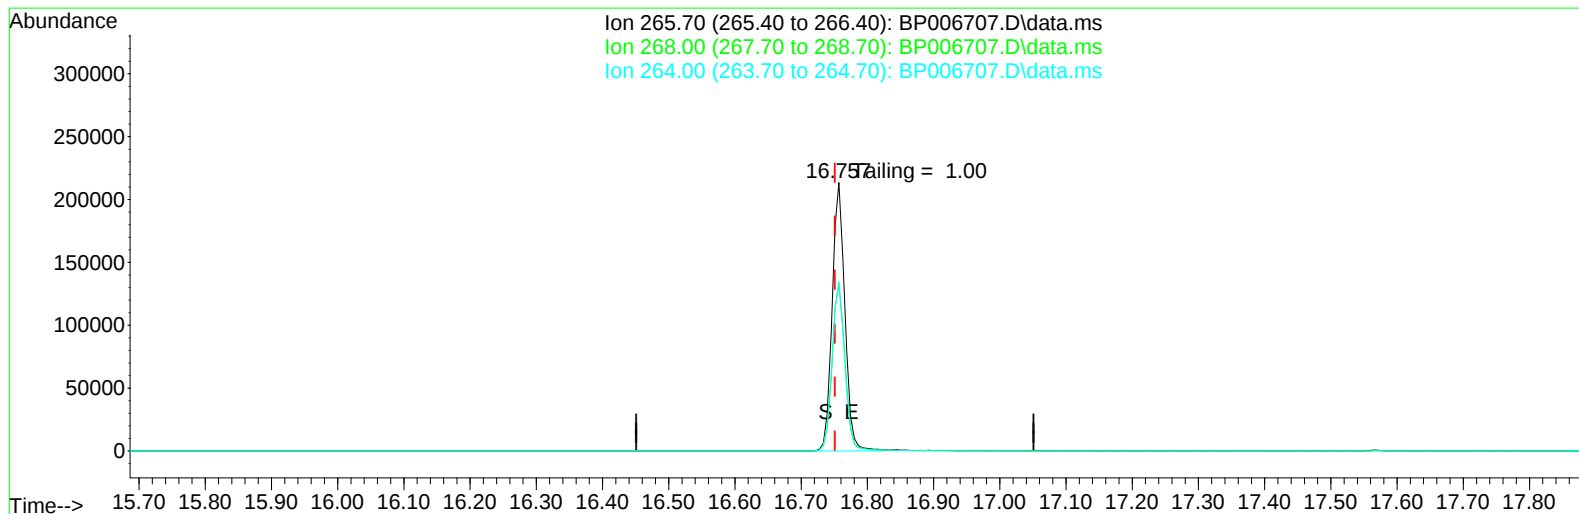

TIC: BP006707.D\data.ms

(70) Pentachlorophenol (C)

16.757min (+ 0.006) 16962.56 ng




response 288611

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.50	62.25
264.00	62.90	63.09
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081721\
 Data File : BP006707.D
 Acq On : 17 Aug 2021 08:40
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Quant Time: Aug 17 11:27:24 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP080321.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Aug 16 18:17:59 2021
 Response via : Initial Calibration

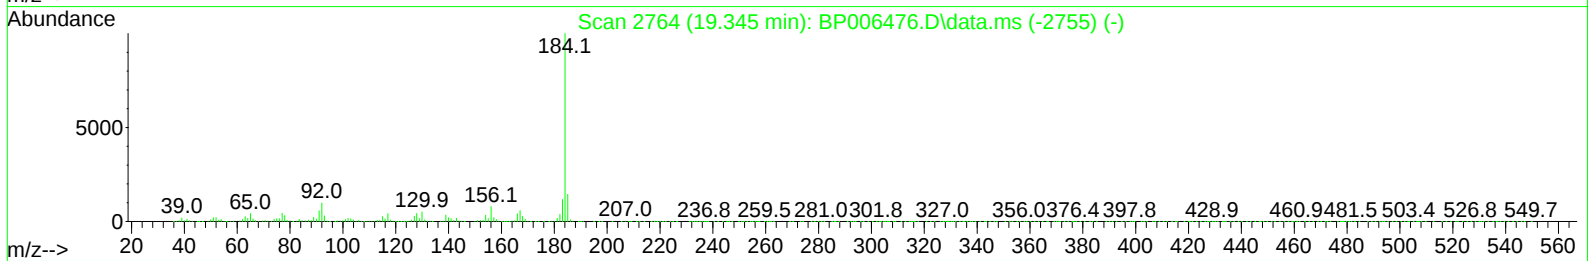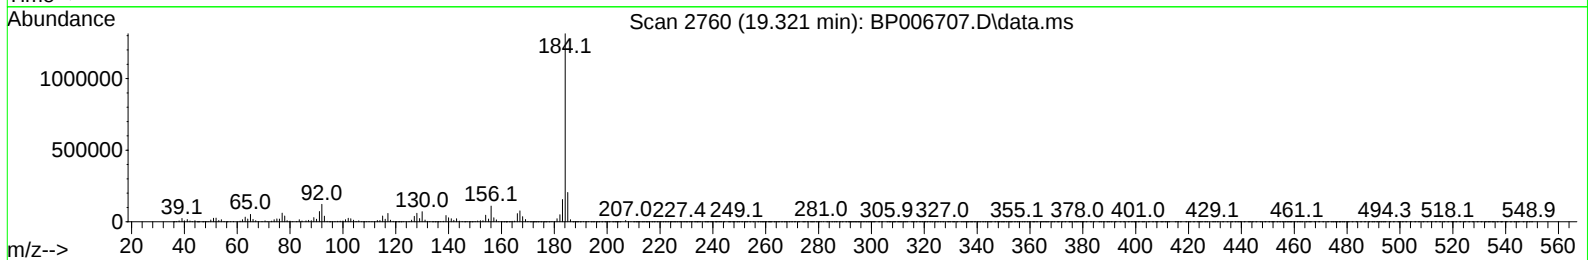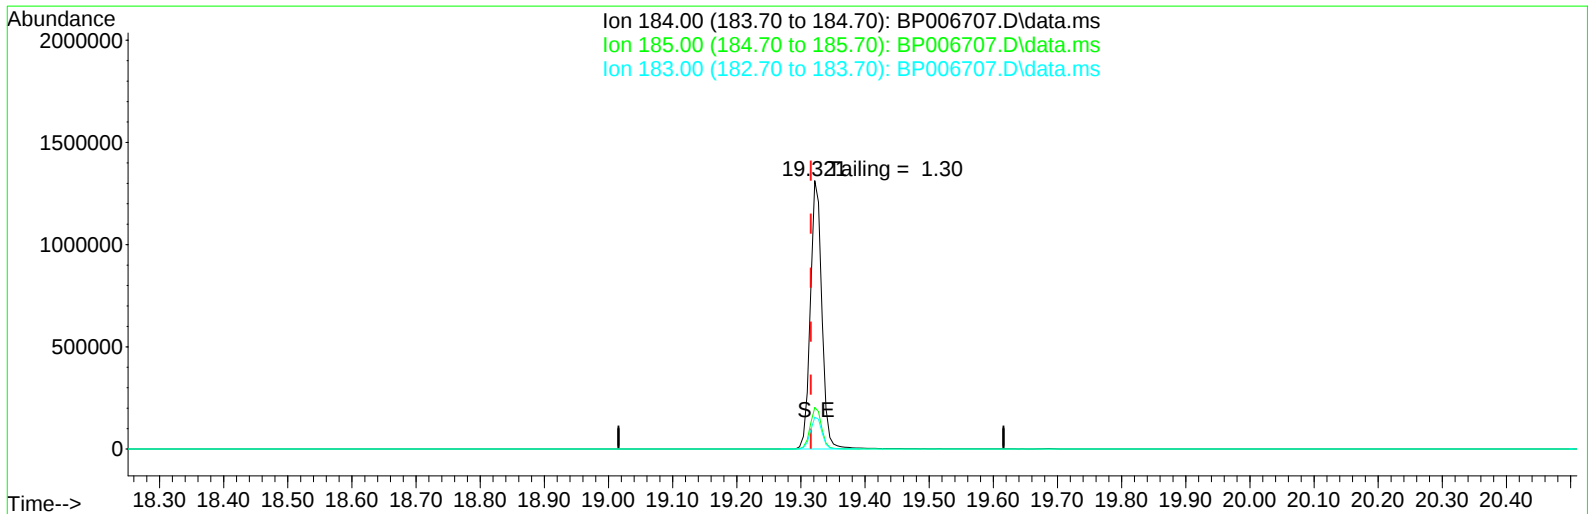

TIC: BP006707.D\data.ms

(77) Benzidine

19.321min (+ 0.006) 3727.76 ng

response 1652751

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.70	15.54
183.00	11.90	11.87
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
8/17/2021	BNA_P	<u>BP006707.D</u>
Compound Name	Response	Retention Time
DDT	737559	20.52
DDD	53815	20.09
DDE	1787	19.59
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
55602	793161	7.01

Instrument :
BNA_P
ClientSampleId :
DFTPP