
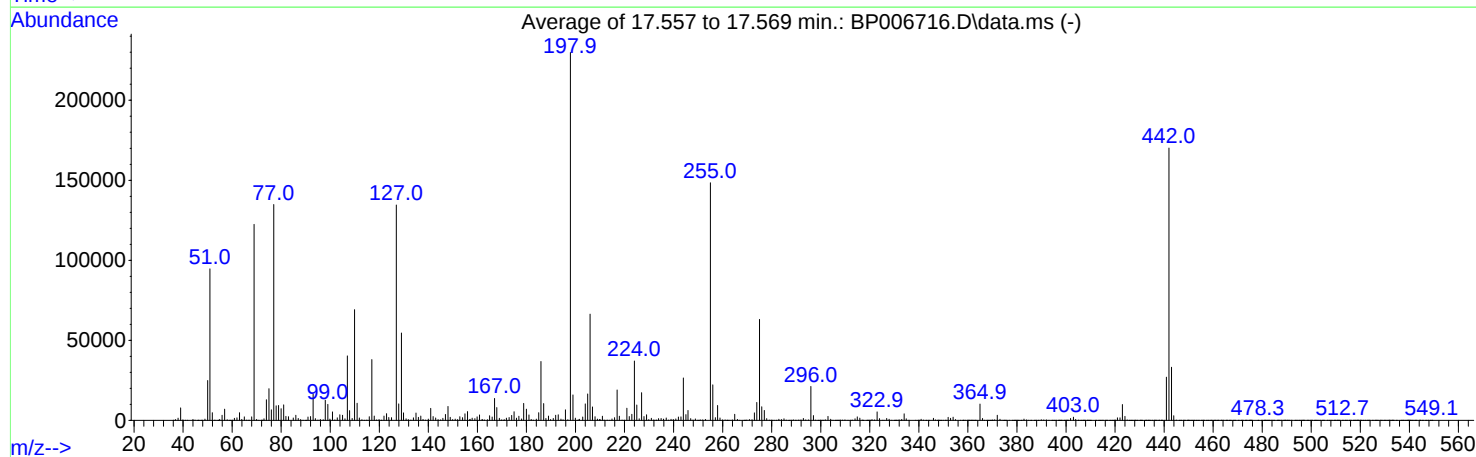


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081721\
 Data File : BP006716.D
 Acq On : 17 Aug 2021 14:00
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP080321.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Aug 16 18:17:59 2021

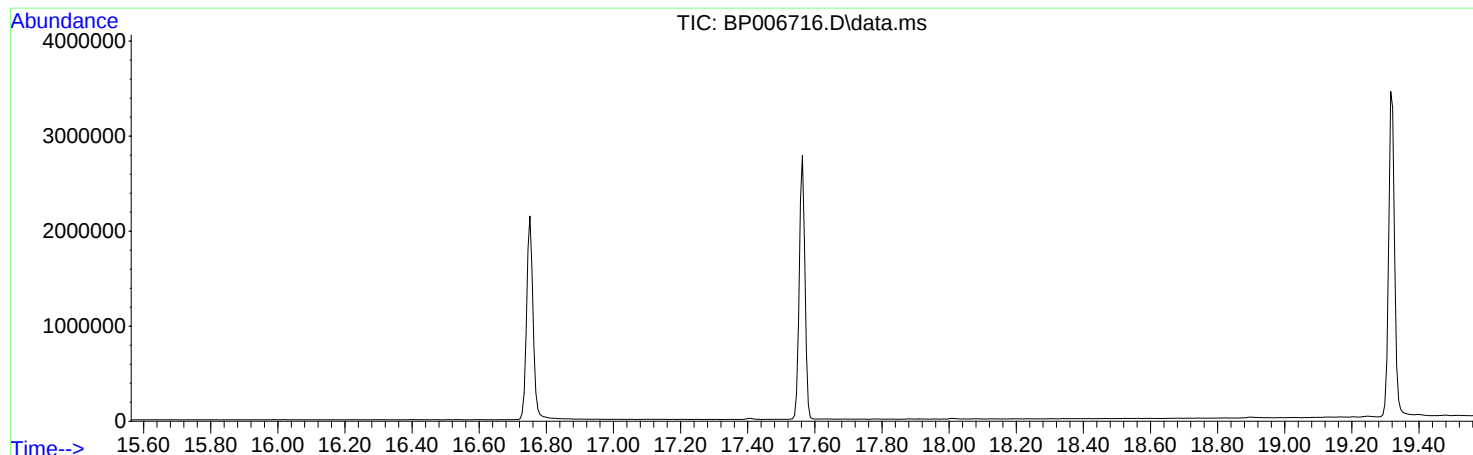




AutoFind: Scans 2460, 2461, 2462; Background Corrected with Scan 2452

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	41.2	94715	PASS
68	69	0.00	2	1.8	2213	PASS
69	198	0.00	100	53.3	122490	PASS
70	69	0.00	2	0.5	579	PASS
127	198	10	80	58.5	134567	PASS
197	198	0.00	2	0.2	416	PASS
198	198	100	100	100.0	229840	PASS
199	198	5	9	6.9	15949	PASS
275	198	10	60	27.5	63117	PASS
365	198	1	100	4.4	10194	PASS
441	198	0.01	100	11.7	27003	PASS
442	442	100	100	100.0	170183	PASS
443	442	15	24	19.5	33208	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081721\
Data File : BP006716.D
Acq On : 17 Aug 2021 14:00
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: Aug 17 14:36:48 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP080321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Aug 16 18:17:59 2021
Response via : Initial Calibration

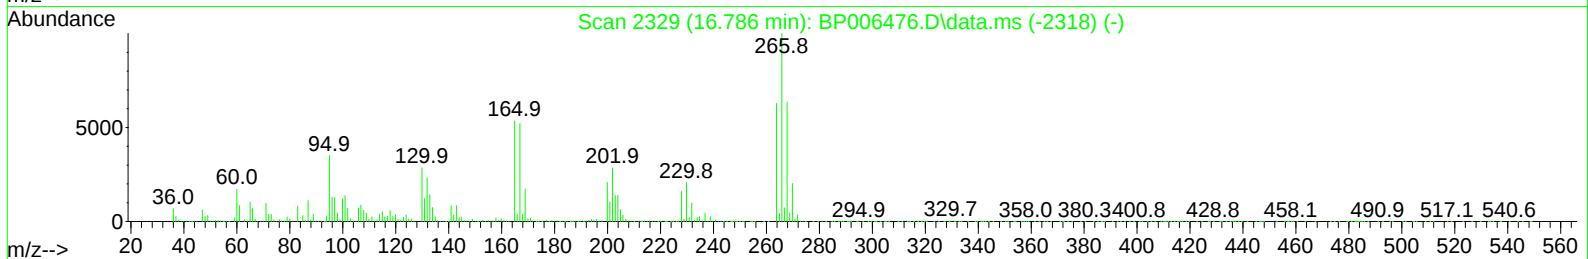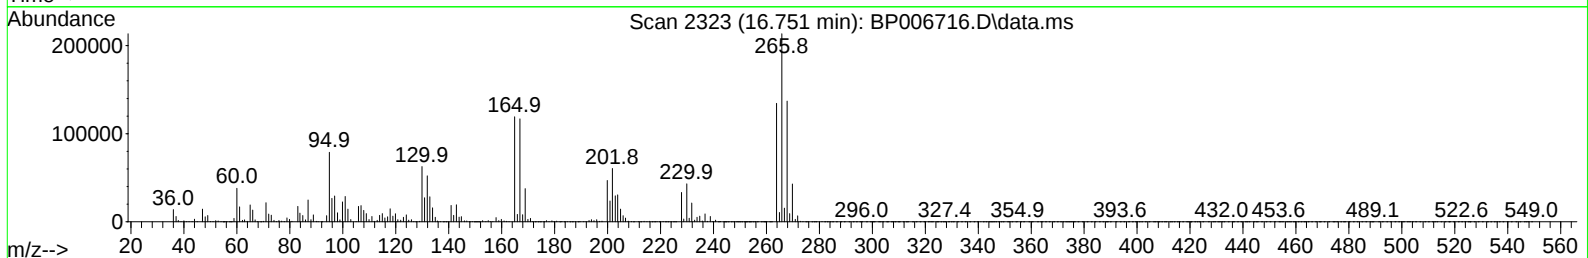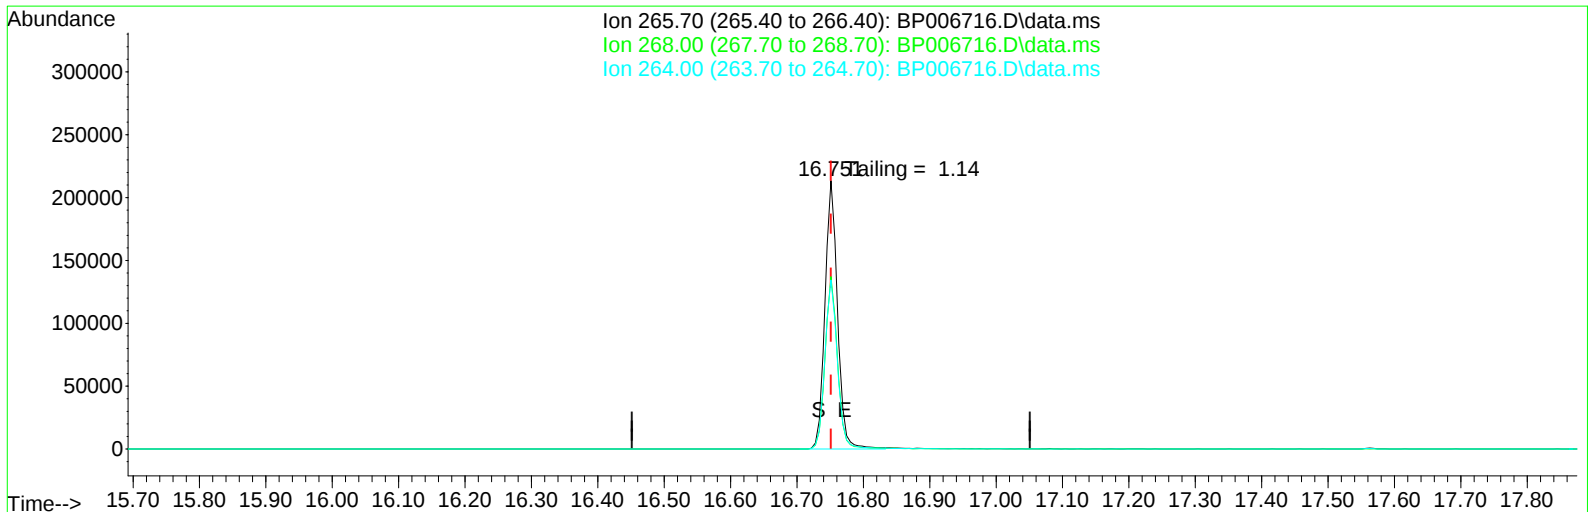

TIC: BP006716.D\data.ms

(70) Pentachlorophenol (C)

16.751min (+ 0.000) 2143062.96 ng




response 282086

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.50	64.21
264.00	62.90	62.95
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081721\
 Data File : BP006716.D
 Acq On : 17 Aug 2021 14:00
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Quant Time: Aug 17 14:36:48 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP080321.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Aug 16 18:17:59 2021
 Response via : Initial Calibration

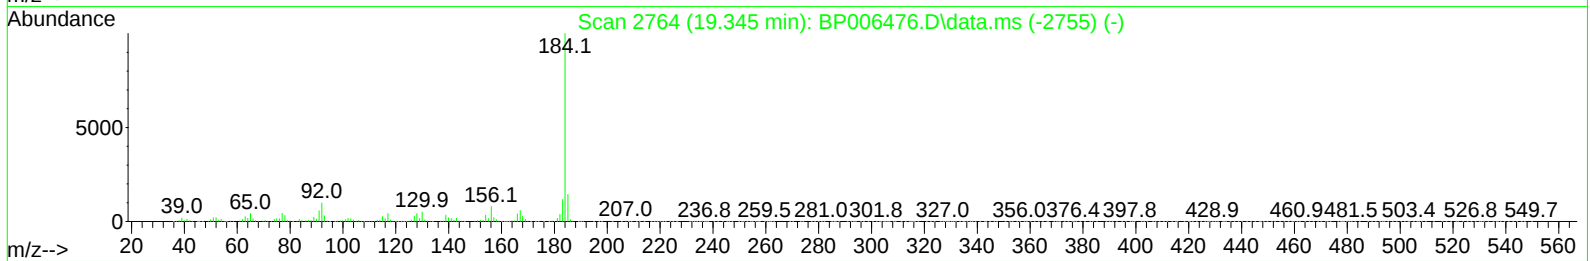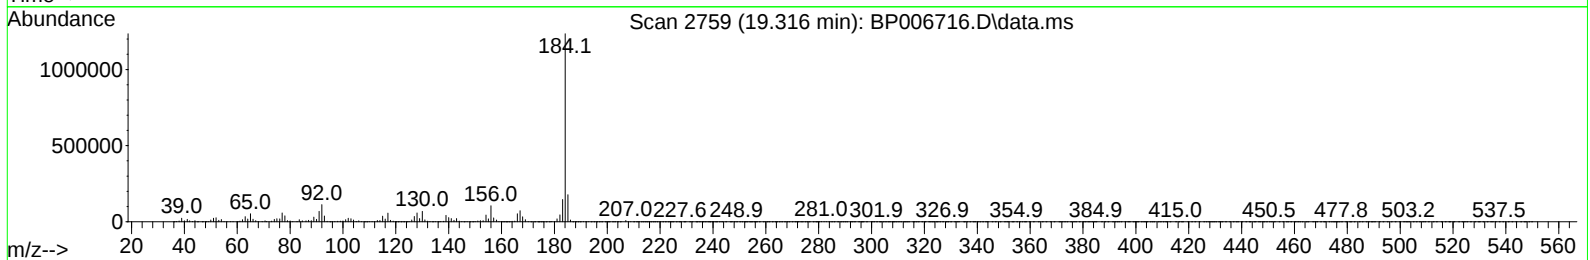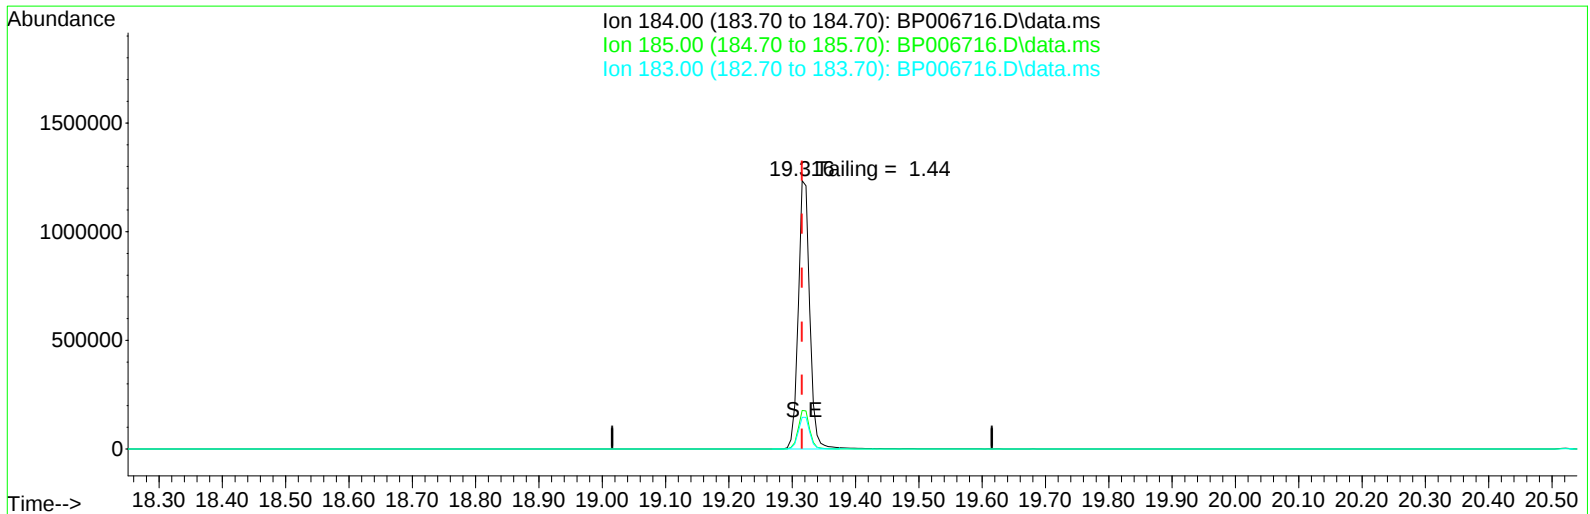

TIC: BP006716.D\data.ms

(77) Benzidine

19.316min (+ 0.000) 23909.43 ng

response 1559751

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.70	14.40
183.00	11.90	11.85
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
8/17/2021	BNA_P	<u>BP006716.D</u>
Compound Name	Response	Retention Time
DDT	710556	20.52
DDD	50323	20.09
DDE	2151	19.59
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
52474	763030	6.88

Instrument :
BNA_P
ClientSampleId :
DFTPP