

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081722\
 Data File : BP011472.D
 Acq On : 17 Aug 2022 21:38
 Operator : CG/JU
 Sample : N4028-03 10X
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :

Quant Time: Aug 17 23:33:43 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP081622.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Aug 17 01:58:37 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.557	152	95964	20.000	ng/u1	0.00
20) Naphthalene-d8	10.346	136	400733	20.000	ng/u1	0.00
38) Acenaphthene-d10	14.234	164	222228	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.004	188	440442	20.000	ng/u1	0.00
79) Chrysene-d12	21.133	240	424735	20.000	ng/u1	0.00
88) Perylene-d12	23.427	264	451818	20.000	ng/u1	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.069	96	6605	2.136	ng/uL	0.00
4) Pyridine-d5	3.481	84	65543	8.278	ng/u1	0.00
7) Phenol-d5	6.740	99	49190	5.578	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	6.905	67	154823	27.023	ng/u1	0.00
11) 2-Chlorophenol-d4	7.093	132	149844	23.102	ng/u1	0.00
15) 4-Methylphenol-d8	8.281	113	92872	13.158	ng/u1	0.00
21) Nitrobenzene-d5	8.722	128	92591	32.094	ng/u1	0.00
24) 2-Nitrophenol-d4	9.440	143	94547	32.201	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	9.975	165	141038	26.023	ng/u1	0.00
31) 4-Chloroaniline-d4	10.498	131	222569	24.670	ng/u1	0.00
46) Dimethylphthalate-d6	13.657	166	498218	31.698	ng/u1	0.00
49) Acenaphthylene-d8	13.922	160	557642	31.921	ng/u1	0.00
54) 4-Nitrophenol-d4	14.469	143	11089	3.662	ng/u1	0.00
60) Fluorene-d10	15.234	176	429745	32.499	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.375	200	68496	28.781	ng/u1	0.00
73) Anthracene-d10	17.104	188	718978	36.858	ng/u1	0.00
81) Pyrene-d10	19.363	212	793895	36.944	ng/u1	0.00
92) Benzo(a)pyrene-d12	23.274	264	814935	37.079	ng/u1	0.00
Target Compounds						
					Qvalue	
16) Acetophenone	8.393	105	12299	1.047	ng/u1	98
71) Pentachlorophenol	16.651	266	7666	2.729	ng/u1	88


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081722\
Data File : BP011472.D
Acq On : 17 Aug 2022 21:38
Operator : CG/JU
Sample : N4028-03 10X
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :

Quant Time: Aug 17 23:33:43 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP081622.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Aug 17 01:58:37 2022
Response via : Initial Calibration




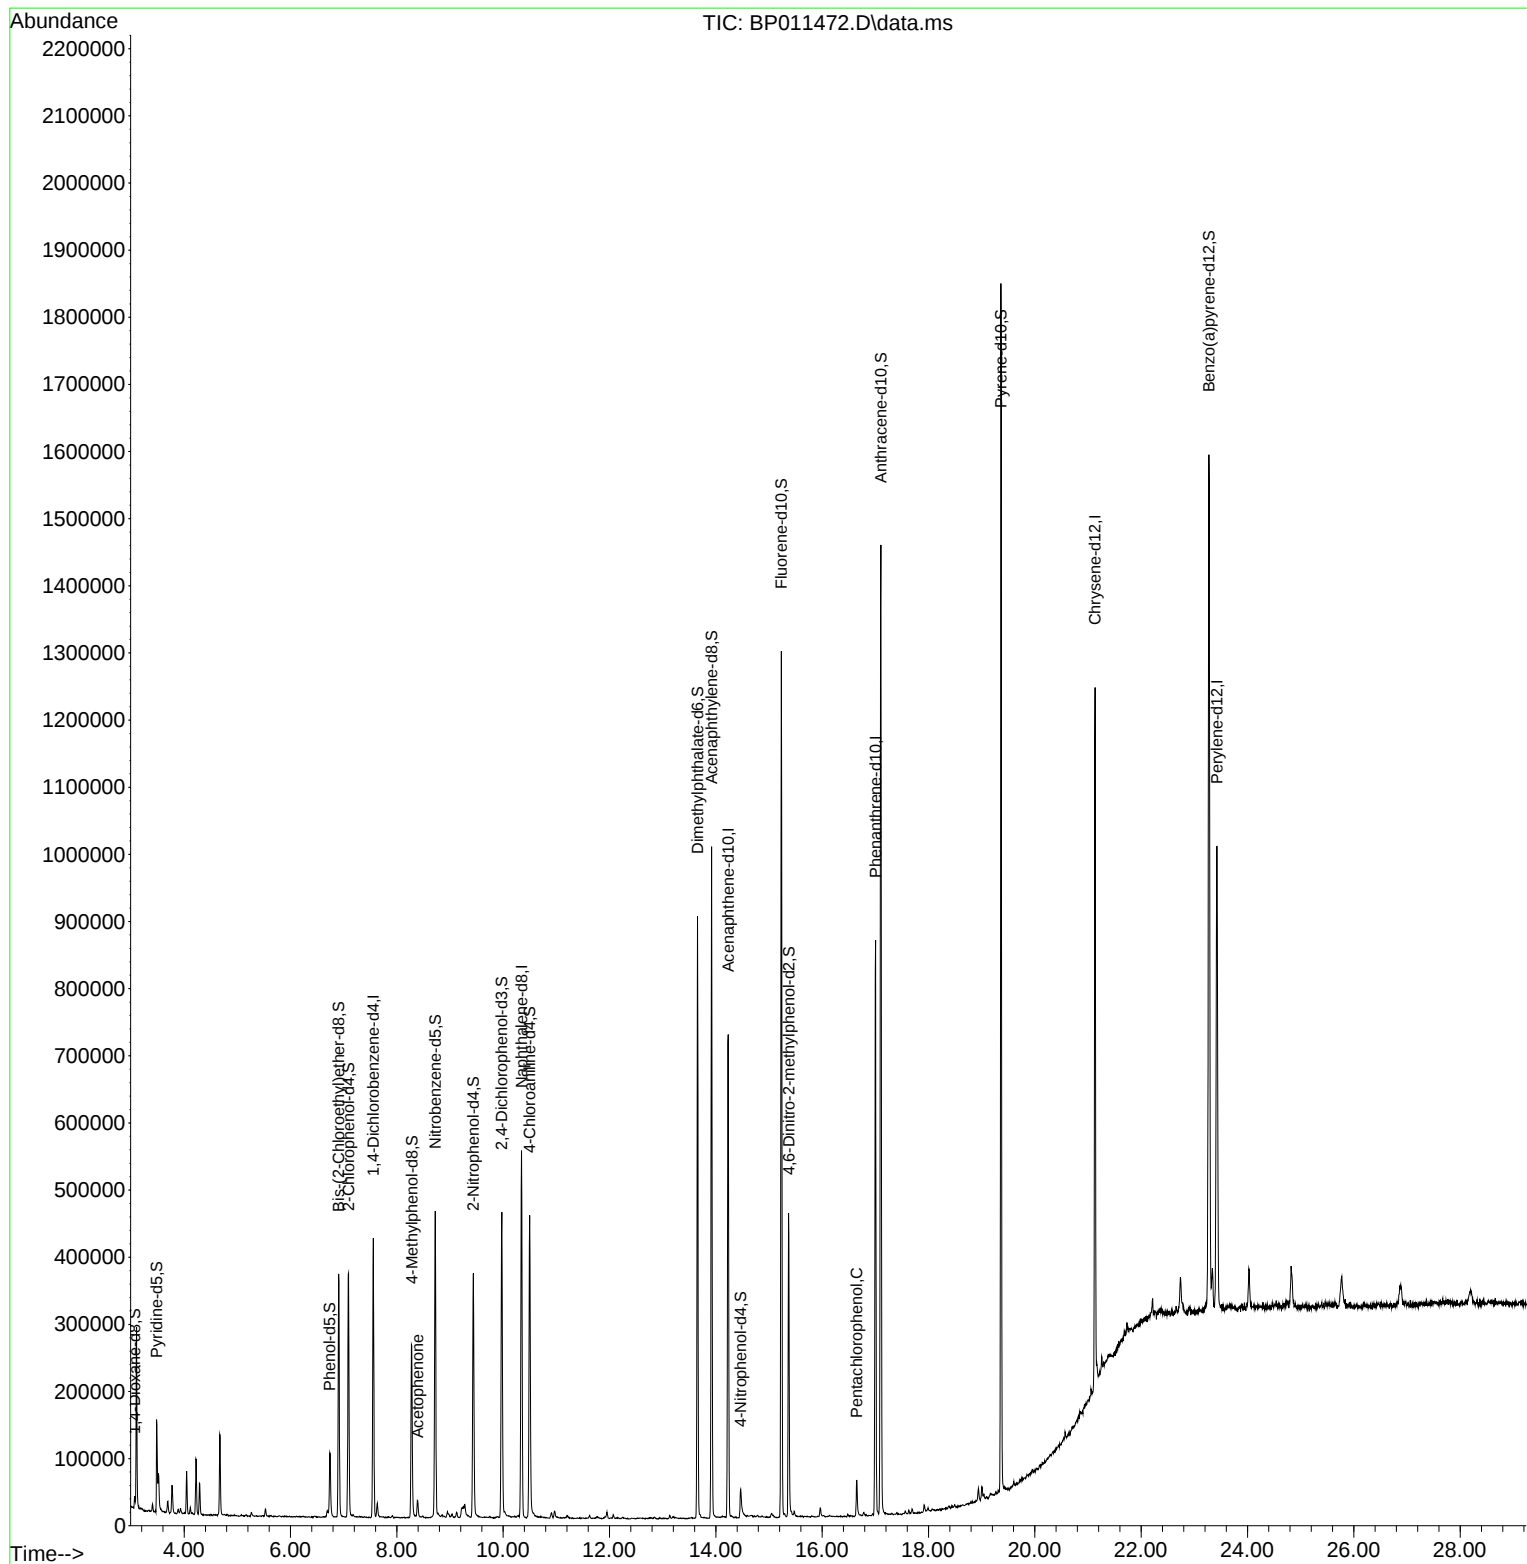


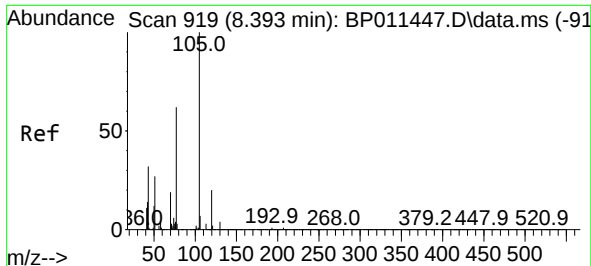

#16
Acetophenone
Concen: 1.047 ng/ul
RT: 8.393 min Scan# 919
Delta R.T. -0.000 min
Lab File: BP011472.D
Acq: 17 Aug 2022 21:38

Instrument :
BNA_P
ClientSampleId :

Tgt Ion:105 Resp: 12299
Ion Ratio Lower Upper
105 100
77 81.3 66.4 99.6
51 35.8 28.2 42.4

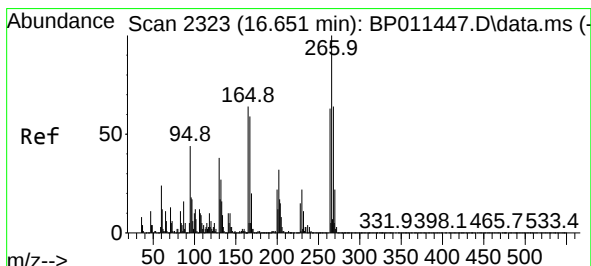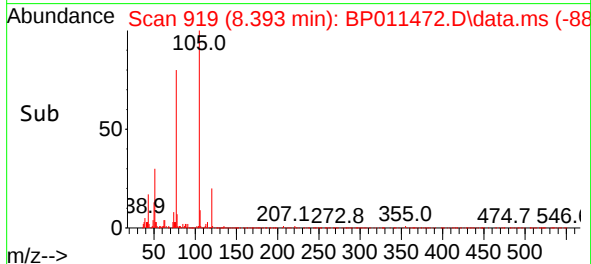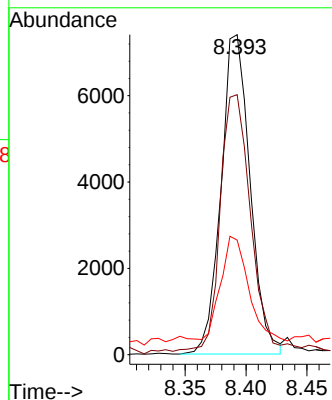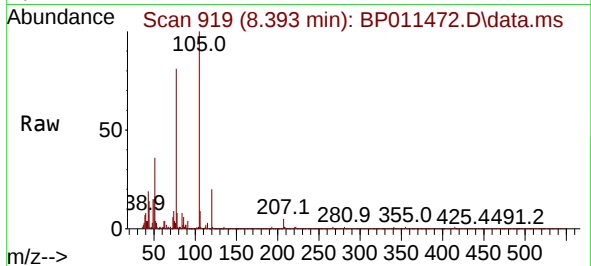

#71
Pentachlorophenol
Concen: 2.729 ng/ul
RT: 16.651 min Scan# 2323
Delta R.T. -0.000 min
Lab File: BP011472.D
Acq: 17 Aug 2022 21:38

Tgt Ion:266 Resp: 7666
Ion Ratio Lower Upper
266 100
264 75.4 50.6 76.0
268 57.8 51.3 76.9

