




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081722\
 Data File : BP011462.D
 Acq On : 17 Aug 2022 14:47
 Operator : CG/JU
 Sample : N4173-13MS
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 EX7Q8MS

Manual IntegrationsAPPROVED

Quant Time: Aug 17 23:28:09 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP081622.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Aug 17 01:58:37 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 08/18/2022
 Supervised By :Sohil Jodhani 08/18/2022

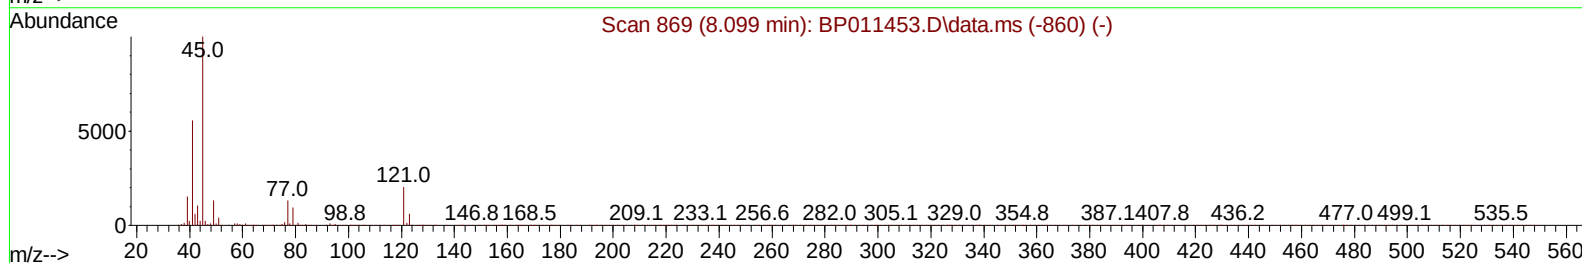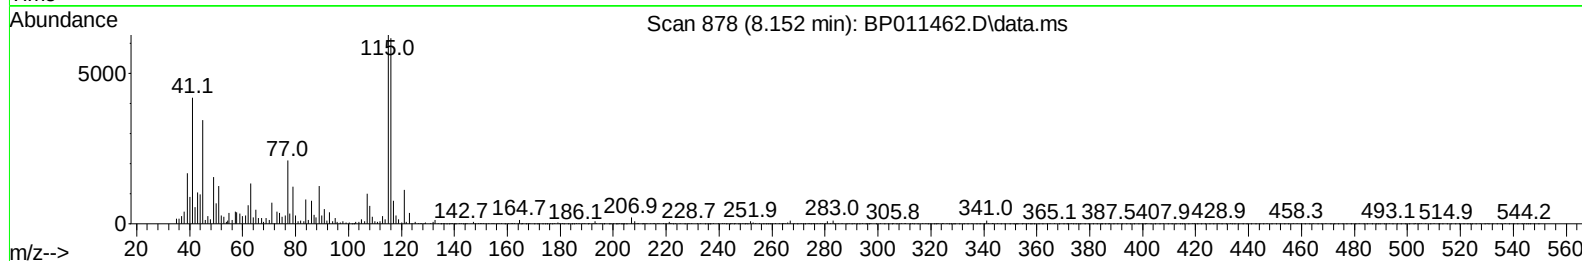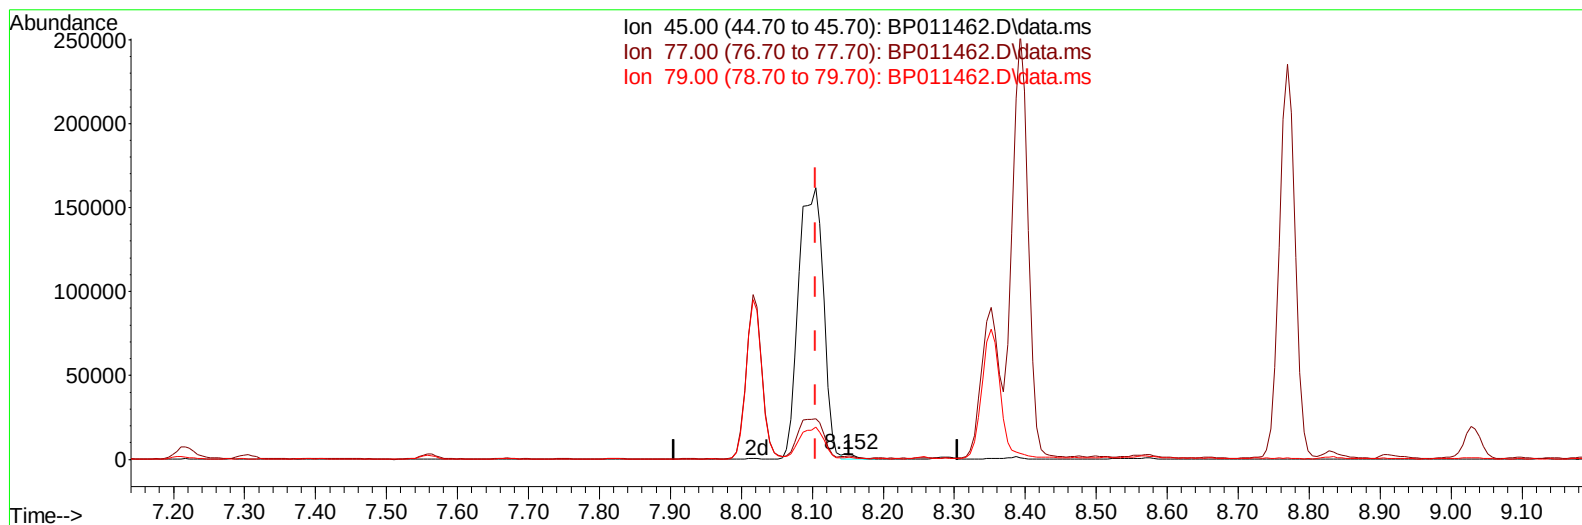

TIC: BP011462.D\data.ms

(14) 2,2'-oxybis(1-Chloropropane)

8.152min (+ 0.047) 0.34 ng/ul

response 4097

Ion	Exp%	Act%
45.00	100.00	100.00
77.00	14.20	60.68#
79.00	10.80	35.54#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081722\
Data File : BP011462.D
Acq On : 17 Aug 2022 14:47
Operator : CG/JU
Sample : N4173-13MS
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
EX7Q8MS

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 08/18/2022
Supervised By :Sohil Jodhani 08/18/2022

Quant Time: Aug 17 23:28:09 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP081622.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Aug 17 01:58:37 2022
Response via : Initial Calibration

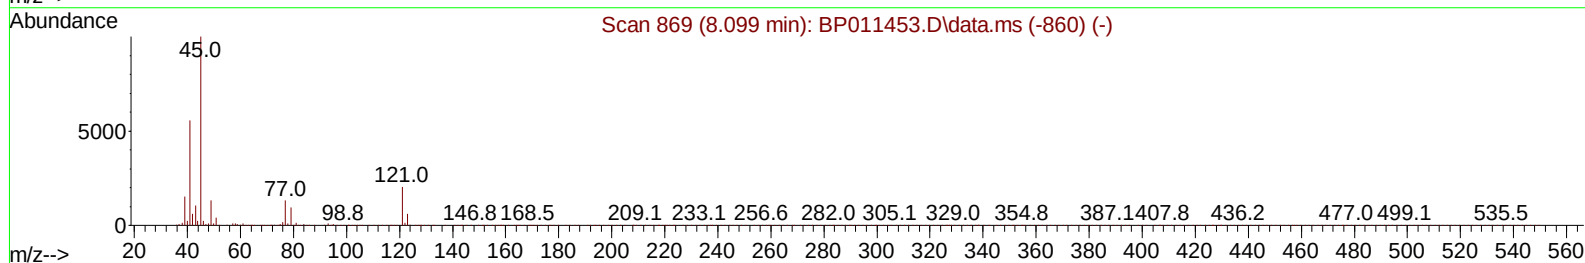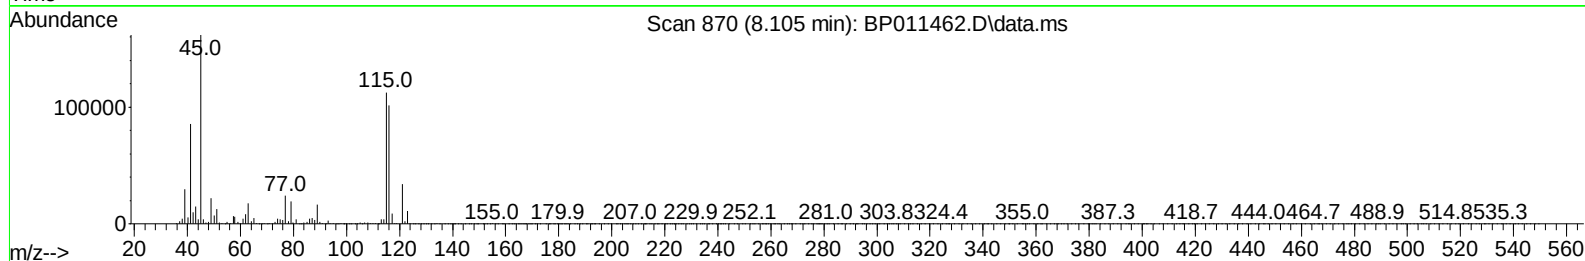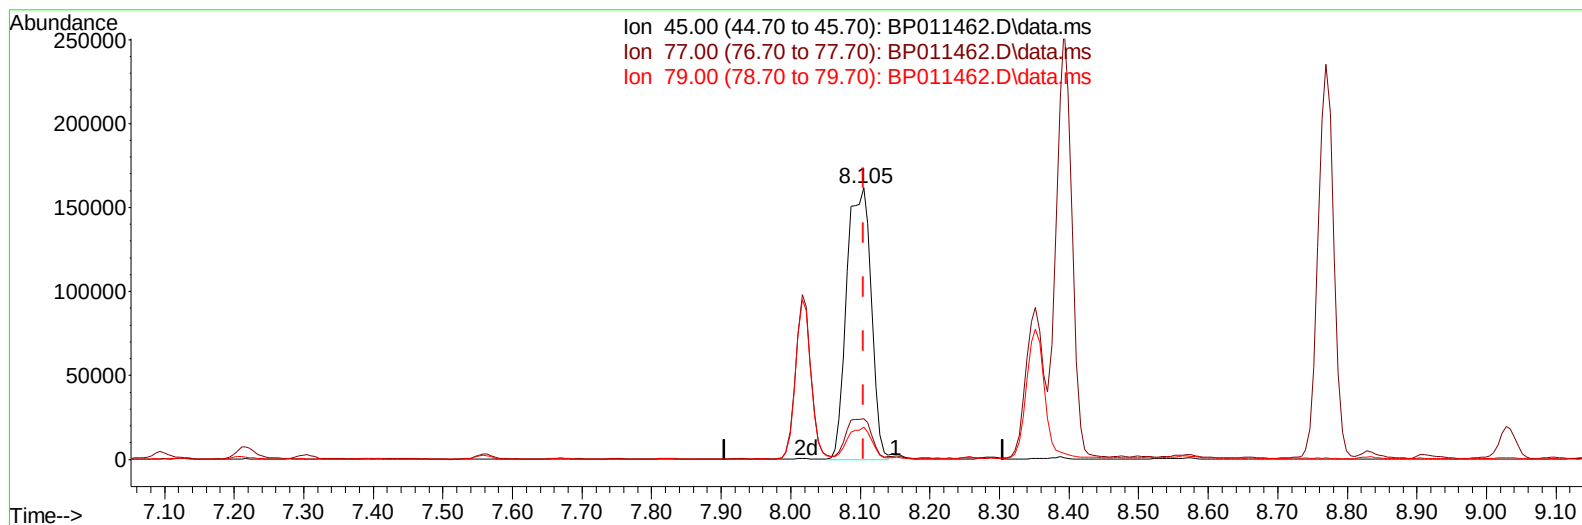

TIC: BP011462.D\data.ms

(14) 2,2'-oxybis(1-Chloropropane)

8.105min (-0.000) 32.47 ng/ul m

response 394296

Ion	Exp%	Act%
45.00	100.00	100.00
77.00	14.20	15.09
79.00	10.80	12.00
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081722\
 Data File : BP011462.D
 Acq On : 17 Aug 2022 14:47
 Operator : CG/JU
 Sample : N4173-13MS
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 EX7Q8MS

Manual IntegrationsAPPROVED

Quant Time: Aug 17 23:28:09 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP081622.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Aug 17 01:58:37 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 08/18/2022
 Supervised By :Sohil Jodhani 08/18/2022

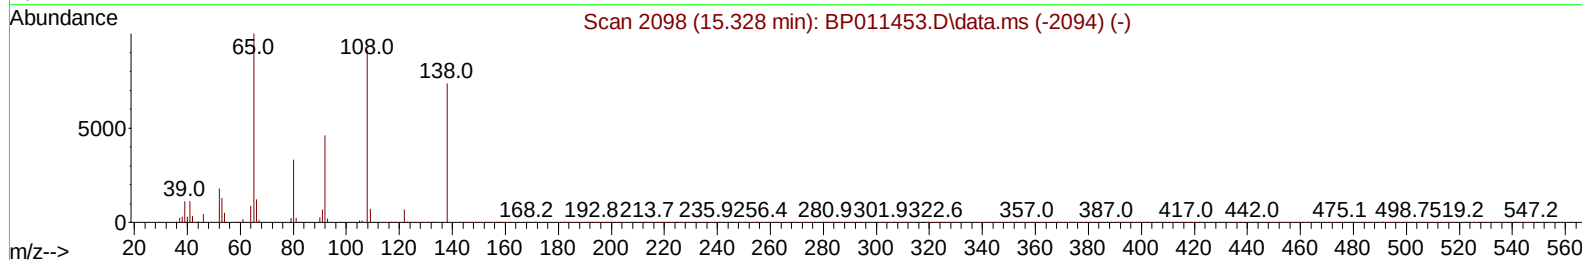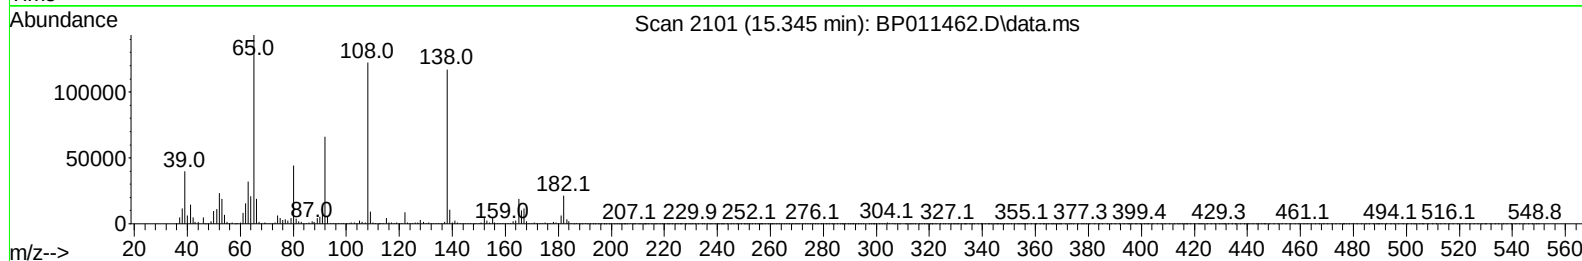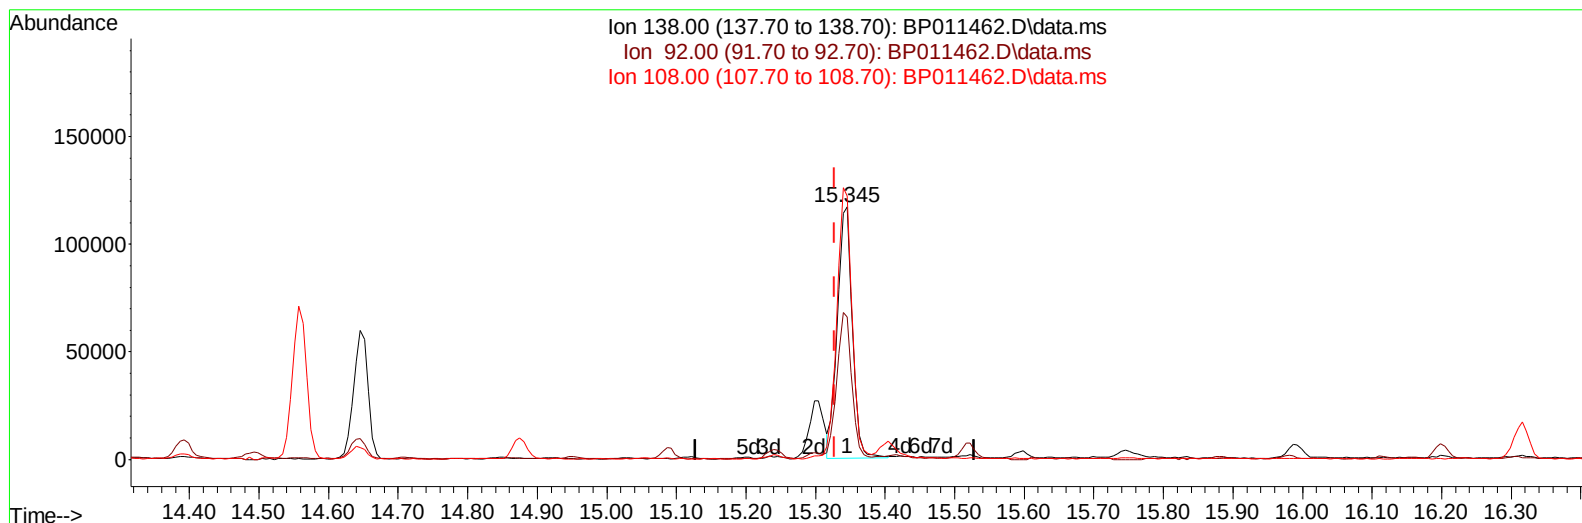

TIC: BP011462.D\data.ms

(63) 4-Nitroaniline

15.345min (+ 0.018) 47.17 ng/ul

response 174441

Ion	Exp%	Act%
138.00	100.00	100.00
92.00	61.90	56.37
108.00	117.10	104.32
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081722\
Data File : BP011462.D
Acq On : 17 Aug 2022 14:47
Operator : CG/JU
Sample : N4173-13MS
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
EX7Q8MS

Manual IntegrationsAPPROVED

Quant Time: Aug 17 23:28:09 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP081622.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Aug 17 01:58:37 2022
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 08/18/2022
Supervised By :Sohil Jodhani 08/18/2022

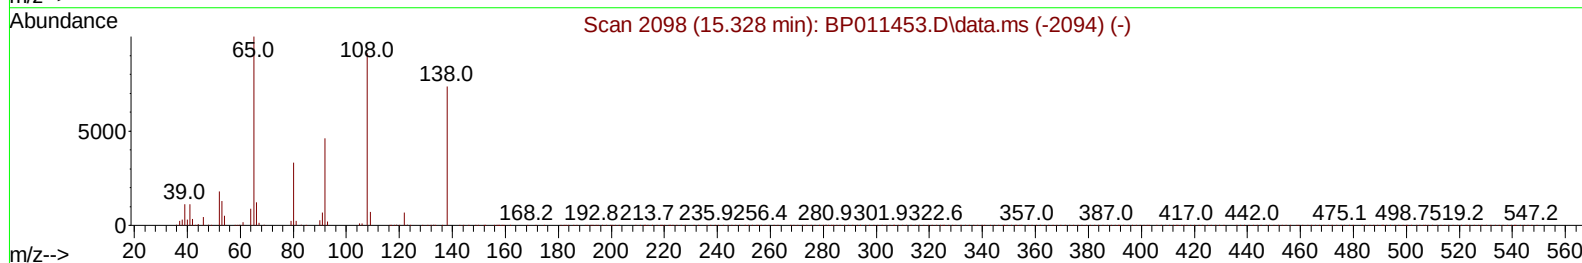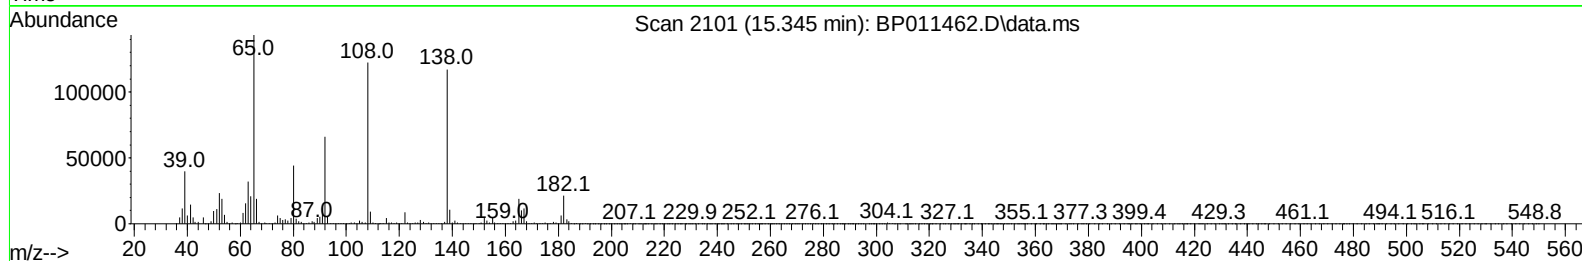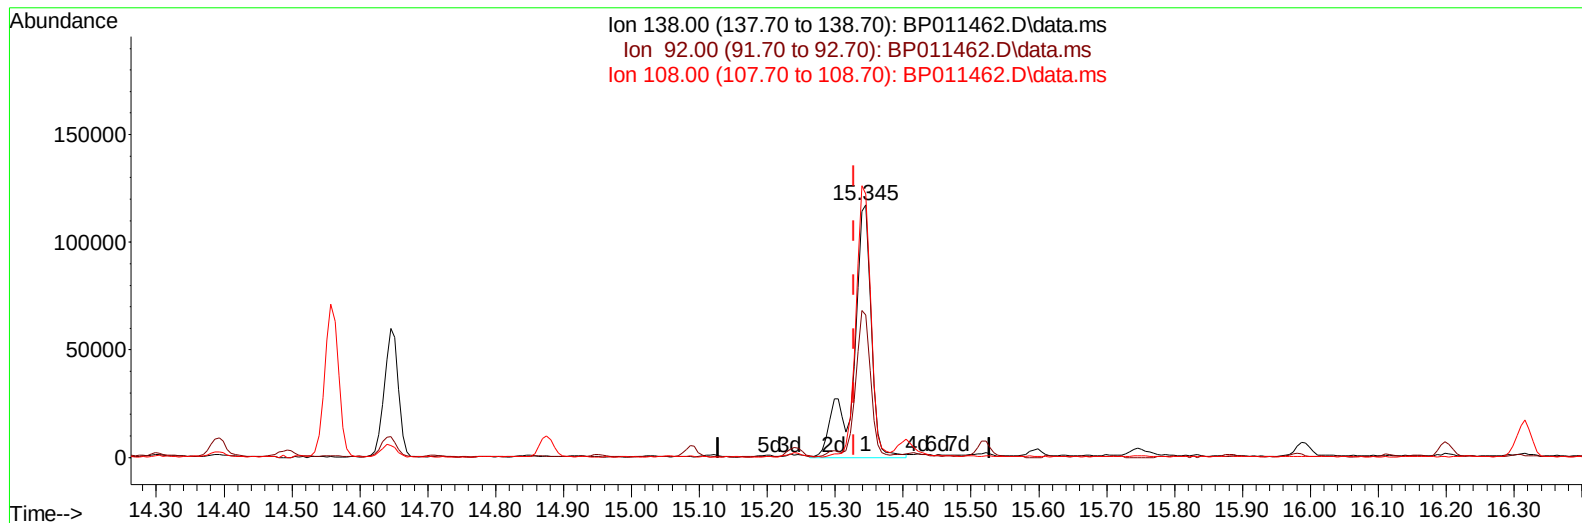

TIC: BP011462.D\data.ms

(63) 4-Nitroaniline

15.345min (+ 0.018) 59.38 ng/ul m

response 219609

Ion	Exp%	Act%
138.00	100.00	100.00
92.00	61.90	56.37
108.00	117.10	104.32
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081722\
 Data File : BP011462.D
 Acq On : 17 Aug 2022 14:47
 Operator : CG/JU
 Sample : N4173-13MS
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 EX7Q8MS

Manual IntegrationsAPPROVED

Quant Time: Aug 17 23:28:09 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP081622.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Aug 17 01:58:37 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 08/18/2022
 Supervised By :Sohil Jodhani 08/18/2022

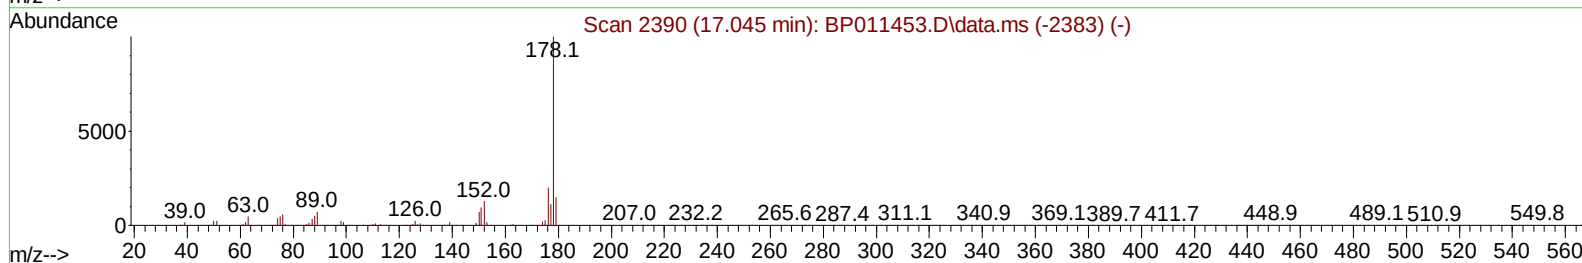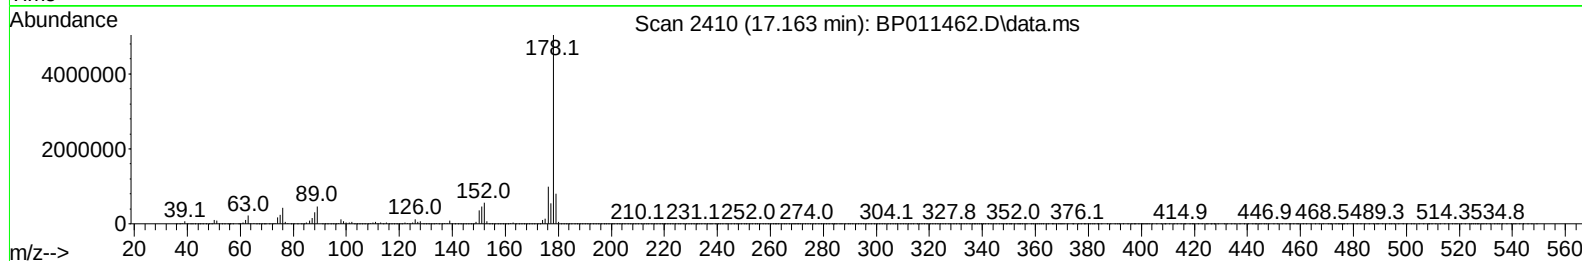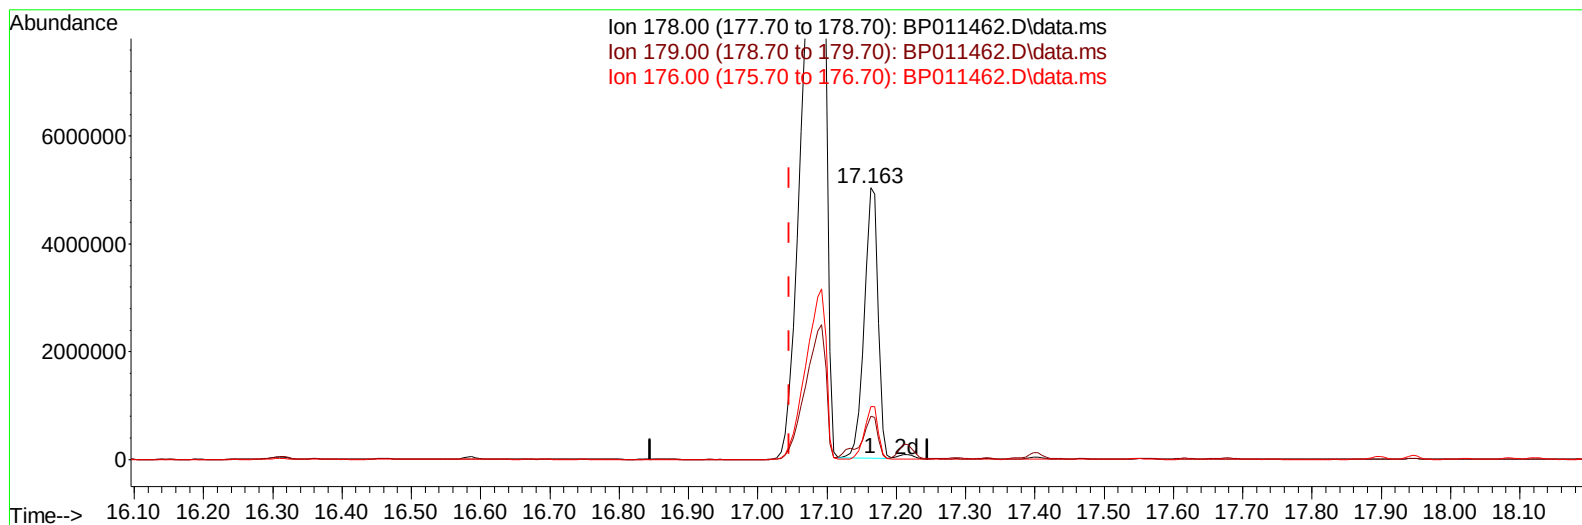

TIC: BP011462.D\data.ms

(72) Phenanthrene

17.163min (+ 0.118) 263.32 ng/uL

response 6964609

Ion	Exp%	Act%
178.00	100.00	100.00
179.00	15.70	15.96
176.00	19.80	19.54
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081722\
 Data File : BP011462.D
 Acq On : 17 Aug 2022 14:47
 Operator : CG/JU
 Sample : N4173-13MS
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 EX7Q8MS

Manual IntegrationsAPPROVED

Quant Time: Aug 17 23:28:09 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP081622.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Aug 17 01:58:37 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 08/18/2022
 Supervised By :Sohil Jodhani 08/18/2022

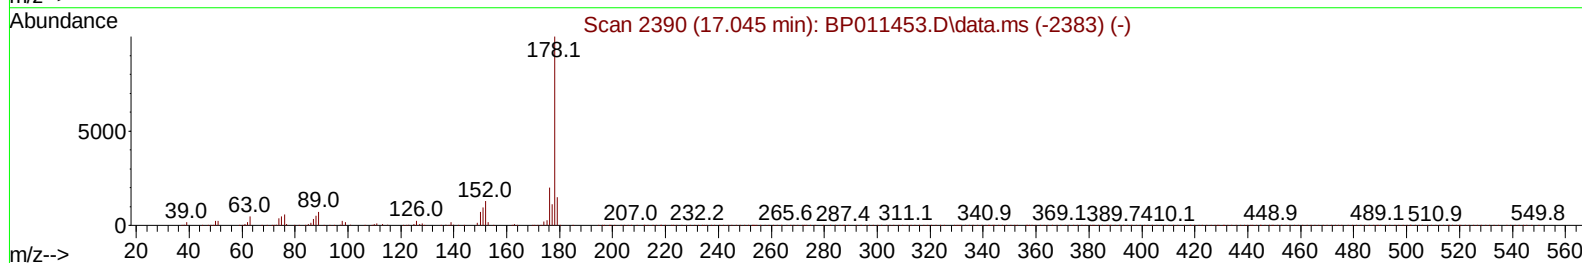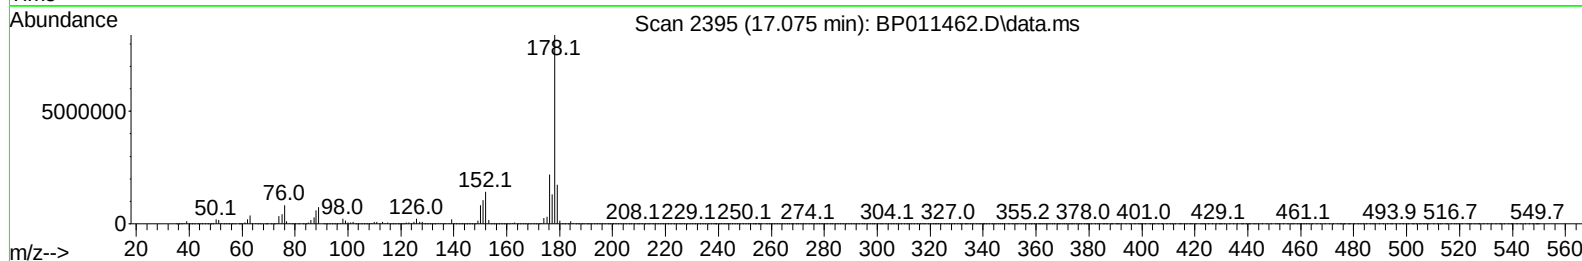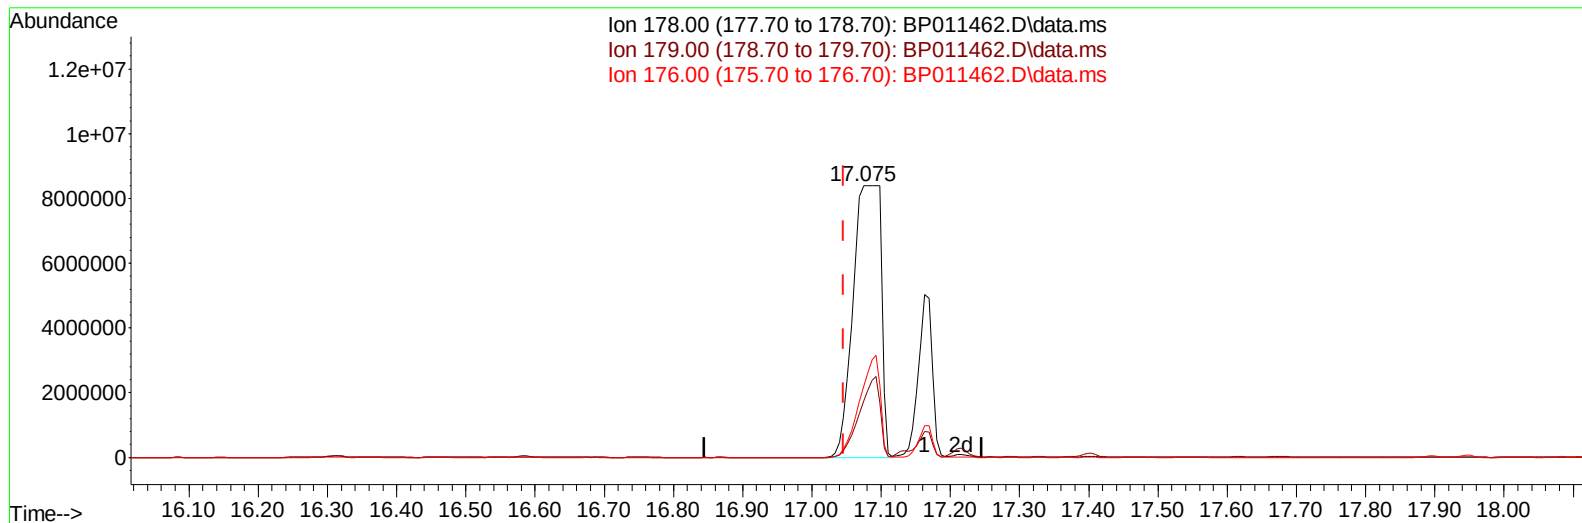

TIC: BP011462.D\data.ms

(72) Phenanthrene

17.075min (+ 0.029) 889.72 ng/ul m

response 23532750

Ion	Exp%	Act%
178.00	100.00	100.00
179.00	15.70	20.82#
176.00	19.80	26.19#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081722\
 Data File : BP011462.D
 Acq On : 17 Aug 2022 14:47
 Operator : CG/JU
 Sample : N4173-13MS
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 EX7Q8MS

Manual IntegrationsAPPROVED

Quant Time: Aug 17 23:28:09 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP081622.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Aug 17 01:58:37 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 08/18/2022
 Supervised By :Sohil Jodhani 08/18/2022

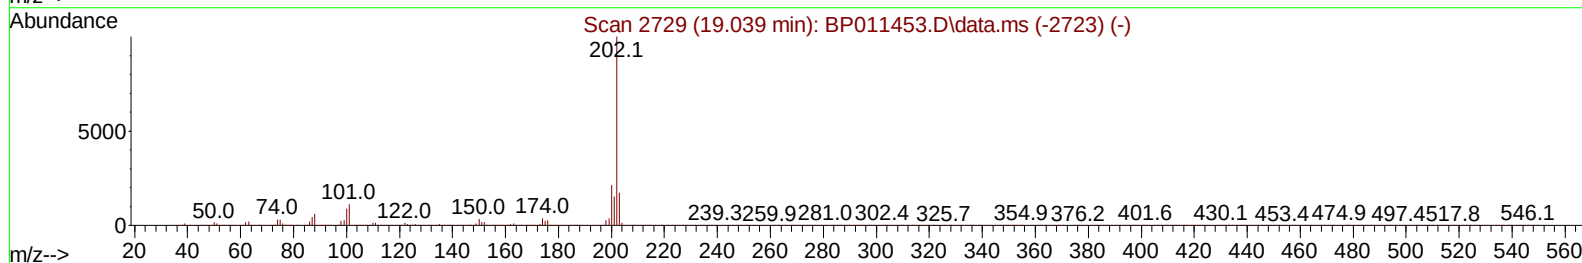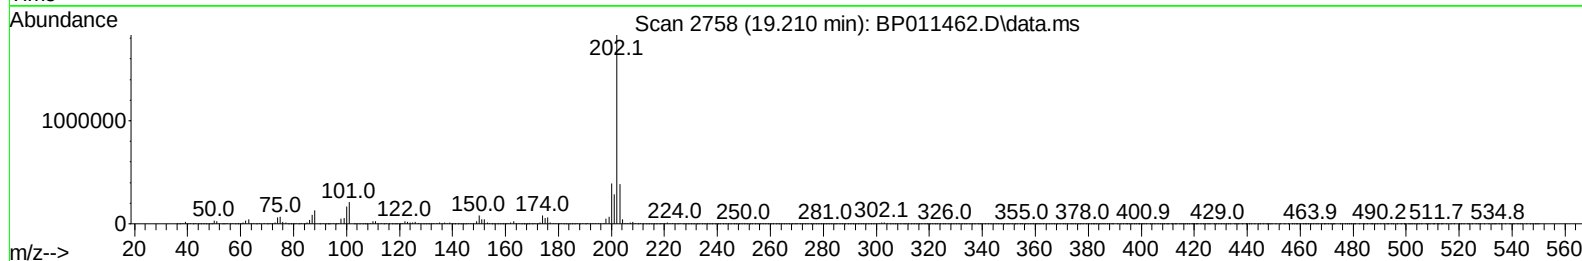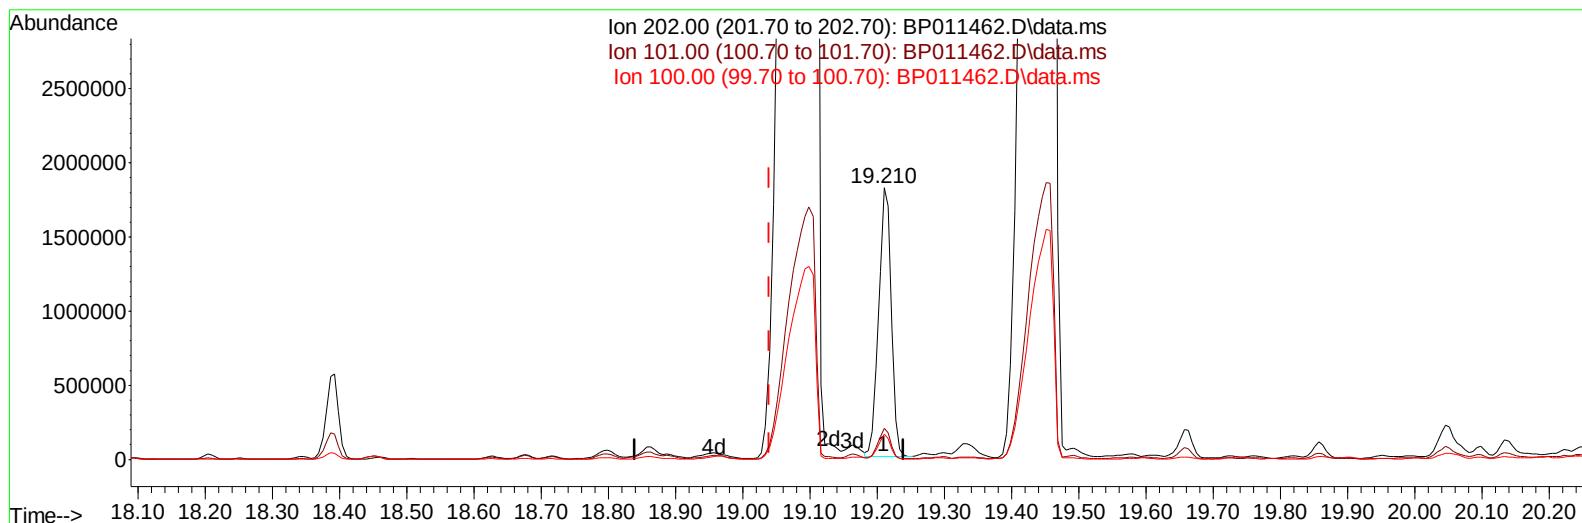

TIC: BP011462.D\data.ms

(80) Fluoranthene

19.210min (+ 0.171) 65.96 ng/ul

response 2364154

Ion	Exp%	Act%
202.00	100.00	100.00
101.00	11.90	11.40
100.00	9.90	9.27
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081722\
 Data File : BP011462.D
 Acq On : 17 Aug 2022 14:47
 Operator : CG/JU
 Sample : N4173-13MS
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 EX7Q8MS

Manual IntegrationsAPPROVED

Quant Time: Aug 17 23:28:09 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP081622.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Aug 17 01:58:37 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 08/18/2022
 Supervised By :Sohil Jodhani 08/18/2022

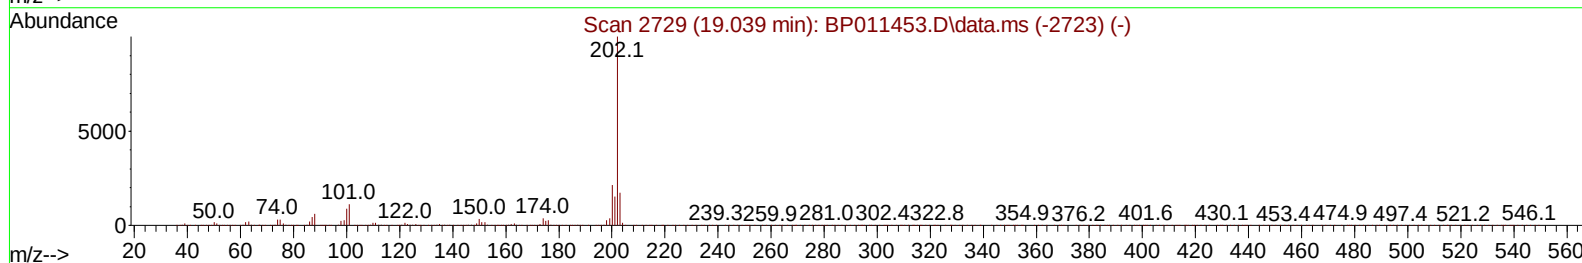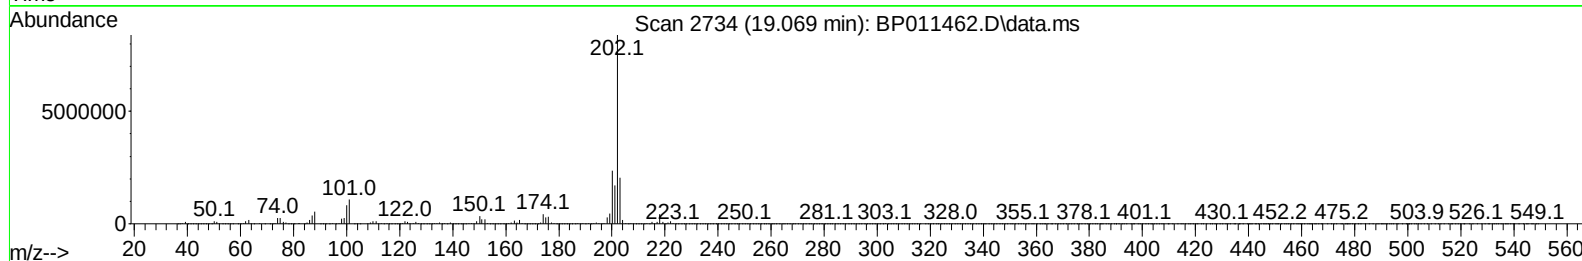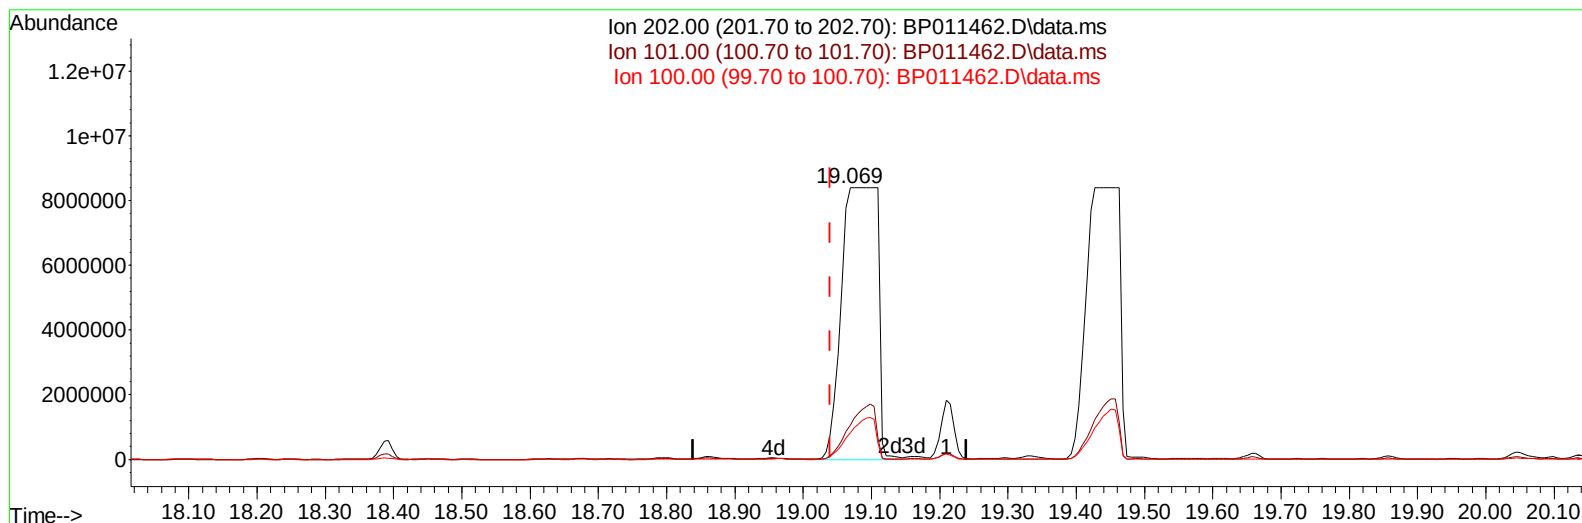

TIC: BP011462.D\data.ms

(80) Fluoranthene

19.069min (+ 0.029) 858.56 ng/ul m

response 30772453

Ion	Exp%	Act%
202.00	100.00	100.00
101.00	11.90	12.73
100.00	9.90	9.82
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081722\
 Data File : BP011462.D
 Acq On : 17 Aug 2022 14:47
 Operator : CG/JU
 Sample : N4173-13MS
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 EX7Q8MS

Manual IntegrationsAPPROVED

Quant Time: Aug 17 23:28:09 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP081622.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Aug 17 01:58:37 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 08/18/2022
 Supervised By :Sohil Jodhani 08/18/2022

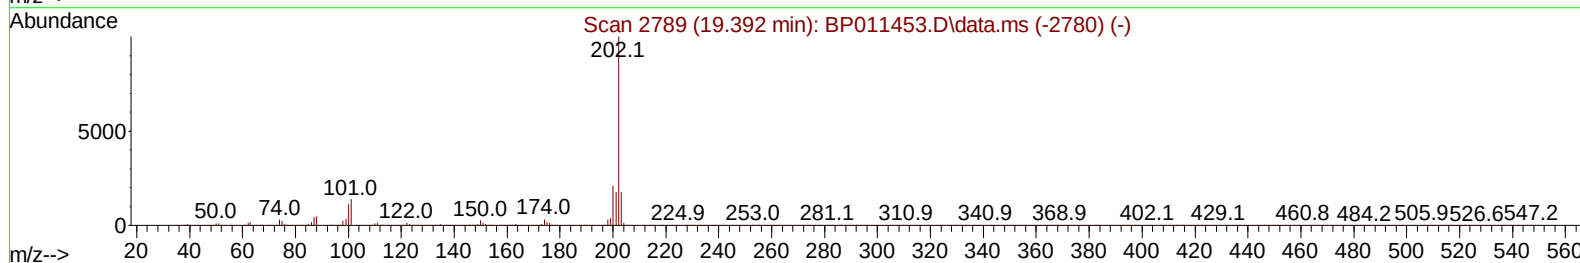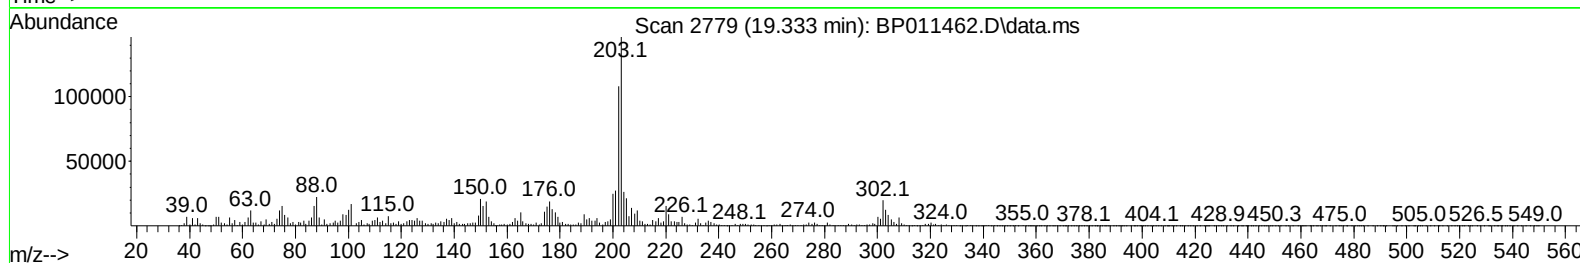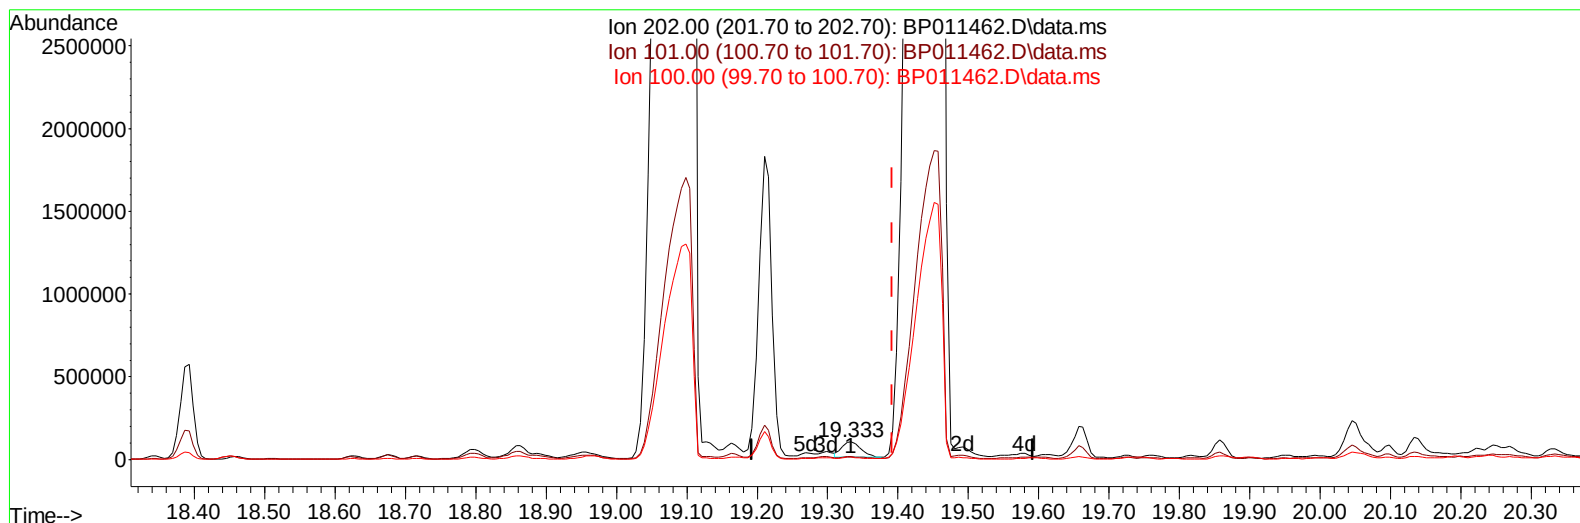

TIC: BP011462.D\data.ms

(82) Pyrene

19.333min (-0.059) 4.78 ng/ul

response 180033

Ion	Exp%	Act%
202.00	100.00	100.00
101.00	14.30	15.39
100.00	11.70	11.55
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081722\
Data File : BP011462.D
Acq On : 17 Aug 2022 14:47
Operator : CG/JU
Sample : N4173-13MS
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
EX7Q8MS

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 08/18/2022
Supervised By :Sohil Jodhani 08/18/2022

Quant Time: Aug 17 23:28:09 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP081622.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Aug 17 01:58:37 2022
Response via : Initial Calibration

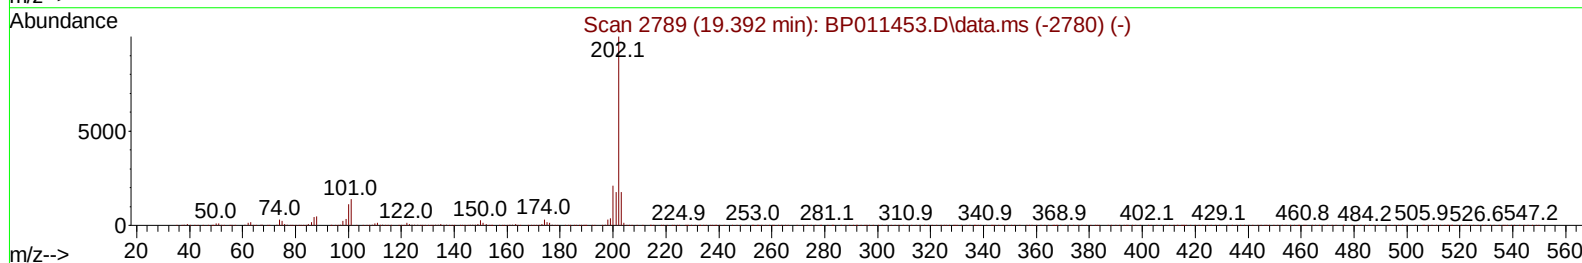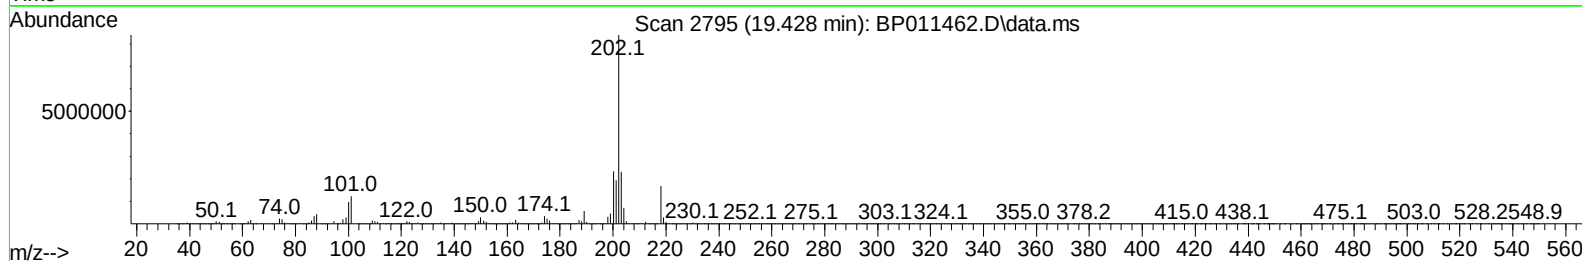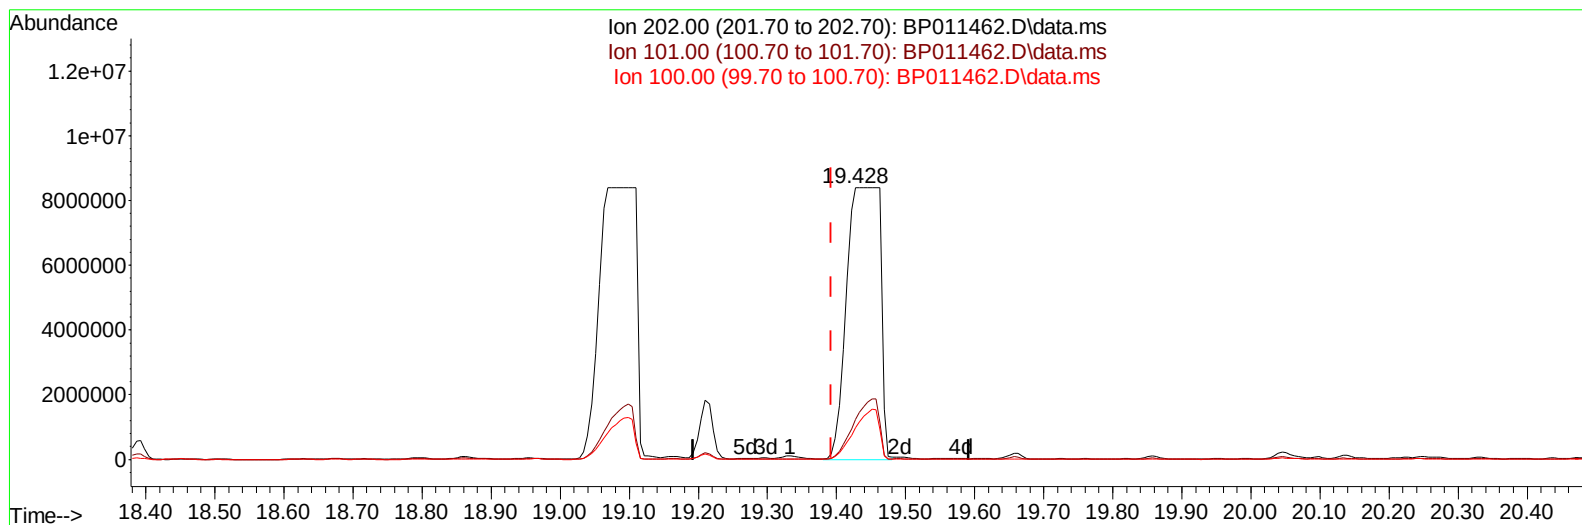

TIC: BP011462.D\data.ms

(82) Pyrene

19.428min (+ 0.035) 746.42 ng/uL m

response 28110539

Ion	Exp%	Act%
202.00	100.00	100.00
101.00	14.30	14.73
100.00	11.70	11.59
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081722\
 Data File : BP011462.D
 Acq On : 17 Aug 2022 14:47
 Operator : CG/JU
 Sample : N4173-13MS
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 EX7Q8MS

Manual IntegrationsAPPROVED

Quant Time: Aug 17 23:28:09 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP081622.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Aug 17 01:58:37 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 08/18/2022
 Supervised By :Sohil Jodhani 08/18/2022

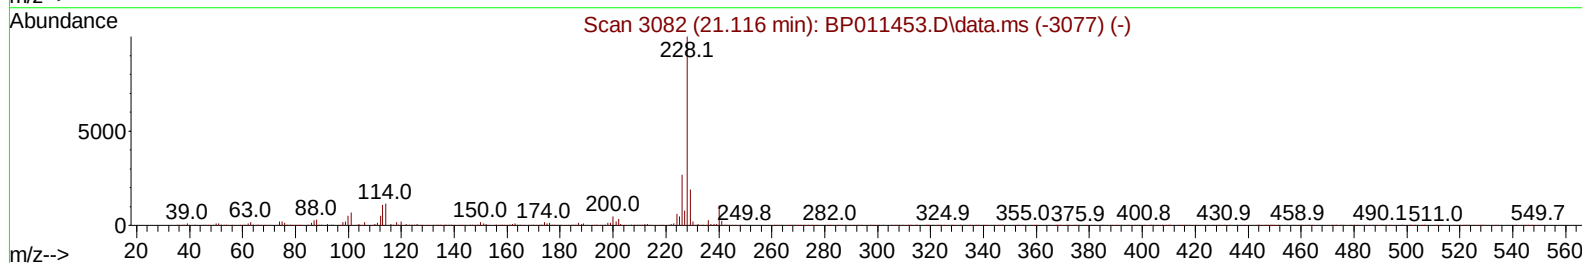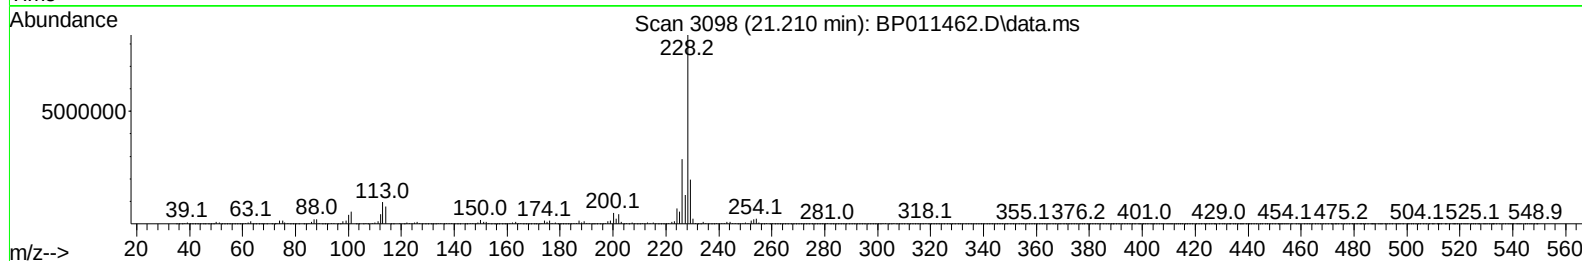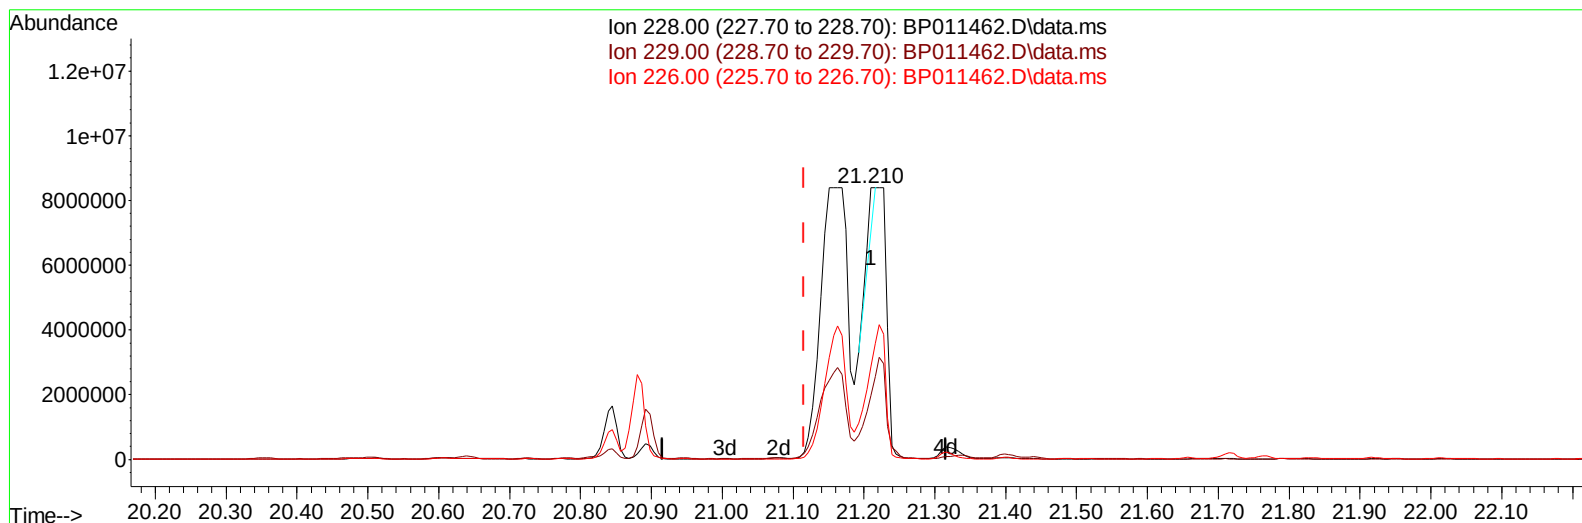

TIC: BP011462.D\data.ms

(85) Benzo(a)anthracene

21.210min (+ 0.094) 56.70 ng/ul

response 1990084

Ion	Exp%	Act%
228.00	100.00	100.00
229.00	20.00	23.57
226.00	28.20	34.18#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081722\
 Data File : BP011462.D
 Acq On : 17 Aug 2022 14:47
 Operator : CG/JU
 Sample : N4173-13MS
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 EX7Q8MS

Manual IntegrationsAPPROVED

Quant Time: Aug 17 23:28:09 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP081622.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Aug 17 01:58:37 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 08/18/2022
 Supervised By :Sohil Jodhani 08/18/2022

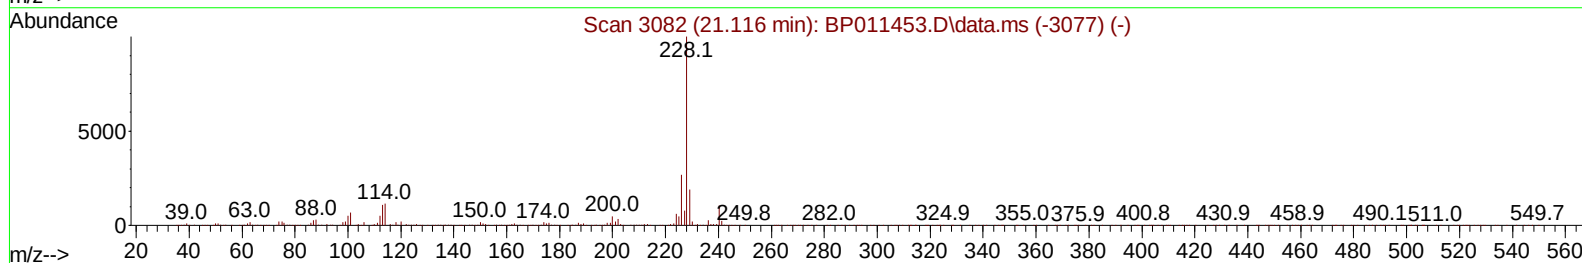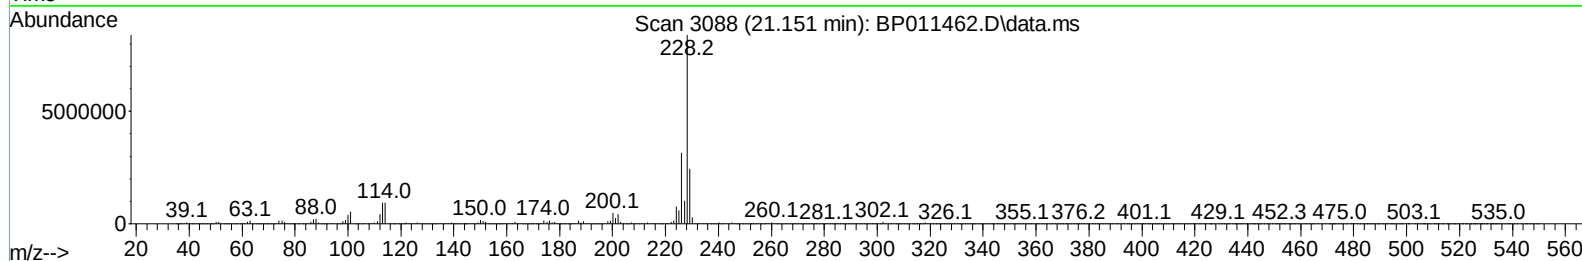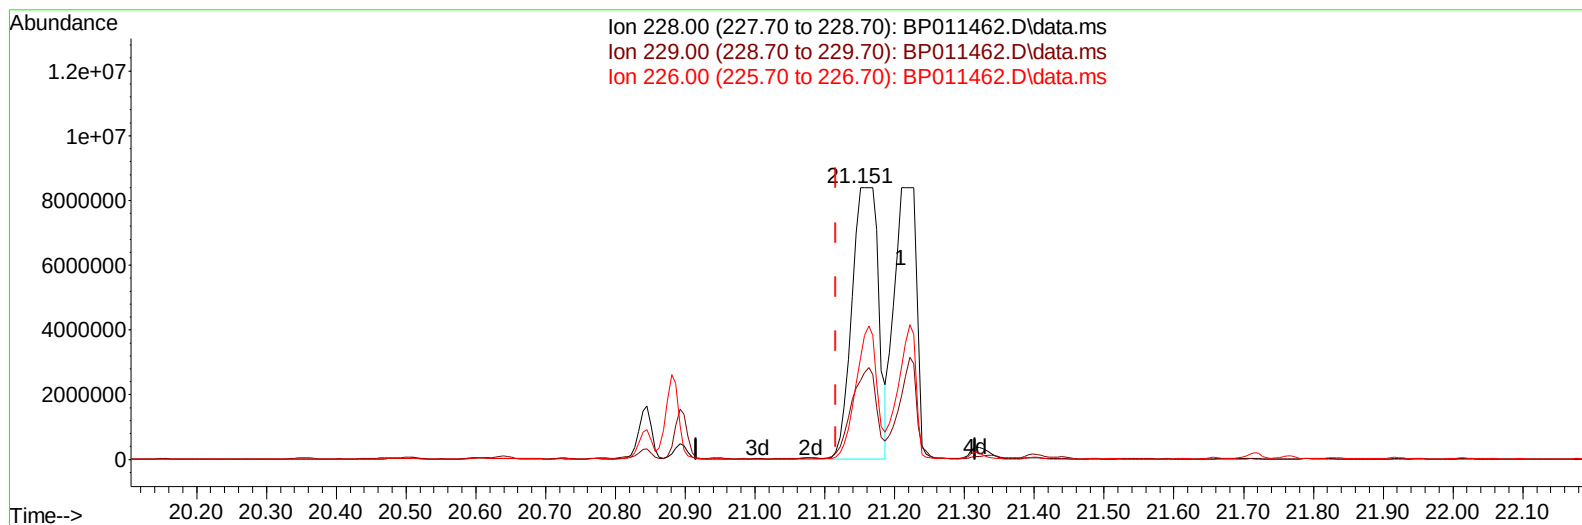

TIC: BP011462.D\data.ms

(85) Benzo(a)anthracene

21.151min (+ 0.035) 637.27 ng/ul m

response 22365525

Ion	Exp%	Act%
228.00	100.00	100.00
229.00	20.00	29.08#
226.00	28.20	37.59#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081722\
 Data File : BP011462.D
 Acq On : 17 Aug 2022 14:47
 Operator : CG/JU
 Sample : N4173-13MS
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 EX7Q8MS

Manual IntegrationsAPPROVED

Quant Time: Aug 17 23:28:09 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP081622.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Aug 17 01:58:37 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 08/18/2022
 Supervised By :Sohil Jodhani 08/18/2022

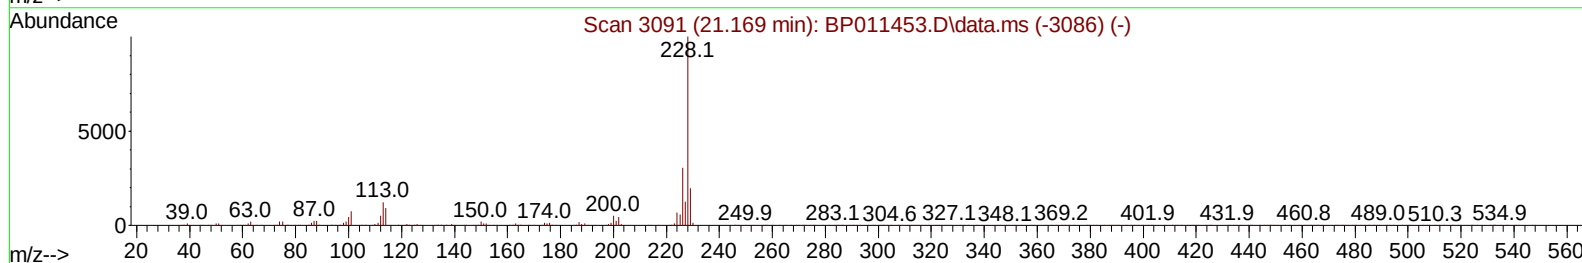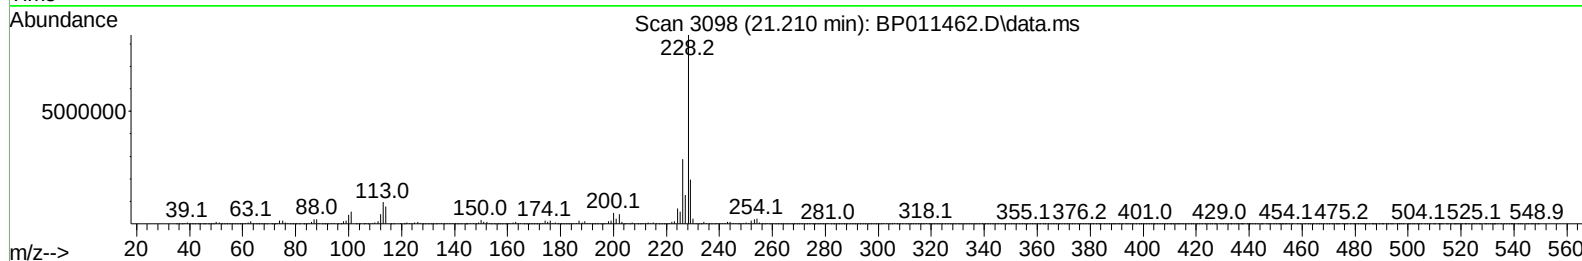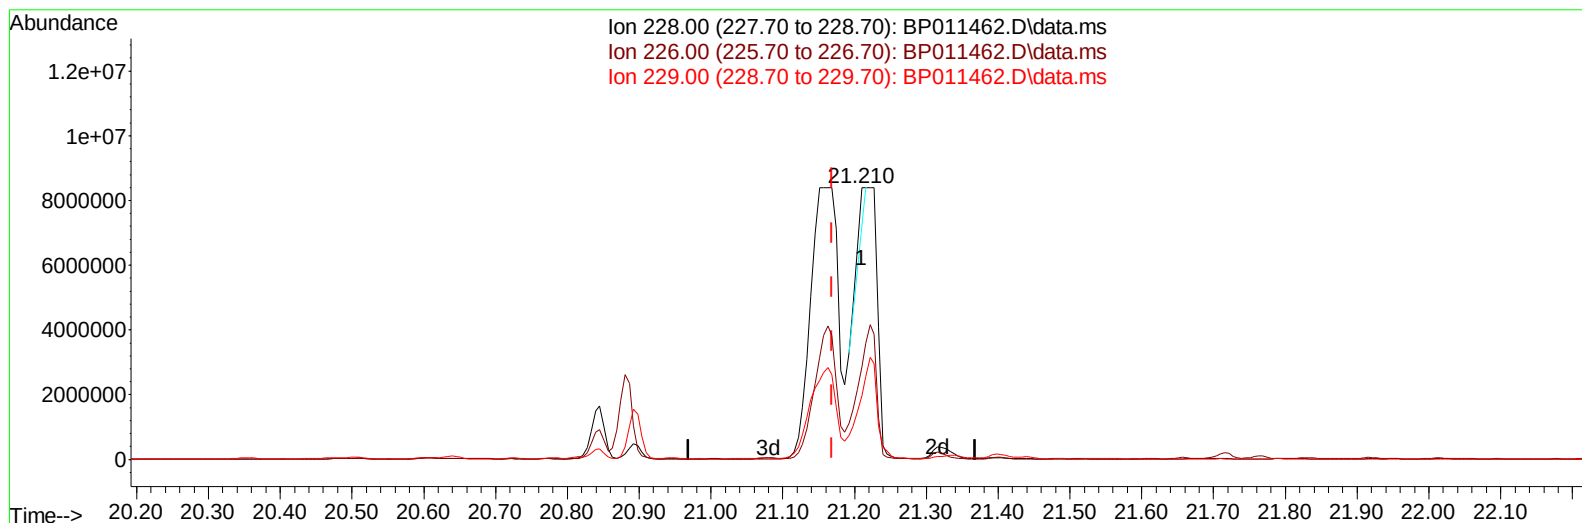

TIC: BP011462.D\data.ms

(87) Chrysene

21.210min (+ 0.041) 57.72 ng/ul

response 1990084

Ion	Exp%	Act%
228.00	100.00	100.00
226.00	29.90	34.18
229.00	20.00	23.57
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081722\
 Data File : BP011462.D
 Acq On : 17 Aug 2022 14:47
 Operator : CG/JU
 Sample : N4173-13MS
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 EX7Q8MS

Manual IntegrationsAPPROVED

Quant Time: Aug 17 23:28:09 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP081622.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Aug 17 01:58:37 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 08/18/2022
 Supervised By :Sohil Jodhani 08/18/2022

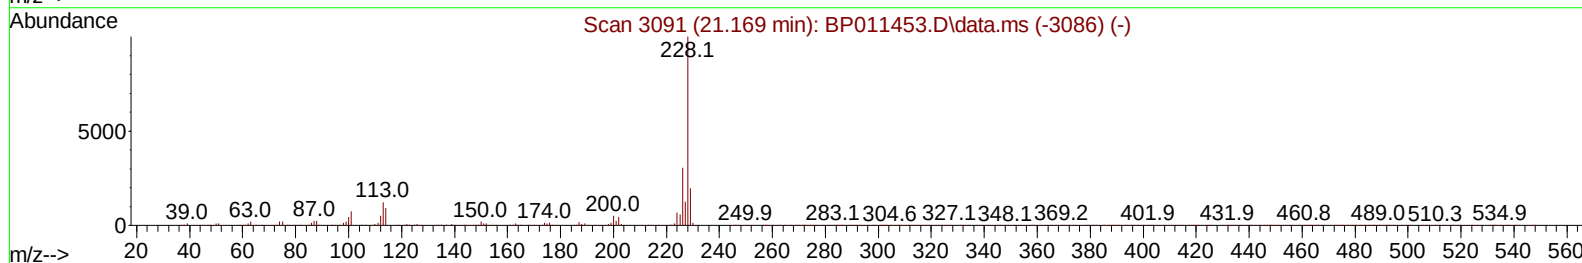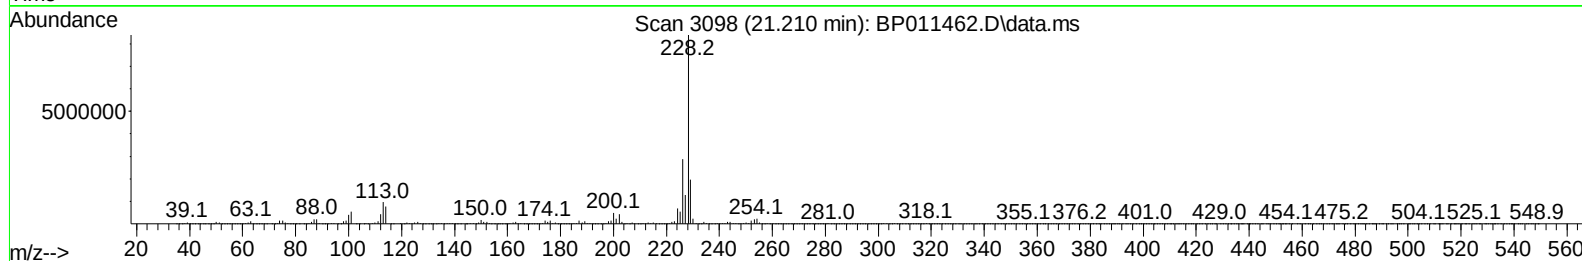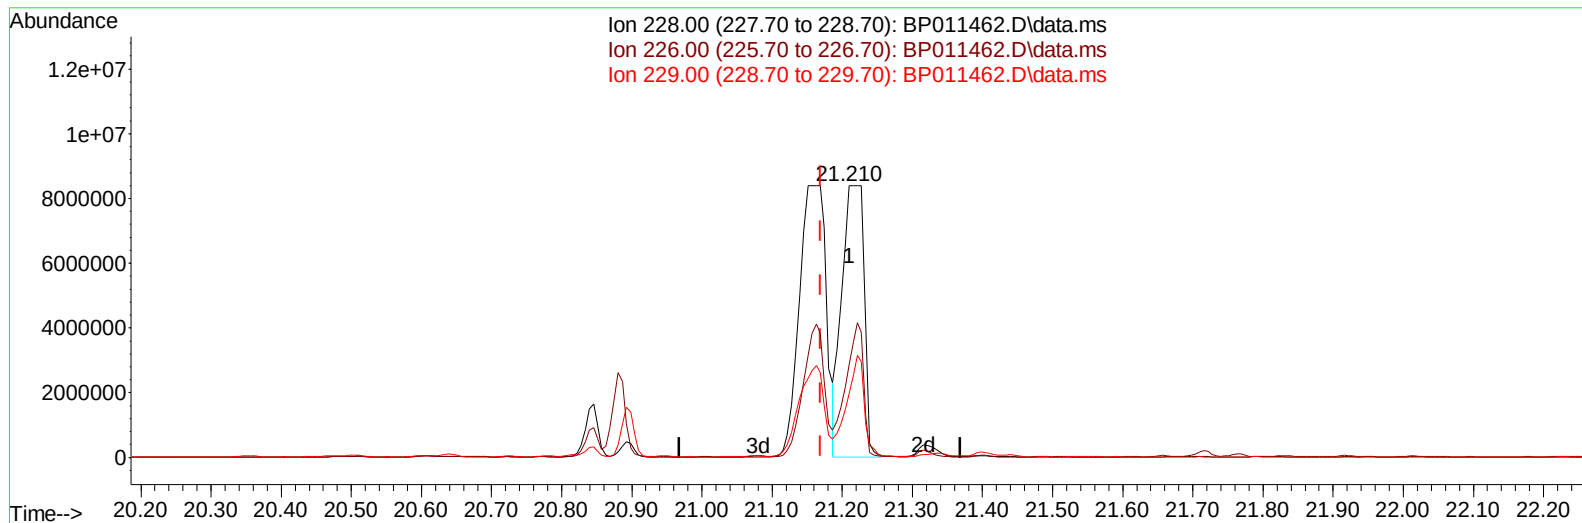

TIC: BP011462.D\data.ms

(87) Chrysene

21.210min (+ 0.041) 541.34 ng/ul m

response 18663110

Ion	Exp%	Act%
228.00	100.00	100.00
226.00	29.90	34.18
229.00	20.00	23.57
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081722\
Data File : BP011462.D
Acq On : 17 Aug 2022 14:47
Operator : CG/JU
Sample : N4173-13MS
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
EX7Q8MS

Manual IntegrationsAPPROVED

Quant Time: Aug 17 23:28:09 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP081622.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Aug 17 01:58:37 2022
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 08/18/2022
Supervised By :Sohil Jodhani 08/18/2022

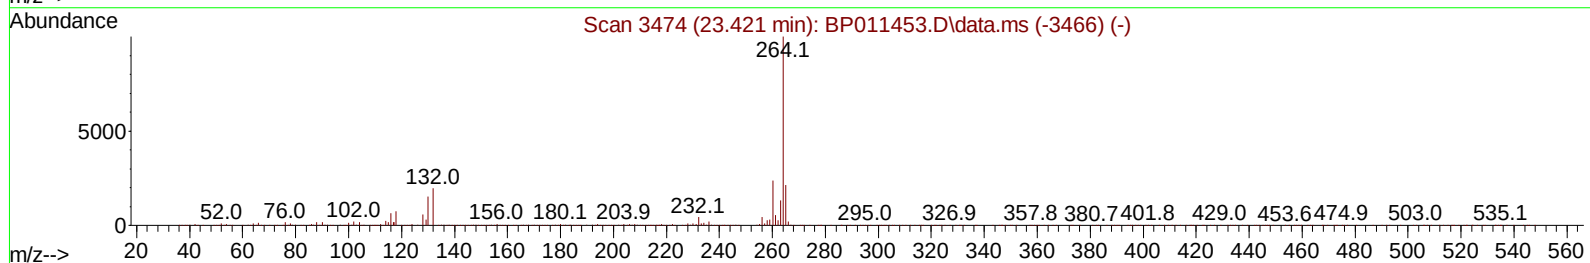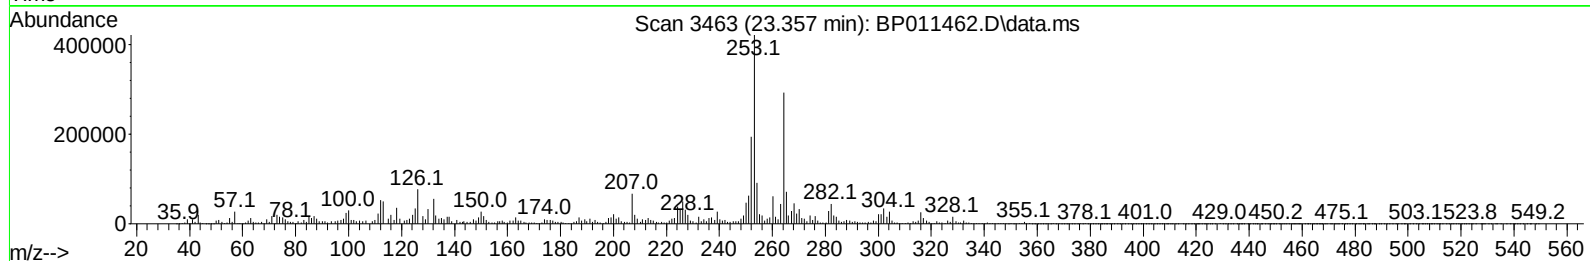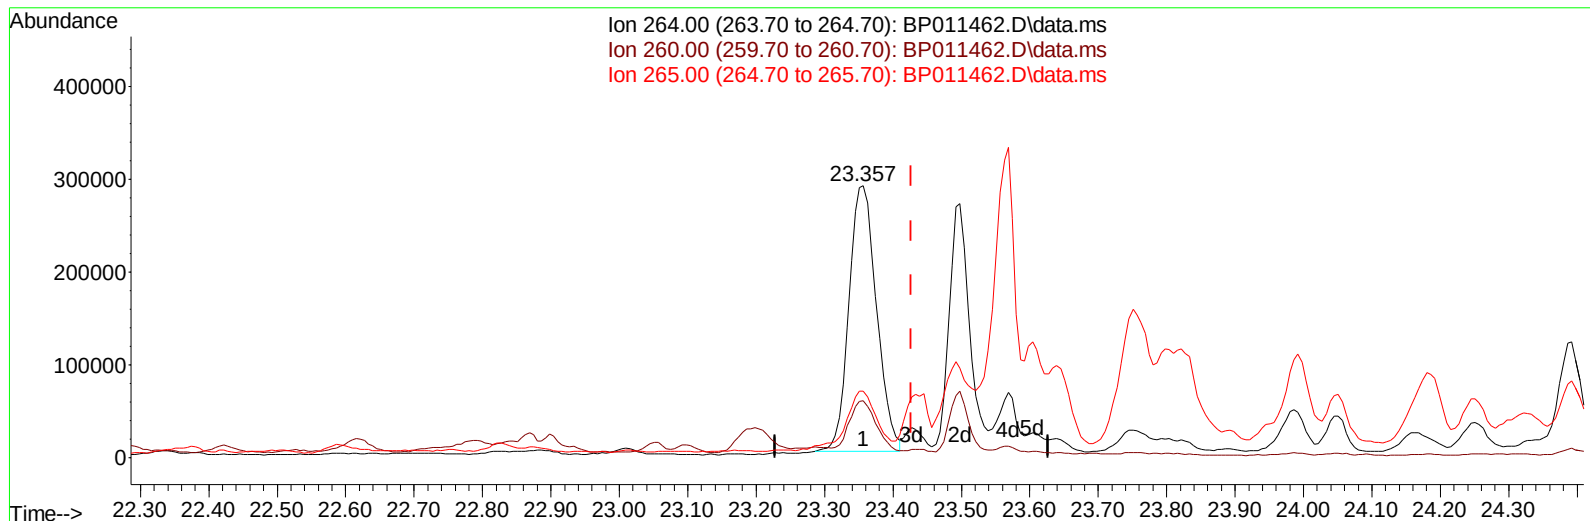

TIC: BP011462.D\data.ms

(88) Perylene-d12 (I)

23.357min (-0.071) 20.00 ng/u1

response 800561

Ion	Exp%	Act%
264.00	100.00	100.00
260.00	24.40	20.90
265.00	22.90	24.40
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081722\
Data File : BP011462.D
Acq On : 17 Aug 2022 14:47
Operator : CG/JU
Sample : N4173-13MS
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
EX7Q8MS

Manual IntegrationsAPPROVED

Quant Time: Aug 17 23:28:09 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP081622.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Aug 17 01:58:37 2022
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 08/18/2022
Supervised By :Sohil Jodhani 08/18/2022

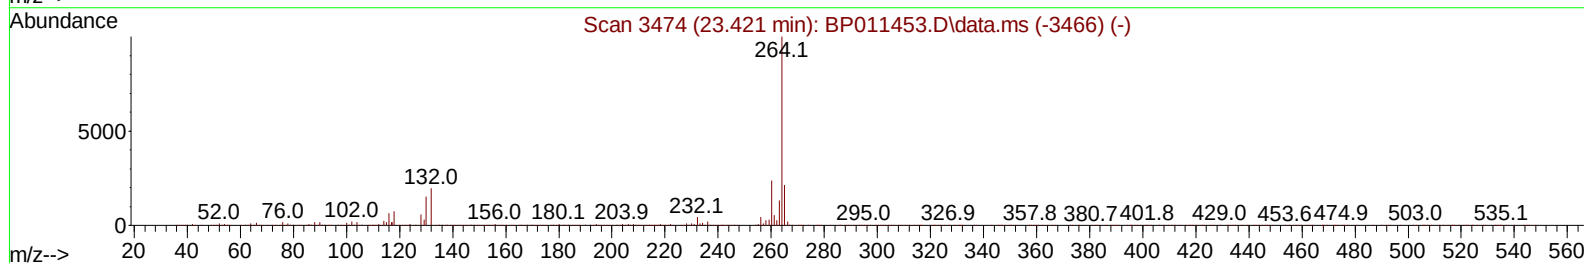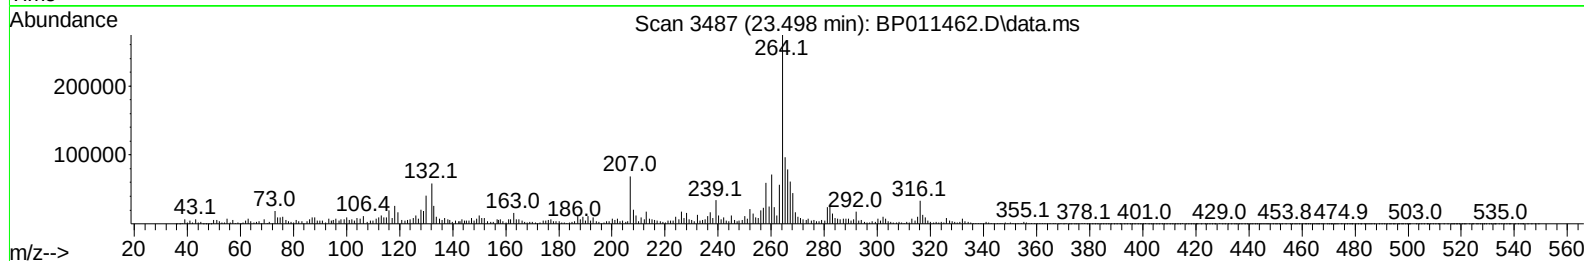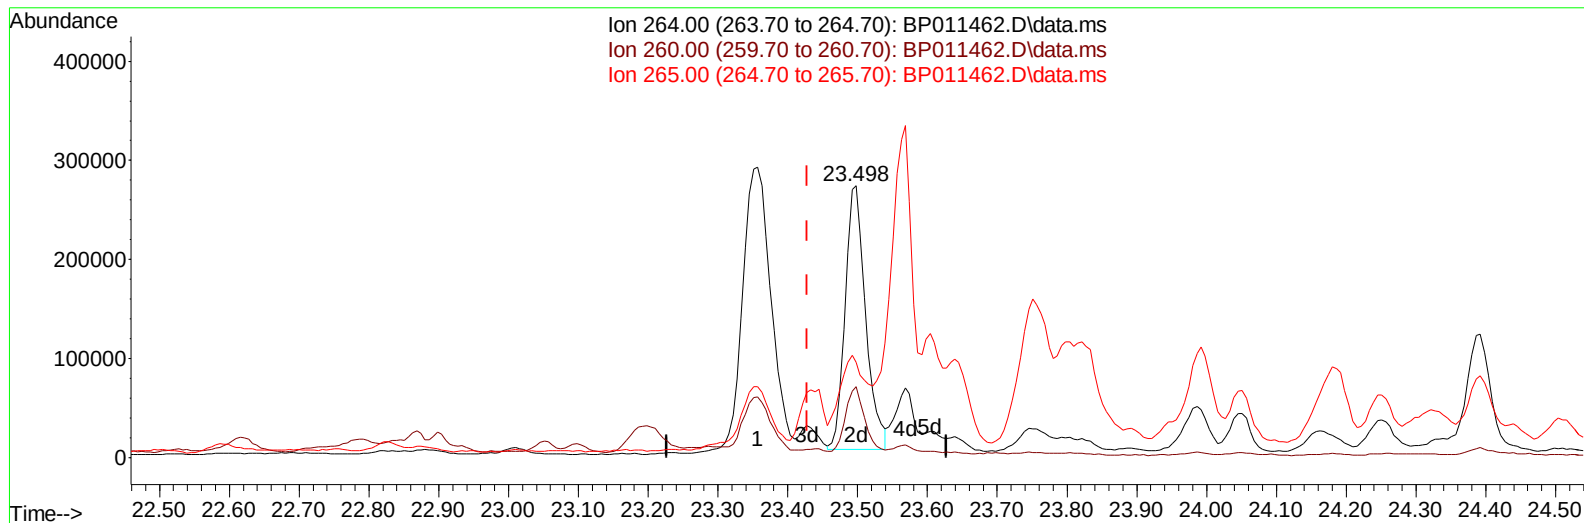

TIC: BP011462.D\data.ms

(88) Perylene-d12 (I)

23.498min (+ 0.071) 20.00 ng/ul m

response 541959

Ion	Exp%	Act%
264.00	100.00	100.00
260.00	24.40	26.07
265.00	22.90	35.12#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081722\
 Data File : BP011462.D
 Acq On : 17 Aug 2022 14:47
 Operator : CG/JU
 Sample : N4173-13MS
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 EX7Q8MS

Manual IntegrationsAPPROVED

Quant Time: Aug 17 23:28:09 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP081622.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Aug 17 01:58:37 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 08/18/2022
 Supervised By :Sohil Jodhani 08/18/2022

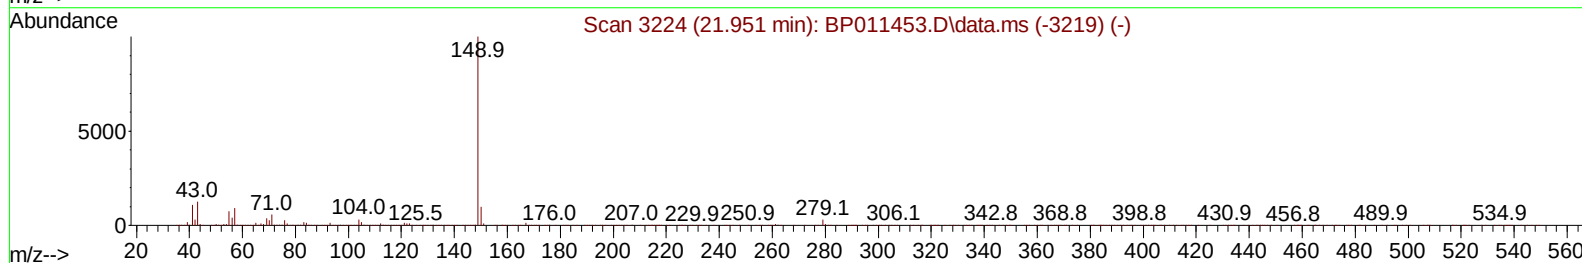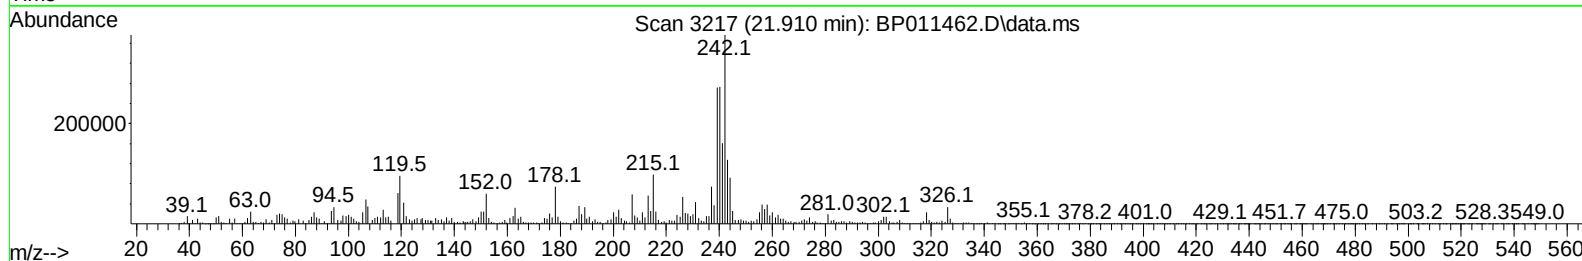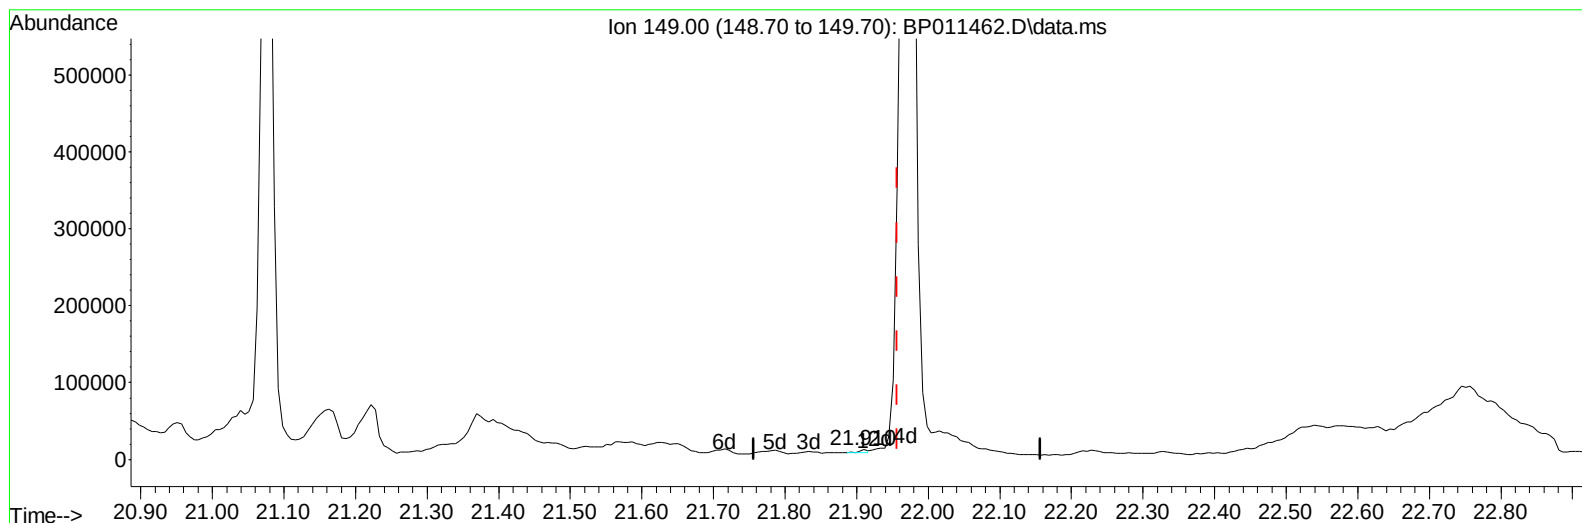

TIC: BP011462.D\data.ms

(89) Di-n-octyl phthalate

21.910min (-0.047) 0.08 ng/u1

response 3415

Ion	Exp%	Act%
149.00	100.00	100.00
0.00	0.00	0.00
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081722\
 Data File : BP011462.D
 Acq On : 17 Aug 2022 14:47
 Operator : CG/JU
 Sample : N4173-13MS
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 EX7Q8MS

Manual IntegrationsAPPROVED

Quant Time: Aug 17 23:28:09 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP081622.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Aug 17 01:58:37 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 08/18/2022
 Supervised By :Sohil Jodhani 08/18/2022

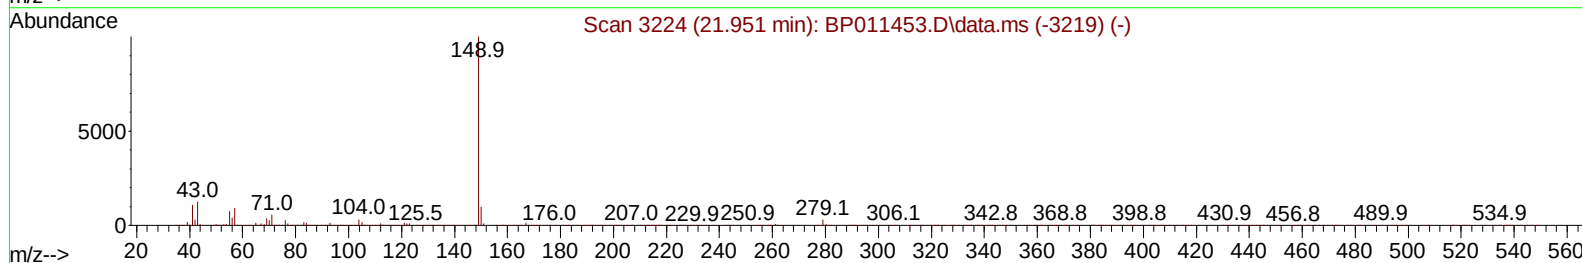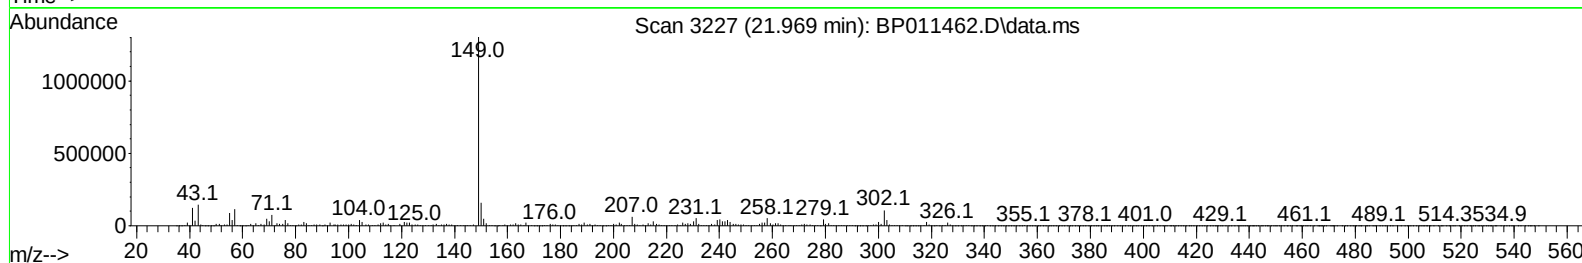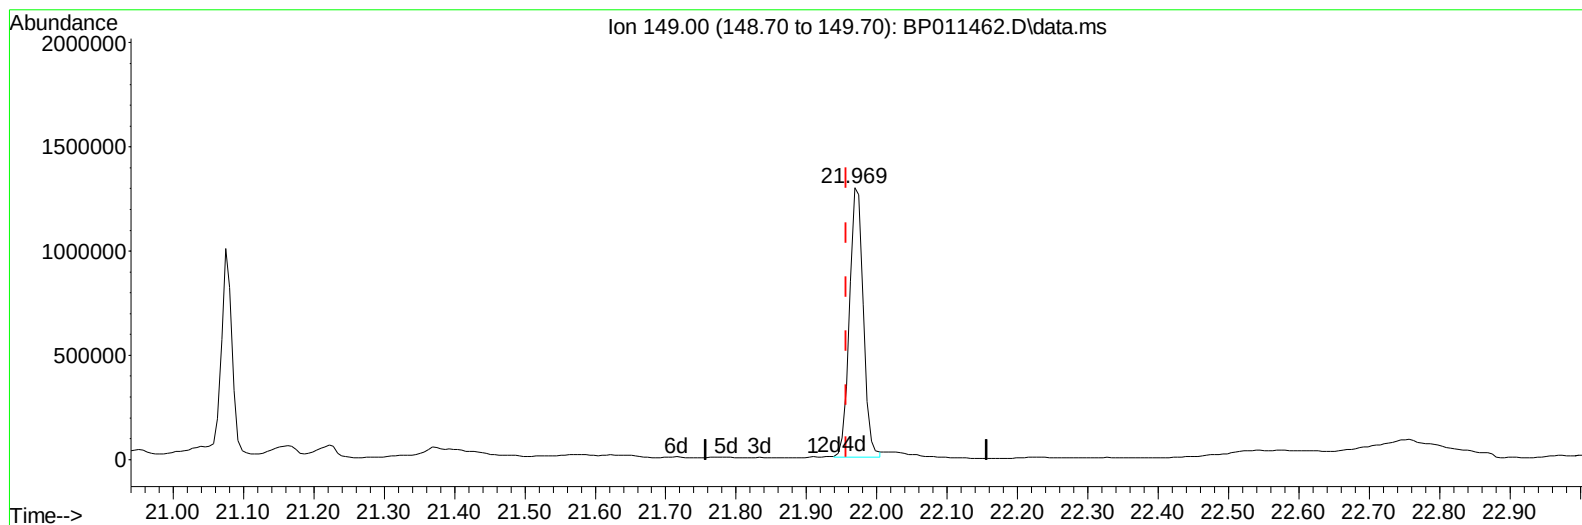

TIC: BP011462.D\data.ms

(89) Di-n-octyl phthalate

21.969min (+ 0.012) 40.27 ng/ul m

response 1754475

Ion	Exp%	Act%
149.00	100.00	100.00
0.00	0.00	0.00
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081722\
 Data File : BP011462.D
 Acq On : 17 Aug 2022 14:47
 Operator : CG/JU
 Sample : N4173-13MS
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 EX7Q8MS

Manual IntegrationsAPPROVED

Quant Time: Aug 17 23:28:09 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP081622.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Aug 17 01:58:37 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 08/18/2022
 Supervised By :Sohil Jodhani 08/18/2022

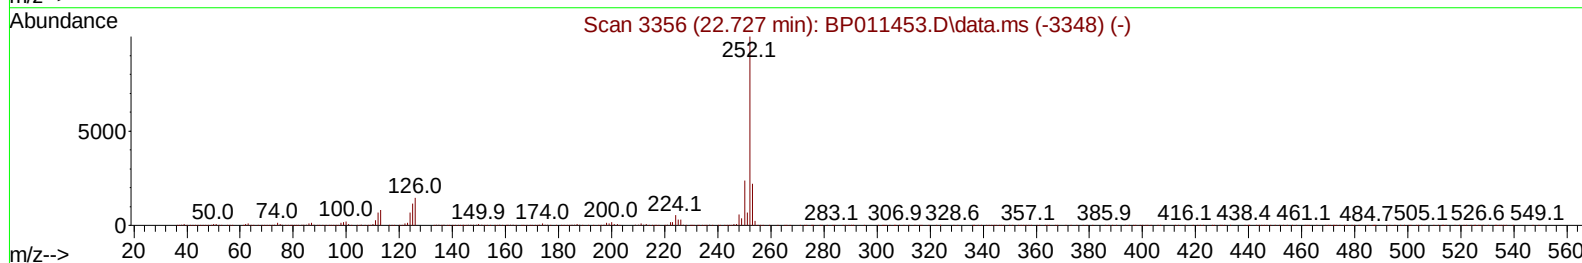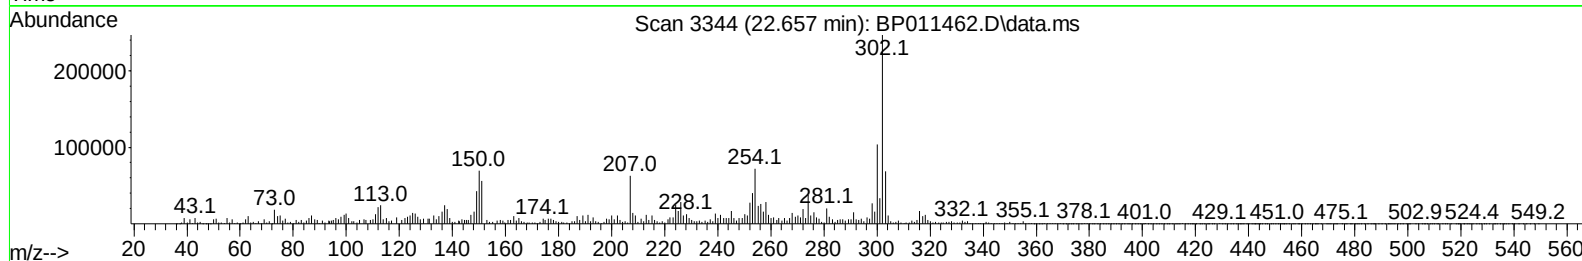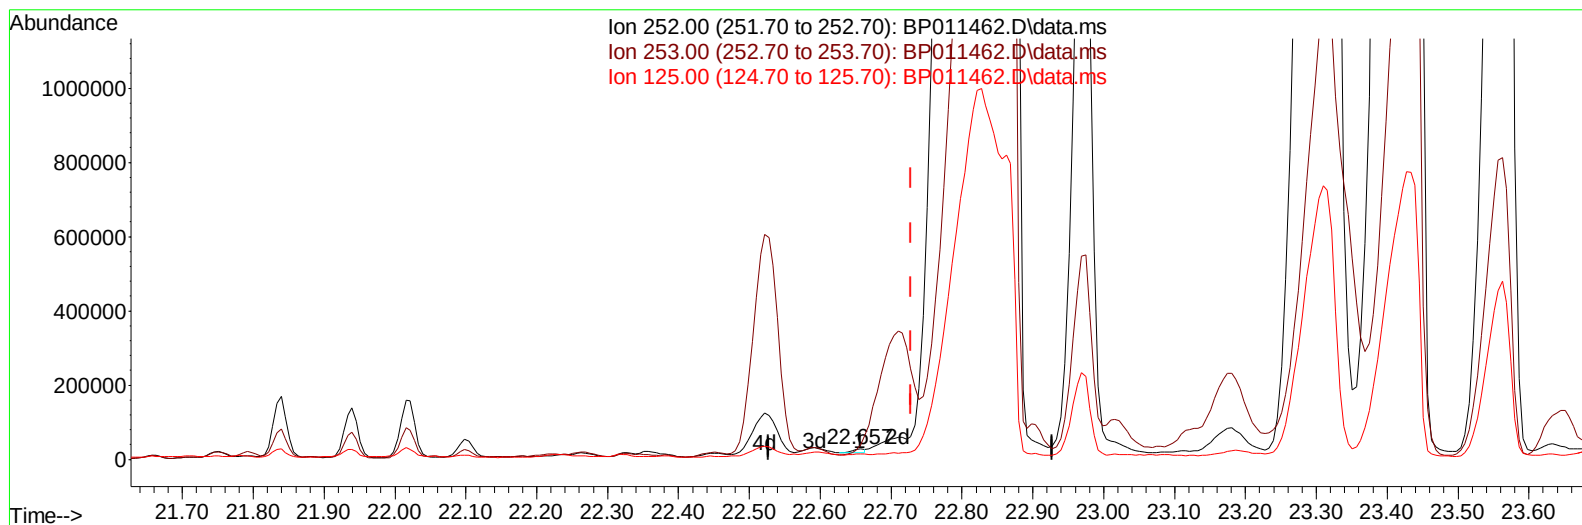

TIC: BP011462.D\data.ms

(90) Benzo(b)fluoranthene

22.657min (-0.071) 0.39 ng/u1

response 13106

Ion	Exp%	Act%
252.00	100.00	100.00
253.00	21.90	141.96#
125.00	11.20	51.20#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081722\
 Data File : BP011462.D
 Acq On : 17 Aug 2022 14:47
 Operator : CG/JU
 Sample : N4173-13MS
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 EX7Q8MS

Manual IntegrationsAPPROVED

Quant Time: Aug 17 23:28:09 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP081622.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Aug 17 01:58:37 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 08/18/2022
 Supervised By :Sohil Jodhani 08/18/2022

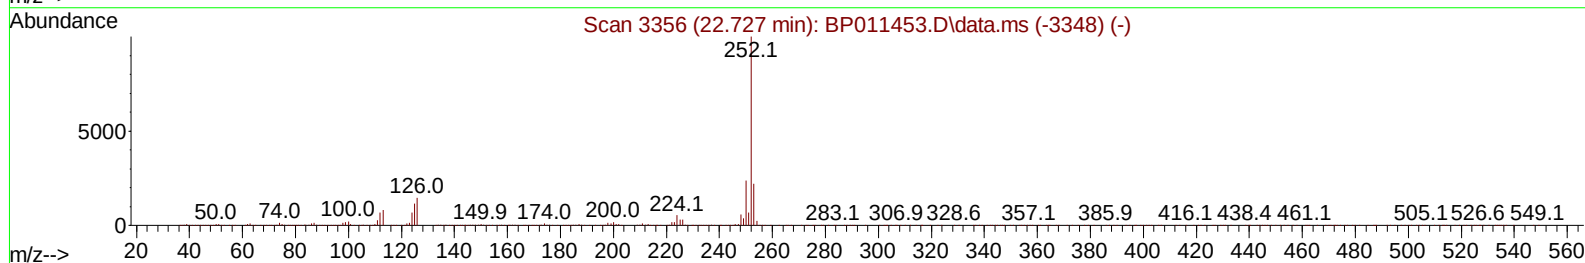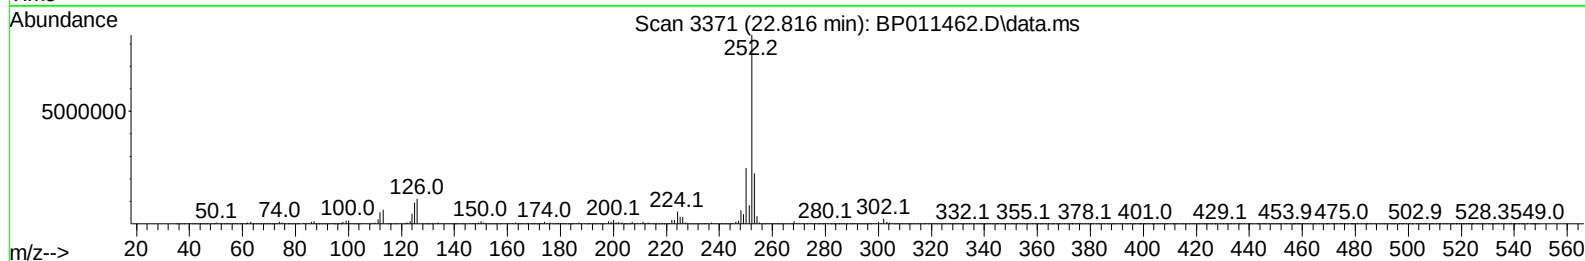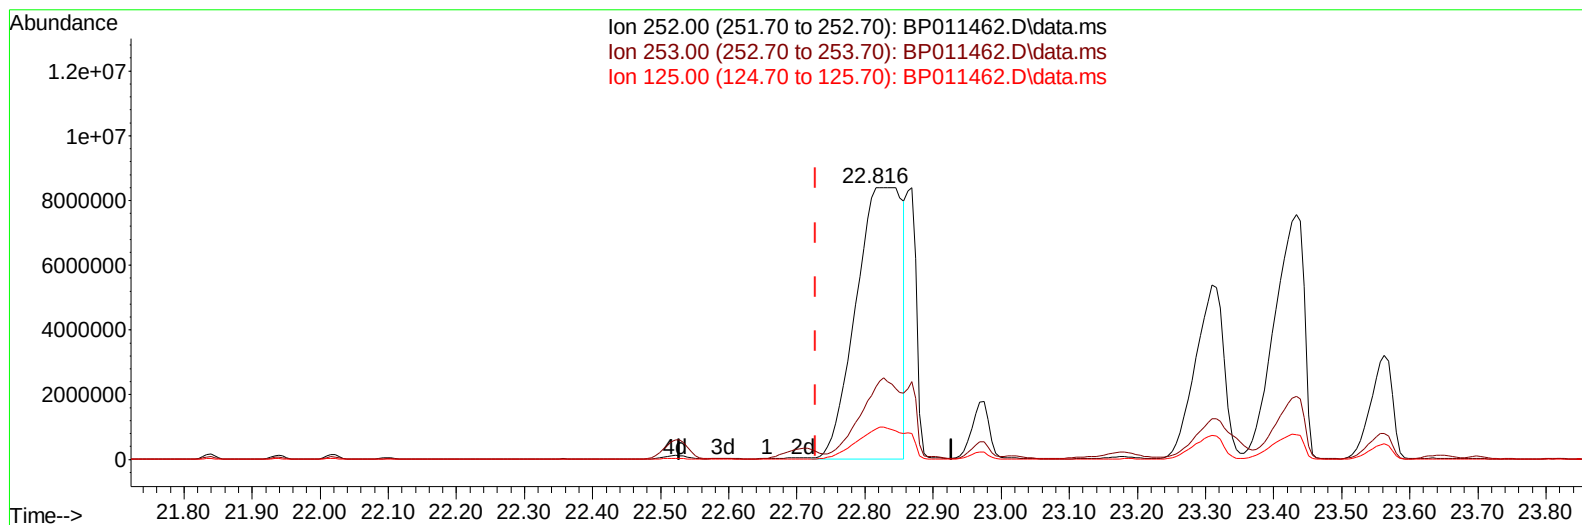

TIC: BP011462.D\data.ms

(90) Benzo(b)fluoranthene

22.816min (+ 0.088) 1174.37 ng/ul m

response 39590525

Ion	Exp%	Act%
252.00	100.00	100.00
253.00	21.90	26.72#
125.00	11.20	11.24
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081722\
 Data File : BP011462.D
 Acq On : 17 Aug 2022 14:47
 Operator : CG/JU
 Sample : N4173-13MS
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 EX7Q8MS

Manual IntegrationsAPPROVED

Quant Time: Aug 17 23:28:09 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP081622.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Aug 17 01:58:37 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 08/18/2022
 Supervised By :Sohil Jodhani 08/18/2022

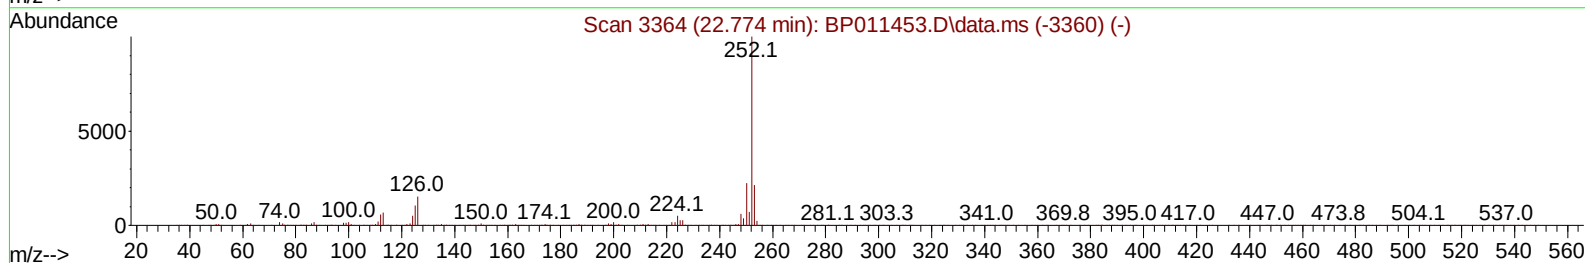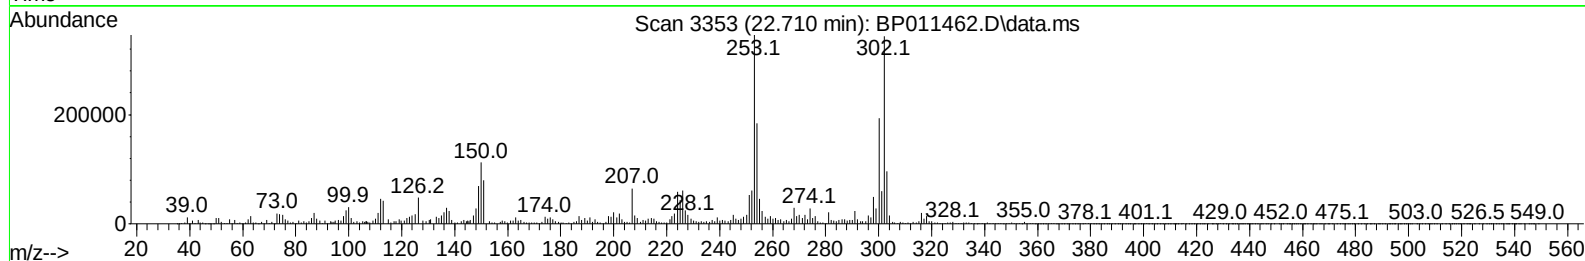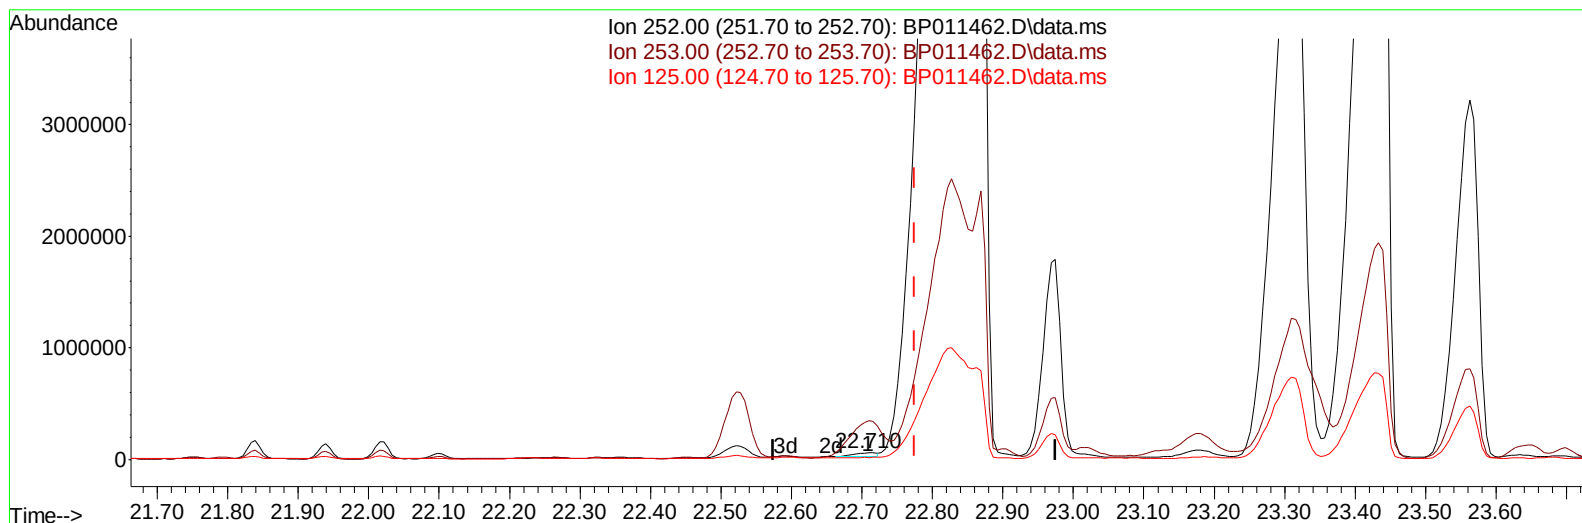

TIC: BP011462.D\data.ms

(91) Benzo(k)fluoranthene

22.710min (-0.065) 2.22 ng/u1

response 71362

Ion	Exp%	Act%
252.00	100.00	100.00
253.00	22.40	571.79#
125.00	12.30	28.35#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081722\
Data File : BP011462.D
Acq On : 17 Aug 2022 14:47
Operator : CG/JU
Sample : N4173-13MS
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
EX7Q8MS

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 08/18/2022
Supervised By :Sohil Jodhani 08/18/2022

Quant Time: Aug 17 23:28:09 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP081622.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Aug 17 01:58:37 2022
Response via : Initial Calibration

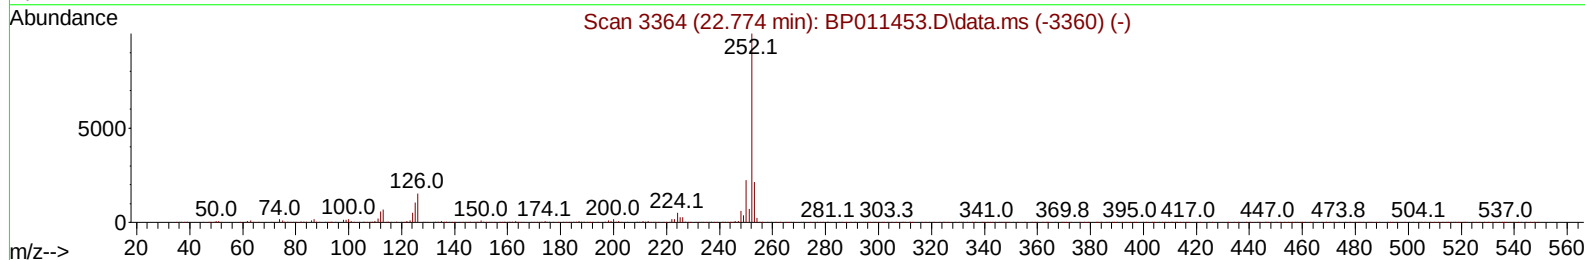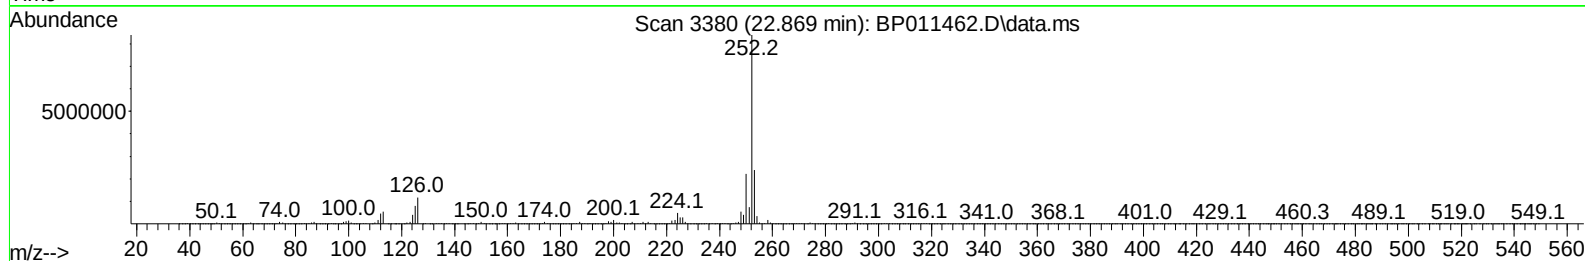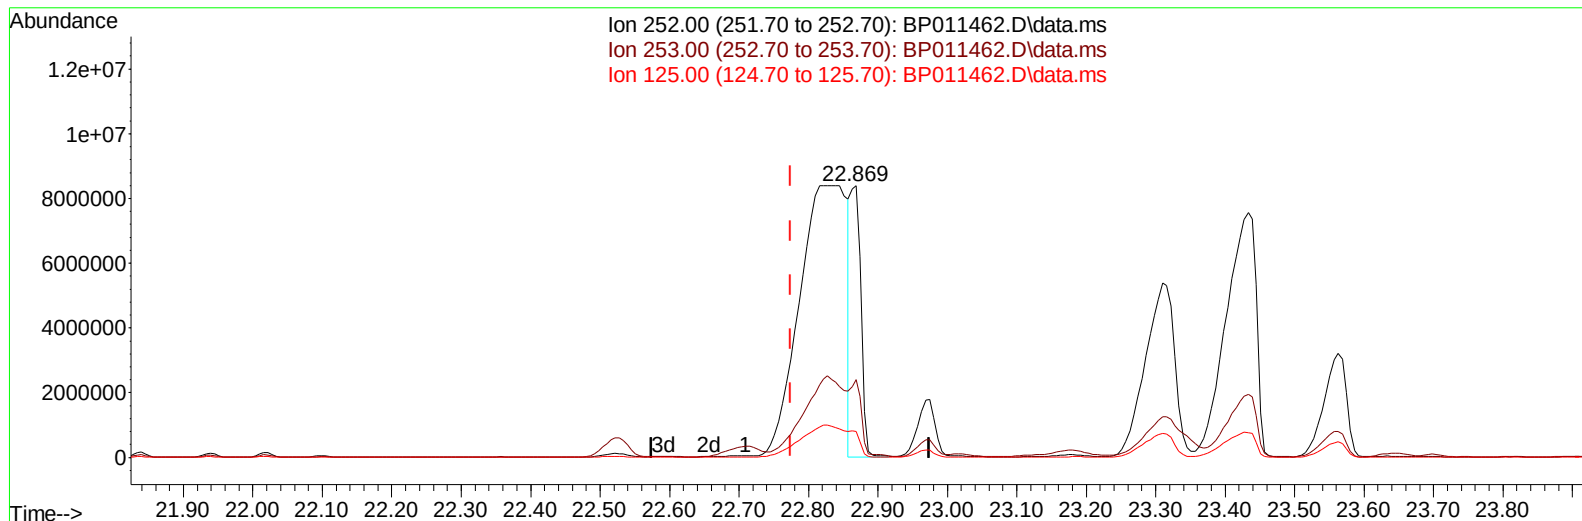

TIC: BP011462.D\data.ms

(91) Benzo(k)fluoranthene

22.869min (+ 0.094) 271.12 ng/ul m

response 8722211

Ion	Exp%	Act%
252.00	100.00	100.00
253.00	22.40	28.65#
125.00	12.30	9.50#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081722\
 Data File : BP011462.D
 Acq On : 17 Aug 2022 14:47
 Operator : CG/JU
 Sample : N4173-13MS
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 EX7Q8MS

Manual IntegrationsAPPROVED

Quant Time: Aug 17 23:28:09 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP081622.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Aug 17 01:58:37 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 08/18/2022
 Supervised By :Sohil Jodhani 08/18/2022

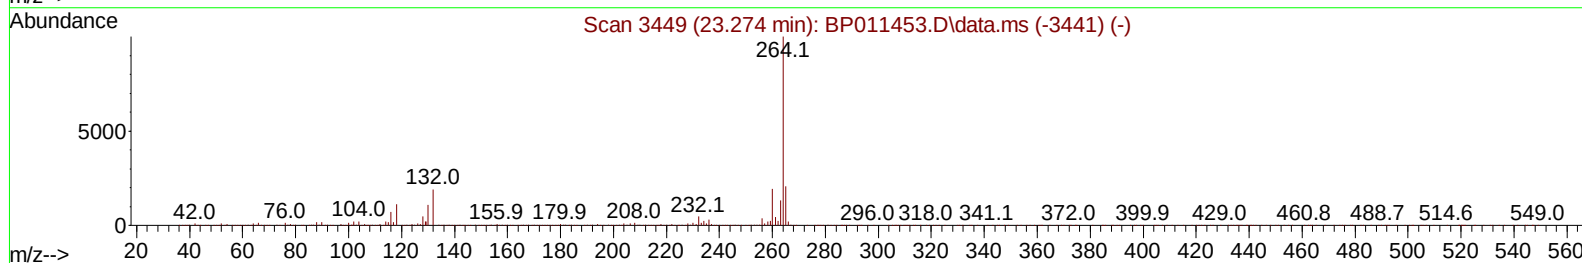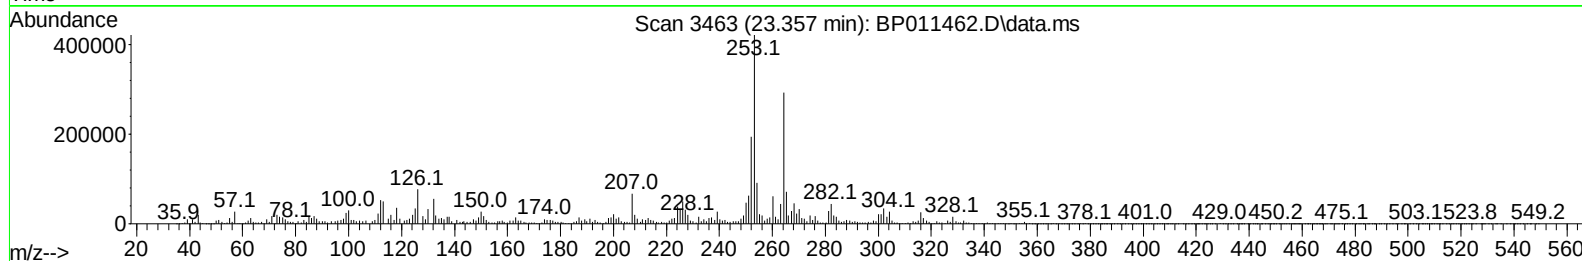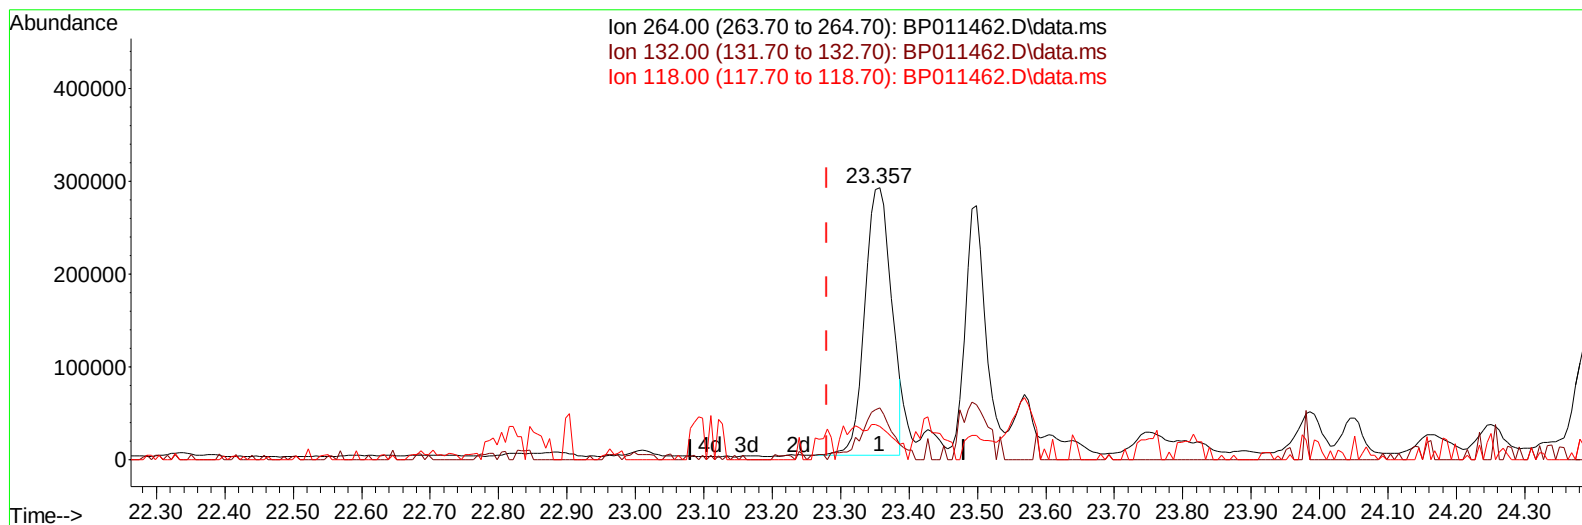

TIC: BP011462.D\data.ms

(92) Benzo(a)pyrene-d12 (S)

23.357min (+ 0.076) 29.59 ng/ul

response 780037

Ion	Exp%	Act%
264.00	100.00	100.00
132.00	17.60	18.90
118.00	11.10	12.21
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081722\
Data File : BP011462.D
Acq On : 17 Aug 2022 14:47
Operator : CG/JU
Sample : N4173-13MS
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
EX7Q8MS

Manual IntegrationsAPPROVED

Quant Time: Aug 17 23:28:09 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP081622.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Aug 17 01:58:37 2022
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 08/18/2022
Supervised By :Sohil Jodhani 08/18/2022

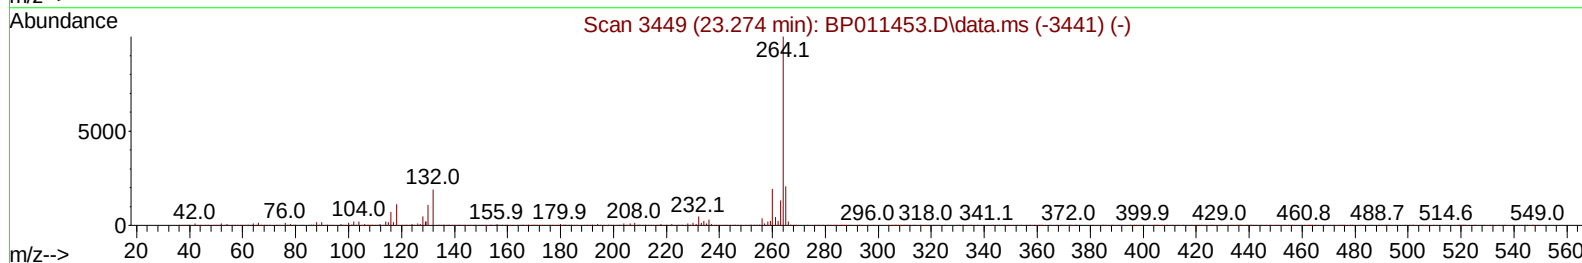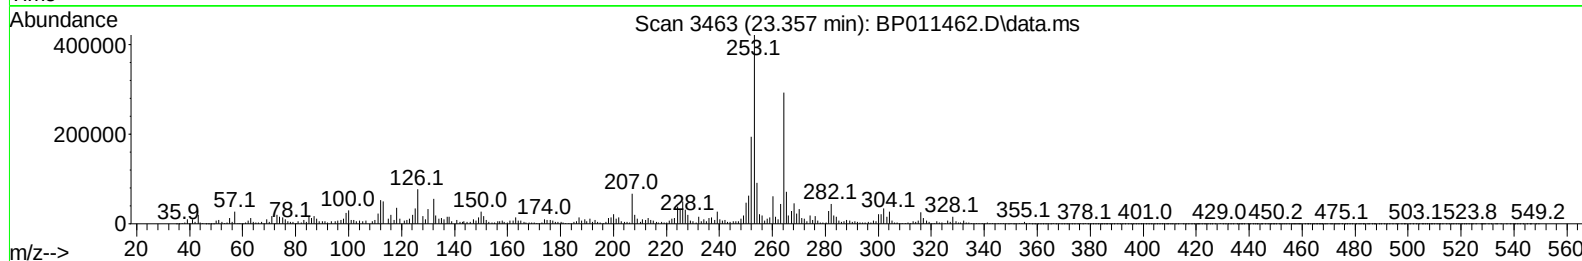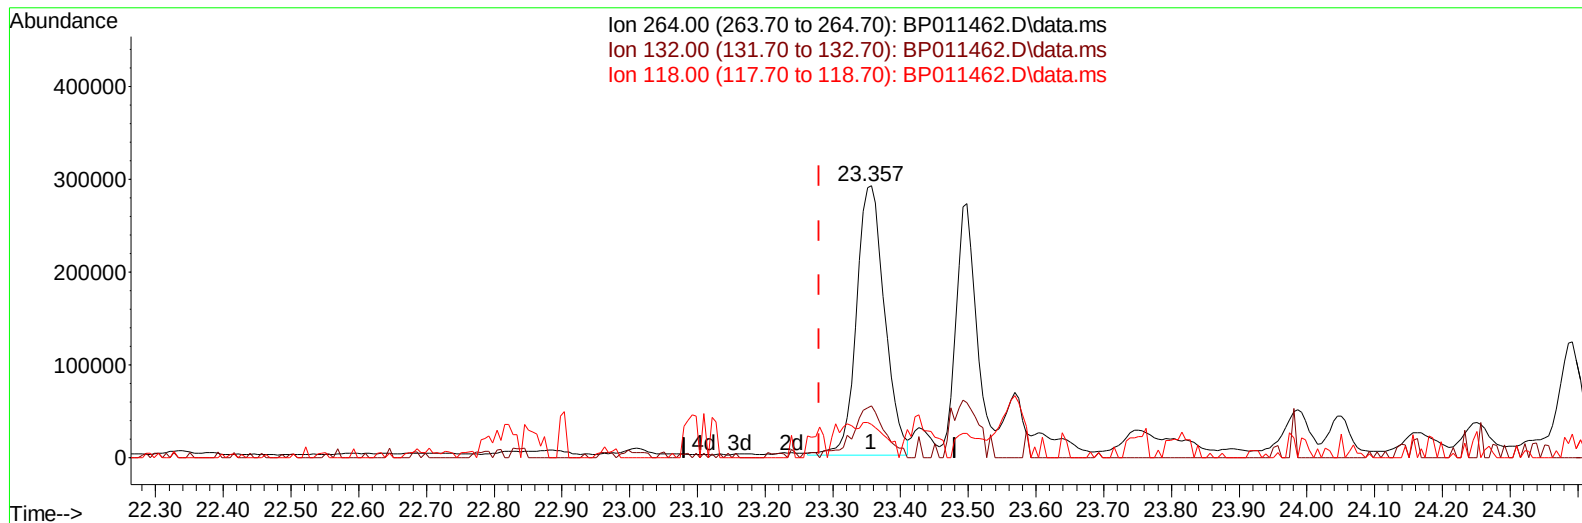

TIC: BP011462.D\data.ms

(92) Benzo(a)pyrene-d12 (S)

23.357min (+ 0.076) 31.84 ng/ul m

response 839453

Ion	Exp%	Act%
264.00	100.00	100.00
132.00	17.60	18.90
118.00	11.10	12.21
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081722\
 Data File : BP011462.D
 Acq On : 17 Aug 2022 14:47
 Operator : CG/JU
 Sample : N4173-13MS
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 EX7Q8MS

Manual IntegrationsAPPROVED

Quant Time: Aug 17 23:28:09 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP081622.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Aug 17 01:58:37 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 08/18/2022
 Supervised By :Sohil Jodhani 08/18/2022

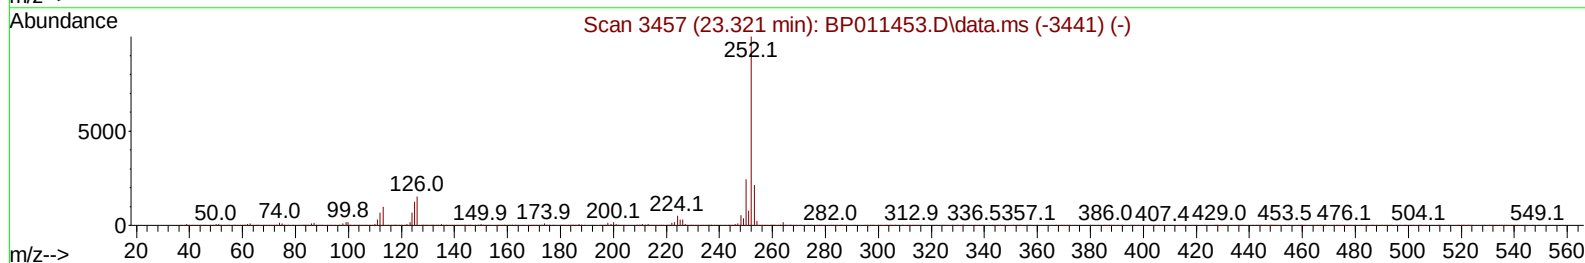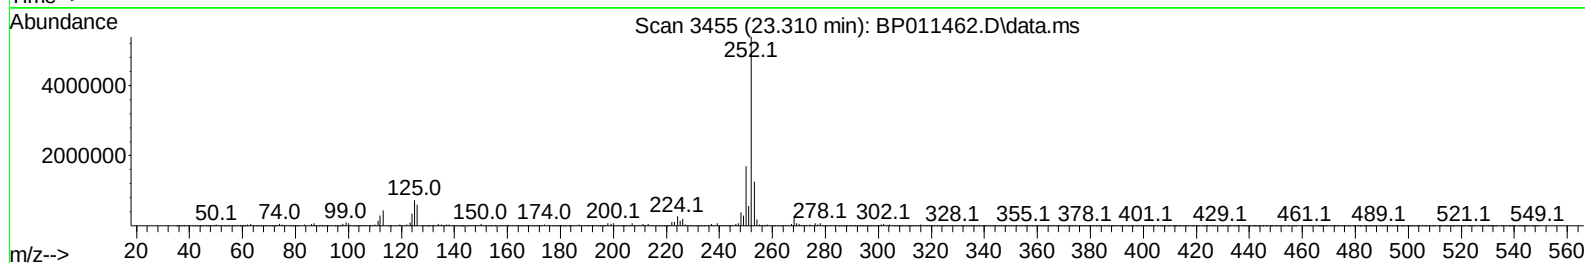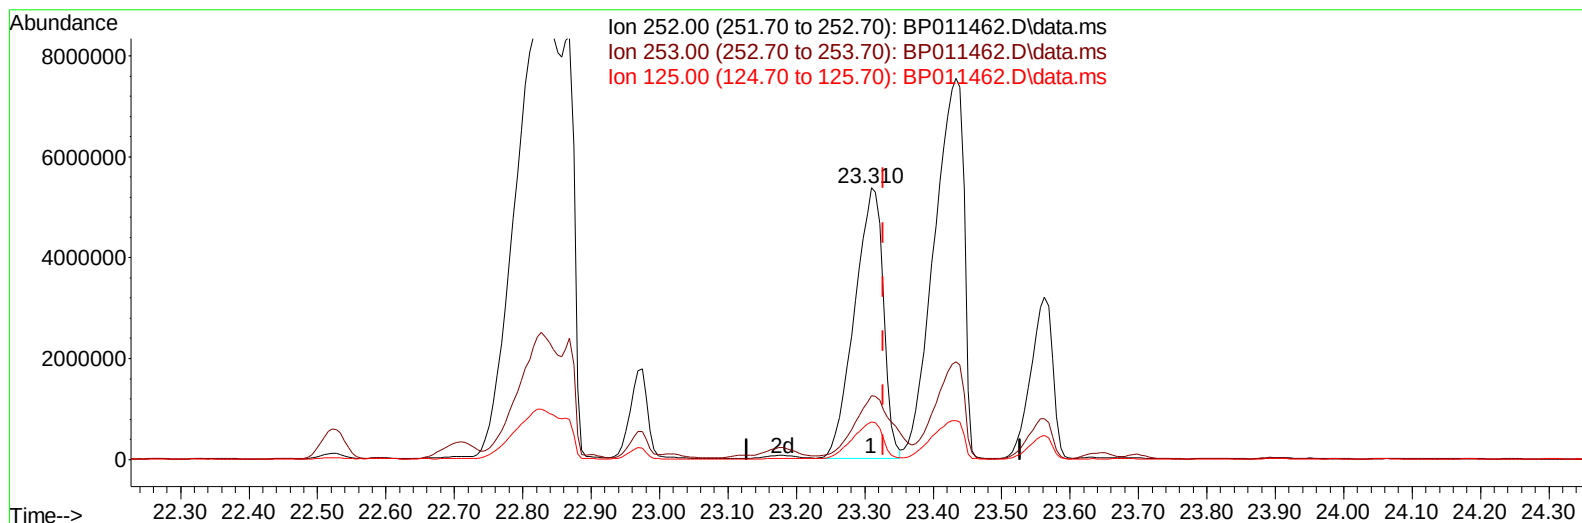

TIC: BP011462.D\data.ms

(93) Benzo(a)pyrene (C)

23.310min (-0.018) 475.14 ng/ul

response 15638671

Ion	Exp%	Act%
252.00	100.00	100.00
253.00	21.00	23.52
125.00	12.40	13.71
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081722\
 Data File : BP011462.D
 Acq On : 17 Aug 2022 14:47
 Operator : CG/JU
 Sample : N4173-13MS
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 EX7Q8MS

Manual IntegrationsAPPROVED

Quant Time: Aug 17 23:28:09 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP081622.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Aug 17 01:58:37 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 08/18/2022
 Supervised By :Sohil Jodhani 08/18/2022

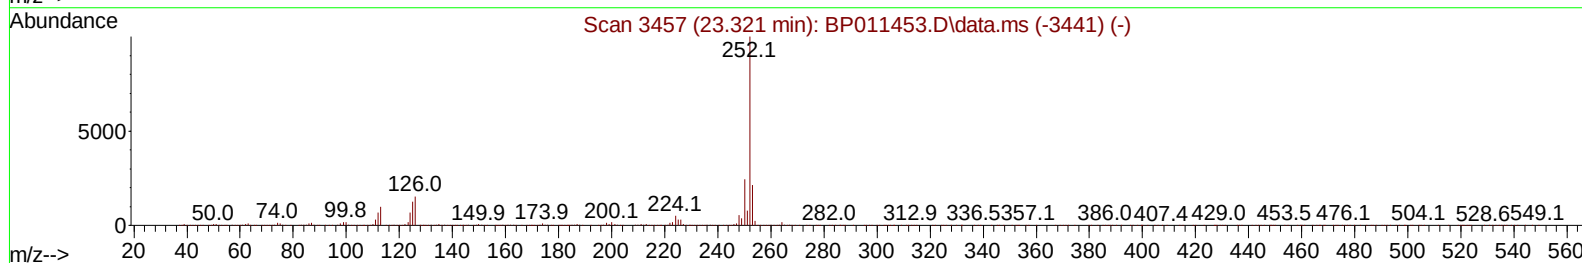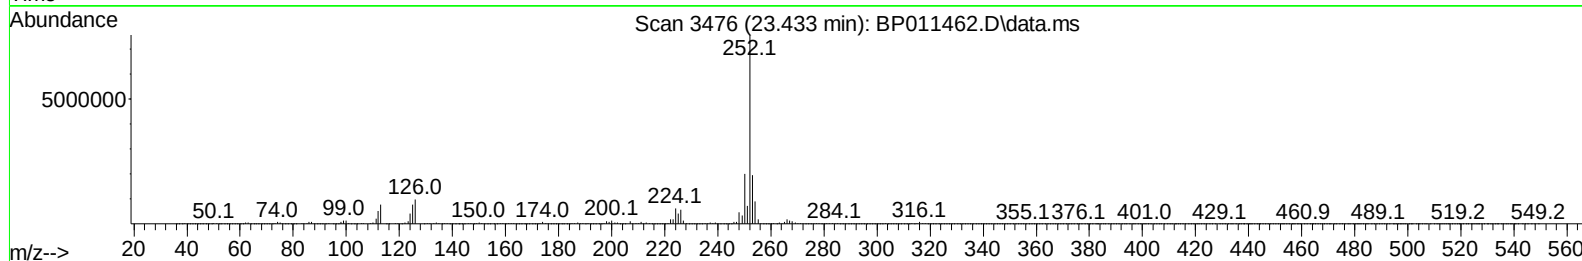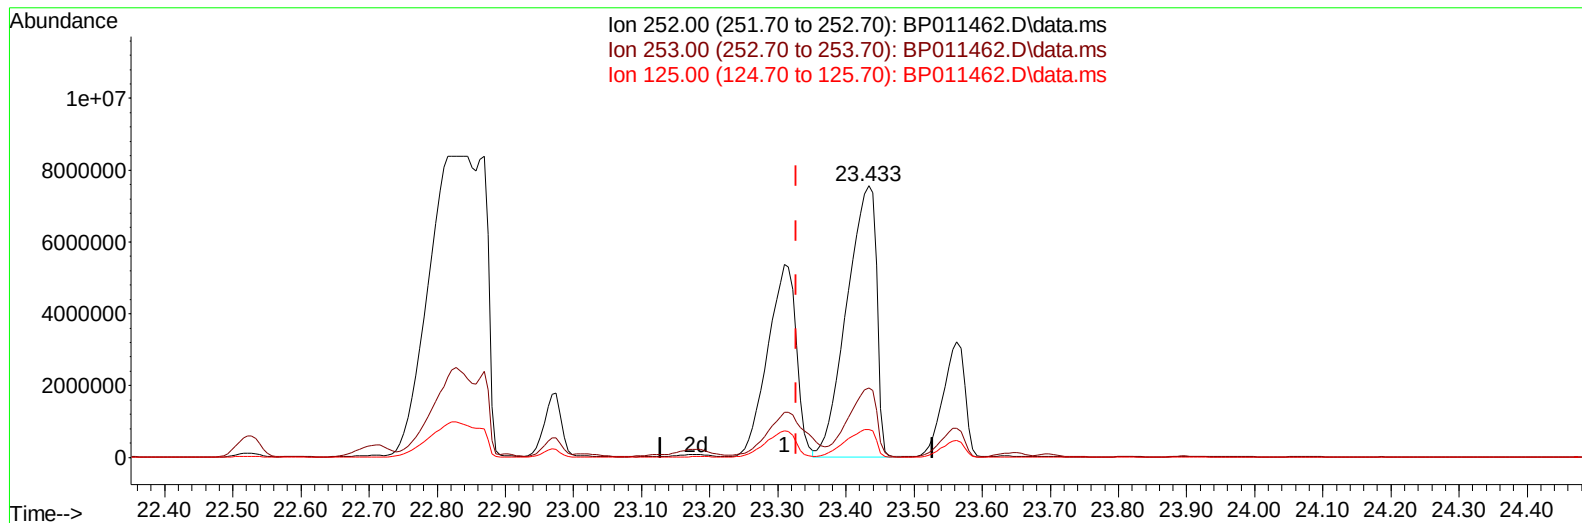

TIC: BP011462.D\data.ms

(93) Benzo(a)pyrene (C)

23.433min (+ 0.106) 696.65 ng/ul m

response 22929271

Ion	Exp%	Act%
252.00	100.00	100.00
253.00	21.00	25.66#
125.00	12.40	10.23
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081722\
 Data File : BP011462.D
 Acq On : 17 Aug 2022 14:47
 Operator : CG/JU
 Sample : N4173-13MS
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 EX7Q8MS

Manual IntegrationsAPPROVED

Quant Time: Aug 17 23:28:09 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP081622.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Aug 17 01:58:37 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 08/18/2022
 Supervised By :Sohil Jodhani 08/18/2022

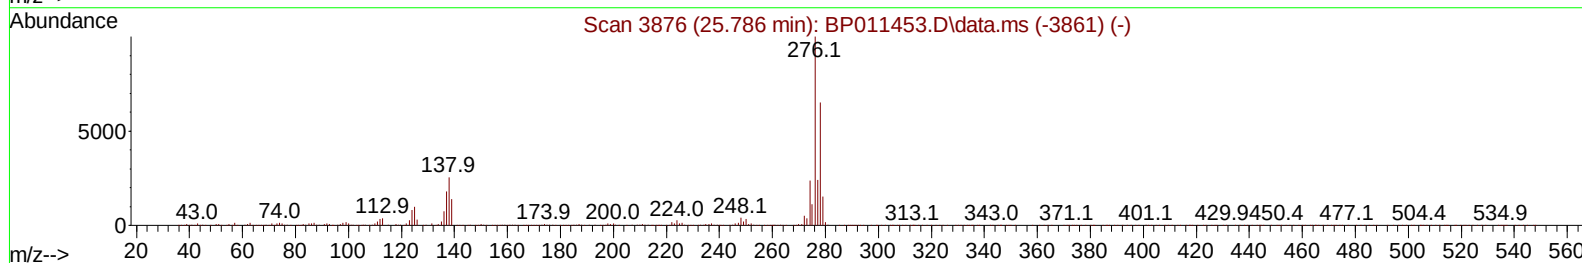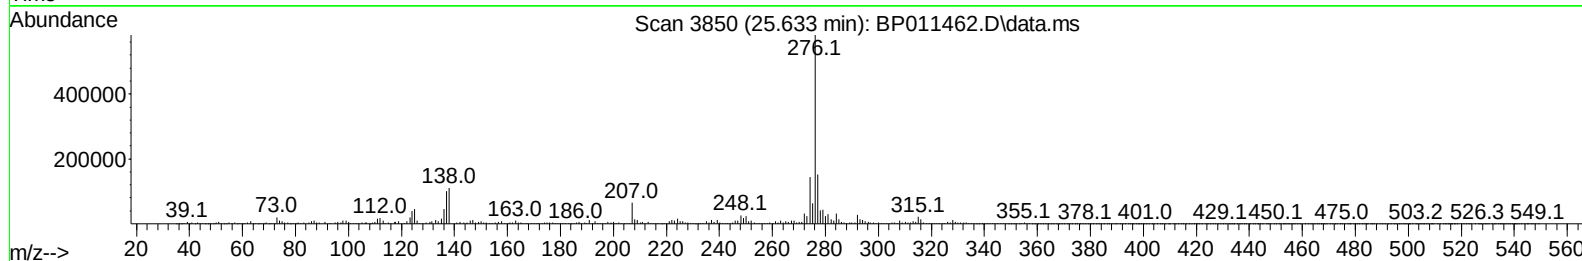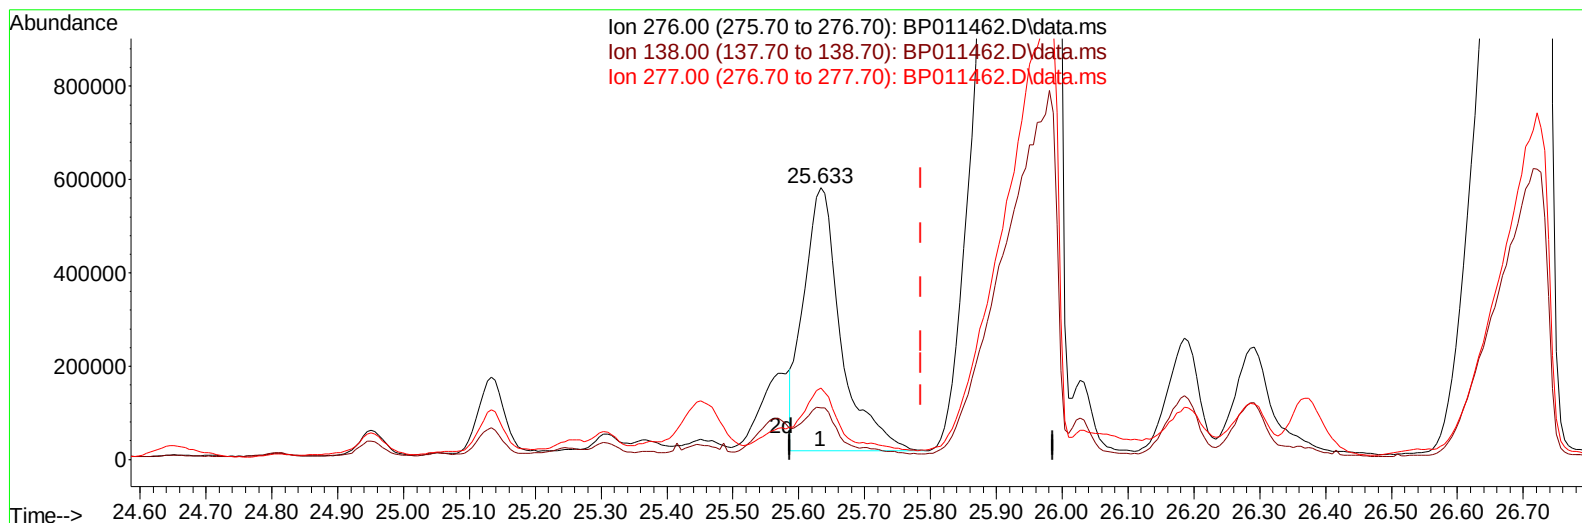

TIC: BP011462.D\data.ms

(94) Indeno(1,2,3-cd)pyrene

25.633min (-0.153) 60.00 ng/u1

response 2202555

Ion	Exp%	Act%
276.00	100.00	100.00
138.00	25.30	19.04#
277.00	25.10	26.20
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081722\
Data File : BP011462.D
Acq On : 17 Aug 2022 14:47
Operator : CG/JU
Sample : N4173-13MS
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
EX7Q8MS

Manual IntegrationsAPPROVED

Quant Time: Aug 17 23:28:09 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP081622.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Aug 17 01:58:37 2022
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 08/18/2022
Supervised By :Sohil Jodhani 08/18/2022

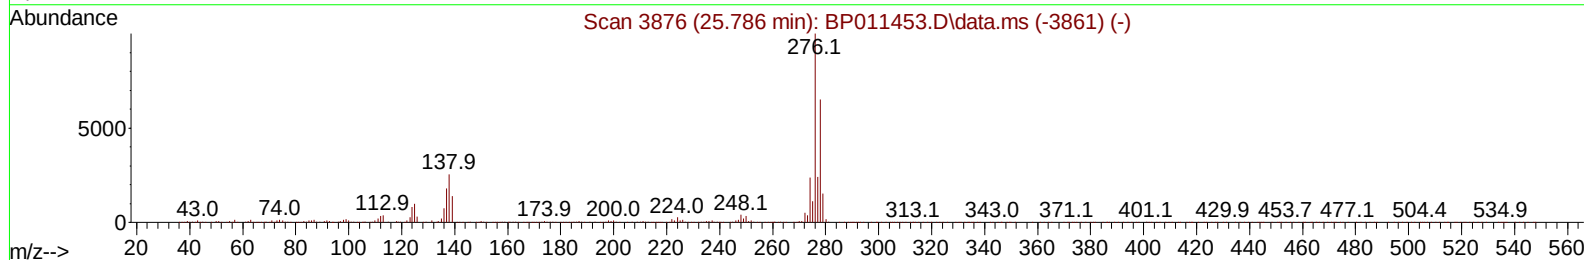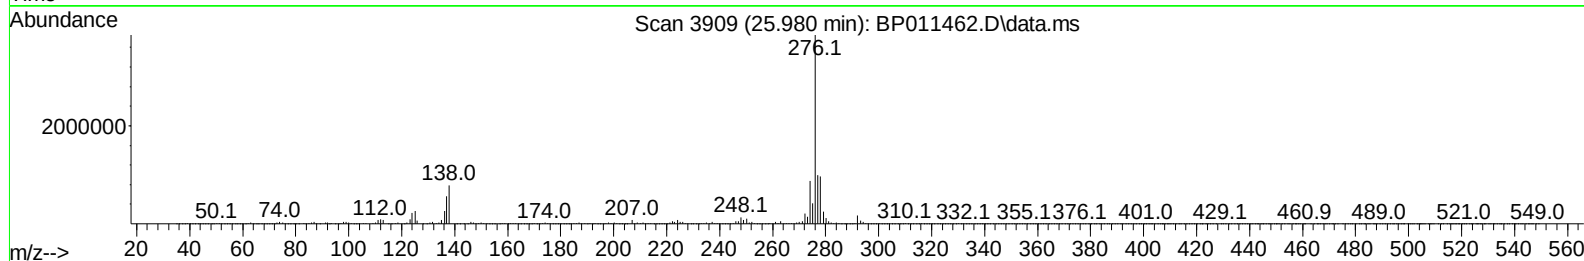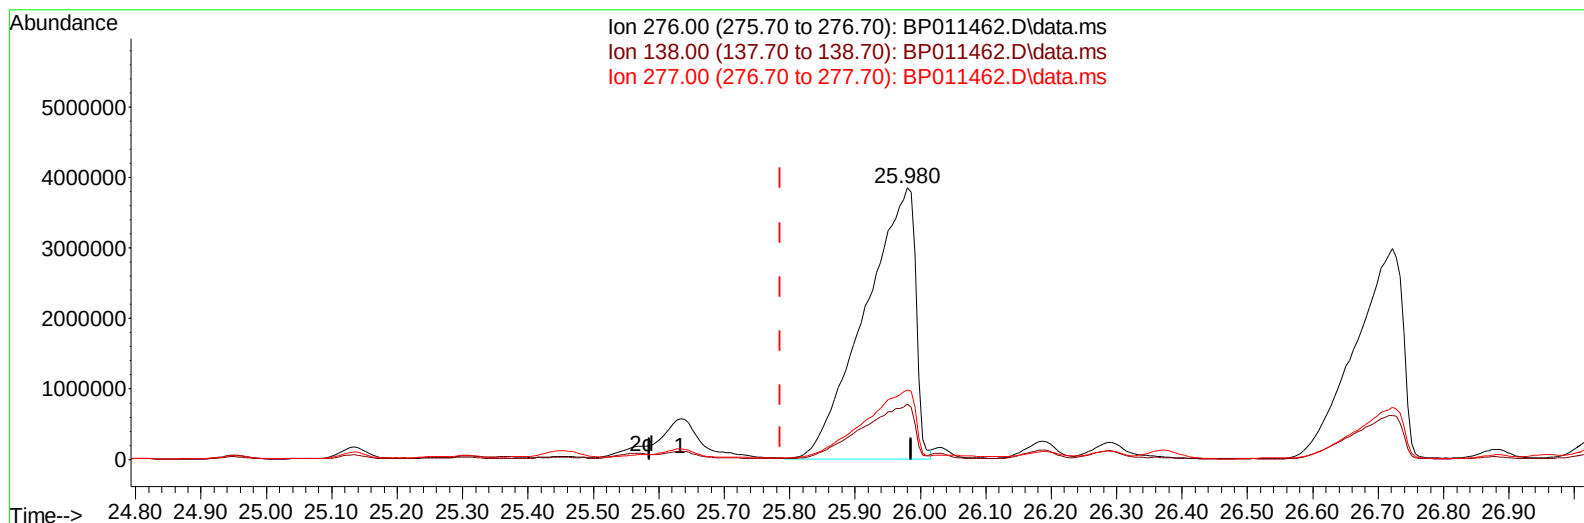

TIC: BP011462.D\data.ms

(94) Indeno(1,2,3-cd)pyrene

25.980min (+ 0.194) 562.04 ng/ul m

response 20633368

Ion	Exp%	Act%
276.00	100.00	100.00
138.00	25.30	20.51
277.00	25.10	25.71
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081722\
 Data File : BP011462.D
 Acq On : 17 Aug 2022 14:47
 Operator : CG/JU
 Sample : N4173-13MS
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 EX7Q8MS

Manual IntegrationsAPPROVED

Quant Time: Aug 17 23:28:09 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP081622.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Aug 17 01:58:37 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 08/18/2022
 Supervised By :Sohil Jodhani 08/18/2022

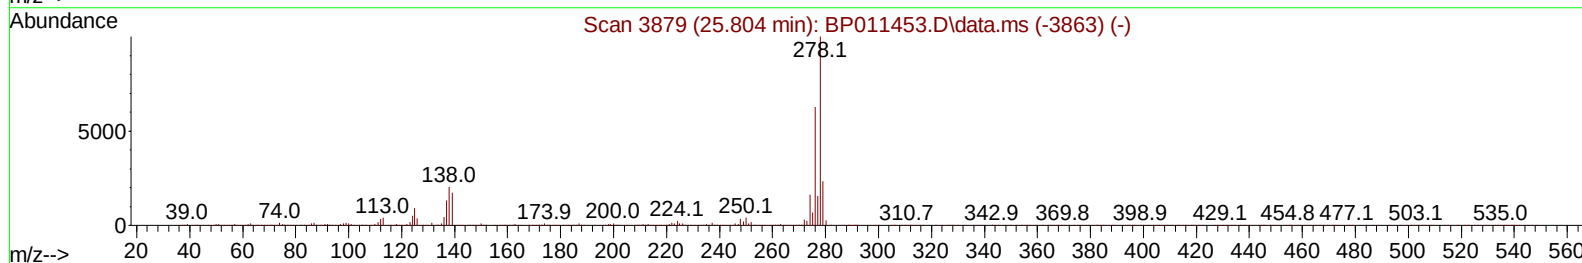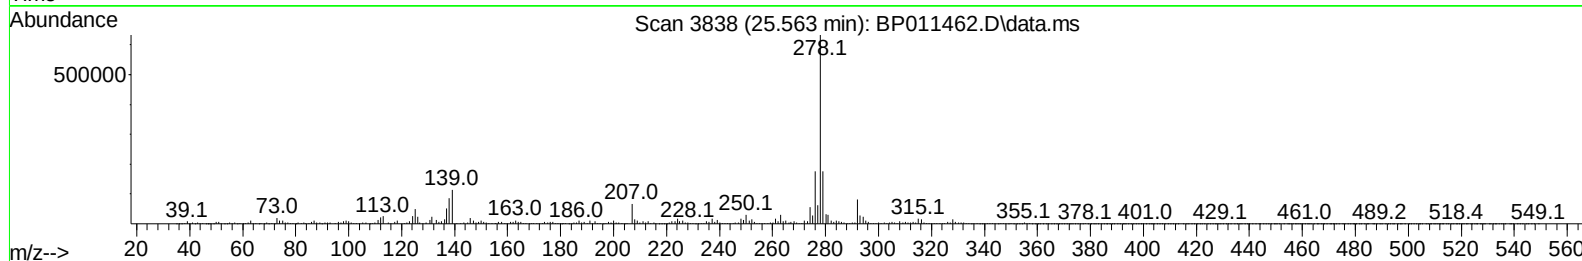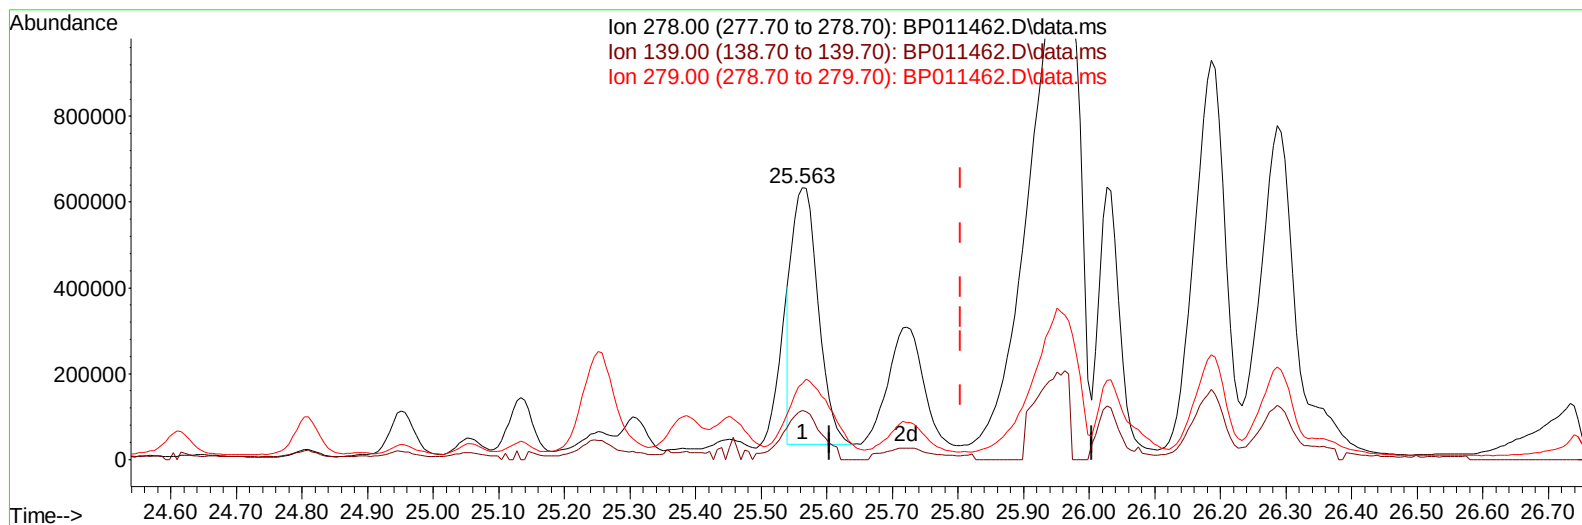

TIC: BP011462.D\data.ms

(95) Dibenzo(a,h)anthracene

25.563min (-0.241) 52.74 ng/u1

response 1667293

Ion	Exp%	Act%
278.00	100.00	100.00
139.00	19.20	18.00
279.00	24.10	27.95
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081722\
Data File : BP011462.D
Acq On : 17 Aug 2022 14:47
Operator : CG/JU
Sample : N4173-13MS
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
EX7Q8MS

Manual IntegrationsAPPROVED

Quant Time: Aug 17 23:28:09 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP081622.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Aug 17 01:58:37 2022
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 08/18/2022
Supervised By :Sohil Jodhani 08/18/2022

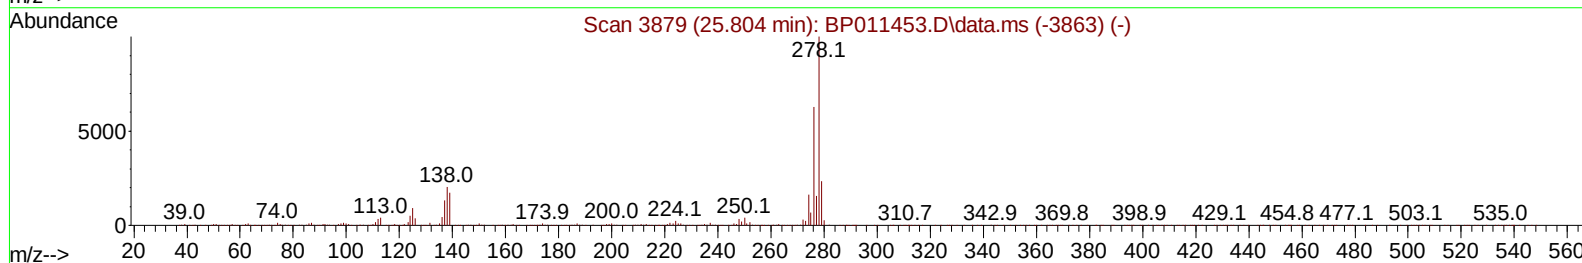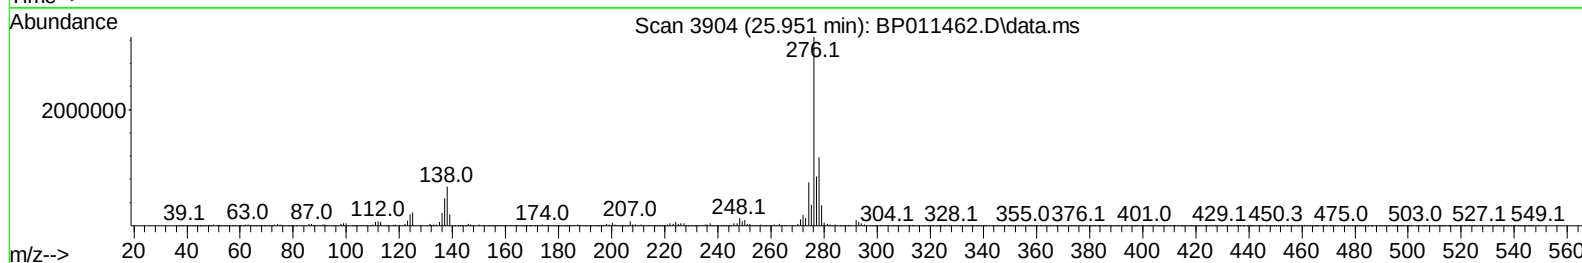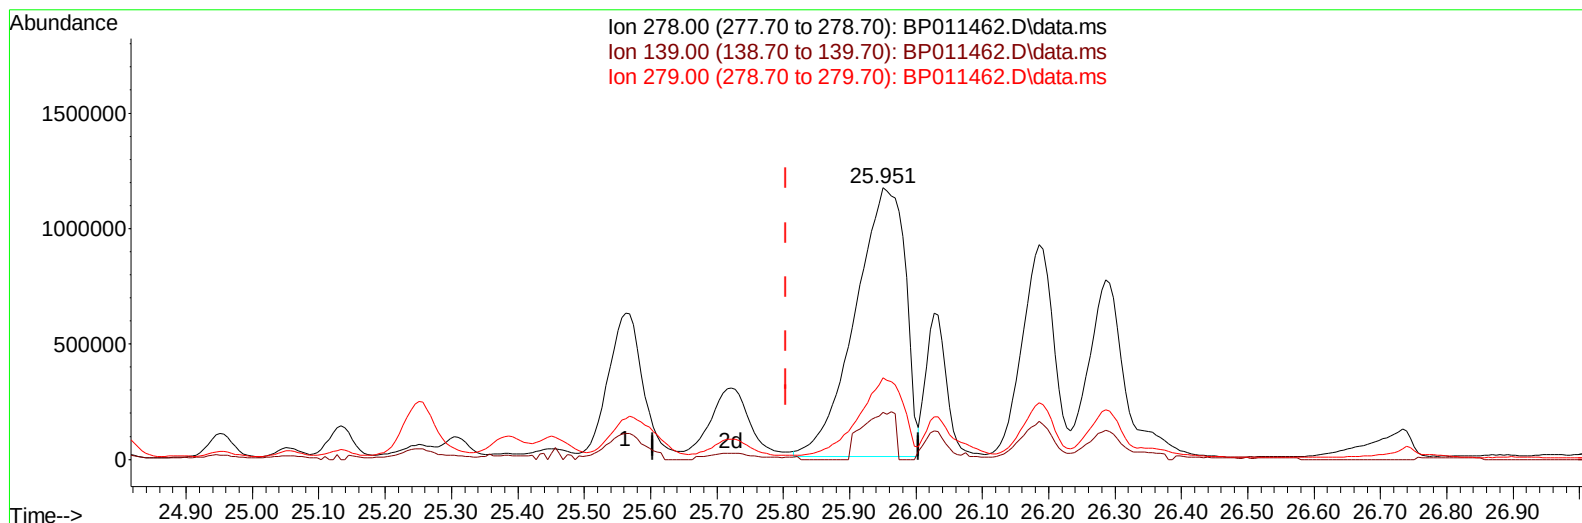

TIC: BP011462.D\data.ms

(95) Dibenzo(a,h)anthracene

25.951min (+ 0.147) 193.72 ng/ul m

response 6123576

Ion	Exp%	Act%
278.00	100.00	100.00
139.00	19.20	17.32
279.00	24.10	29.97#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081722\
Data File : BP011462.D
Acq On : 17 Aug 2022 14:47
Operator : CG/JU
Sample : N4173-13MS
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
EX7Q8MS

Manual IntegrationsAPPROVED

Quant Time: Aug 17 23:28:09 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP081622.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Aug 17 01:58:37 2022
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 08/18/2022
Supervised By :Sohil Jodhani 08/18/2022

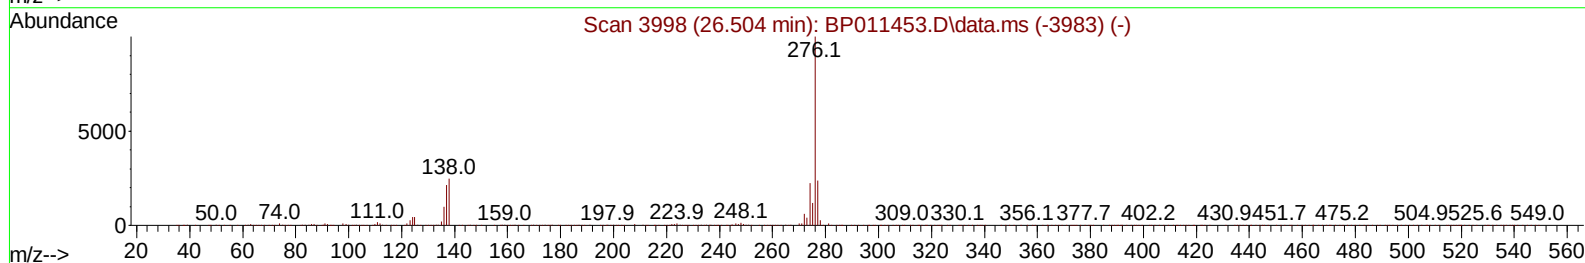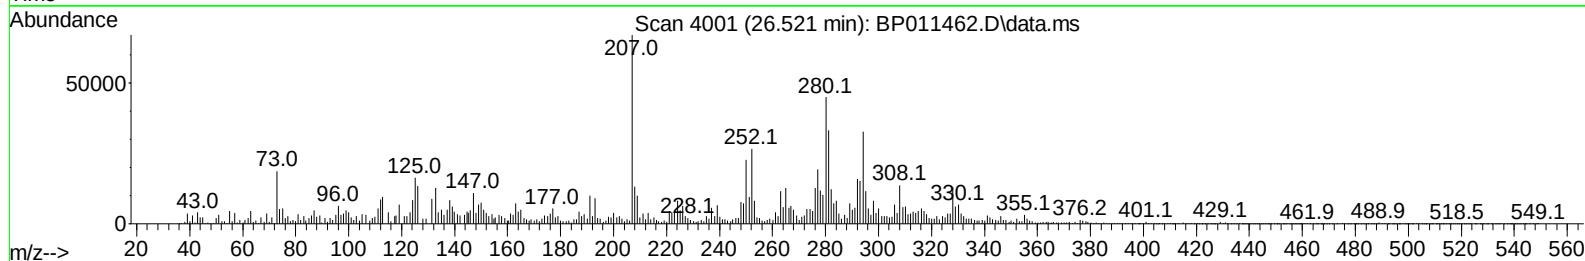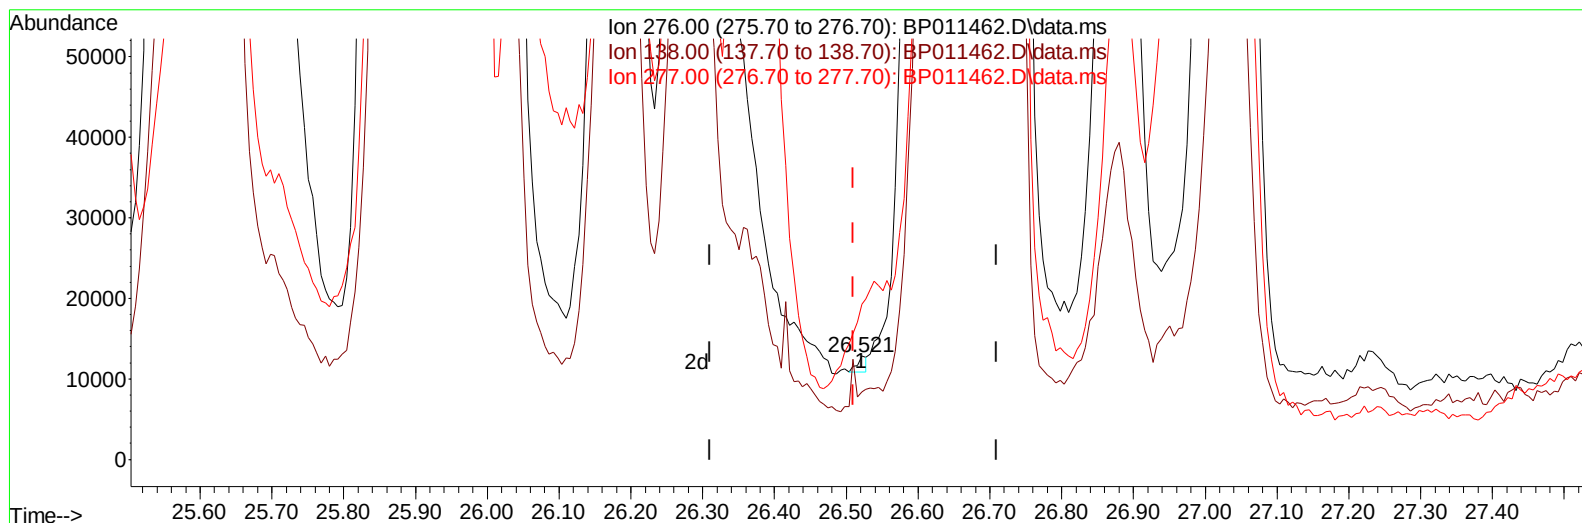

TIC: BP011462.D\data.ms

(96) Benzo(g,h,i)perylene

26.521min (+ 0.012) 0.06 ng/u1

response 1920

Ion	Exp%	Act%
276.00	100.00	100.00
138.00	24.30	65.26#
277.00	23.90	150.56#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081722\
 Data File : BP011462.D
 Acq On : 17 Aug 2022 14:47
 Operator : CG/JU
 Sample : N4173-13MS
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 EX7Q8MS

Manual IntegrationsAPPROVED

Quant Time: Aug 17 23:28:09 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP081622.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Aug 17 01:58:37 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 08/18/2022
 Supervised By :Sohil Jodhani 08/18/2022

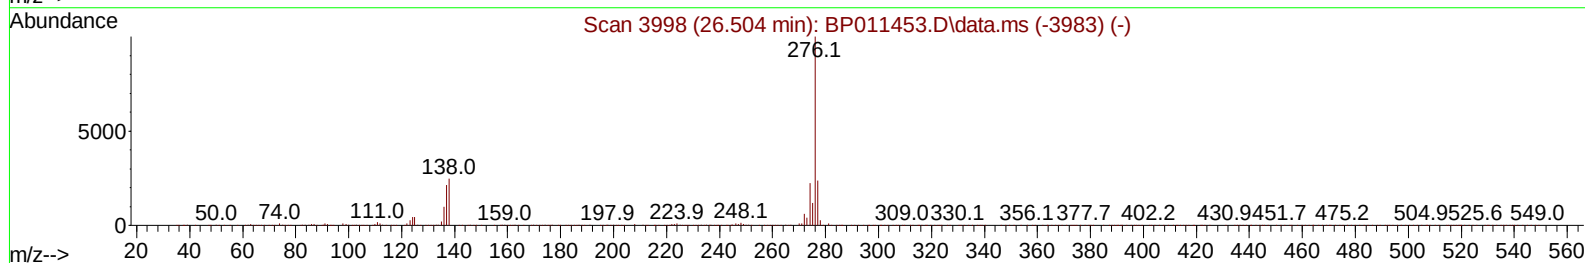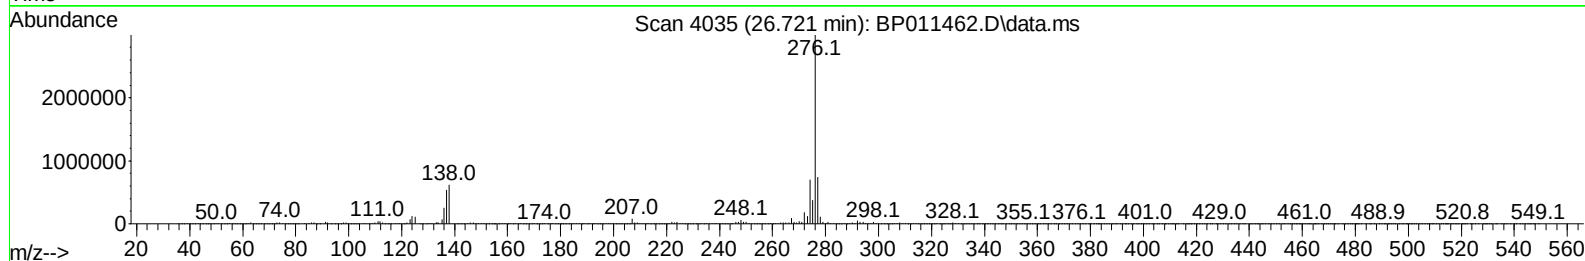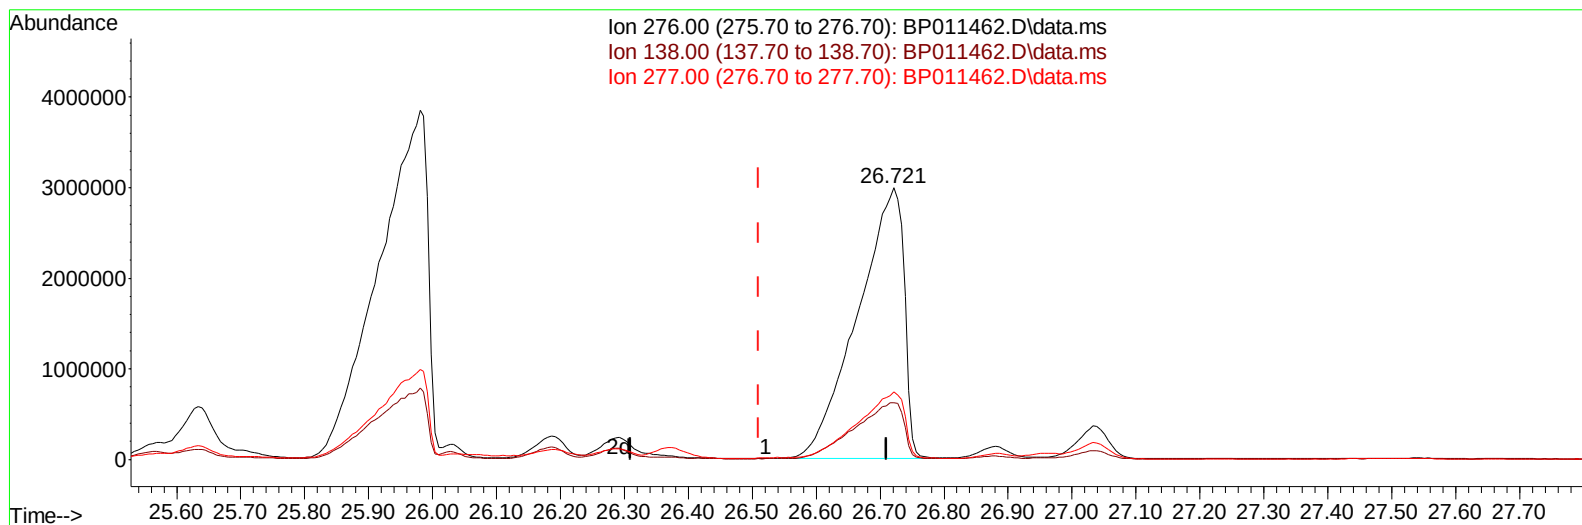

TIC: BP011462.D\data.ms

(96) Benzo(g,h,i)perylene

26.721min (+ 0.212) 483.33 ng/ul m

response 15093245

Ion	Exp%	Act%
276.00	100.00	100.00
138.00	24.30	20.78
277.00	23.90	24.79
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081722\
 Data File : BP011462.D
 Acq On : 17 Aug 2022 14:47
 Operator : CG/JU
 Sample : N4173-13MS
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 EX7Q8MS

Manual IntegrationsAPPROVED

Quant Time: Aug 17 23:28:09 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP081622.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Aug 17 01:58:37 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 08/18/2022
 Supervised By :Sohil Jodhani 08/18/2022

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.558	152	111270	20.000	ng/ul	0.00
20) Naphthalene-d8	10.352	136	473077	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.234	164	267444	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.022	188	488662	20.000	ng/ul	0.02
79) Chrysene-d12	21.175	240	576051	20.000	ng/ul	0.04
88) Perylene-d12	23.498	264	541959m	20.000	ng/ul	0.07
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.070	96	13504	3.766	ng/uL	0.00
4) Pyridine-d5	3.481	84	110711	12.060	ng/ul	0.00
7) Phenol-d5	6.746	99	274947	26.889	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	6.911	67	168059	25.298	ng/ul	0.00
11) 2-Chlorophenol-d4	7.093	132	220782	29.357	ng/ul	0.00
15) 4-Methylphenol-d8	8.287	113	226310	27.652	ng/ul	0.00
21) Nitrobenzene-d5	8.728	128	108353	31.814	ng/ul	0.00
24) 2-Nitrophenol-d4	9.446	143	111279	32.104	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	9.981	165	203296	31.774	ng/ul	0.00
31) 4-Chloroaniline-d4	10.505	131	279155	26.210	ng/ul	0.00
46) Dimethylphthalate-d6	13.663	166	560387	29.625	ng/ul	0.00
49) Acenaphthylene-d8	13.928	160	663459	31.558	ng/ul	0.00
54) 4-Nitrophenol-d4	14.475	143	81972	22.492	ng/ul	0.01
60) Fluorene-d10	15.240	176	474448	29.814	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.404	200	35288	13.364	ng/ul	0.04
73) Anthracene-d10	17.128	188	736703	34.040	ng/ul	0.02
81) Pyrene-d10	19.398	212	803561	27.571	ng/ul	0.04
92) Benzo(a)pyrene-d12	23.357	264	839453m	31.842	ng/ul	0.08
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.105	88	39981	10.693	ng/uL	96
5) Pyridine	3.499	79	208334	22.735	ng/ul	93
6) Benzaldehyde	6.716	77	187883	40.039	ng/ul	97
8) Phenol	6.775	94	428555	40.784	ng/ul	95
10) Bis(2-Chloroethyl)ether	7.005	93	282133	34.420	ng/ul	98
12) 2-Chlorophenol	7.128	128	311136	38.447	ng/ul	98
13) 2-Methylphenol	8.016	108	311569	40.249	ng/ul	99
14) 2,2'-oxybis(1-Chloropr...	8.105	45	394296m	32.471	ng/ul	
16) Acetophenone	8.393	105	479969	35.253	ng/ul	98
17) N-Nitroso-di-n-propyla...	8.387	70	240176	35.465	ng/ul	93
18) 4-Methylphenol	8.352	108	368401	42.986	ng/ul	99
19) Hexachloroethane	8.622	117	127774	34.808	ng/ul	97
22) Nitrobenzene	8.769	77	362801	37.792	ng/ul	95
23) Isophorone	9.299	82	668069	39.644	ng/ul	99
25) 2-Nitrophenol	9.475	139	167205	42.280	ng/ul	97
26) 2,4-Dimethylphenol	9.546	107	402112	42.823	ng/ul	94
27) Bis(2-Chloroethoxy)met...	9.787	93	377722	37.082	ng/ul	98
29) 2,4-Dichlorophenol	10.010	162	277907	42.442	ng/ul	98
30) Naphthalene	10.410	128	8193761	328.030	ng/ul	99
32) 4-Chloroaniline	10.528	127	296164	26.839	ng/ul	99
33) Hexachlorobutadiene	10.681	225	153123	36.733	ng/ul	96
34) Caprolactam	11.340	113	93665	39.450	ng/ul	91
35) 4-Chloro-3-methylphenol	11.669	107	341138	41.207	ng/ul	97

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081722\
 Data File : BP011462.D
 Acq On : 17 Aug 2022 14:47
 Operator : CG/JU
 Sample : N4173-13MS
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 EX7Q8MS

Manual IntegrationsAPPROVED

Quant Time: Aug 17 23:28:09 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP081622.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Aug 17 01:58:37 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 08/18/2022
 Supervised By :Sohil Jodhani 08/18/2022

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
36) 2-Methylnaphthalene	12.034	142	1880952	115.742	ng/ul	98
37) 1-Methylnaphthalene	12.252	142	1524520	92.492	ng/ul	97
39) 1,2,4,5-Tetrachloroben...	12.404	216	280342	41.299	ng/ul	96
40) Hexachlorocyclopentadiene	12.375	237	30669	7.283	ng/ul	96
41) 2,4,6-Trichlorophenol	12.657	196	198276	45.384	ng/ul	99
42) 2,4,5-Trichlorophenol	12.728	196	213832	43.968	ng/ul	97
43) 1,1'-Biphenyl	13.063	154	1330405	66.761	ng/ul	100
44) 2-Chloronaphthalene	13.099	162	610381	40.647	ng/ul	100
45) 2-Nitroaniline	13.328	65	230823	45.037	ng/ul	94
47) Dimethylphthalate	13.710	163	772448	39.510	ng/ul	99
48) 2,6-Dinitrotoluene	13.840	165	162744	46.301	ng/ul	91
50) Acenaphthylene	13.963	152	4341570	173.828	ng/ul	99
51) 3-Nitroaniline	14.163	138	168860	44.105	ng/ul	99
52) Acenaphthene	14.304	153	932685	55.753	ng/ul	98
53) 2,4-Dinitrophenol	14.393	184	43635	20.283	ng/ul#	73
55) 4-Nitrophenol	14.493	109	156668	36.079	ng/ul	94
56) Dibenzofuran	14.645	168	4047543	175.453	ng/ul	100
57) 2,4-Dinitrotoluene	14.640	165	244456	46.458	ng/ul#	4
58) 2,3,4,6-Tetrachlorophenol	14.875	232	162701	42.611	ng/ul	98
59) Diethylphthalate	15.087	149	834367	38.965	ng/ul	99
61) Fluorene	15.304	166	2510678	133.032	ng/ul	99
62) 4-Chlorophenyl-phenyle...	15.298	204	330005	38.707	ng/ul	98
63) 4-Nitroaniline	15.345	138	219609m	59.384	ng/ul	
66) 4,6-Dinitro-2-methylph...	15.416	198	57905	21.200	ng/ul#	89
67) N-Nitrosodiphenylamine	15.522	169	638317	44.524	ng/ul	98
68) 4-Bromophenyl-phenylether	16.198	248	194969	44.695	ng/ul	95
69) Hexachlorobenzene	16.316	284	221432	44.046	ng/ul	97
70) Atrazine	16.504	200	124295	23.231	ng/ul	99
71) Pentachlorophenol	16.675	266	121627	39.018	ng/ul	99
72) Phenanthrene	17.075	178	23532750m	889.719	ng/ul	
74) Anthracene	17.163	178	6965616	261.038	ng/ul	99
75) 1,2,3,4-Tetrachloroben...	13.022	216	280729	44.691	ng/uL	98
76) Pentachlorobenzene	14.563	250	266575	44.724	ng/uL	98
77) Carbazole	17.439	167	3122776	124.418	ng/ul	99
78) Di-n-butylphthalate	18.004	149	1420855	45.970	ng/ul	99
80) Fluoranthene	19.069	202	30772453m	858.559	ng/ul	
82) Pyrene	19.428	202	28110539m	746.422	ng/ul	
83) Butylbenzylphthalate	20.310	149	713886	42.257	ng/ul	88
84) 3,3'-Dichlorobenzidine	21.098	252	369900	33.920	ng/ul	99
85) Benzo(a)anthracene	21.151	228	22365525m	637.265	ng/ul	
86) Bis(2-ethylhexyl)phtha...	21.075	149	1072866	42.914	ng/ul	98
87) Chrysene	21.210	228	18663110m	541.336	ng/ul	
89) Di-n-octyl phthalate	21.969	149	1754475m	40.272	ng/ul	
90) Benzo(b)fluoranthene	22.816	252	39590525m	1174.367	ng/ul	
91) Benzo(k)fluoranthene	22.869	252	8722211m	271.117	ng/ul	
93) Benzo(a)pyrene	23.433	252	22929271m	696.653	ng/ul	
94) Indeno(1,2,3-cd)pyrene	25.980	276	20633368m	562.043	ng/ul	
95) Dibenzo(a,h)anthracene	25.951	278	6123576m	193.720	ng/ul	
96) Benzo(g,h,i)perylene	26.721	276	15093245m	483.328	ng/ul	

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Instrument :

BNA_P

ClientSampleId :

EX7Q8MS

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 08/18/2022
Supervised By :Sohil Jodhani 08/18/2022

Manual IntegrationsAPPROVED

Quant Time: Aug 17 23:28:09 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP081622.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Aug 17 01:58:37 2022
Response via : Initial Calibration

