

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081722\
 Data File : BP011470.D
 Acq On : 17 Aug 2022 20:29
 Operator : CG/JU
 Sample : N4028-01 10X
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0QB0

Quant Time: Aug 17 23:33:00 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP081622.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Aug 17 01:58:37 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.558	152	112887	20.000	ng/ul	0.00
20) Naphthalene-d8	10.346	136	490698	20.000	ng/ul	# 0.00
38) Acenaphthene-d10	14.234	164	292126	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.004	188	595079	20.000	ng/ul	0.00
79) Chrysene-d12	21.133	240	551094	20.000	ng/ul	0.00
88) Perylene-d12	23.427	264	561900	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.070	96	6956	1.912	ng/uL	0.00
4) Pyridine-d5	3.487	84	77411	8.312	ng/ul	0.00
7) Phenol-d5	6.740	99	58890	5.677	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	6.905	67	190767	28.305	ng/ul	0.00
11) 2-Chlorophenol-d4	7.093	132	182977	23.982	ng/ul	0.00
15) 4-Methylphenol-d8	8.281	113	111323	13.407	ng/ul	0.00
21) Nitrobenzene-d5	8.722	128	117172	33.168	ng/ul	0.00
24) 2-Nitrophenol-d4	9.440	143	120956	33.643	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	9.975	165	178665	26.922	ng/ul	0.00
31) 4-Chloroaniline-d4	10.499	131	255314	23.111	ng/ul	0.00
46) Dimethylphthalate-d6	13.657	166	699345	33.847	ng/ul	0.00
49) Acenaphthylene-d8	13.922	160	747328	32.544	ng/ul	0.00
54) 4-Nitrophenol-d4	14.463	143	18406	4.624	ng/ul	0.00
60) Fluorene-d10	15.234	176	591507	34.029	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.375	200	111639	34.719	ng/ul	0.00
73) Anthracene-d10	17.104	188	1023695	38.842	ng/ul	0.00
81) Pyrene-d10	19.369	212	1131258	40.573	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.280	264	1093254	39.998	ng/ul	0.00
Target Compounds						
71) Pentachlorophenol	16.651	266	17586	4.633	ng/ul	Qvalue 99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081722\
Data File : BP011470.D
Acq On : 17 Aug 2022 20:29
Operator : CG/JU
Sample : N4028-01 10X
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0QB0

Quant Time: Aug 17 23:33:00 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP081622.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Aug 17 01:58:37 2022
Response via : Initial Calibration

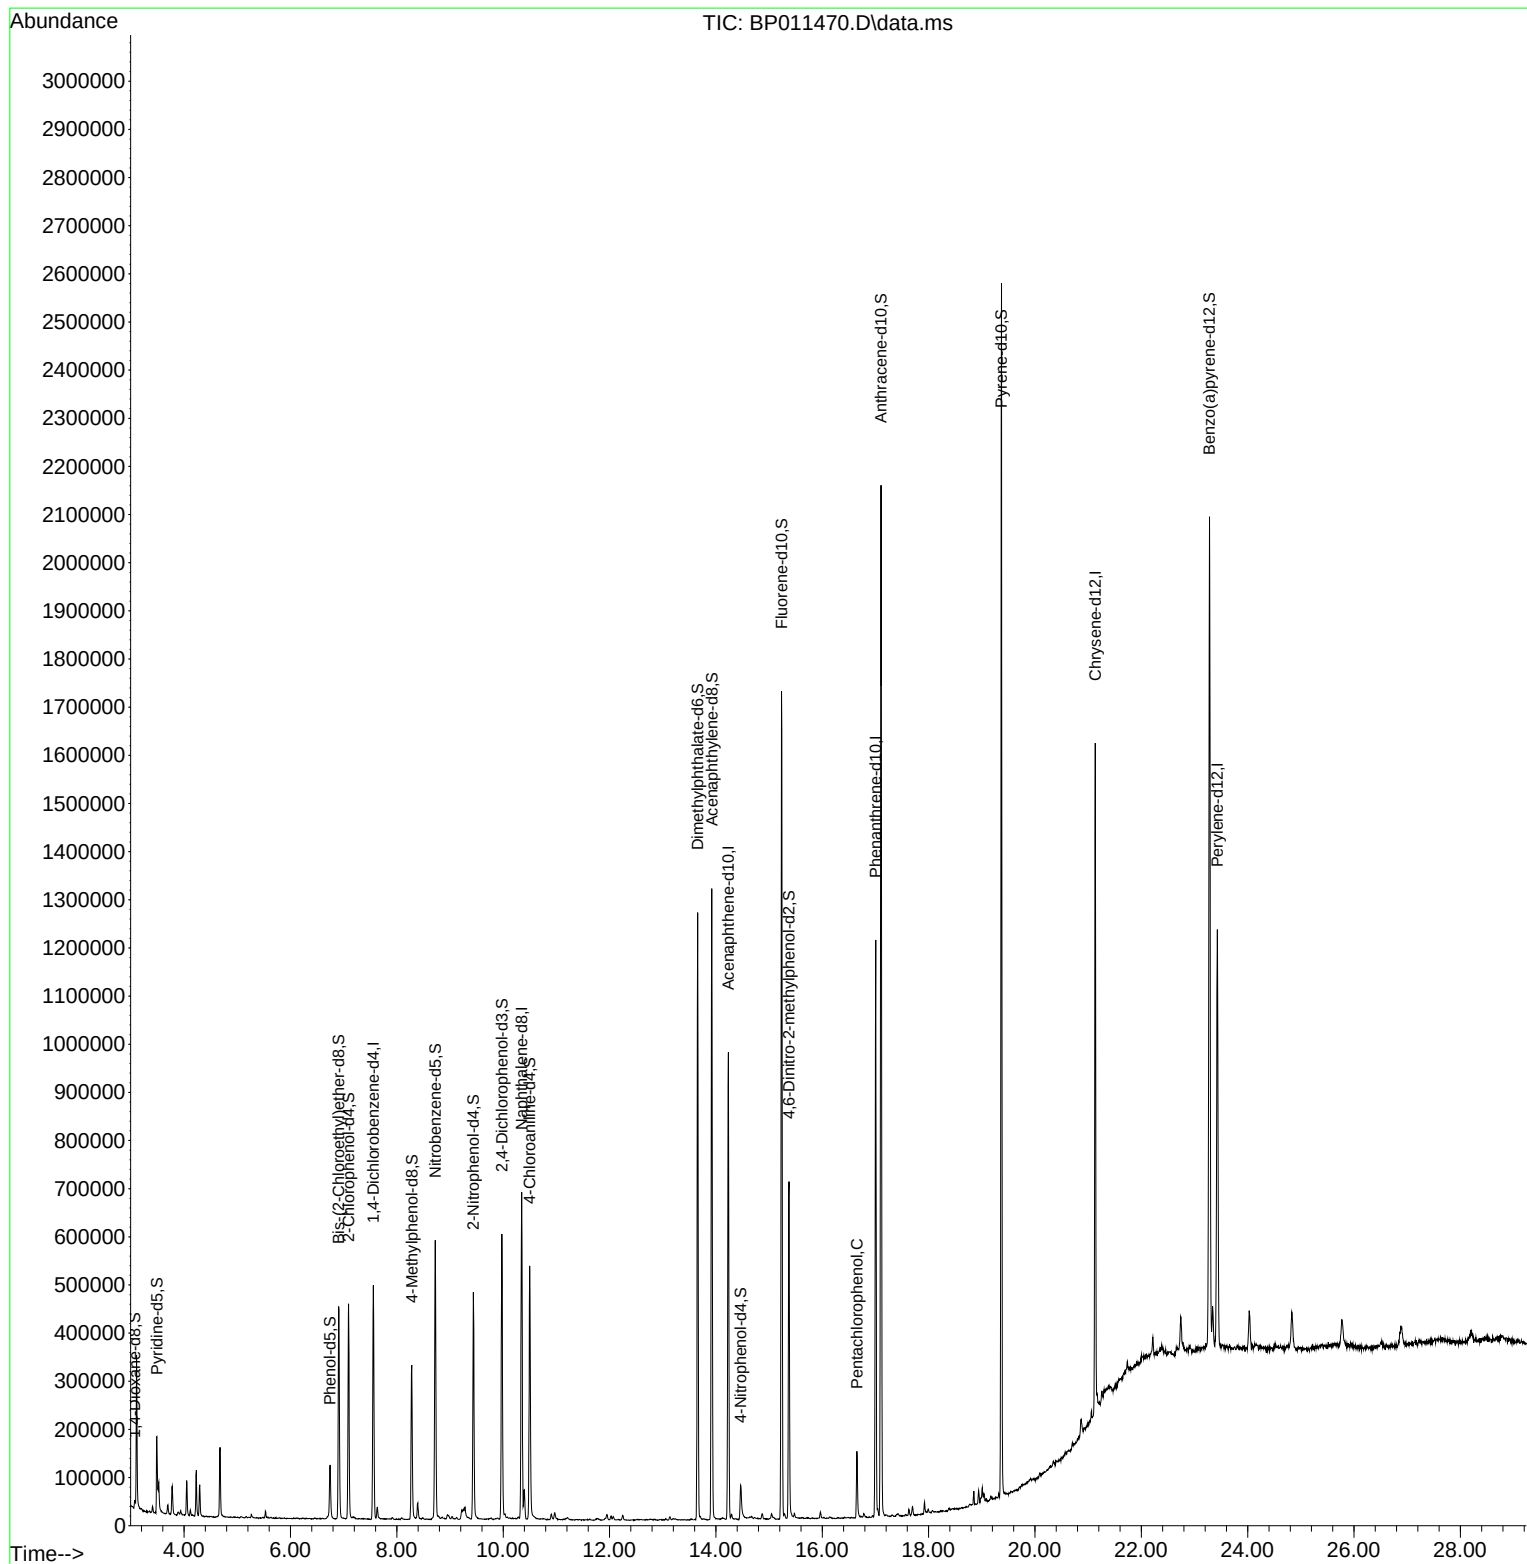

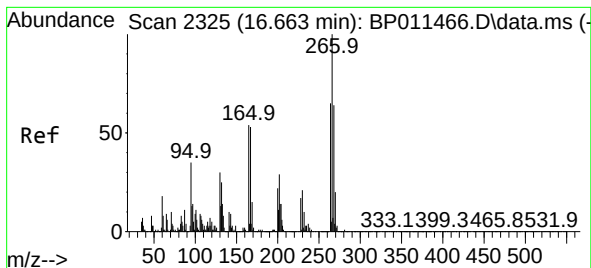

#71

Pentachlorophenol

Concen: 4.633 ng/ul

RT: 16.651 min Scan# 21

Delta R.T. 0.000 min

Lab File: BP011470.D


Acq: 17 Aug 2022 20:29

Instrument :

BNA_P

ClientSampleId :

C0QB0

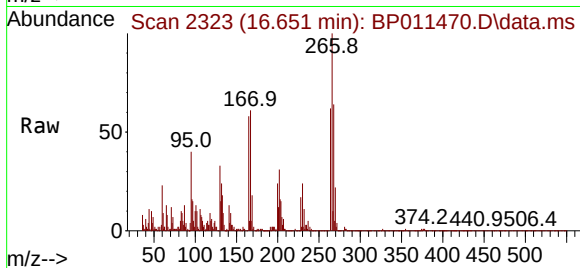

Tgt Ion:266 Resp: 17586

Ion Ratio Lower Upper

266 100

264 62.4 50.6 76.0

268 64.0 51.3 76.9

