

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081722\
 Data File : BP011473.D
 Acq On : 17 Aug 2022 22:12
 Operator : CG/JU
 Sample : N4028-04 10X
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0QB4

Quant Time: Aug 17 23:34:02 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP081622.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Aug 17 01:58:37 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.558	152	96043	20.000	ng/ul	0.00
20) Naphthalene-d8	10.346	136	403366	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.228	164	226517	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.004	188	454768	20.000	ng/ul	0.00
79) Chrysene-d12	21.133	240	424758	20.000	ng/ul	0.00
88) Perylene-d12	23.421	264	444309	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.070	96	6143	1.985	ng/uL	0.00
4) Pyridine-d5	3.493	84	24524	3.095	ng/ul	0.01
7) Phenol-d5	6.746	99	51379	5.821	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	6.905	67	157832	27.525	ng/ul	0.00
11) 2-Chlorophenol-d4	7.093	132	149808	23.078	ng/ul	0.00
15) 4-Methylphenol-d8	8.275	113	93424	13.225	ng/ul	0.00
21) Nitrobenzene-d5	8.722	128	95367	32.840	ng/ul	0.00
24) 2-Nitrophenol-d4	9.440	143	94884	32.105	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	9.975	165	144431	26.475	ng/ul	0.00
31) 4-Chloroaniline-d4	10.499	131	211931	23.337	ng/ul	0.00
46) Dimethylphthalate-d6	13.657	166	529316	33.038	ng/ul	0.00
49) Acenaphthylene-d8	13.922	160	584232	32.810	ng/ul	0.00
54) 4-Nitrophenol-d4	14.469	143	12658	4.101	ng/ul	0.00
60) Fluorene-d10	15.234	176	439276	32.591	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.369	200	71070	28.921	ng/ul	0.00
73) Anthracene-d10	17.098	188	724936	35.993	ng/ul	0.00
81) Pyrene-d10	19.363	212	792381	36.871	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.274	264	800021	37.016	ng/ul	0.00
Target Compounds						Qvalue
71) Pentachlorophenol	16.651	266	3579	1.234	ng/ul	95


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081722\
Data File : BP011473.D
Acq On : 17 Aug 2022 22:12
Operator : CG/JU
Sample : N4028-04 10X
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0QB4

Quant Time: Aug 17 23:34:02 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP081622.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Aug 17 01:58:37 2022
Response via : Initial Calibration

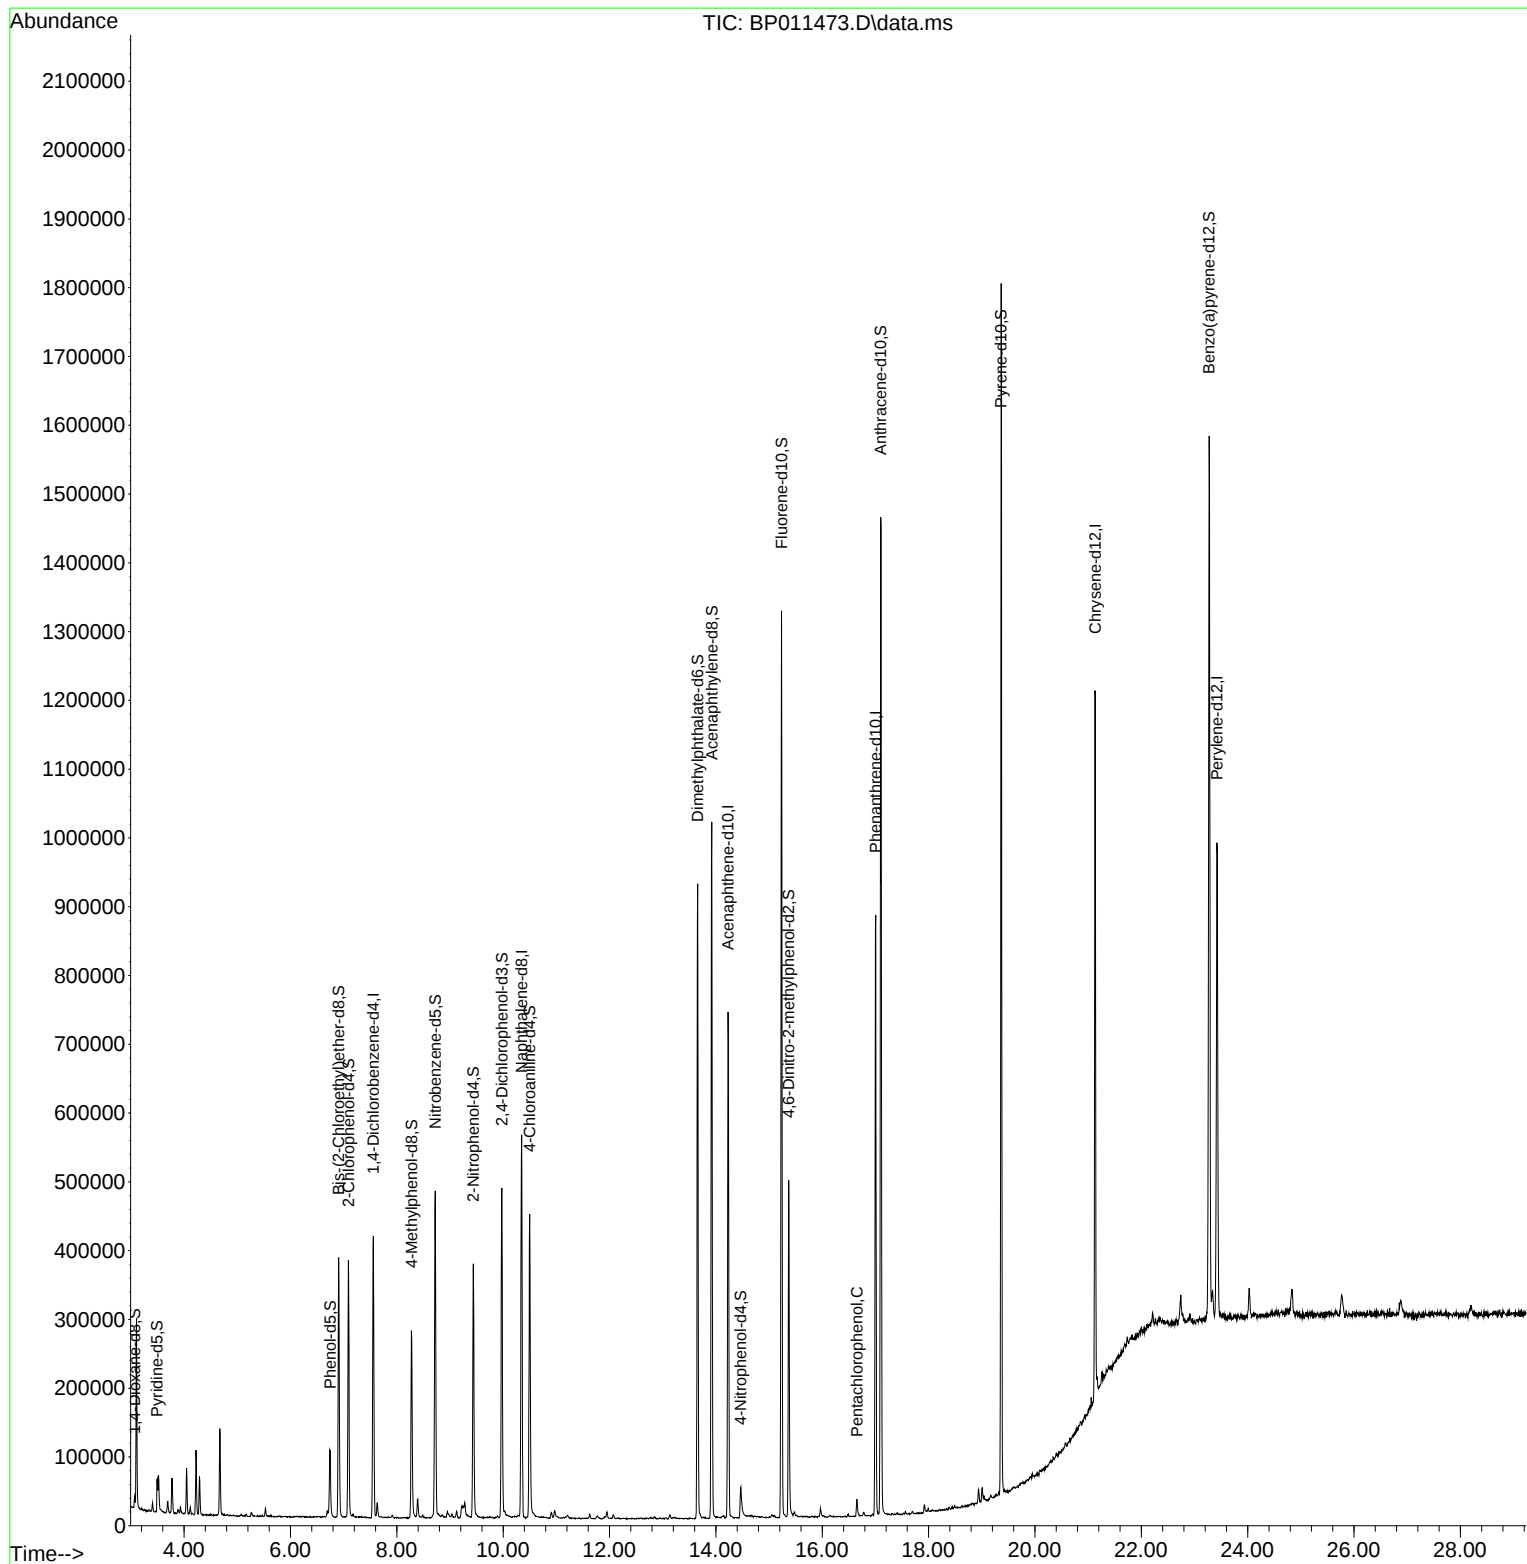

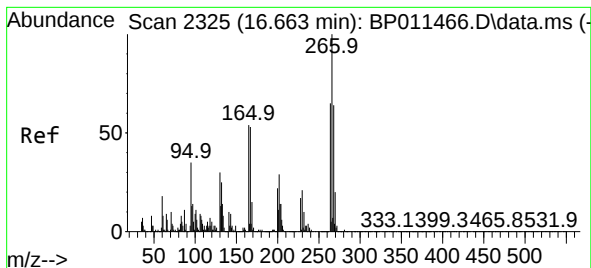

#71

Pentachlorophenol

Concen: 1.234 ng/ul

RT: 16.651 min Scan# 21

Delta R.T. -0.000 min

Lab File: BP011473.D


Acq: 17 Aug 2022 22:12

Instrument :

BNA_P

ClientSampleId :

C0QB4

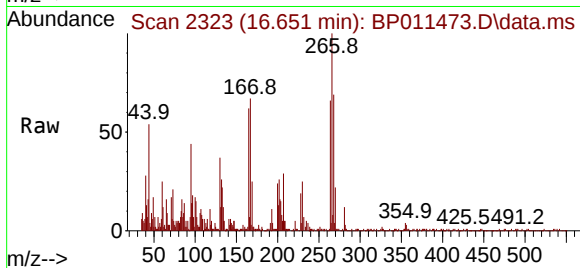

Tgt Ion:266 Resp: 3579

Ion Ratio Lower Upper

266 100

264 65.9 50.6 76.0

268 69.2 51.3 76.9

