

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081722\
 Data File : BP011474.D
 Acq On : 17 Aug 2022 22:46
 Operator : CG/JU
 Sample : N4028-05 10X
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0QB5

Quant Time: Aug 17 23:34:21 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP081622.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Aug 17 01:58:37 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.558	152	94151	20.000	ng/u1	0.00
20) Naphthalene-d8	10.346	136	389848	20.000	ng/u1	0.00
38) Acenaphthene-d10	14.228	164	215954	20.000	ng/u1	0.00
64) Phenanthrene-d10	16.998	188	421801	20.000	ng/u1	0.00
79) Chrysene-d12	21.133	240	406331	20.000	ng/u1	0.00
88) Perylene-d12	23.421	264	434452	20.000	ng/u1	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.070	96	5335	1.758	ng/uL	0.00
4) Pyridine-d5	3.487	84	45232	5.823	ng/u1	0.00
7) Phenol-d5	6.740	99	41991	4.853	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	6.905	67	134206	23.875	ng/u1	0.00
11) 2-Chlorophenol-d4	7.087	132	127373	20.016	ng/u1	0.00
15) 4-Methylphenol-d8	8.275	113	78593	11.349	ng/u1	0.00
21) Nitrobenzene-d5	8.722	128	78684	28.035	ng/u1	0.00
24) 2-Nitrophenol-d4	9.440	143	78312	27.417	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	9.975	165	118834	22.538	ng/u1	0.00
31) 4-Chloroaniline-d4	10.499	131	185437	21.128	ng/u1	0.00
46) Dimethylphthalate-d6	13.657	166	432977	28.347	ng/u1	0.00
49) Acenaphthylene-d8	13.922	160	470816	27.734	ng/u1	0.00
54) 4-Nitrophenol-d4	14.463	143	9362	3.181	ng/u1	0.00
60) Fluorene-d10	15.234	176	371337	28.898	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.369	200	61789	27.110	ng/u1	0.00
73) Anthracene-d10	17.098	188	638764	34.193	ng/u1	0.00
81) Pyrene-d10	19.363	212	701699	34.132	ng/u1	0.00
92) Benzo(a)pyrene-d12	23.274	264	720307	34.084	ng/u1	0.00
Target Compounds						Qvalue
71) Pentachlorophenol	16.651	266	4187	1.556	ng/u1	95


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081722\
Data File : BP011474.D
Acq On : 17 Aug 2022 22:46
Operator : CG/JU
Sample : N4028-05 10X
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0QB5

Quant Time: Aug 17 23:34:21 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP081622.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Aug 17 01:58:37 2022
Response via : Initial Calibration

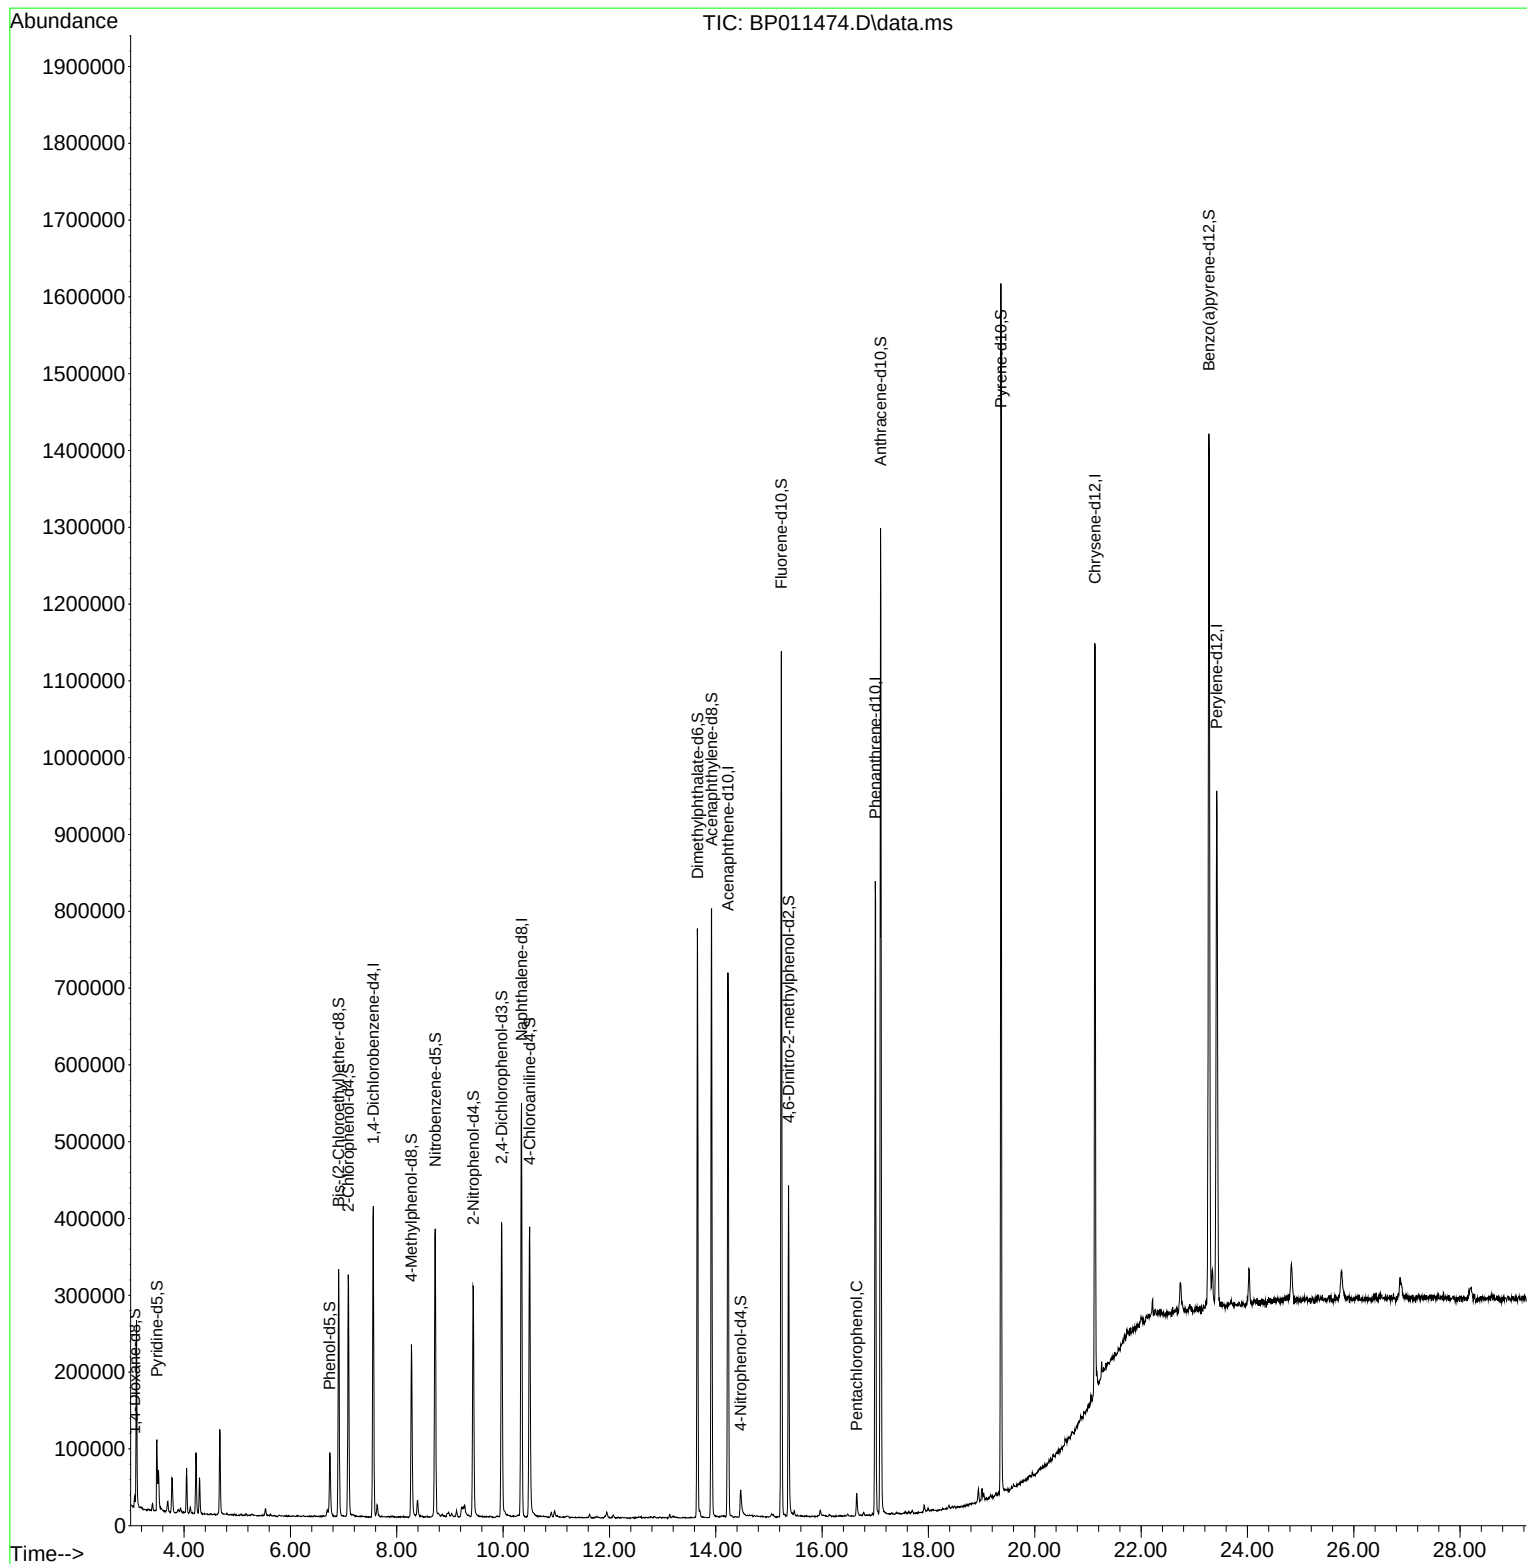

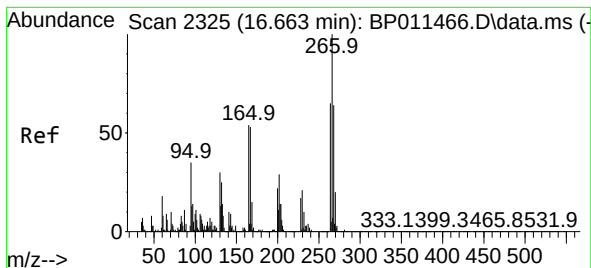

#71

Pentachlorophenol

Concen: 1.556 ng/ul

RT: 16.651 min Scan# 21

Delta R.T. -0.000 min

Lab File: BP011474.D


Acq: 17 Aug 2022 22:46

Instrument :

BNA_P

ClientSampleId :

C0QB5

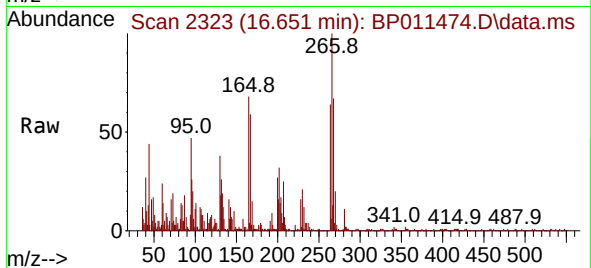

Tgt Ion:266 Resp: 4187

Ion Ratio Lower Upper

266 100

264 64.1 50.6 76.0

268 71.1 51.3 76.9

