

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081722\
 Data File : BP011454.D
 Acq On : 17 Aug 2022 10:13
 Operator : CG/JU
 Sample : PB147024BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK024

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP081622.M
 Title : SVOA CALIBRATION

Signal : TIC: BP011454.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.070	10	14	20	rVB	33178	40444	1.88%	0.170%
2	3.475	81	83	98	rBV	376509	556219	25.84%	2.337%
3	3.781	131	135	141	rVB3	6725	10793	0.50%	0.045%
4	4.946	331	333	340	rBV8	1505	2630	0.12%	0.011%
5	6.740	631	638	657	rBV	427519	650969	30.24%	2.736%
6	6.905	660	666	676	rVV	316921	482456	22.41%	2.027%
7	7.087	690	697	713	rBV	421105	654588	30.40%	2.751%
8	7.558	770	777	789	rBV	343326	540944	25.13%	2.273%
9	8.275	890	899	916	rBV	491542	800878	37.20%	3.366%
10	8.722	967	975	990	rBV	401281	663075	30.80%	2.786%
11	9.128	1037	1044	1045	rBV6	1437	2336	0.11%	0.010%
12	9.440	1088	1097	1108	rBV	329641	546248	25.37%	2.296%
13	9.969	1180	1187	1203	rBV	454543	780801	36.27%	3.281%
14	10.346	1242	1251	1262	rBV	480638	776080	36.05%	3.261%
15	10.499	1267	1277	1290	rBV	489609	844614	39.23%	3.549%
16	11.957	1516	1525	1533	rBV7	5787	15421	0.72%	0.065%
17	13.657	1807	1814	1825	rBV	954286	1336230	62.07%	5.615%
18	13.922	1851	1859	1871	rBV	936205	1353707	62.88%	5.689%
19	14.228	1905	1911	1921	rBV	680784	979507	45.50%	4.116%
20	14.457	1943	1950	1966	rBV	405213	656352	30.49%	2.758%
21	15.234	2075	2082	2096	rBV	1264508	1736949	80.68%	7.299%
22	15.369	2098	2105	2118	rVV	447292	638002	29.63%	2.681%
23	15.475	2119	2123	2129	rVB3	12866	19389	0.90%	0.081%
24	16.028	2212	2217	2223	rVB10	3157	6244	0.29%	0.026%
25	16.681	2323	2328	2334	rBV9	2630	5175	0.24%	0.022%
26	16.998	2373	2382	2393	rBV	810908	1141844	53.04%	4.798%
27	17.104	2393	2400	2417	rVV	1355735	1966611	91.35%	8.264%
28	17.686	2495	2499	2506	rBV8	3160	4995	0.23%	0.021%
29	17.810	2517	2520	2523	rBV5	1536	2742	0.13%	0.012%
30	18.939	2708	2712	2717	rBV3	15471	23021	1.07%	0.097%
31	19.010	2720	2724	2729	rVB	14628	21993	1.02%	0.092%
32	19.363	2778	2784	2793	rBV	1665496	2152943	100.00%	9.047%
33	21.127	3080	3084	3092	rBV	913837	1167916	54.25%	4.908%
34	23.274	3443	3449	3457	rBV2	1147426	2048869	95.17%	8.610%
35	23.421	3468	3474	3485	rVB2	622648	1165299	54.13%	4.897%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081722\
Data File : BP011454.D
Acq On : 17 Aug 2022 10:13
Operator : CG/JU
Sample : PB147024BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK024

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP081622.M
Title : SVOA CALIBRATION




Sum of corrected areas: 23796284

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081722\
Data File : BP011454.D
Acq On : 17 Aug 2022 10:13
Operator : CG/JU
Sample : PB147024BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK024

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP081622.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

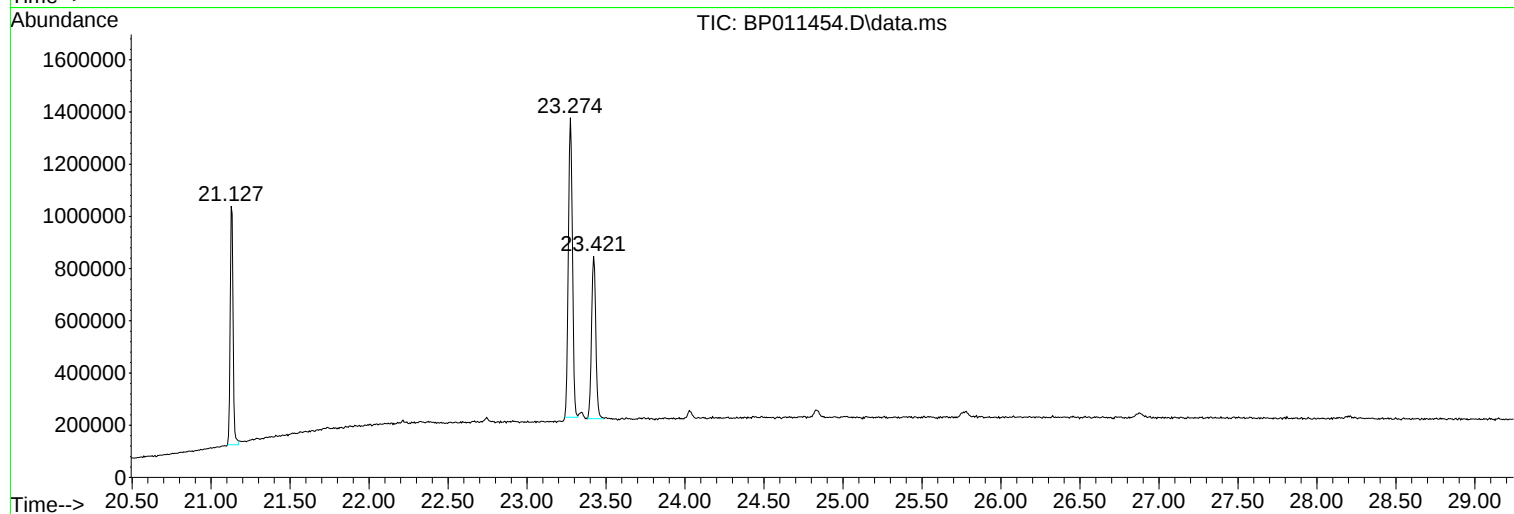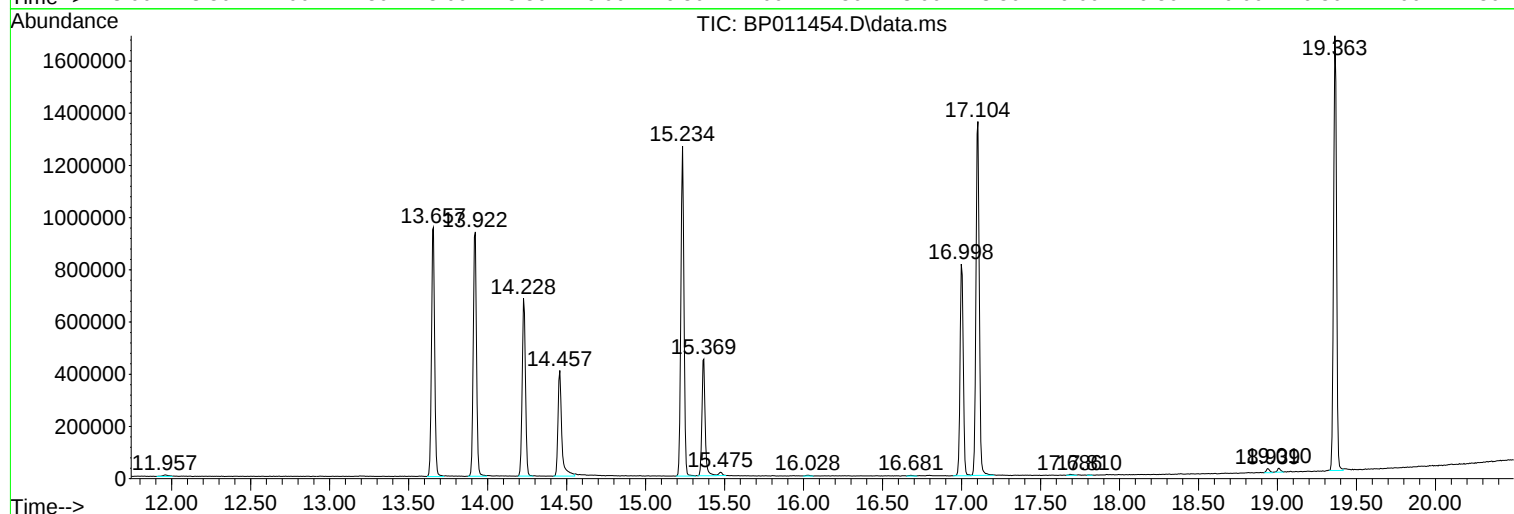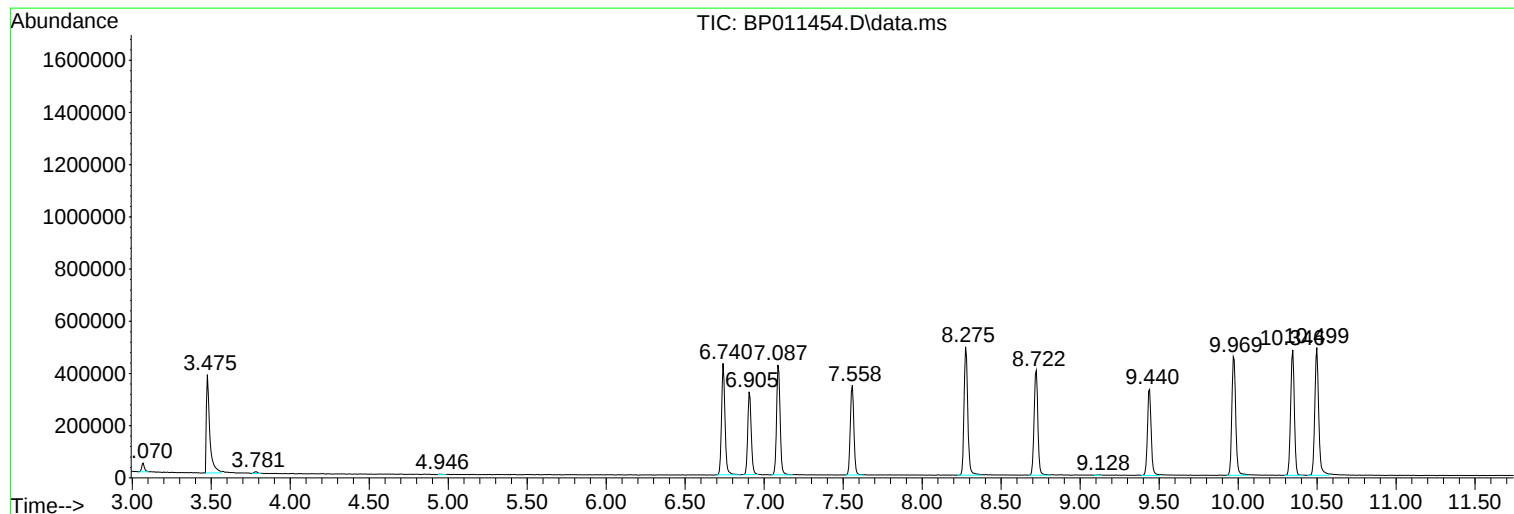

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081722\
Data File : BP011454.D
Acq On : 17 Aug 2022 10:13
Operator : CG/JU
Sample : PB147024BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK024

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP081622.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081722\
Data File : BP011454.D
Acq On : 17 Aug 2022 10:13
Operator : CG/JU
Sample : PB147024BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK024

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP081622.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc