
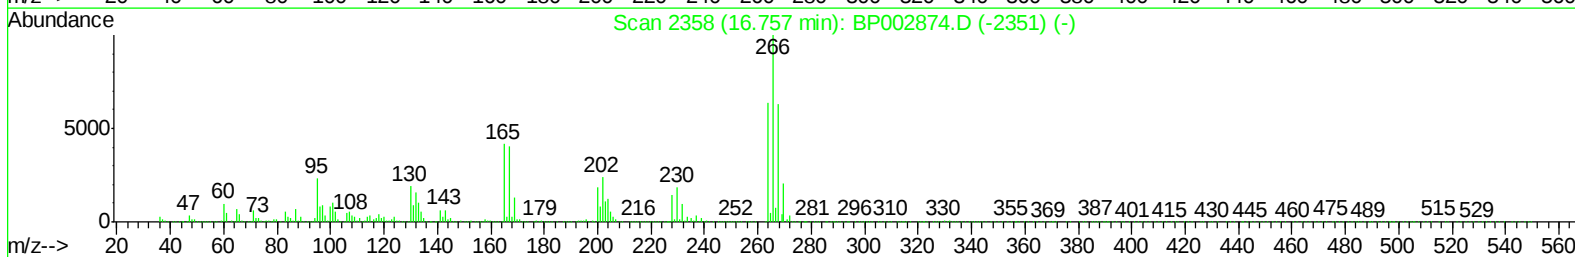
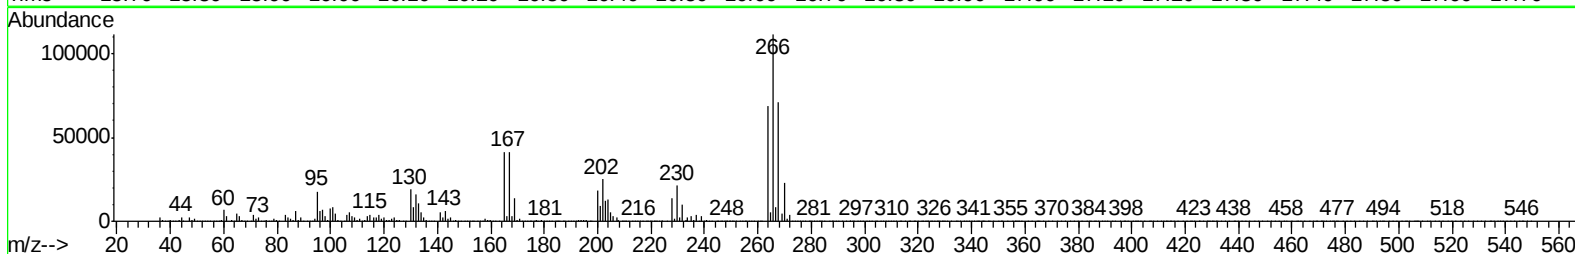


Data Path : Z:\svoasrv\HPCHEM1\BNA P\Data\BP081820\
 Data File : BP003011.D
 Acq On : 18 Aug 2020 10:24
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 19 06:45:19 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA P\METHODS\8270-BP073020.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Aug 17 14:07:35 2020
 Response via : Initial Calibration

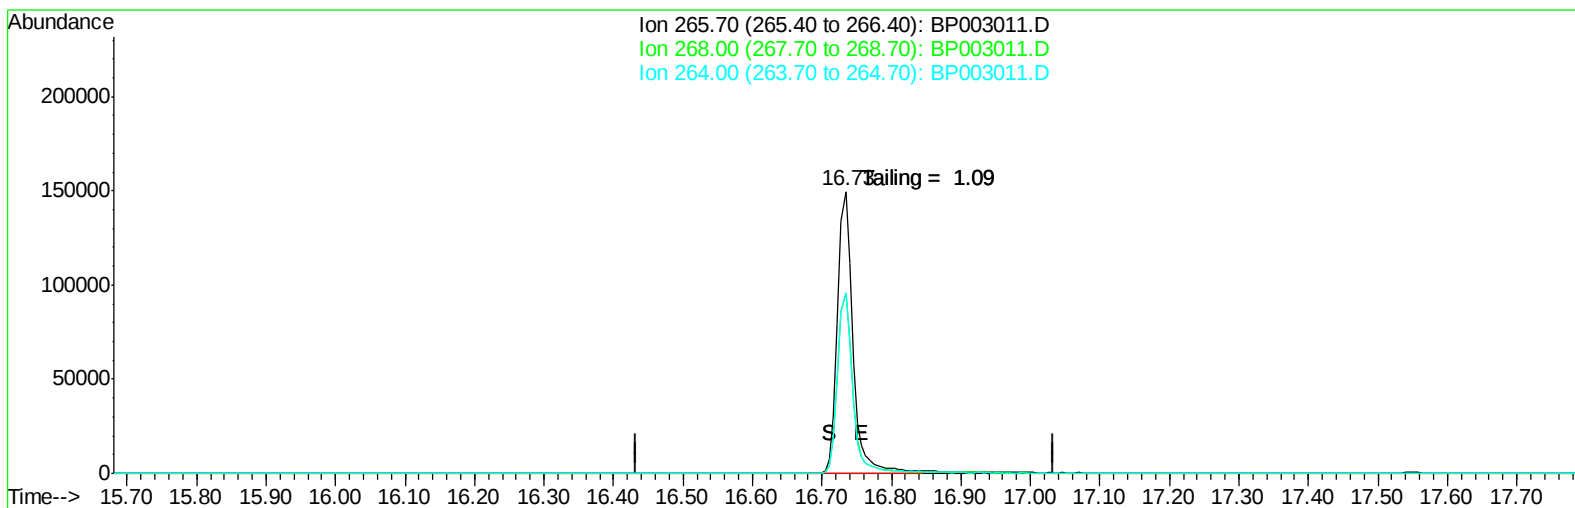

TIC: BP003011.D

(70) Pentachlorophenol (C)




16.734min (-16.734) 0.00ng

response 0

Ion	Exp%	Act%
265.70	100	0.00
268.00	63.60	0.00#
264.00	63.00	0.00#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA P\Data\BP081820\
 Data File : BP003011.D
 Acq On : 18 Aug 2020 10:24
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 19 06:45:19 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA P\METHODS\8270-BP073020.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Aug 17 14:07:35 2020
 Response via : Initial Calibration

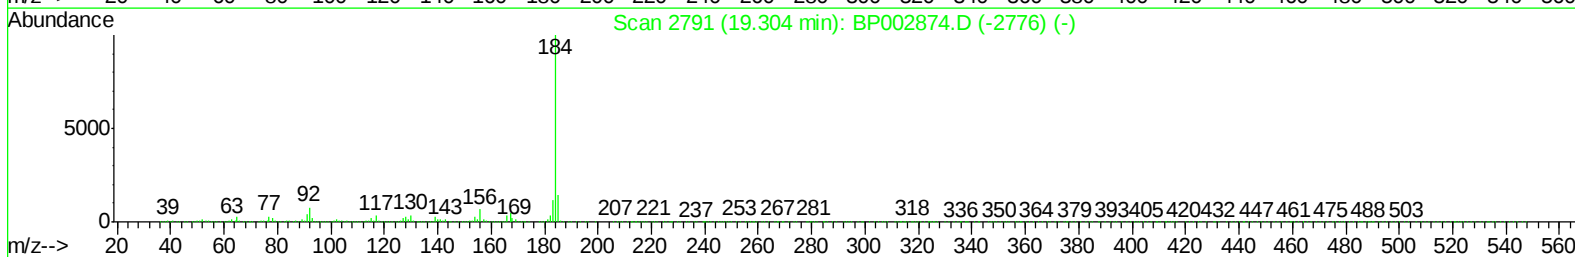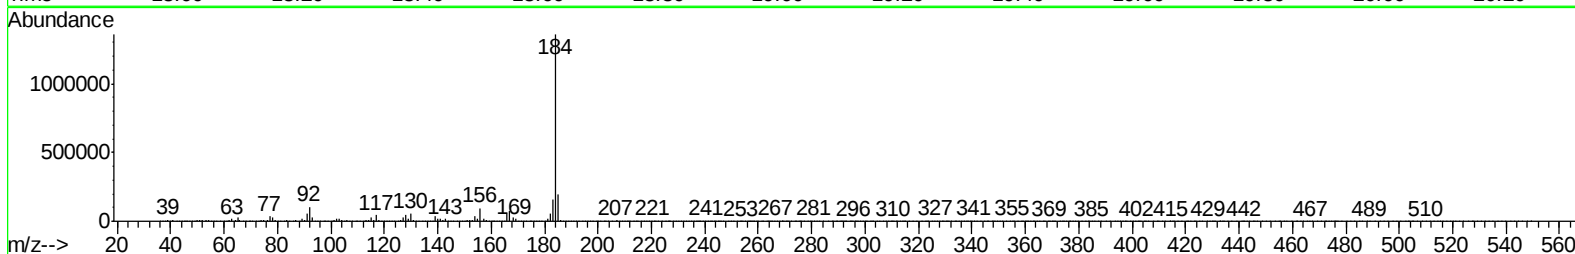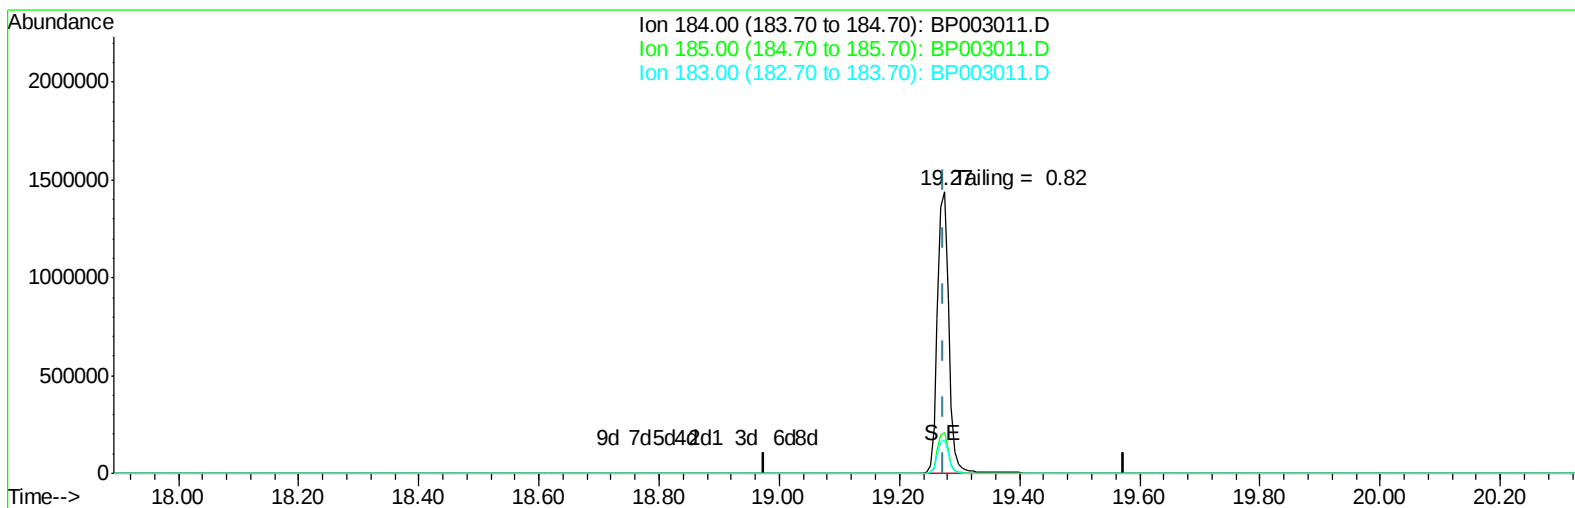

TIC: BP003011.D

(77) Benzidine

18.898min (-0.376) 6.41ng

response 26

Ion	Exp%	Act%
184.00	100	100
185.00	14.40	145.61#
183.00	11.70	70.18#
0.00	0.00	0.00