

Data Path : Z:\SVOASRV\HPCHEM1\BNA_P\DATA\BP081820\
 Data File : BP003026.D
 Acq On : 18 Aug 2020 20:14
 Operator : CG/JU
 Sample : L3700-10
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 EB-02-081420-SO-N

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0
 Filtering: 5
 Min Area: 3 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP073020.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.951	7	11	31	rVB	3231565	4253324	32.24%	7.255%
2	5.287	402	408	425	rBV	1409255	2155469	16.34%	3.677%
3	6.857	661	675	692	rBV	828372	1395393	10.58%	2.380%
4	7.681	808	815	824	rBV	850799	1337321	10.14%	2.281%
5	8.828	1000	1010	1027	rBV	2039302	3362509	25.48%	5.736%
6	10.463	1280	1288	1307	rBV	1151201	1958175	14.84%	3.340%
7	12.945	1702	1710	1729	rBV	5602650	8610551	65.26%	14.688%
8	13.780	1846	1852	1865	rBV	476505	692197	5.25%	1.181%
9	14.321	1937	1944	1960	rBV2	1763427	2629374	19.93%	4.485%
10	15.816	2190	2198	2222	rBV	4131048	6063913	45.96%	10.344%
11	17.074	2405	2412	2418	rBV	2246907	3170716	24.03%	5.408%
12	19.651	2844	2850	2862	rBV	10547920	13194716	100.00%	22.507%
13	20.903	3058	3063	3068	rVV2	425832	642073	4.87%	1.095%
14	20.951	3068	3071	3078	rVB	264087	359944	2.73%	0.614%
15	21.162	3102	3107	3113	rBV	3385326	4163770	31.56%	7.102%
16	23.409	3482	3489	3500	rVB2	2448356	4635571	35.13%	7.907%


Sum of corrected areas: 58625016

Data Path : Z:\SVOASRV\HPCHEM1\BNA P\DATA\BP081820\
Data File : BP003026.D
Acq On : 18 Aug 2020 20:14
Operator : CG/JU
Sample : L3700-10
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
EB-02-081420-SO-N

Quant Method : Z:\SVOASRV\HPCHEM1\BNA P\METHODS\8270-BP073020.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

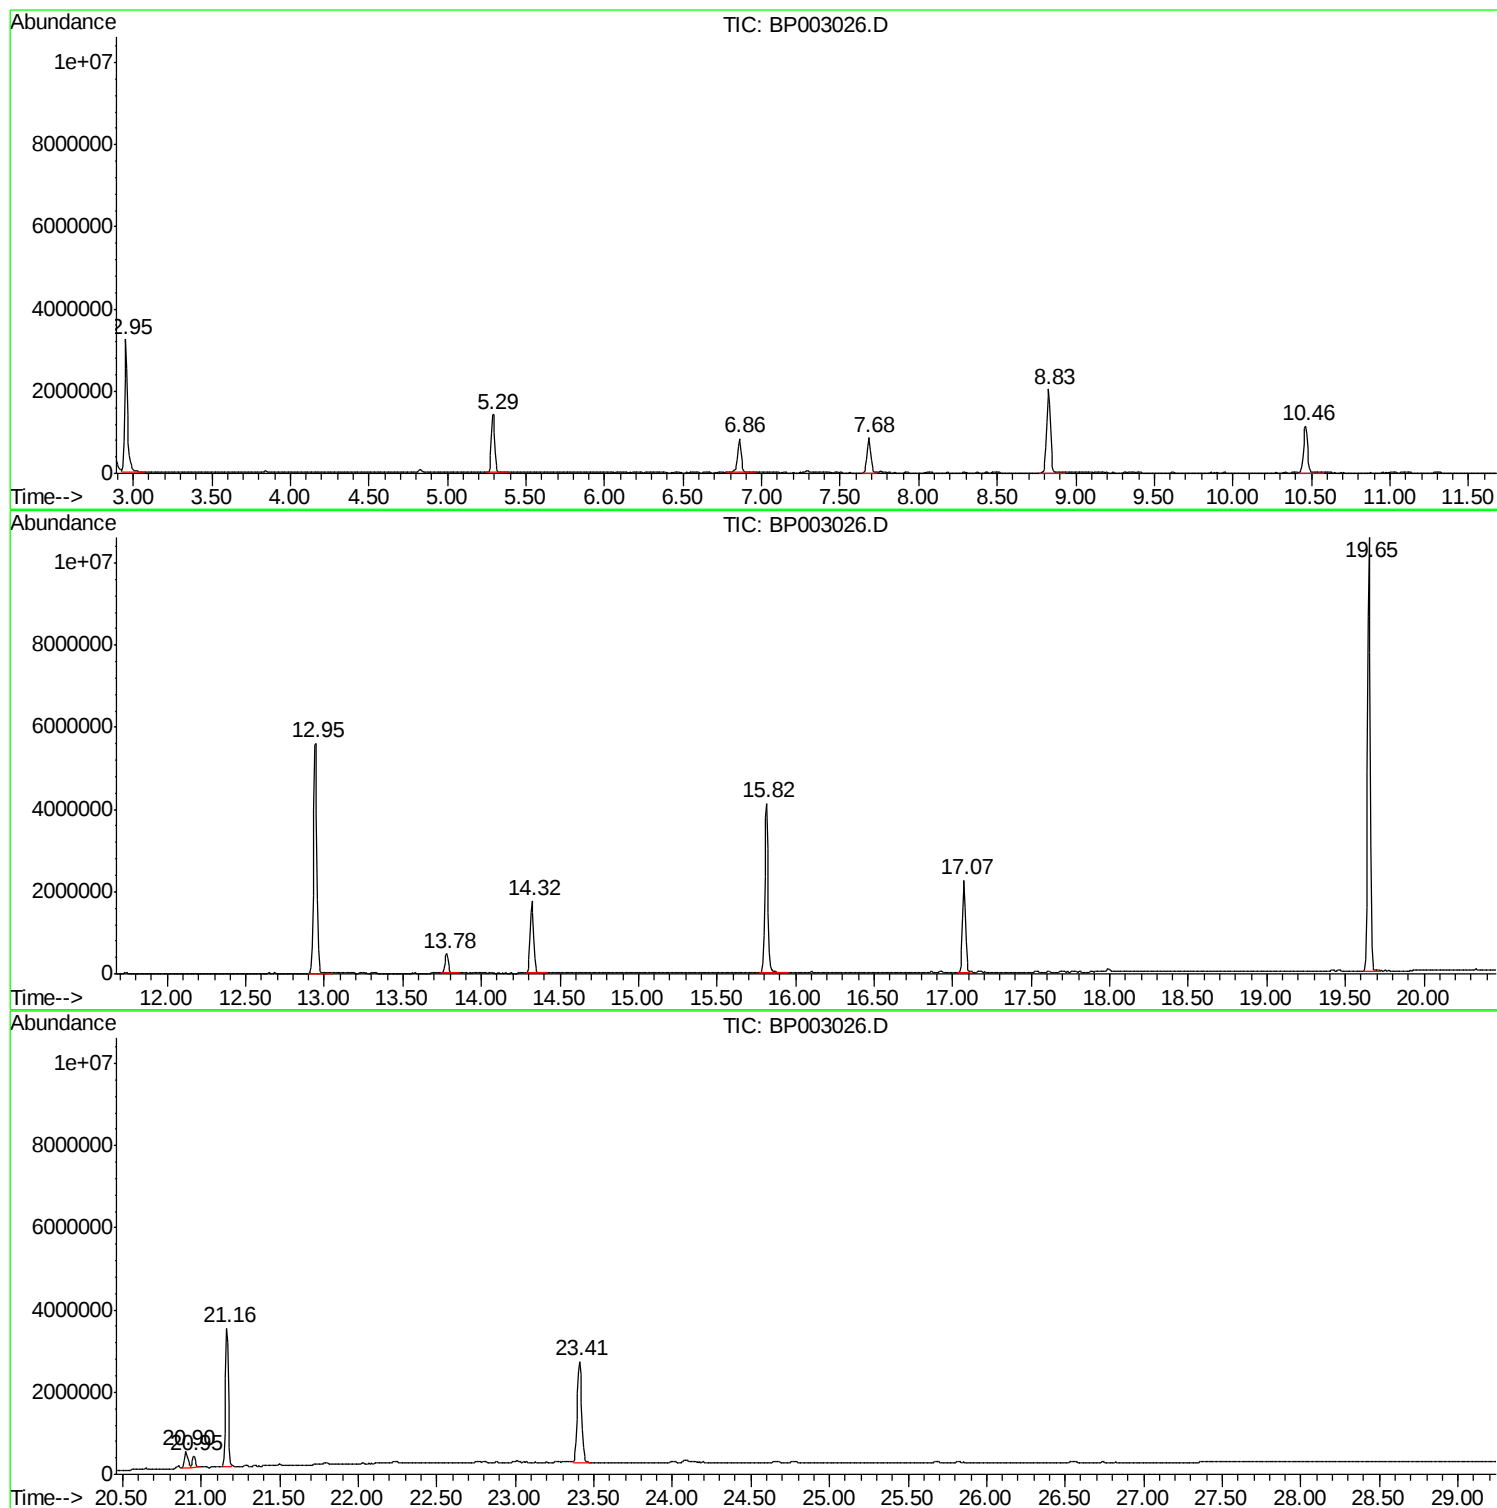

Data Path : Z:\SVOASRV\HPCHEM1\BNA P\DATA\BP081820\
Data File : BP003026.D
Acq On : 18 Aug 2020 20:14
Operator : CG/JU
Sample : L3700-10
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
EB-02-081420-SO-N










Quant Method : Z:\SVOASRV\HPCHEM1\BNA P\METHODS\8270-BP073020.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Butane, 2-methoxy-2-methyl- Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
2.95	63.61 ng	4253320	1,4-Dichlorobenzene-d4	7.68

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	Butane, 2-methoxy-2-methyl-	102	C6H14O	000994-05-8	64
2		2,2,4-Trimethyl-3-pentanol	130	C8H18O	005162-48-1	40
3		Pentane, 3-methoxy-	102	C6H14O	036839-67-5	12
4		N-Ethylformamide	73	C3H7NO	000627-45-2	9
5		3-Hexanol, 2-methyl-	116	C7H16O	000617-29-8	9

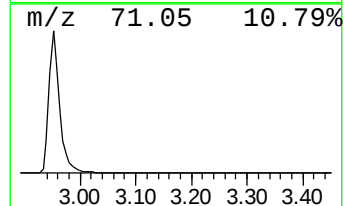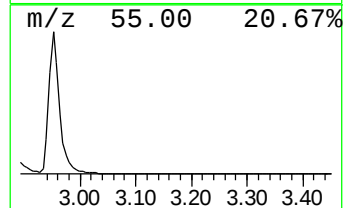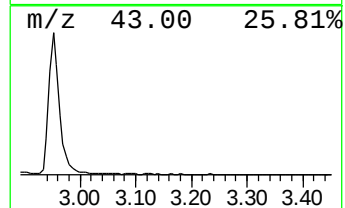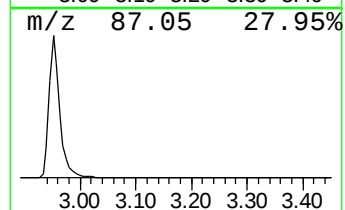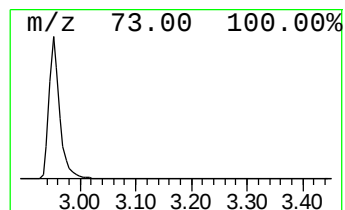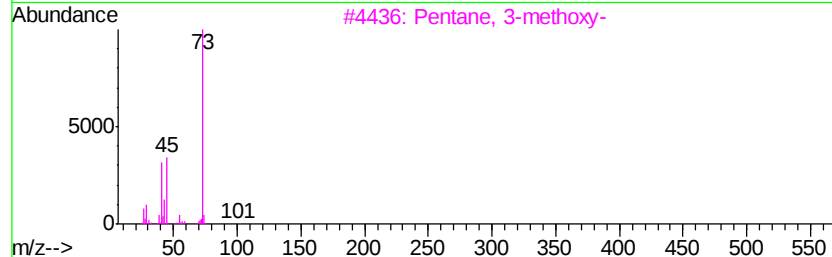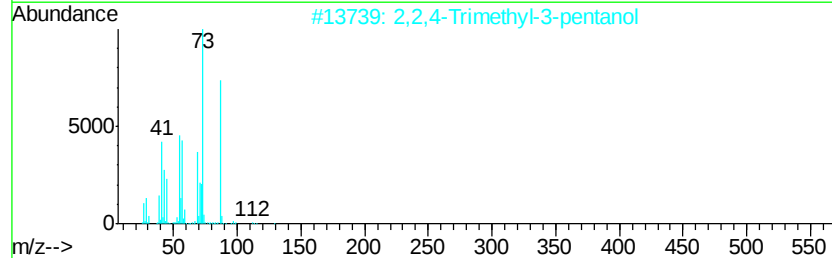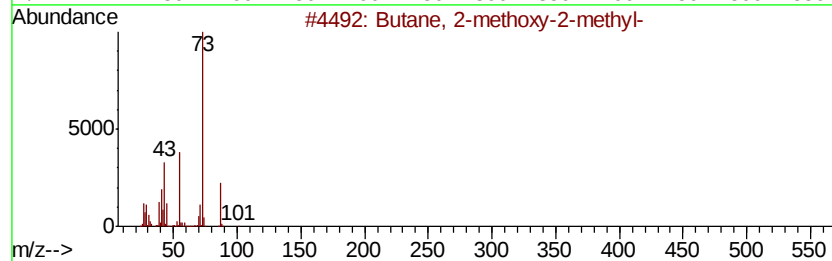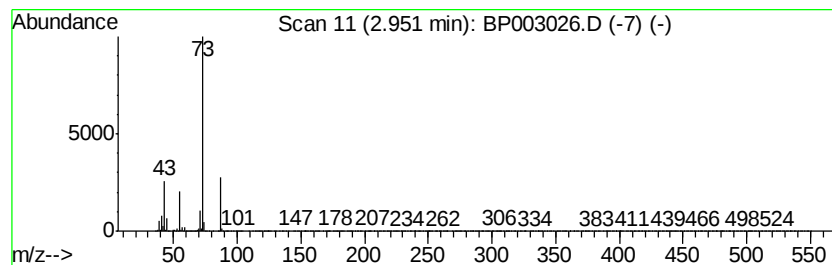

Data Path : Z:\SVOASRV\HPCHEM1\BNA P\DATA\BP081820\
Data File : BP003026.D
Acq On : 18 Aug 2020 20:14
Operator : CG/JU
Sample : L3700-10
Misc :
ALS Vial : 16 Sample Multiplier: 1










Instrument :
BNA_P
ClientSampleId :
EB-02-081420-SO-N

Quant Method : Z:\SVOASRV\HPCHEM1\BNA P\METHODS\8270-BP073020.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 2 Nonadecyl trifluoroacetate Concentration Rank 2

R.T.	EstConc	Area	Relative to ISTD		R.T.	
20.90	3.08 ng	642073	Chrysene-d12		21.16	
Hit# of	5	Tentative ID	MW	MolForm	CAS#	Qual
1		Nonadecyl trifluoroacetate	380	C21H39F3O2	1000351-76-3	93
2		1-Heptacosanol	396	C27H56O	002004-39-9	93
3		n-Tetracosanol-1	354	C24H50O	000506-51-4	91
4		Behenic alcohol	326	C22H46O	000661-19-8	91
5		1-Docosene	308	C22H44	001599-67-3	87

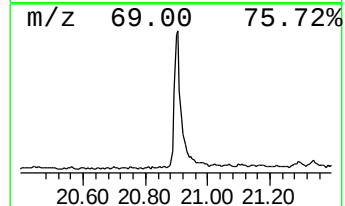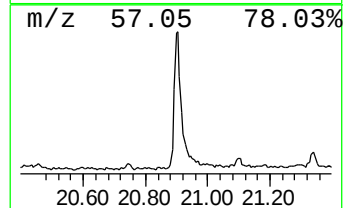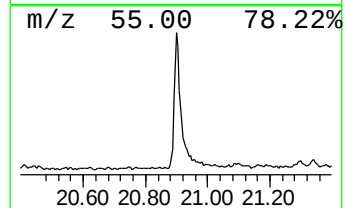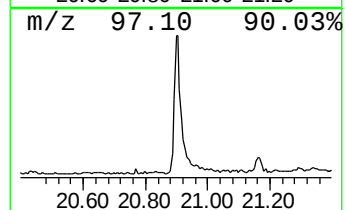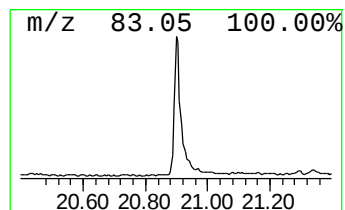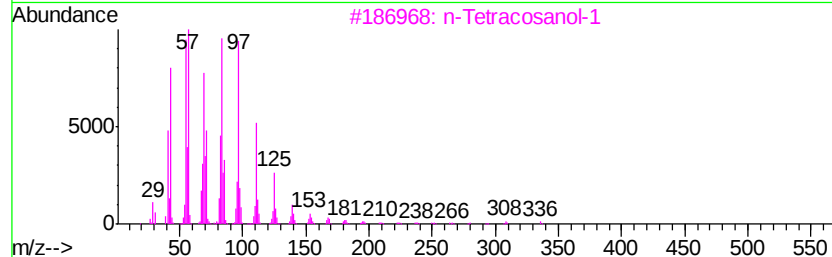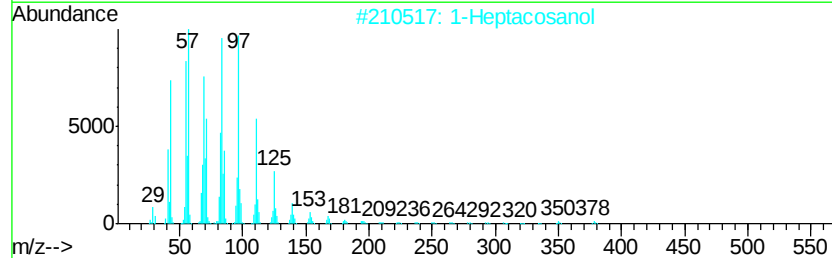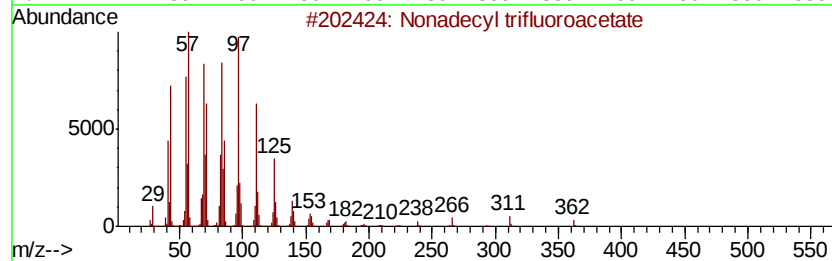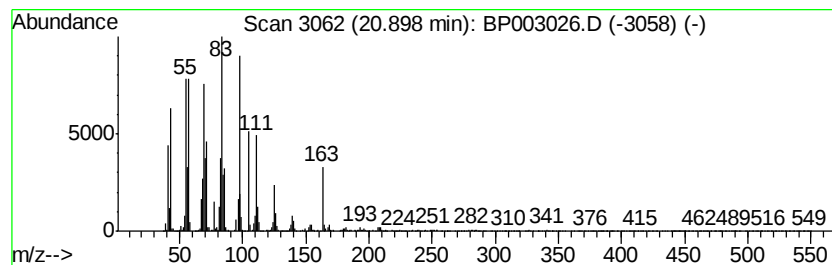

Data Path : Z:\SVOASRV\HPCHEM1\BNA_P\DATA\BP081820\
Data File : BP003026.D
Acq On : 18 Aug 2020 20:14
Operator : CG/JU
Sample : L3700-10
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
EB-02-081420-SO-N

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP073020.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	---Internal Standard---			
					#	RT	Resp	Conc
Butane, 2-methoxy...	2.95	63.6	ng	4253320	1	7.68	1337320	20.0
Nonadecyl trifluo...	20.90	3.1	ng	642073	5	21.16	4163770	20.0