




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081822\
Data File : BP011483.D
Acq On : 18 Aug 2022 15:47
Operator : CG/JU
Sample : N4220-01
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
A43K4

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 08/19/2022
Supervised By :Sohil Jodhani 08/22/2022

Quant Time: Aug 18 23:16:56 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP081622.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Aug 17 01:58:37 2022
Response via : Initial Calibration

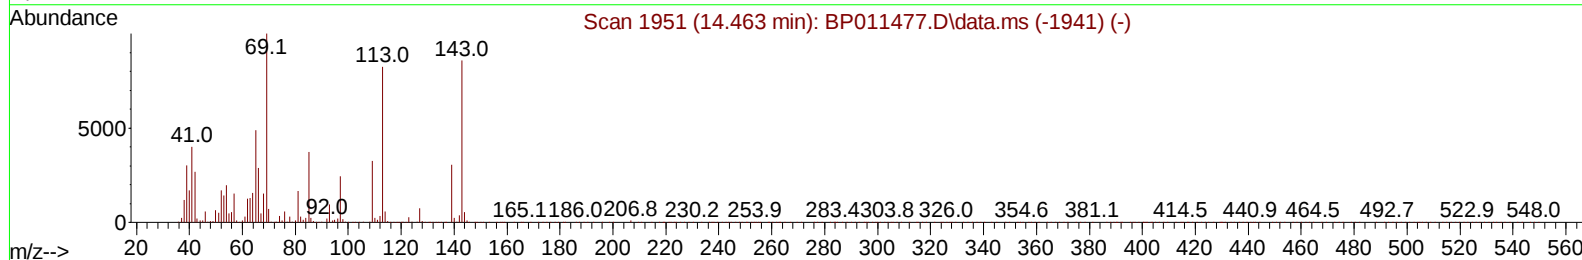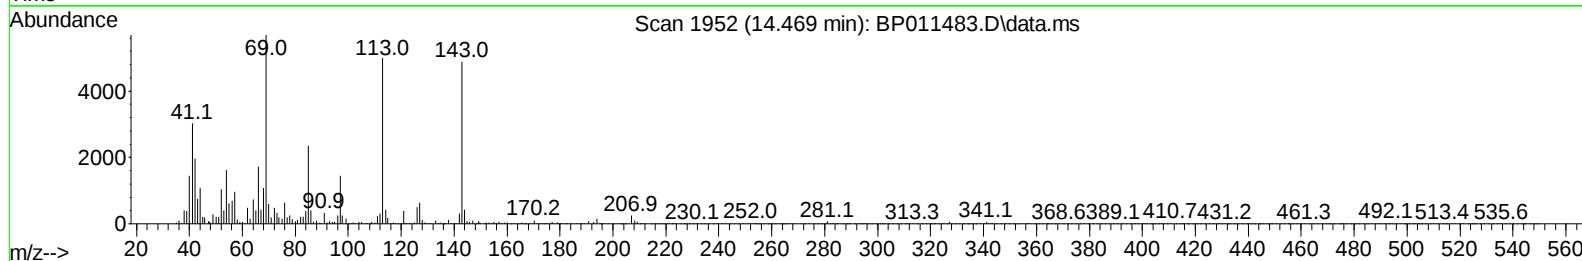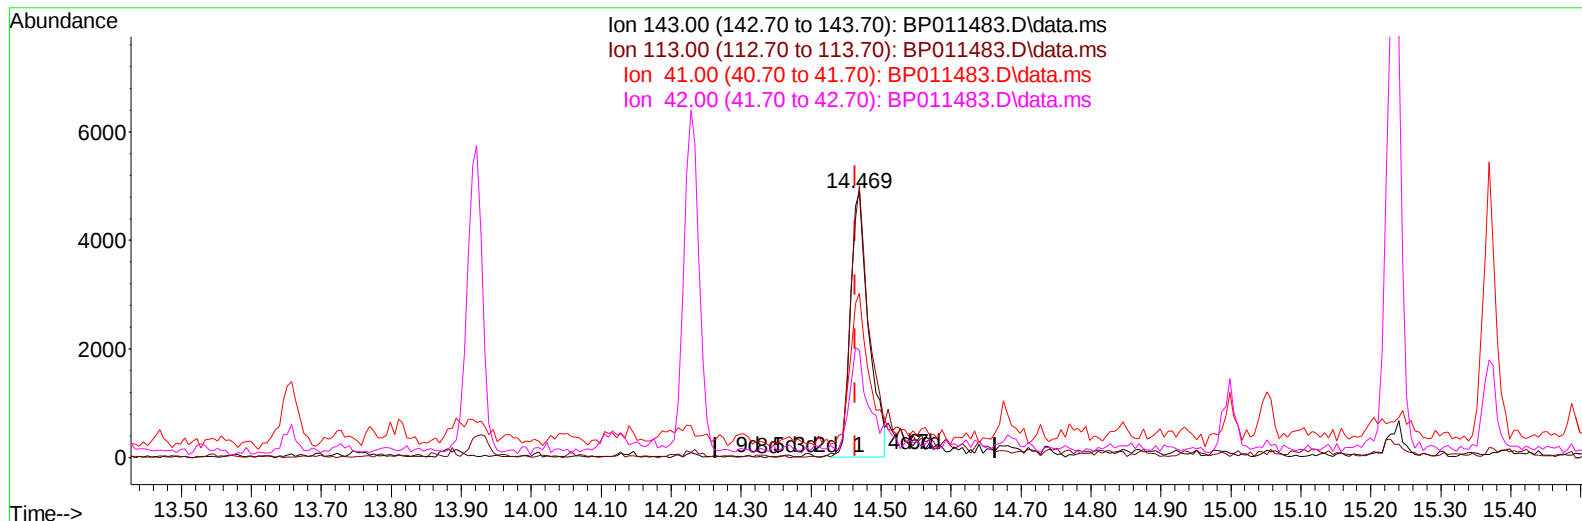

TIC: BP011483.D\data.ms

(54) 4-Nitrophenol-d4 (S)**14.469min (+ 0.006) 3.47 ng/u1****response 8748**

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	109.60	102.44
41.00	52.50	61.97
42.00	35.70	40.41




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081822\
 Data File : BP011483.D
 Acq On : 18 Aug 2022 15:47
 Operator : CG/JU
 Sample : N4220-01
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 A43K4

Manual IntegrationsAPPROVED

Quant Time: Aug 18 23:16:56 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP081622.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Aug 17 01:58:37 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 08/19/2022
 Supervised By :Sohil Jodhani 08/22/2022

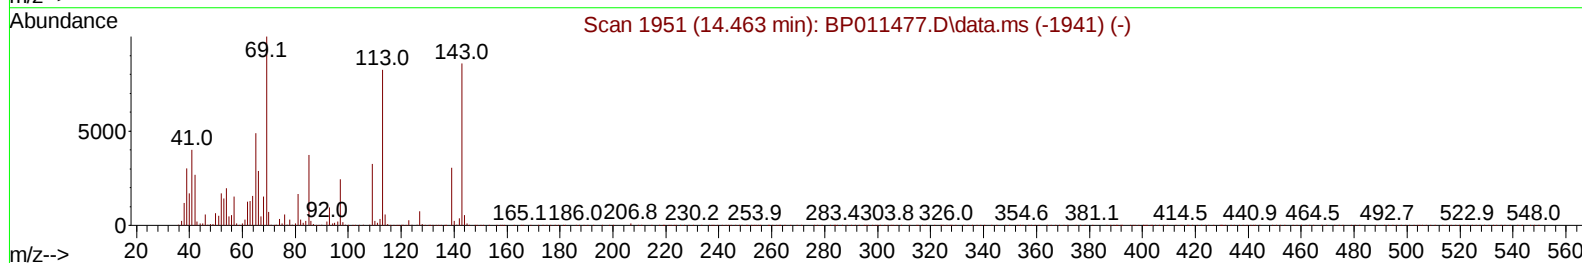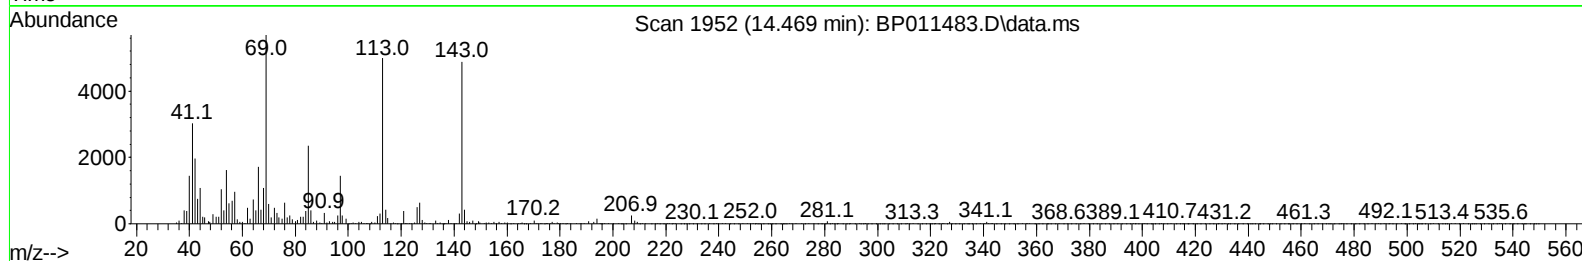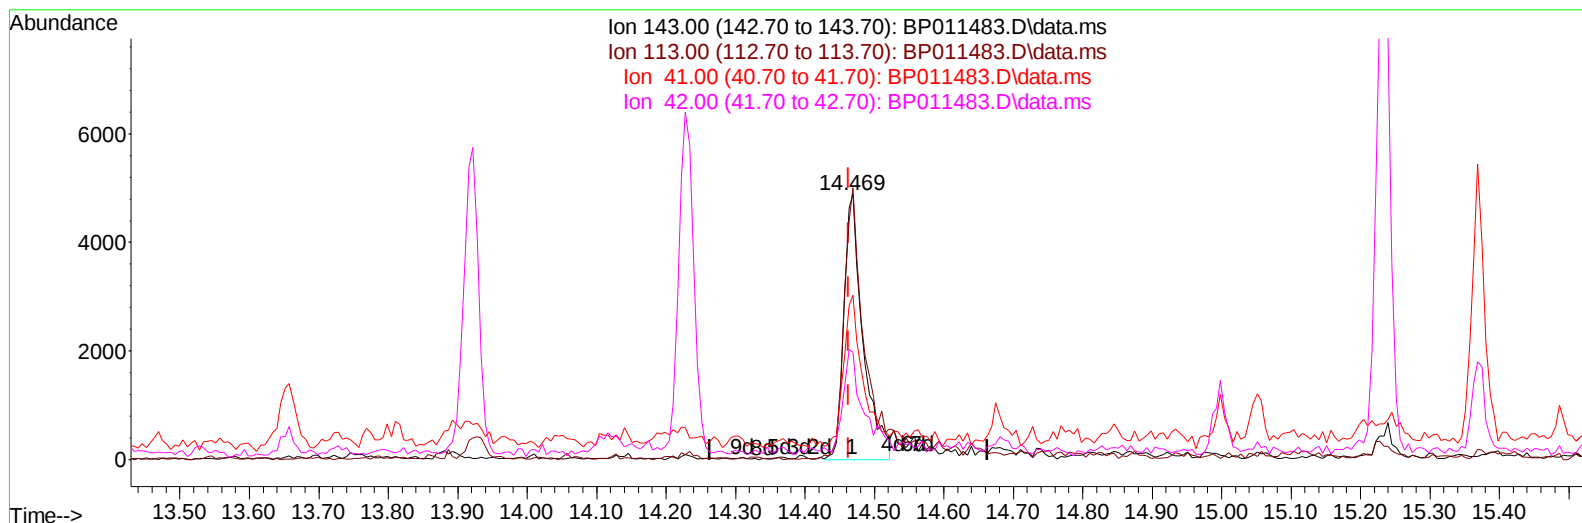

TIC: BP011483.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.469min (+ 0.006) 3.70 ng/ul m

response 9326

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	109.60	102.44
41.00	52.50	61.97
42.00	35.70	40.41

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081822\
 Data File : BP011483.D
 Acq On : 18 Aug 2022 15:47
 Operator : CG/JU
 Sample : N4220-01
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 A43K4

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 08/19/2022
 Supervised By :Sohil Jodhani 08/22/2022

Quant Time: Aug 18 23:16:56 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP081622.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Aug 17 01:58:37 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.558	152	87139	20.000	ng/ul	0.00
20) Naphthalene-d8	10.346	136	351102	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.228	164	185074	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.004	188	353471	20.000	ng/ul	0.00
79) Chrysene-d12	21.139	240	370461	20.000	ng/ul	0.00
88) Perylene-d12	23.433	264	418799	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.070	96	10911	3.886	ng/uL	0.00
4) Pyridine-d5	3.481	84	67091	9.332	ng/ul	0.00
7) Phenol-d5	6.746	99	36790	4.594	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	6.905	67	116916	22.473	ng/ul	0.00
11) 2-Chlorophenol-d4	7.093	132	108261	18.382	ng/ul	0.00
15) 4-Methylphenol-d8	8.281	113	59951	9.354	ng/ul	0.00
21) Nitrobenzene-d5	8.722	128	66786	26.422	ng/ul	0.00
24) 2-Nitrophenol-d4	9.440	143	62961	24.475	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	9.975	165	106787	22.488	ng/ul	0.00
31) 4-Chloroaniline-d4	10.499	131	103773	13.128	ng/ul	0.00
46) Dimethylphthalate-d6	13.657	166	376422	28.756	ng/ul	0.00
49) Acenaphthylene-d8	13.922	160	399239	27.442	ng/ul	0.00
54) 4-Nitrophenol-d4	14.469	143	9326m	3.698	ng/ul	0.00
60) Fluorene-d10	15.234	176	310703	28.214	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.369	200	46343	24.263	ng/ul	0.00
73) Anthracene-d10	17.104	188	489136	31.245	ng/ul	0.00
81) Pyrene-d10	19.369	212	570280	30.426	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.286	264	646325	31.726	ng/ul	0.00

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081822\
Data File : BP011483.D
Acq On : 18 Aug 2022 15:47
Operator : CG/JU
Sample : N4220-01
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
A43K4

Manual IntegrationsAPPROVED

Quant Time: Aug 18 23:16:56 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP081622.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Aug 17 01:58:37 2022
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 08/19/2022
Supervised By :Sohil Jodhani 08/22/2022

