

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081822\
 Data File : BP011486.D
 Acq On : 18 Aug 2022 17:30
 Operator : CG/JU
 Sample : N4221-14
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0KN6

Quant Time: Aug 18 23:18:01 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP081622.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Aug 17 01:58:37 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.557	152	78998	20.000	ng/u1	0.00
20) Naphthalene-d8	10.345	136	328602	20.000	ng/u1	0.00
38) Acenaphthene-d10	14.228	164	182026	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.004	188	355657	20.000	ng/u1	0.00
79) Chrysene-d12	21.133	240	348160	20.000	ng/u1	0.00
88) Perylene-d12	23.427	264	378014	20.000	ng/u1	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.069	96	14553	5.717	ng/uL	0.00
4) Pyridine-d5	3.493	84	21177	3.249	ng/u1	0.01
7) Phenol-d5	6.740	99	38158	5.256	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	6.904	67	125891	26.692	ng/u1	0.00
11) 2-Chlorophenol-d4	7.093	132	116681	21.853	ng/u1	0.00
15) 4-Methylphenol-d8	8.275	113	71309	12.272	ng/u1	0.00
21) Nitrobenzene-d5	8.722	128	71669	30.295	ng/u1	0.00
24) 2-Nitrophenol-d4	9.440	143	70417	29.247	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	9.969	165	111971	25.195	ng/u1	0.00
31) 4-Chloroaniline-d4	10.498	131	134505	18.181	ng/u1	0.00
46) Dimethylphthalate-d6	13.657	166	401222	31.164	ng/u1	0.00
49) Acenaphthylene-d8	13.922	160	441178	30.832	ng/u1	0.00
54) 4-Nitrophenol-d4	14.463	143	10510	4.237	ng/u1	0.00
60) Fluorene-d10	15.233	176	325530	30.055	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.369	200	56564	29.433	ng/u1	0.00
73) Anthracene-d10	17.104	188	561219	35.629	ng/u1	0.00
81) Pyrene-d10	19.363	212	617178	35.037	ng/u1	0.00
92) Benzo(a)pyrene-d12	23.280	264	655241	35.634	ng/u1	0.00
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.099	88	299501	112.830	ng/uL	100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081822\
Data File : BP011486.D
Acq On : 18 Aug 2022 17:30
Operator : CG/JU
Sample : N4221-14
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0KN6


Quant Time: Aug 18 23:18:01 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP081622.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Aug 17 01:58:37 2022
Response via : Initial Calibration

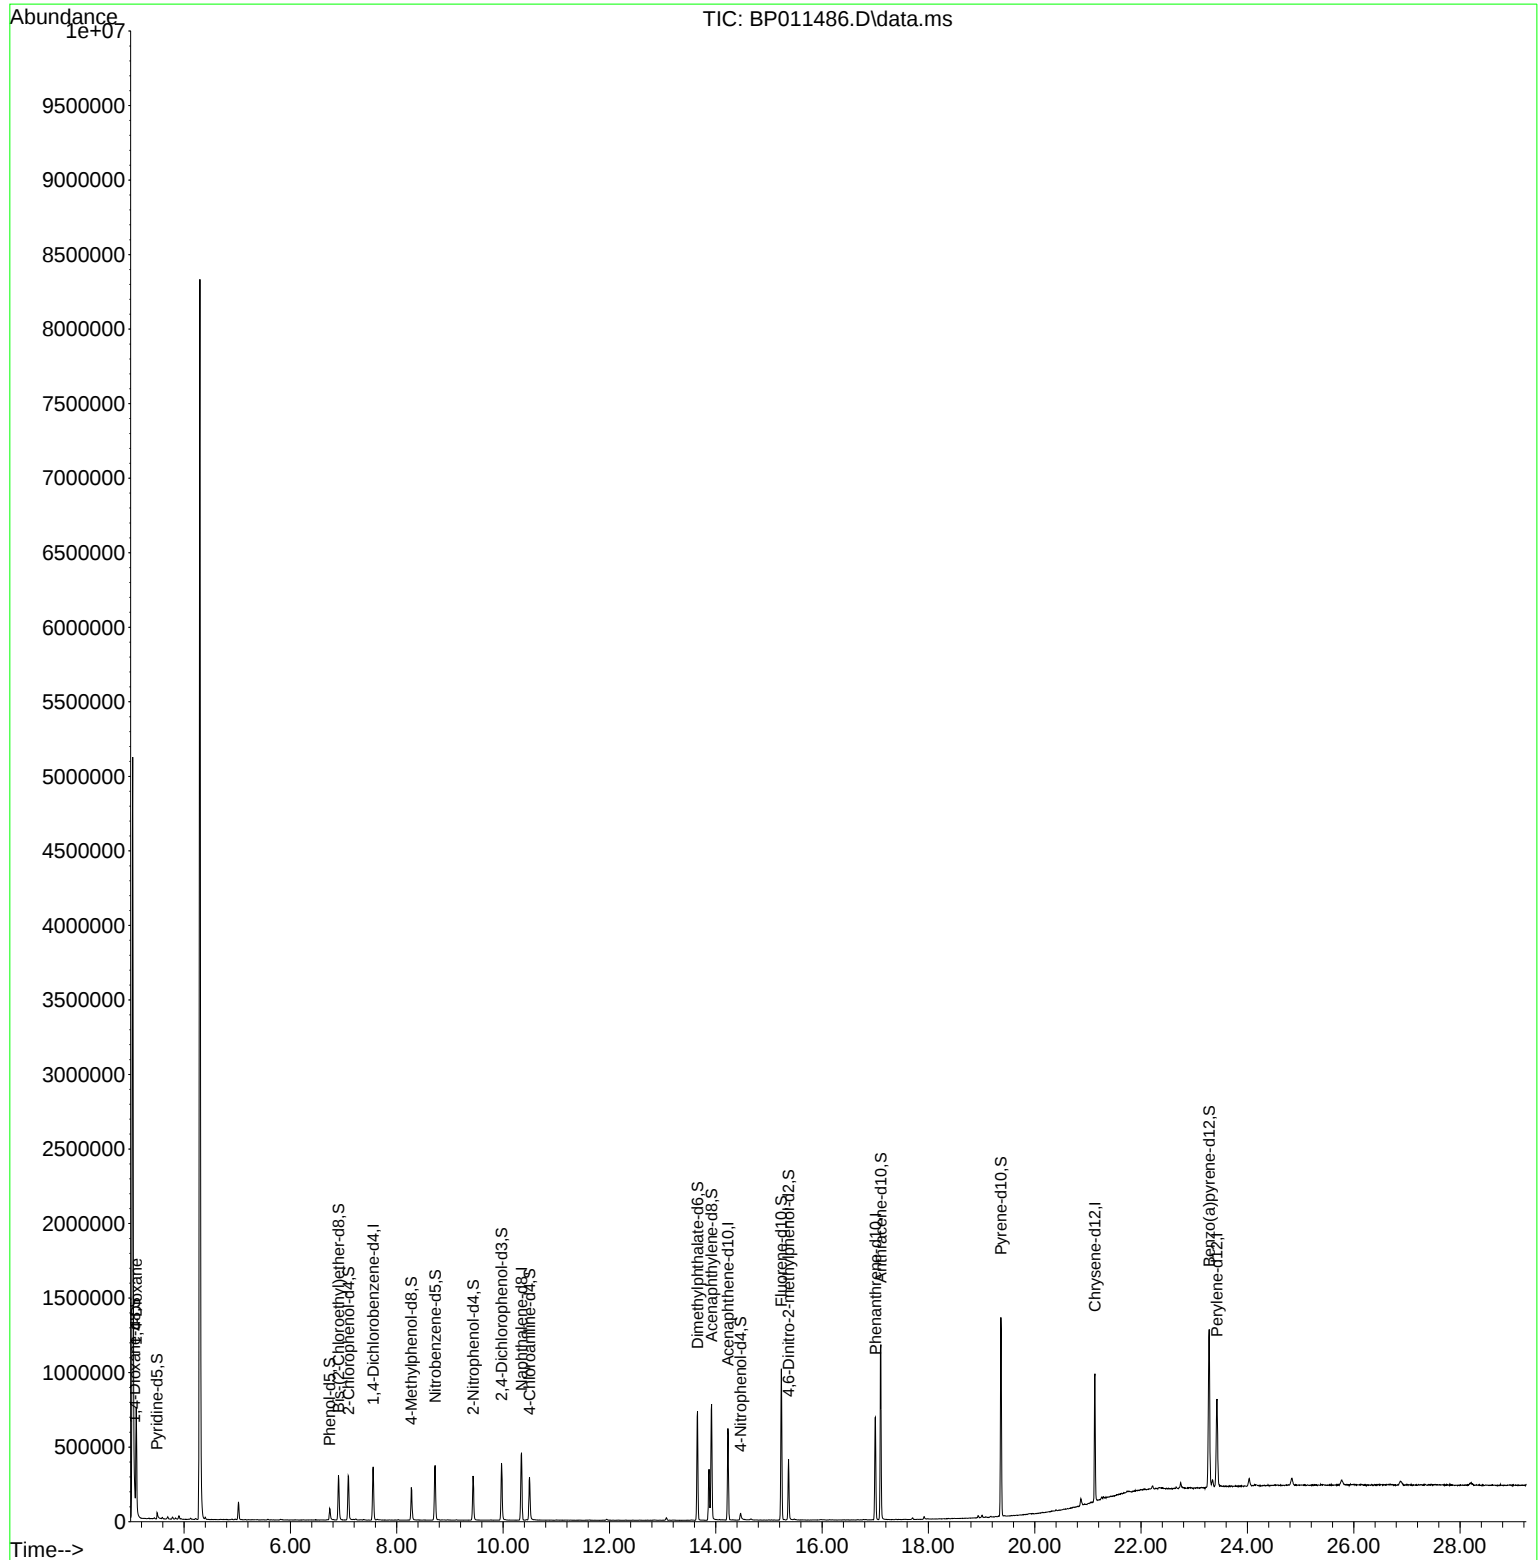

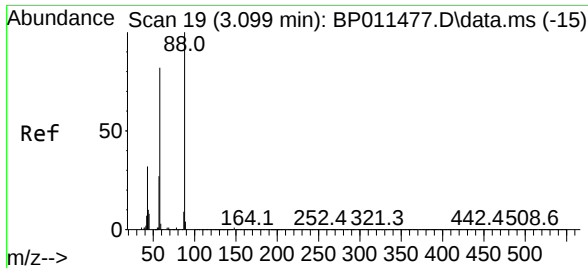

#2
 1,4-Dioxane
 Concen: 112.830 ng/uL
 RT: 3.099 min Scan# 19
 Delta R.T. -0.006 min
 Lab File: BP011486.D
 Acq: 18 Aug 2022 17:30

Instrument :
 BNA_P
 ClientSampleId :
 C0KN6

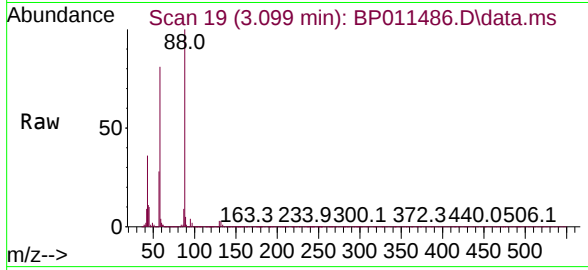

Tgt Ion: 88 Resp: 299501
 Ion Ratio Lower Upper
 88 100
 43 36.2 29.0 43.4
 58 81.4 64.7 97.1

