

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081822\
 Data File : BP011487.D
 Acq On : 18 Aug 2022 18:05
 Operator : CG/JU
 Sample : N4221-15
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0KN7

Quant Time: Aug 18 23:18:22 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP081622.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Aug 17 01:58:37 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.558	152	80934	20.000	ng/u1	0.00
20) Naphthalene-d8	10.346	136	328847	20.000	ng/u1	0.00
38) Acenaphthene-d10	14.228	164	180196	20.000	ng/u1	0.00
64) Phenanthrene-d10	16.998	188	357135	20.000	ng/u1	0.00
79) Chrysene-d12	21.133	240	348198	20.000	ng/u1	0.00
88) Perylene-d12	23.427	264	377360	20.000	ng/u1	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.070	96	12970	4.973	ng/uL	0.00
4) Pyridine-d5	3.487	84	40384	6.048	ng/u1	0.00
7) Phenol-d5	6.740	99	40020	5.381	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	6.905	67	121757	25.198	ng/u1	0.00
11) 2-Chlorophenol-d4	7.087	132	115565	21.126	ng/u1	0.00
15) 4-Methylphenol-d8	8.275	113	71304	11.978	ng/u1	0.00
21) Nitrobenzene-d5	8.722	128	67628	28.566	ng/u1	0.00
24) 2-Nitrophenol-d4	9.434	143	67663	28.083	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	9.969	165	107962	24.275	ng/u1	0.00
31) 4-Chloroaniline-d4	10.499	131	152327	20.575	ng/u1	0.00
46) Dimethylphthalate-d6	13.657	166	398622	31.277	ng/u1	0.00
49) Acenaphthylene-d8	13.916	160	416528	29.405	ng/u1	0.00
54) 4-Nitrophenol-d4	14.469	143	12131	4.940	ng/u1	0.00
60) Fluorene-d10	15.234	176	322926	30.117	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.369	200	54390	28.184	ng/u1	0.00
73) Anthracene-d10	17.098	188	544027	34.395	ng/u1	0.00
81) Pyrene-d10	19.363	212	609418	34.593	ng/u1	0.00
92) Benzo(a)pyrene-d12	23.274	264	637477	34.728	ng/u1	0.00
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.099	88	287631	105.766	ng/uL	100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081822\
Data File : BP011487.D
Acq On : 18 Aug 2022 18:05
Operator : CG/JU
Sample : N4221-15
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0KN7

Quant Time: Aug 18 23:18:22 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP081622.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Aug 17 01:58:37 2022
Response via : Initial Calibration

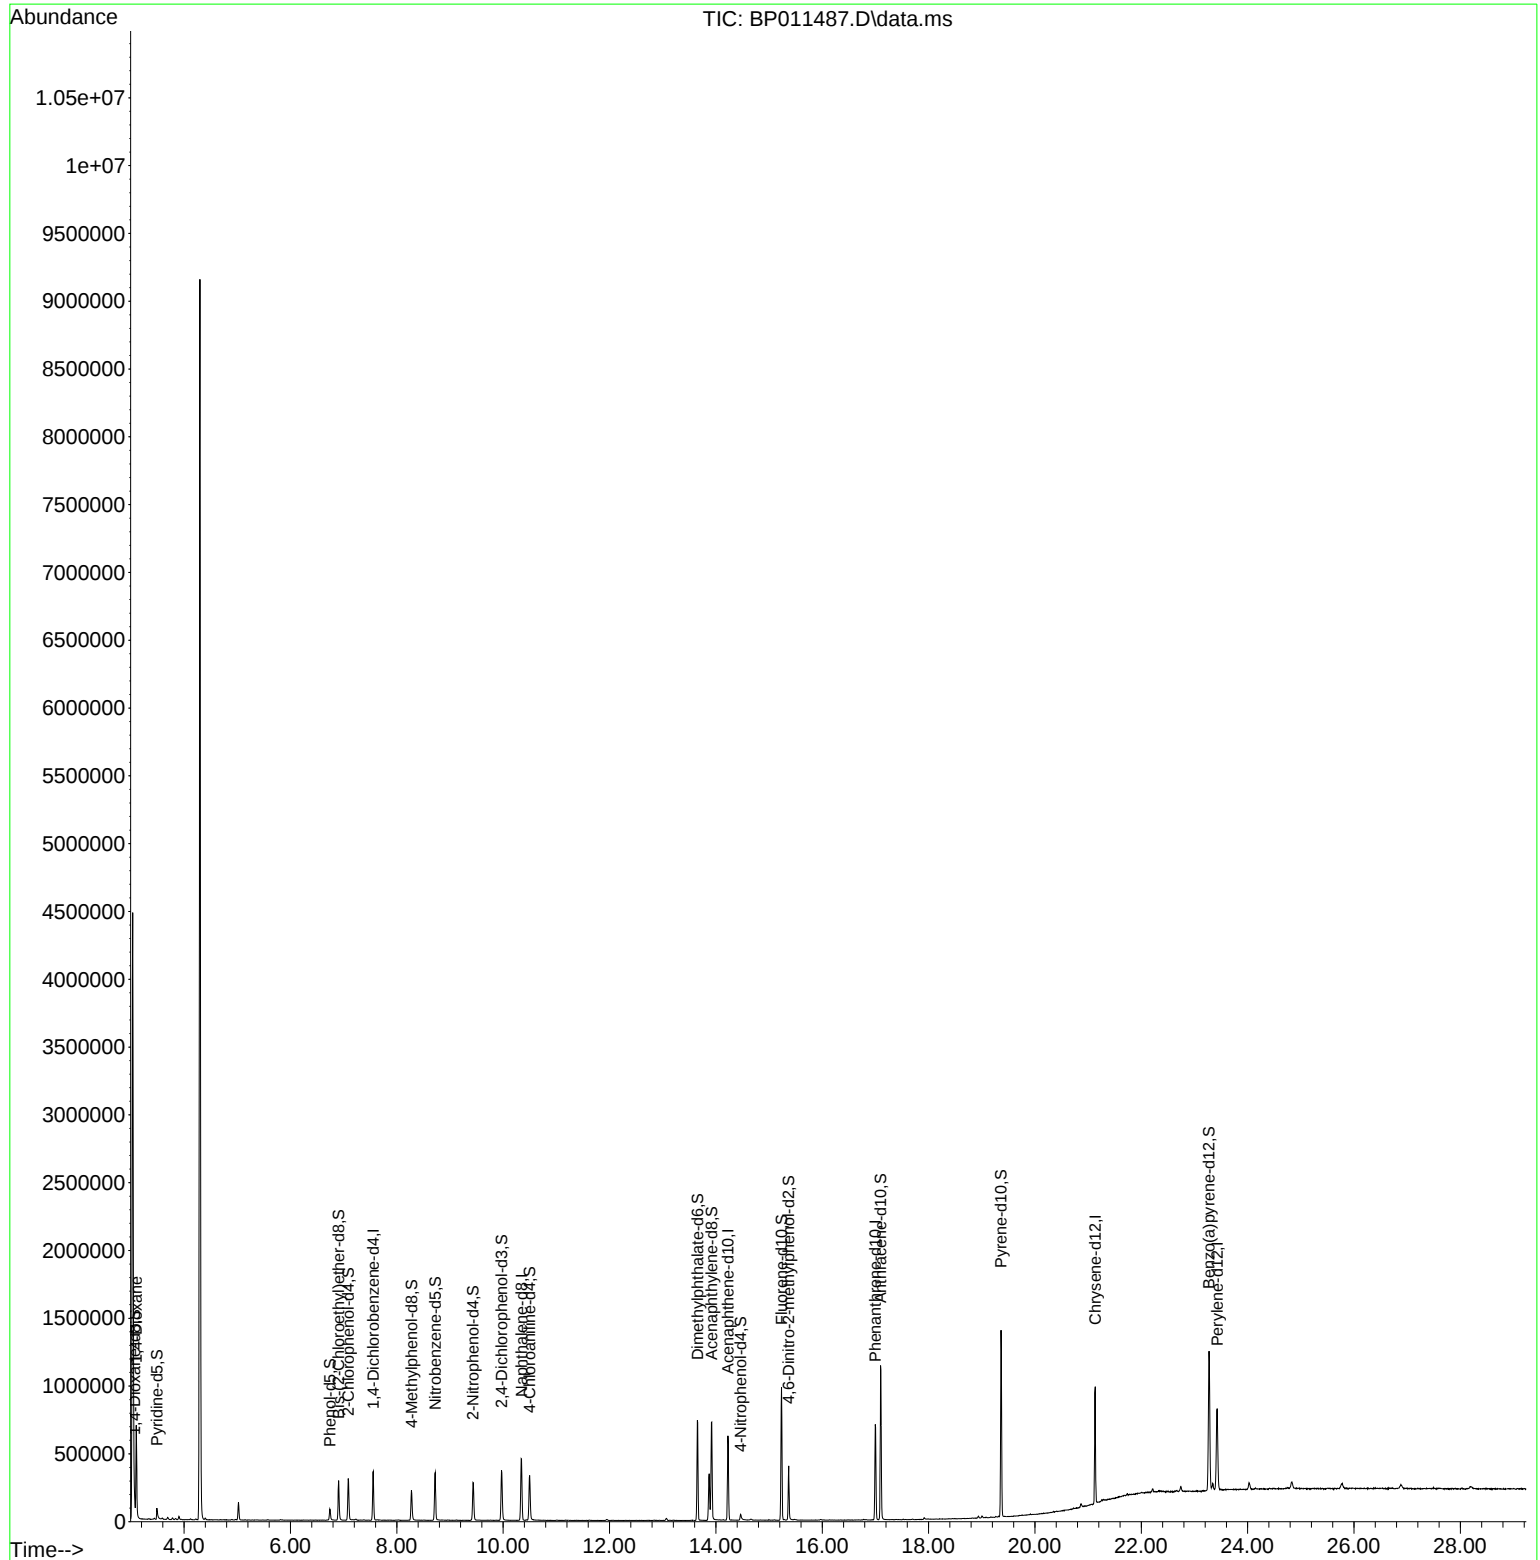

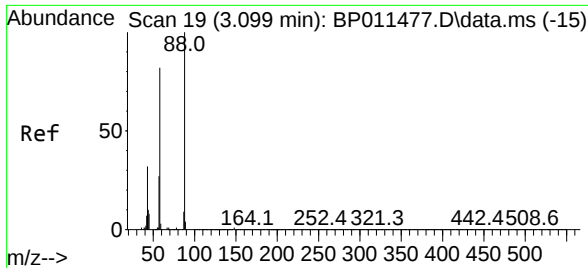

#2
 1,4-Dioxane
 Concen: 105.766 ng/uL
 RT: 3.099 min Scan# 19
 Delta R.T. -0.006 min
 Lab File: BP011487.D
 Acq: 18 Aug 2022 18:05

Instrument :
 BNA_P
 ClientSampleId :
 C0KN7

Tgt Ion: 88 Resp: 287631
 Ion Ratio Lower Upper
 88 100
 43 35.9 29.0 43.4
 58 81.1 64.7 97.1

