

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081822\
 Data File : BP011478.D
 Acq On : 18 Aug 2022 12:12
 Operator : CG/JU
 Sample : PB147103BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK103

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP081622.M
 Title : SVOA CALIBRATION

Signal : TIC: BP011478.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.069	11	14	22	rVB	36459	47742	2.68%	0.211%
2	3.481	81	84	103	rBV	348935	527404	29.59%	2.334%
3	3.787	132	136	141	rVB	9521	12296	0.69%	0.054%
4	5.898	491	495	498	rBV6	1733	2811	0.16%	0.012%
5	6.740	632	638	649	rBV	439031	708080	39.72%	3.134%
6	6.910	660	667	678	rVB	335130	525119	29.46%	2.324%
7	7.093	691	698	709	rBV	471247	734800	41.22%	3.252%
8	7.557	769	777	786	rBV	420618	637291	35.75%	2.820%
9	8.281	892	900	910	rBV	507879	844089	47.35%	3.736%
10	8.722	968	975	989	rBV	423825	684454	38.40%	3.029%
11	8.851	995	997	1000	rBV3	1560	1856	0.10%	0.008%
12	9.439	1089	1097	1111	rBV	367019	585809	32.86%	2.593%
13	9.975	1181	1188	1203	rBV	485971	818141	45.90%	3.621%
14	10.345	1243	1251	1263	rBV	544045	871970	48.91%	3.859%
15	10.498	1270	1277	1289	rBV	446465	777344	43.61%	3.440%
16	10.981	1358	1359	1366	rVB6	1597	1871	0.10%	0.008%
17	11.963	1516	1526	1529	rBV5	6960	14800	0.83%	0.065%
18	12.428	1602	1605	1610	rBV7	874	1848	0.10%	0.008%
19	12.739	1656	1658	1662	rBV5	1139	1862	0.10%	0.008%
20	12.951	1688	1694	1697	rVB8	1161	2006	0.11%	0.009%
21	13.122	1720	1723	1725	rBV3	1647	1925	0.11%	0.009%
22	13.198	1732	1736	1738	rBV5	2381	3016	0.17%	0.013%
23	13.657	1807	1814	1824	rBV	866351	1143266	64.13%	5.060%
24	13.922	1852	1859	1874	rBV	882566	1265859	71.01%	5.602%
25	14.233	1905	1912	1922	rBV	710836	1015783	56.98%	4.495%
26	14.463	1943	1951	1973	rBV	304316	570613	32.01%	2.525%
27	15.233	2076	2082	2090	rBV	1105006	1530860	85.88%	6.775%
28	15.369	2098	2105	2118	rBV	411228	582276	32.66%	2.577%
29	15.474	2119	2123	2130	rVB	11381	18582	1.04%	0.082%
30	15.810	2176	2180	2185	rBV8	1701	3100	0.17%	0.014%
31	16.027	2213	2217	2222	rVB6	3801	4953	0.28%	0.022%
32	16.139	2232	2236	2238	rBV5	1670	1925	0.11%	0.009%
33	16.792	2342	2347	2350	rBV6	2974	4565	0.26%	0.020%
34	17.004	2377	2383	2390	rBV	827477	1120729	62.87%	4.960%
35	17.104	2394	2400	2416	rVV	1210025	1636947	91.83%	7.244%
36	17.210	2416	2418	2423	rVB6	2266	2385	0.13%	0.011%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081822\
Data File : BP011478.D
Acq On : 18 Aug 2022 12:12
Operator : CG/JU
Sample : PB147103BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK103

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0.1 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP081622.M

Title : SVOA CALIBRATION

37	17.321	2435	2437	2442	rVB6	1556	1801	0.10%	0.008%
38	17.927	2536	2540	2544	rBV6	3659	5951	0.33%	0.026%
39	18.386	2614	2618	2622	rBV6	2202	4635	0.26%	0.021%
40	18.939	2708	2712	2716	rBV4	13723	20104	1.13%	0.089%
41	19.010	2721	2724	2730	rVV	10605	15668	0.88%	0.069%
42	19.368	2779	2785	2794	rBV	1380800	1742585	97.75%	7.712%
43	21.133	3081	3085	3094	rBV	900209	1126410	63.19%	4.985%
44	23.286	3444	3451	3457	rBV2	954127	1782628	100.00%	7.889%
45	23.433	3470	3476	3488	rVB2	626040	1187896	66.64%	5.257%




Sum of corrected areas: 22596055

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081822\
Data File : BP011478.D
Acq On : 18 Aug 2022 12:12
Operator : CG/JU
Sample : PB147103BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK103

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP081622.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

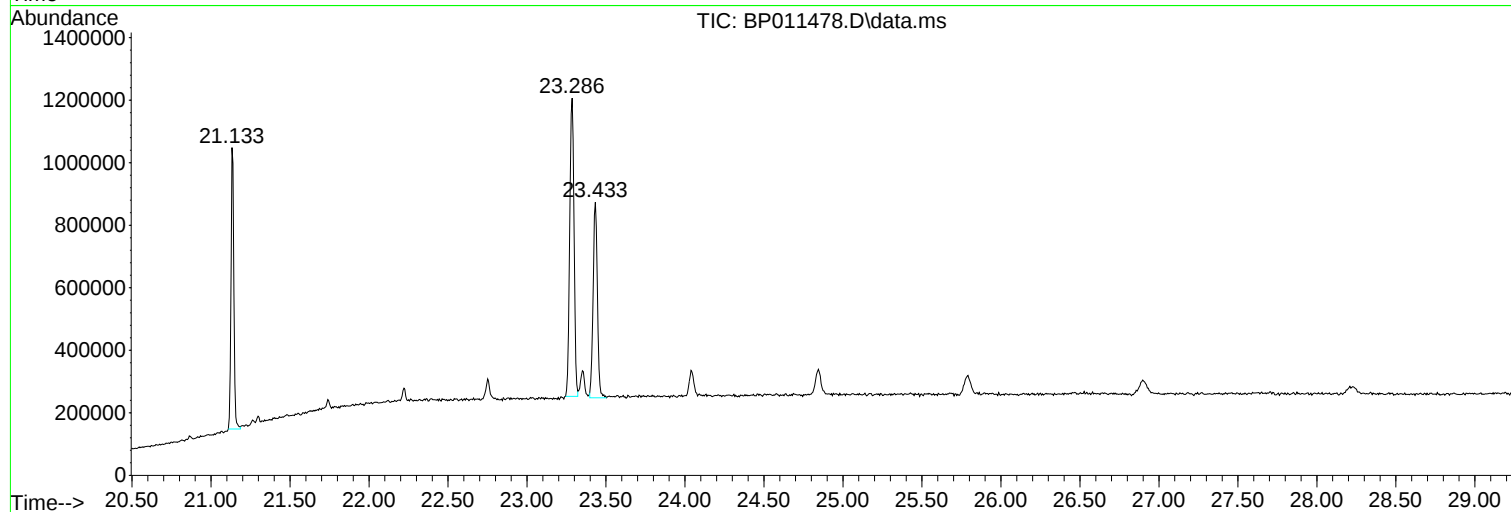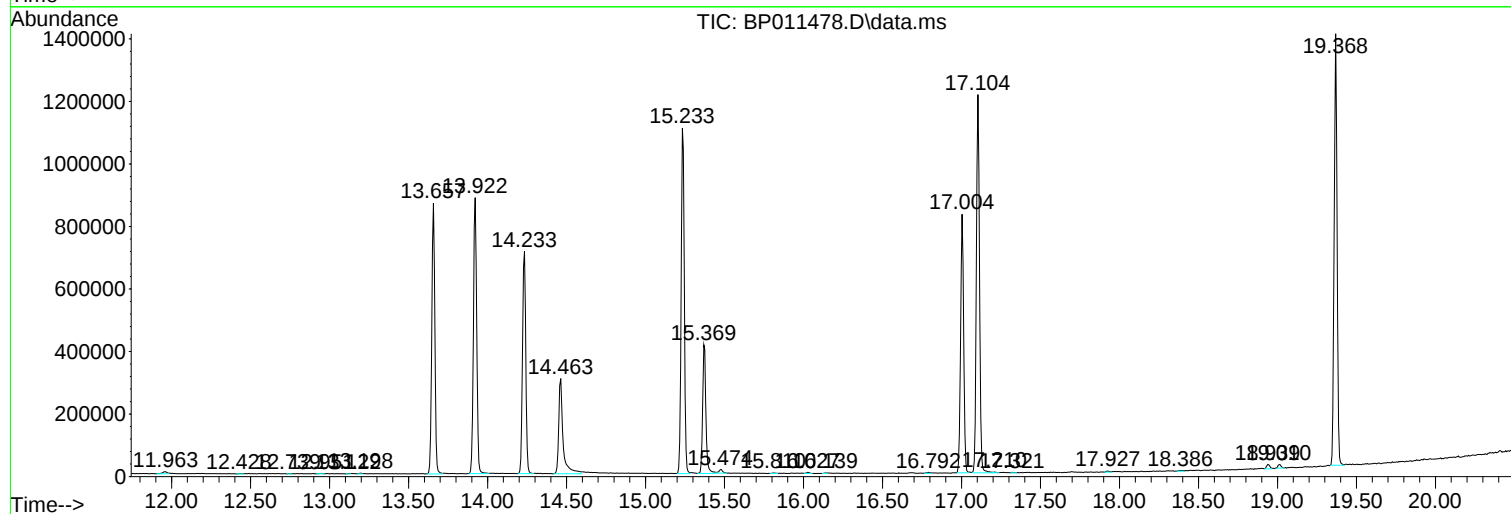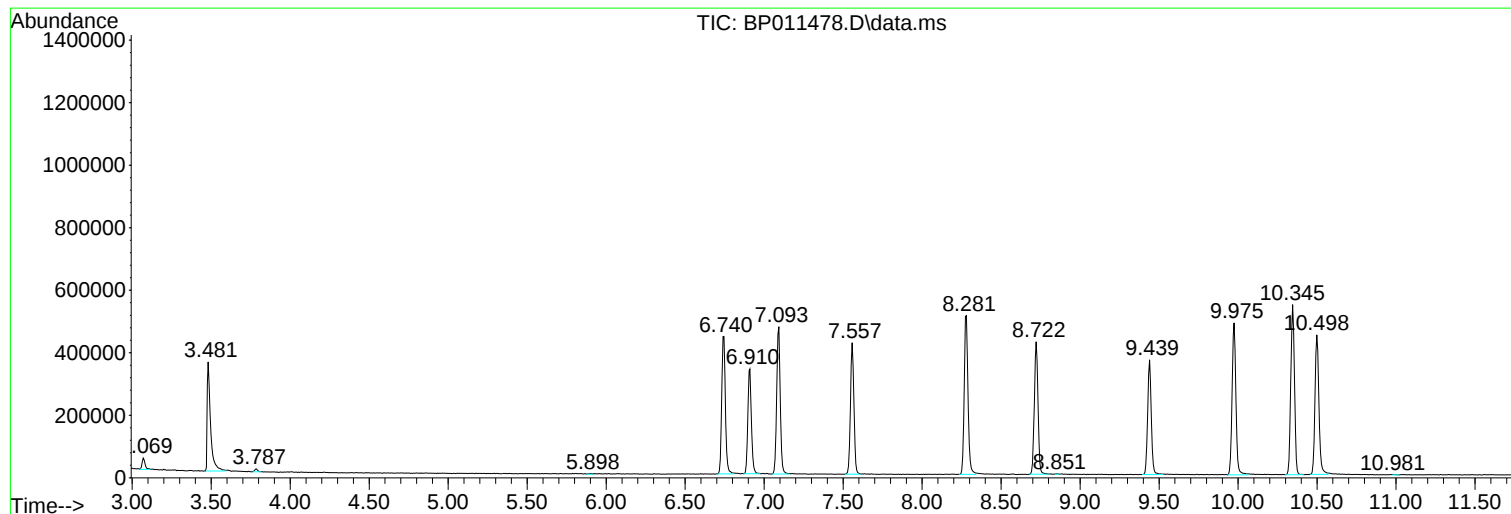

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081822\
Data File : BP011478.D
Acq On : 18 Aug 2022 12:12
Operator : CG/JU
Sample : PB147103BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK103

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP081622.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081822\
Data File : BP011478.D
Acq On : 18 Aug 2022 12:12
Operator : CG/JU
Sample : PB147103BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK103

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP081622.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc