

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081822\
 Data File : BP011481.D
 Acq On : 18 Aug 2022 14:38
 Operator : CG/JU
 Sample : PB147077BL
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK077

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP081622.M
 Title : SVOA CALIBRATION

Signal : TIC: BP011481.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.070	11	14	22	rVB	47273	59106	3.35%	0.244%
2	3.481	80	84	99	rBV	473508	740882	41.95%	3.055%
3	3.787	132	136	141	rVB2	9547	13792	0.78%	0.057%
4	4.005	171	173	177	rVB5	2164	2267	0.13%	0.009%
5	6.746	632	639	654	rBV	532808	814319	46.11%	3.358%
6	6.911	661	667	677	rVB	402950	597556	33.83%	2.464%
7	7.093	691	698	708	rBV	547182	824548	46.68%	3.400%
8	7.564	771	778	788	rBV	457561	721152	40.83%	2.974%
9	8.281	893	900	912	rBV	588673	939661	53.20%	3.875%
10	8.728	968	976	987	rBV	461589	767655	43.46%	3.166%
11	9.440	1089	1097	1108	rBV	395289	656088	37.15%	2.706%
12	9.975	1181	1188	1205	rBV	528739	899460	50.93%	3.709%
13	10.352	1243	1252	1265	rBV	600342	959885	54.35%	3.958%
14	10.505	1269	1278	1293	rBV	525461	910784	51.57%	3.756%
15	11.957	1519	1525	1530	rBV3	8197	13687	0.77%	0.056%
16	13.204	1727	1737	1743	rBV3	3109	7337	0.42%	0.030%
17	13.528	1789	1792	1796	rVB6	1209	1913	0.11%	0.008%
18	13.663	1807	1815	1827	rBV	863741	1183704	67.02%	4.881%
19	13.757	1829	1831	1837	rVB7	1944	3236	0.18%	0.013%
20	13.928	1853	1860	1873	rBV	966797	1349073	76.38%	5.563%
21	14.240	1906	1913	1921	rBV	751295	1100276	62.30%	4.537%
22	14.293	1921	1922	1930	rVB8	4075	5588	0.32%	0.023%
23	14.469	1943	1952	1969	rBV	321743	576598	32.65%	2.378%
24	14.969	2032	2037	2040	rBV7	1432	1795	0.10%	0.007%
25	15.051	2047	2051	2054	rBV6	2180	3313	0.19%	0.014%
26	15.246	2077	2084	2093	rBV	1101648	1598563	90.51%	6.592%
27	15.381	2100	2107	2119	rBV	402237	574143	32.51%	2.368%
28	15.487	2121	2125	2130	rVB6	5635	10417	0.59%	0.043%
29	16.145	2232	2237	2243	rBV7	4919	8834	0.50%	0.036%
30	16.304	2258	2264	2266	rBV7	1237	2199	0.12%	0.009%
31	16.340	2266	2270	2273	rVV6	1336	1971	0.11%	0.008%
32	16.493	2294	2296	2302	rVB7	1635	1822	0.10%	0.008%
33	16.787	2344	2346	2347	rBV2	2603	2068	0.12%	0.009%
34	16.951	2371	2374	2378	rBV5	3614	5403	0.31%	0.022%
35	17.010	2378	2384	2395	rVV	866334	1198234	67.84%	4.941%
36	17.110	2395	2401	2420	rVB	1228012	1682018	95.23%	6.936%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081822\
 Data File : BP011481.D
 Acq On : 18 Aug 2022 14:38
 Operator : CG/JU
 Sample : PB147077BL
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK077

Integration Parameters: LSCINT.P
 Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0.1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP081622.M
 Title : SVOA CALIBRATION

37	17.410	2450	2452	2456	rBV5	1412	2111	0.12%	0.009%
38	17.569	2477	2479	2482	rBV4	1626	1815	0.10%	0.007%
39	17.716	2499	2504	2507	rBV7	2819	4570	0.26%	0.019%
40	17.928	2538	2540	2545	rVB5	4578	4287	0.24%	0.018%
41	18.451	2627	2629	2633	rVB5	2724	3204	0.18%	0.013%
42	18.951	2709	2714	2720	rBV4	16267	23606	1.34%	0.097%
43	19.022	2722	2726	2730	rVV	13366	18518	1.05%	0.076%
44	19.375	2780	2786	2794	rBV	1346432	1758569	99.57%	7.252%
45	21.145	3082	3087	3097	rBV	943175	1197403	67.79%	4.938%
46	23.298	3446	3453	3460	rBV2	965502	1766212	100.00%	7.284%
47	23.445	3472	3478	3489	rVB2	666034	1229731	69.63%	5.071%




Sum of corrected areas: 24249373

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081822\
Data File : BP011481.D
Acq On : 18 Aug 2022 14:38
Operator : CG/JU
Sample : PB147077BL
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK077

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP081622.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

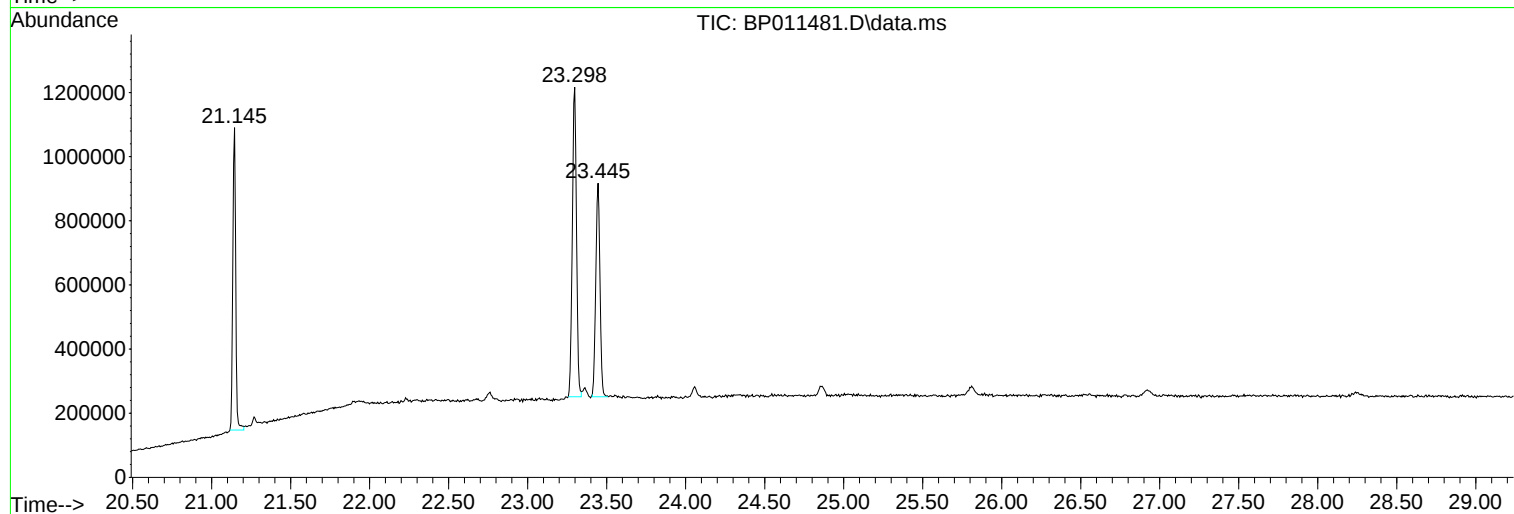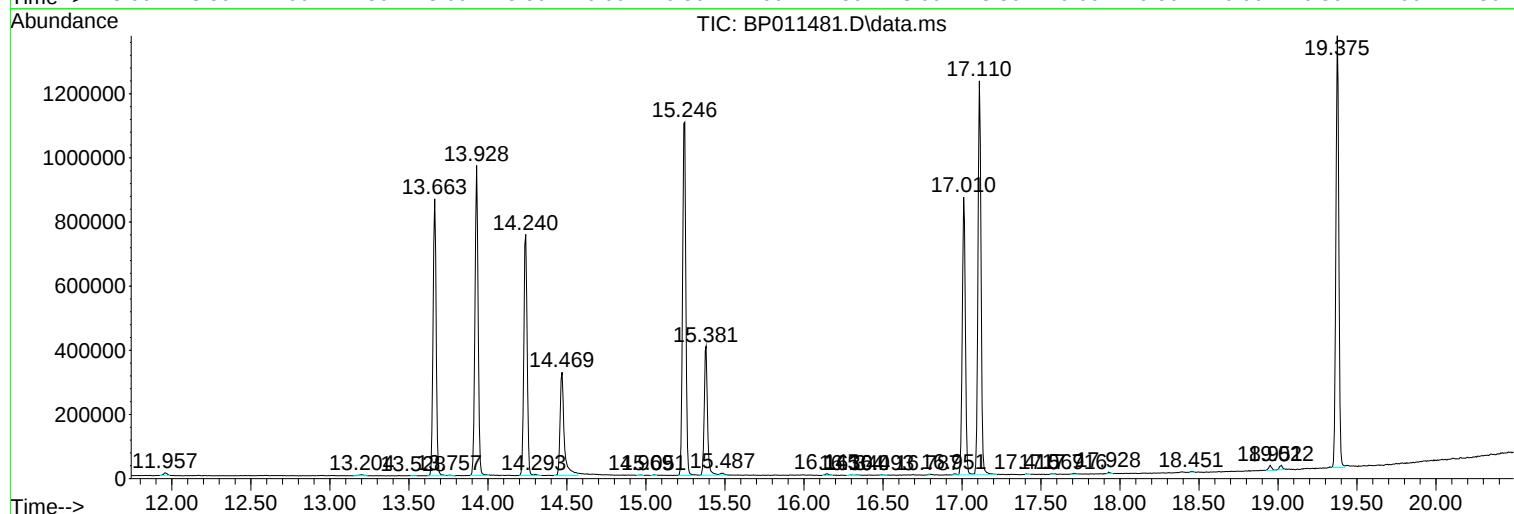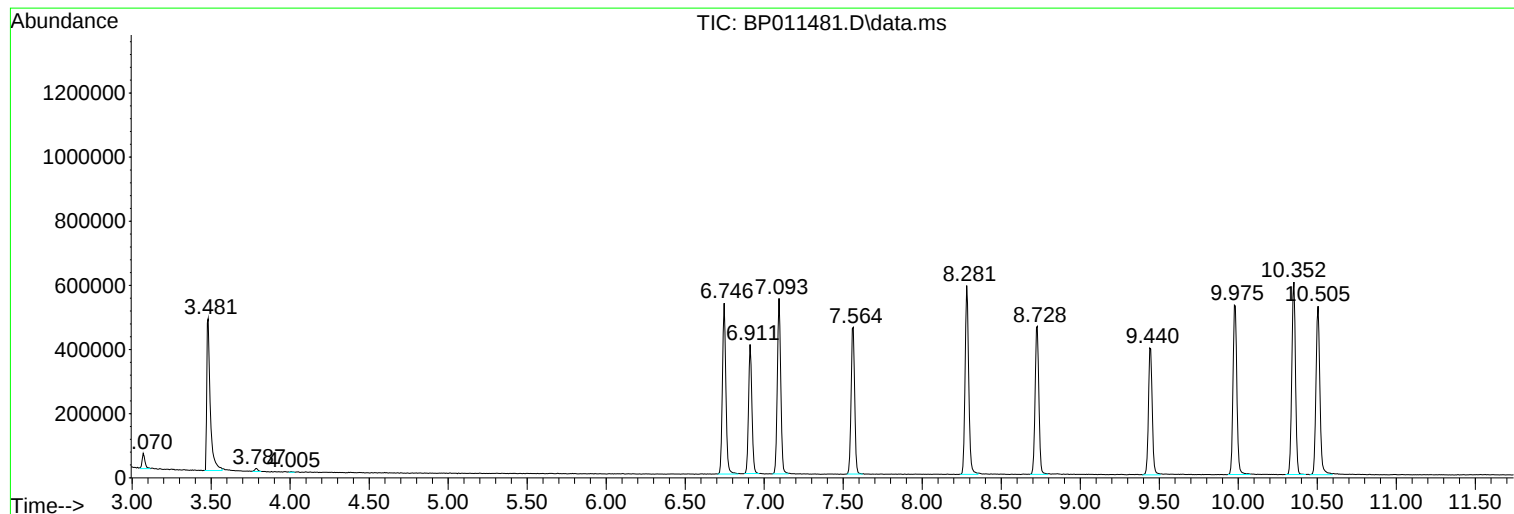

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081822\
Data File : BP011481.D
Acq On : 18 Aug 2022 14:38
Operator : CG/JU
Sample : PB147077BL
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK077

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP081622.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081822\
Data File : BP011481.D
Acq On : 18 Aug 2022 14:38
Operator : CG/JU
Sample : PB147077BL
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK077

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP081622.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc