

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081822\
 Data File : BP011488.D
 Acq On : 18 Aug 2022 18:40
 Operator : CG/JU
 Sample : N4221-16
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 COKN8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP081622.M
 Title : SVOA CALIBRATION

Signal : TIC: BP011488.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.034	3	8	12	rBV	185036	277262	9.92%	1.309%
2	3.070	12	14	18	rVB	26587	29971	1.07%	0.142%
3	3.487	82	85	102	rBV	104296	168419	6.02%	0.795%
4	3.693	116	120	124	rVB2	13853	20126	0.72%	0.095%
5	3.781	131	135	143	rVB	21997	32803	1.17%	0.155%
6	4.217	205	209	213	rBV	5872	7376	0.26%	0.035%
7	4.299	216	223	237	rVB	1928585	2796141	100.00%	13.204%
8	4.893	319	324	331	rVB	15363	23849	0.85%	0.113%
9	6.687	626	629	632	rBV5	3059	3942	0.14%	0.019%
10	6.746	633	639	646	rVV	64608	105839	3.79%	0.500%
11	6.905	659	666	675	rBV	291873	443554	15.86%	2.095%
12	7.087	690	697	707	rBV	283565	452388	16.18%	2.136%
13	7.558	770	777	789	rBV	350562	547370	19.58%	2.585%
14	8.275	892	899	911	rBV	189773	317798	11.37%	1.501%
15	8.722	966	975	983	rBV	357722	588479	21.05%	2.779%
16	9.122	1038	1043	1047	rBV5	2767	4158	0.15%	0.020%
17	9.440	1089	1097	1112	rBV	277951	471178	16.85%	2.225%
18	9.969	1181	1187	1200	rBV	357888	611833	21.88%	2.889%
19	10.346	1242	1251	1261	rBV	447248	734445	26.27%	3.468%
20	10.440	1263	1267	1270	rVV4	3971	5968	0.21%	0.028%
21	10.499	1270	1277	1293	rVV	338043	598137	21.39%	2.825%
22	11.199	1389	1396	1402	rVB	1433	3101	0.11%	0.015%
23	11.616	1463	1467	1472	rBV4	2747	5039	0.18%	0.024%
24	11.951	1518	1524	1530	rBV5	6829	12363	0.44%	0.058%
25	12.834	1669	1674	1677	rBV7	1790	2875	0.10%	0.014%
26	13.198	1732	1736	1742	rBV7	1782	3051	0.11%	0.014%
27	13.651	1806	1813	1826	rBV	715672	992124	35.48%	4.685%
28	13.916	1852	1858	1867	rBV	724766	1074264	38.42%	5.073%
29	14.228	1905	1911	1921	rBV	594781	844000	30.18%	3.986%
30	14.469	1945	1952	1964	rBV3	23952	63144	2.26%	0.298%
31	14.675	1981	1987	1989	rBV7	2789	5123	0.18%	0.024%
32	14.998	2037	2042	2047	rVB3	4439	6315	0.23%	0.030%
33	15.234	2075	2082	2098	rBV	990261	1356303	48.51%	6.405%
34	15.369	2098	2105	2117	rVV	363256	504819	18.05%	2.384%
35	15.475	2120	2123	2129	rVB8	6008	9512	0.34%	0.045%
36	15.975	2203	2208	2210	rBV6	2465	3715	0.13%	0.018%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081822\
 Data File : BP011488.D
 Acq On : 18 Aug 2022 18:40
 Operator : CG/JU
 Sample : N4221-16
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 COKN8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP081622.M
 Title : SVOA CALIBRATION

37	16.134	2230	2235	2240	rVB8	1623	2804	0.10%	0.013%
38	16.487	2291	2295	2302	rVB8	3067	4328	0.15%	0.020%
39	16.781	2340	2345	2349	rVB6	4393	6633	0.24%	0.031%
40	16.945	2369	2373	2376	rBV6	1773	3040	0.11%	0.014%
41	16.998	2376	2382	2392	rVV	659165	930191	33.27%	4.393%
42	17.098	2393	2399	2413	rVV2	1111139	1580107	56.51%	7.462%
43	17.387	2444	2448	2453	rBV7	3084	7331	0.26%	0.035%
44	17.522	2467	2471	2474	rVB5	2198	3151	0.11%	0.015%
45	17.698	2497	2501	2504	rBV6	3825	5283	0.19%	0.025%
46	17.916	2534	2538	2545	rBV4	16570	25745	0.92%	0.122%
47	17.986	2548	2550	2554	rVV3	2939	4183	0.15%	0.020%
48	18.445	2624	2628	2630	rBV4	2762	4180	0.15%	0.020%
49	18.939	2708	2712	2717	rVB2	12408	19082	0.68%	0.090%
50	19.010	2719	2724	2727	rBV	14433	20285	0.73%	0.096%
51	19.169	2749	2751	2755	rBV5	5580	5974	0.21%	0.028%
52	19.363	2778	2784	2794	rBV	1337825	1693533	60.57%	7.997%
53	21.127	3080	3084	3092	rBV	772919	954862	34.15%	4.509%
54	23.274	3442	3449	3457	rBV2	941073	1759051	62.91%	8.307%
55	23.421	3468	3474	3485	rVB	548157	1019900	36.48%	4.816%




Sum of corrected areas: 21176447

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081822\
Data File : BP011488.D
Acq On : 18 Aug 2022 18:40
Operator : CG/JU
Sample : N4221-16
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0KN8

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP081622.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

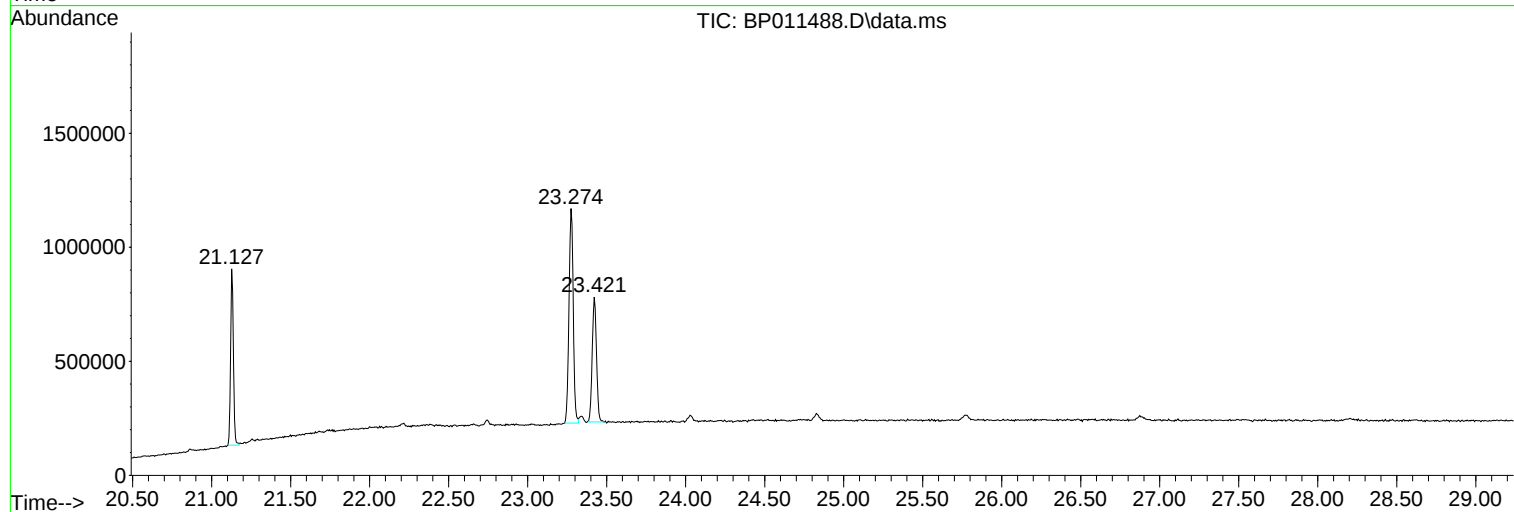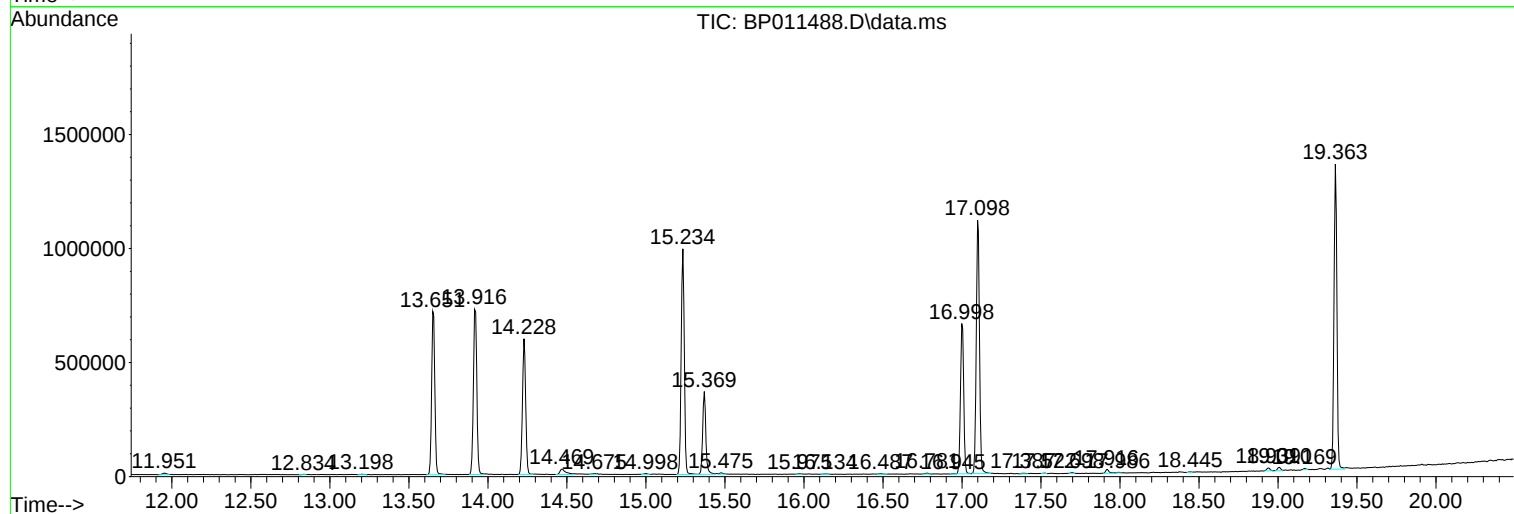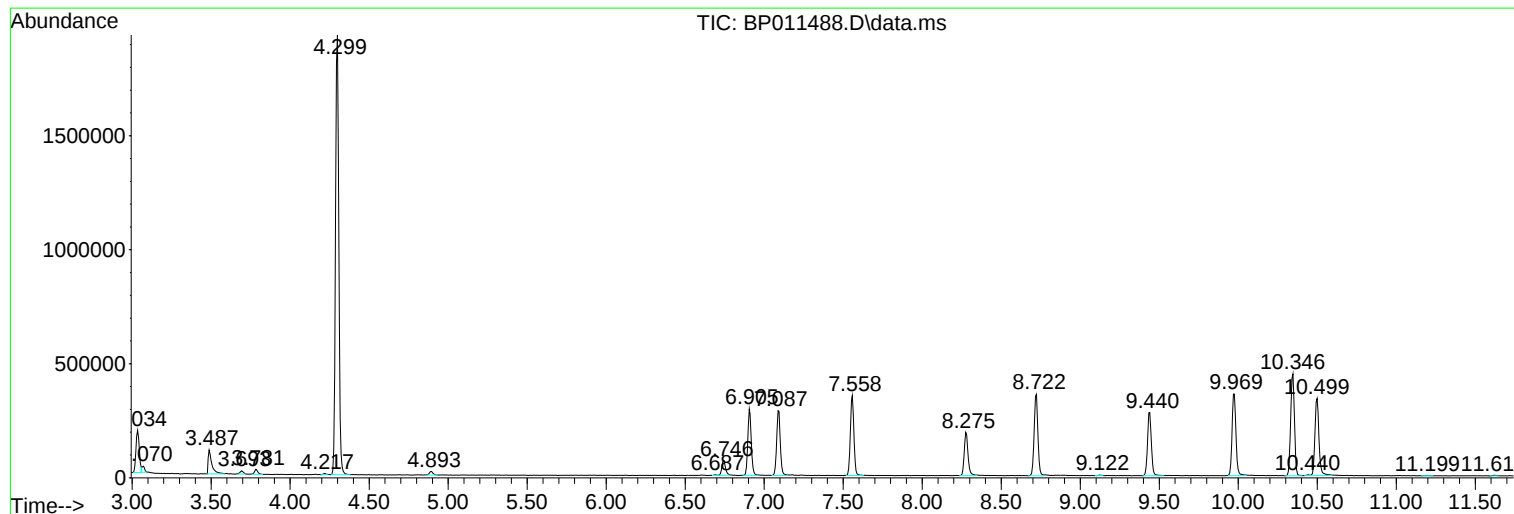

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081822\
Data File : BP011488.D
Acq On : 18 Aug 2022 18:40
Operator : CG/JU
Sample : N4221-16
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0KN8

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP081622.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081822\
Data File : BP011488.D
Acq On : 18 Aug 2022 18:40
Operator : CG/JU
Sample : N4221-16
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0KN8

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP081622.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc