

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081822\
 Data File : BP011489.D
 Acq On : 18 Aug 2022 19:14
 Operator : CG/JU
 Sample : N4221-17
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0KN9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP081622.M
 Title : SVOA CALIBRATION

Signal : TIC: BP011489.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.070	11	14	22	rVB	26161	33010	1.96%	0.178%
2	3.487	83	85	98	rBV	75774	120592	7.15%	0.648%
3	3.693	114	120	124	rVB	15890	22289	1.32%	0.120%
4	3.781	131	135	142	rVB	10519	14525	0.86%	0.078%
5	4.152	193	198	203	rBV	26469	35902	2.13%	0.193%
6	4.217	205	209	215	rVB	6333	10041	0.59%	0.054%
7	4.293	220	222	227	rVB4	2954	3547	0.21%	0.019%
8	4.375	234	236	239	rBV3	1635	1751	0.10%	0.009%
9	5.087	353	357	361	rBV7	1728	2855	0.17%	0.015%
10	5.128	361	364	369	rVB2	4462	5882	0.35%	0.032%
11	5.211	374	378	381	rVB6	1345	1826	0.11%	0.010%
12	5.505	425	428	436	rVB2	6408	9555	0.57%	0.051%
13	5.628	444	449	456	rBV	23813	35462	2.10%	0.191%
14	6.540	600	604	608	rBV7	1417	2477	0.15%	0.013%
15	6.587	609	612	616	rBV5	2054	3237	0.19%	0.017%
16	6.740	625	638	649	rVB2	69880	137453	8.14%	0.739%
17	6.905	660	666	679	rBV	285620	436500	25.86%	2.347%
18	7.087	691	697	707	rBV	284851	452351	26.80%	2.432%
19	7.175	709	712	714	rVB4	1582	2036	0.12%	0.011%
20	7.263	725	727	732	rVB6	2303	2466	0.15%	0.013%
21	7.558	770	777	784	rBV	343926	537845	31.87%	2.892%
22	7.628	784	789	799	rVB	24720	43818	2.60%	0.236%
23	8.169	878	881	886	rVB7	2202	4180	0.25%	0.022%
24	8.275	893	899	910	rBV	192139	320268	18.98%	1.722%
25	8.387	915	918	923	rVB4	4402	5658	0.34%	0.030%
26	8.658	958	964	968	rBV2	13244	23255	1.38%	0.125%
27	8.716	968	974	983	rVV	344917	559592	33.16%	3.009%
28	8.887	997	1003	1017	rVB	156076	265963	15.76%	1.430%
29	9.122	1039	1043	1049	rVB8	2081	3284	0.19%	0.018%
30	9.263	1064	1067	1069	rBV4	1565	2249	0.13%	0.012%
31	9.440	1089	1097	1102	rBV	276727	452974	26.84%	2.436%
32	9.487	1102	1105	1114	rVB	16653	26295	1.56%	0.141%
33	9.634	1123	1130	1134	rBV9	1256	3022	0.18%	0.016%
34	9.710	1139	1143	1147	rVB7	1362	1811	0.11%	0.010%
35	9.969	1181	1187	1200	rBV	357821	595145	35.26%	3.200%
36	10.128	1210	1214	1217	rBV6	1972	3742	0.22%	0.020%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081822\
 Data File : BP011489.D
 Acq On : 18 Aug 2022 19:14
 Operator : CG/JU
 Sample : N4221-17
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 COKN9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP081622.M
 Title : SVOA CALIBRATION

37	10.216	1225	1229	1232	rBV6	2412	3091	0.18%	0.017%
38	10.275	1232	1239	1241	rBV4	4901	7044	0.42%	0.038%
39	10.340	1243	1250	1258	rVV	427857	714381	42.33%	3.841%
40	10.410	1258	1262	1269	rVB3	10000	16736	0.99%	0.090%

41	10.499	1269	1277	1292	rBV	325904	582923	34.54%	3.135%
42	10.840	1333	1335	1341	rVB6	1335	2114	0.13%	0.011%
43	10.916	1343	1348	1352	rVB7	1623	2327	0.14%	0.013%
44	10.975	1353	1358	1361	rBV6	1492	2413	0.14%	0.013%
45	11.010	1361	1364	1366	rBV3	2040	1847	0.11%	0.010%

46	11.169	1387	1391	1398	rVB7	5126	9930	0.59%	0.053%
47	11.487	1442	1445	1450	rBV7	1089	1873	0.11%	0.010%
48	11.663	1469	1475	1485	rVV2	32734	63217	3.75%	0.340%
49	11.734	1485	1487	1493	rVB7	1617	1778	0.11%	0.010%
50	11.951	1518	1524	1533	rVB3	7211	14441	0.86%	0.078%

51	12.434	1603	1606	1610	rBV6	1354	1790	0.11%	0.010%
52	12.522	1615	1621	1626	rBV8	3559	6863	0.41%	0.037%
53	12.575	1626	1630	1635	rBV7	2571	4558	0.27%	0.025%
54	12.834	1670	1674	1681	rVB4	6639	9587	0.57%	0.052%
55	13.163	1719	1730	1742	rBV4	12912	31743	1.88%	0.171%

56	13.463	1777	1781	1785	rBV5	1052	1741	0.10%	0.009%
57	13.651	1807	1813	1827	rBV	670170	932750	55.27%	5.016%
58	13.916	1850	1858	1871	rBV	710901	1025306	60.75%	5.513%
59	14.228	1904	1911	1920	rBV	587462	834590	49.45%	4.488%
60	14.322	1925	1927	1932	rVV5	4819	6249	0.37%	0.034%

61	14.469	1945	1952	1964	rBV3	22015	60688	3.60%	0.326%
62	14.681	1984	1988	1993	rVB8	3780	6184	0.37%	0.033%
63	14.922	2022	2029	2035	rVV	19829	32519	1.93%	0.175%
64	14.998	2039	2042	2048	rVV3	4920	8058	0.48%	0.043%
65	15.057	2048	2052	2061	rVV8	6906	15395	0.91%	0.083%

66	15.234	2075	2082	2094	rBV	930362	1301365	77.11%	6.998%
67	15.369	2099	2105	2115	rVV	333482	444433	26.33%	2.390%
68	15.481	2119	2124	2128	rVV7	5603	13349	0.79%	0.072%
69	15.528	2128	2132	2136	rVB6	6871	10590	0.63%	0.057%
70	15.616	2143	2147	2151	rVB4	4773	6315	0.37%	0.034%

71	15.816	2174	2181	2184	rBV9	2894	4960	0.29%	0.027%
72	15.857	2184	2188	2193	rVB7	3153	4561	0.27%	0.025%
73	15.969	2204	2207	2212	rVV6	2324	3515	0.21%	0.019%
74	16.022	2212	2216	2221	rVB7	1841	3950	0.23%	0.021%
75	16.604	2311	2315	2319	rVB6	3545	4282	0.25%	0.023%

76	16.681	2326	2328	2333	rVB6	1542	1876	0.11%	0.010%
----	--------	------	------	------	------	------	------	-------	--------

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081822\
 Data File : BP011489.D
 Acq On : 18 Aug 2022 19:14
 Operator : CG/JU
 Sample : N4221-17
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0KN9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP081622.M
 Title : SVOA CALIBRATION

77	16.781	2341	2345	2349	rVV6	2988	3941	0.23%	0.021%
78	16.945	2368	2373	2374	rBV5	2507	3074	0.18%	0.017%
79	16.998	2376	2382	2392	rVB	679206	924218	54.76%	4.970%
80	17.098	2392	2399	2411	rBV	1075334	1491131	88.35%	8.018%
81	17.222	2417	2420	2424	rVB6	2310	3346	0.20%	0.018%
82	17.310	2432	2435	2439	rVB3	4089	4678	0.28%	0.025%
83	17.686	2494	2499	2505	rBV	201558	254228	15.06%	1.367%
84	17.857	2525	2528	2532	rBV6	3555	5438	0.32%	0.029%
85	17.916	2534	2538	2542	rBV6	9729	14199	0.84%	0.076%
86	17.992	2547	2551	2557	rVV3	8980	16562	0.98%	0.089%
87	18.110	2567	2571	2574	rBV5	1447	2173	0.13%	0.012%
88	18.157	2576	2579	2584	rVV5	6011	7619	0.45%	0.041%
89	18.204	2584	2587	2592	rVB7	3049	3974	0.24%	0.021%
90	18.245	2592	2594	2597	rVB3	2077	1941	0.12%	0.010%
91	18.286	2597	2601	2602	rBV3	2103	2710	0.16%	0.015%
92	18.751	2677	2680	2684	rBV5	4539	6340	0.38%	0.034%
93	18.933	2708	2711	2718	rBV5	12735	18164	1.08%	0.098%
94	19.010	2720	2724	2727	rBV2	13072	18302	1.08%	0.098%
95	19.169	2748	2751	2754	rBV4	5445	8349	0.49%	0.045%
96	19.316	2773	2776	2778	rBV3	6102	6512	0.39%	0.035%
97	19.363	2778	2784	2792	rVV	1311464	1639729	97.16%	8.817%
98	21.127	3080	3084	3092	rBV	825373	1009975	59.84%	5.431%
99	23.274	3443	3449	3456	rBV2	953557	1687718	100.00%	9.075%
100	23.421	3468	3474	3483	rVB2	574696	1077965	63.87%	5.797%




Sum of corrected areas: 18596476

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081822\
Data File : BP011489.D
Acq On : 18 Aug 2022 19:14
Operator : CG/JU
Sample : N4221-17
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0KN9

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP081622.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

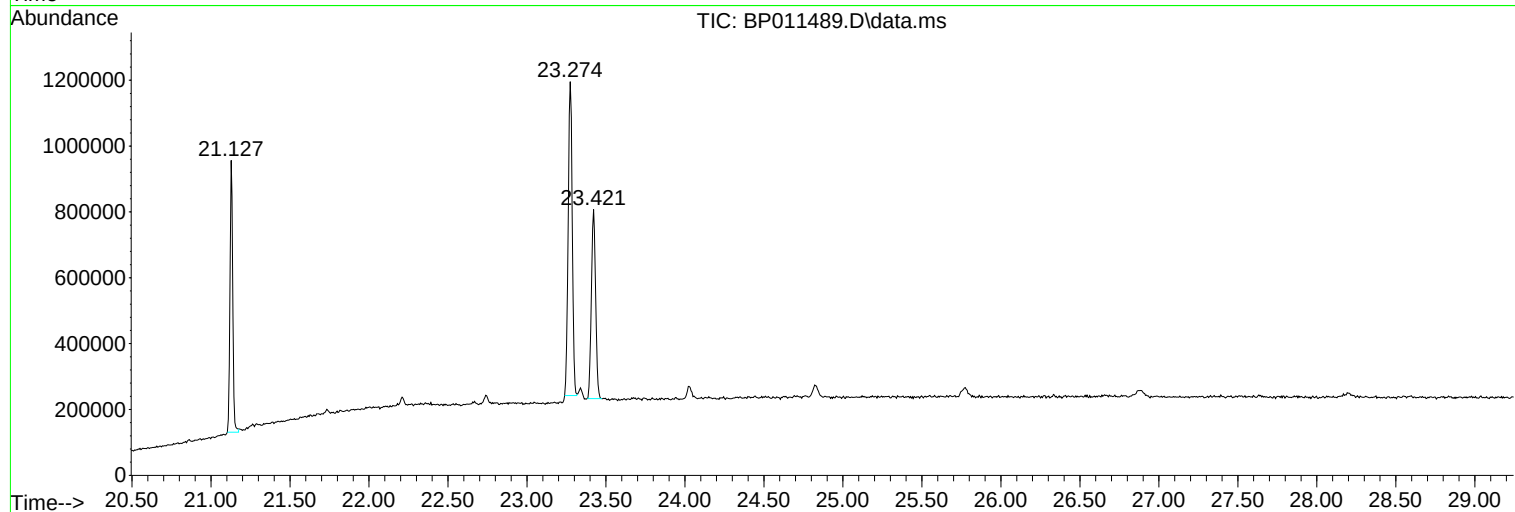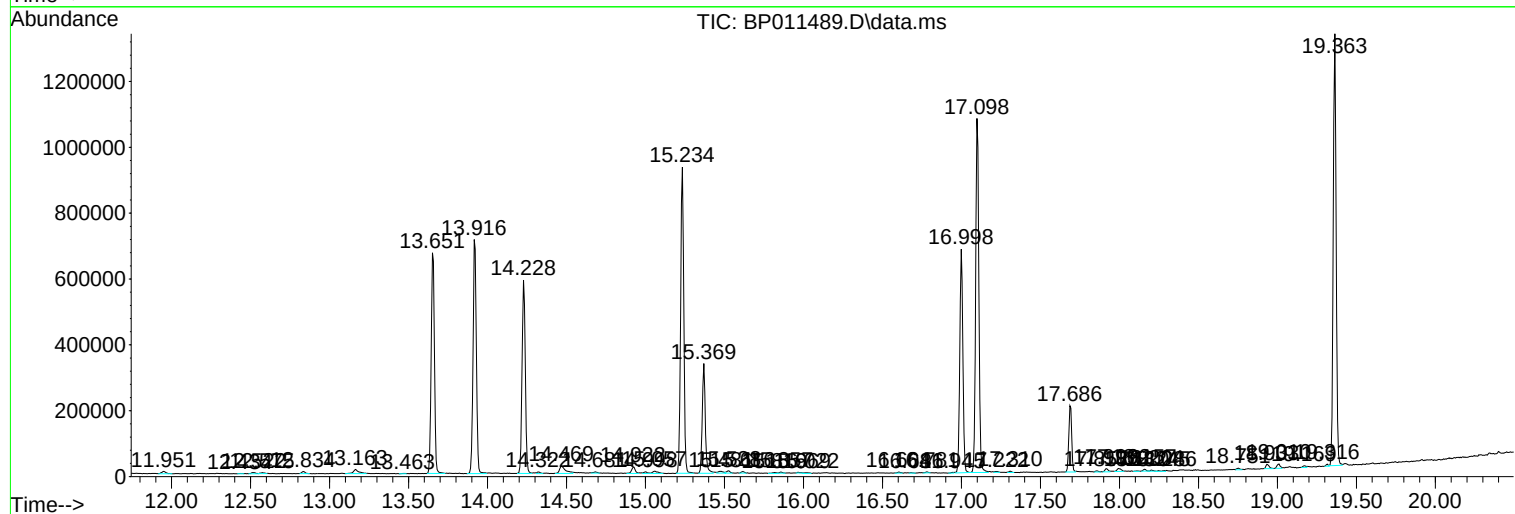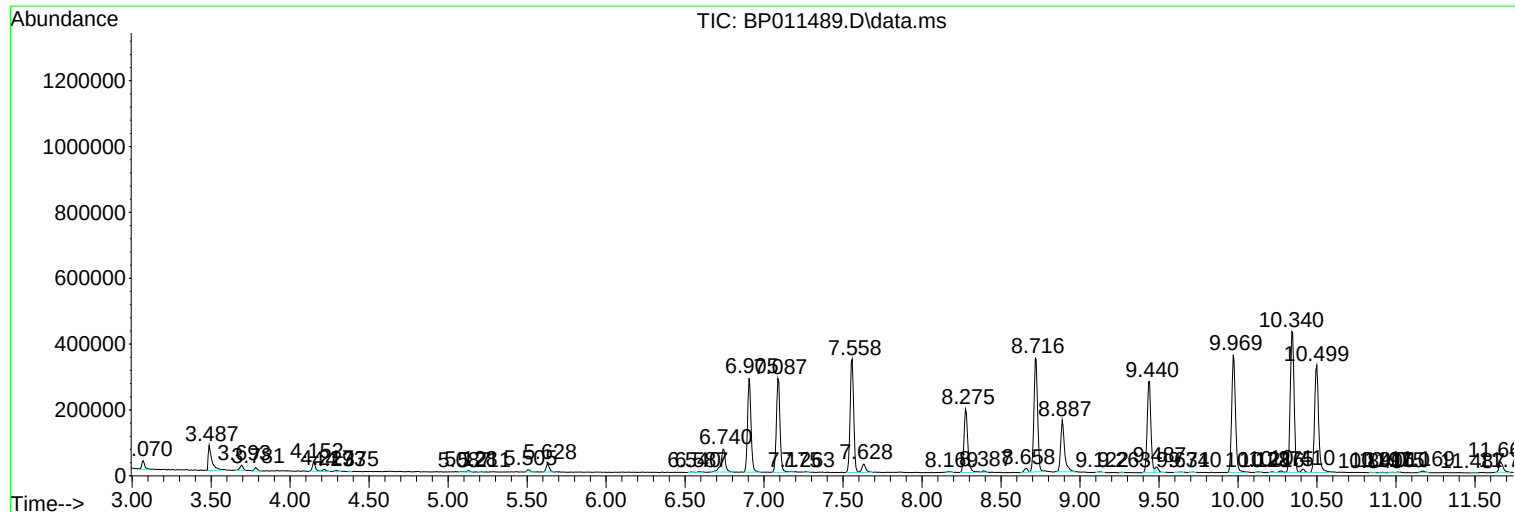

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081822\
Data File : BP011489.D
Acq On : 18 Aug 2022 19:14
Operator : CG/JU
Sample : N4221-17
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0KN9










Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP081622.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Ethanol, 2-(hexyloxy)- Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
8.887	9.89 ng/ul	265963	1,4-Dichlorobenzene-d4	7.558

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Ethanol, 2-(hexyloxy)-	146	C8H18O2	000112-25-4	50
2			Hexane, 1-propoxy-	144	C9H20O	053685-78-2	47
3			3-(Hexyloxy)-1,2-propanediol	176	C9H20O3	010305-38-1	40
4			Heptane, 3,4,5-trimethyl-	142	C10H22	020278-89-1	38
5			Hexane, 3-iodo-	212	C6H13I	031294-91-4	38

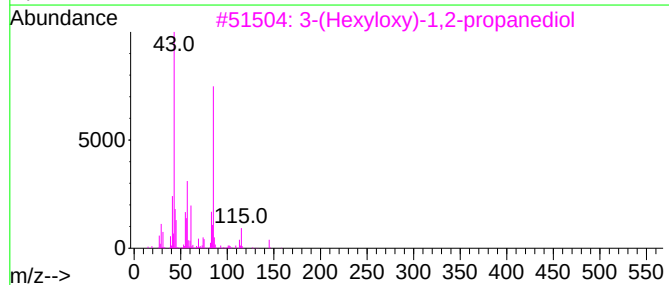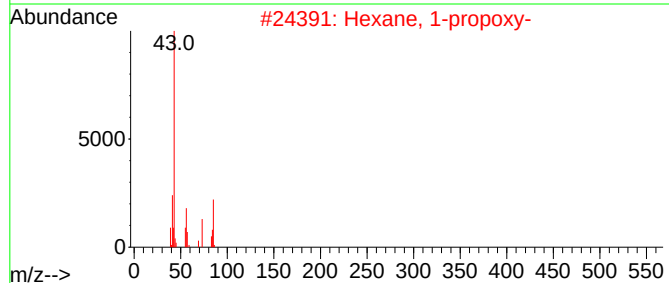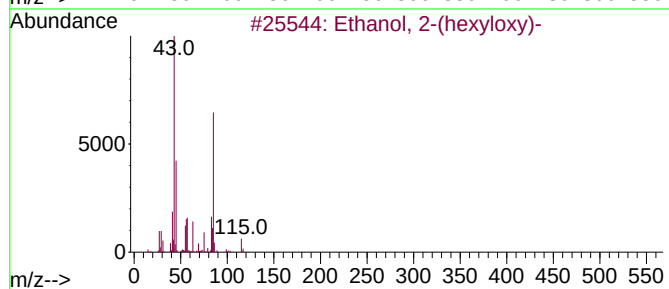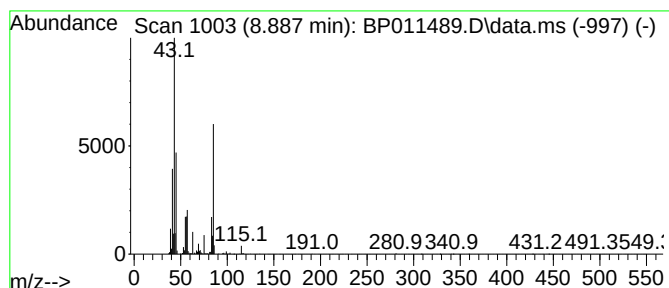

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081822\
Data File : BP011489.D
Acq On : 18 Aug 2022 19:14
Operator : CG/JU
Sample : N4221-17
Misc :
ALS Vial : 14 Sample Multiplier: 1










Instrument :
BNA_P
ClientSampleId :
C0KN9

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP081622.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 2 7,9-Di-tert-butyl-1-oxaspiro... Concentration Rank 2

R.T.	EstConc	Area	Relative to ISTD	R.T.	
17.686	5.50 ng/ul	254228	Phenanthrene-d10	16.998	
Hit# of 5	Tentative ID	MW	MolForm	CAS#	Qual
1	7,9-Di-tert-butyl-1-oxaspiro(4,5...	276	C17H24O3	082304-66-3	96
2	7,9-Di-tert-butyl-1-oxaspiro(4,5...	276	C17H24O3	082304-66-3	87
3	7,9-Di-tert-butyl-1-oxaspiro(4,5...	276	C17H24O3	082304-66-3	70
4	1-(3-Amino-4,6-dimethylthieno[2,...	220	C11H12N2OS	052505-42-7	49
5	2,5-Cyclohexadien-1-one, 2,6-bis...	232	C16H24O	006738-27-8	42

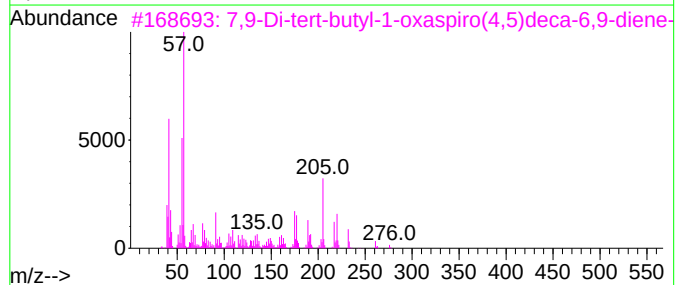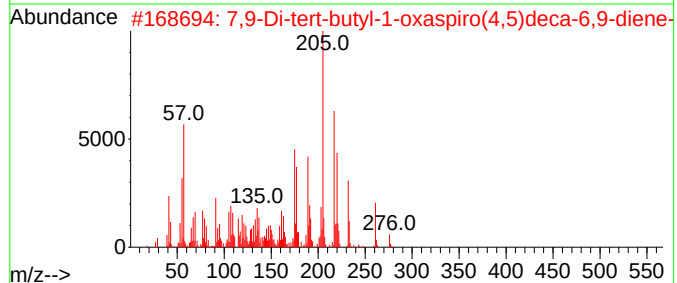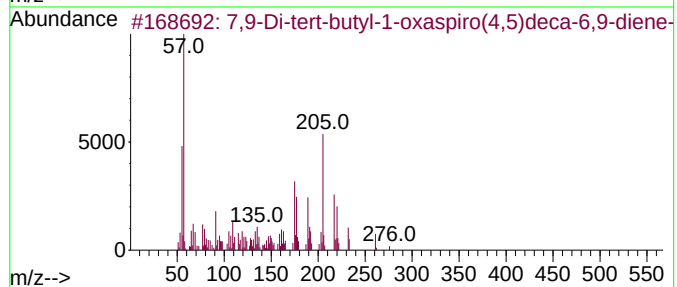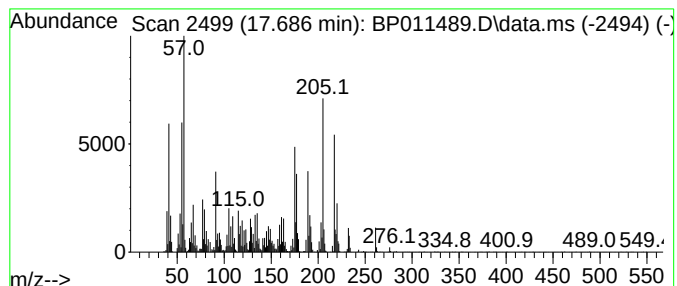

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081822\
Data File : BP011489.D
Acq On : 18 Aug 2022 19:14
Operator : CG/JU
Sample : N4221-17
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0KN9

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP081622.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Ethanol, 2-(hex...	8.887	9.9	ng/ul	265963	1	7.558	537845	20.0
7,9-Di-tert-but...	17.686	5.5	ng/ul	254228	4	16.998	924218	20.0