

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081822\
 Data File : BP011490.D
 Acq On : 18 Aug 2022 19:49
 Operator : CG/JU
 Sample : N4221-18
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 COKP0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP081622.M
 Title : SVOA CALIBRATION

Signal : TIC: BP011490.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.034	3	8	12	rBV	339815	480861	8.57%	2.008%
2	3.105	17	20	25	rVB	16484	23278	0.41%	0.097%
3	3.511	87	89	96	rBV	12834	21762	0.39%	0.091%
4	3.693	115	120	128	rVB	16651	25119	0.45%	0.105%
5	3.781	132	135	140	rVB2	7817	11084	0.20%	0.046%
6	4.217	204	209	214	rVB3	7860	12919	0.23%	0.054%
7	4.299	216	223	237	rVB	3884448	5609239	100.00%	23.428%
8	4.887	318	323	329	rVB	28324	42266	0.75%	0.177%
9	6.687	625	629	633	rBV3	5530	8890	0.16%	0.037%
10	6.740	633	638	653	rVB	79748	128813	2.30%	0.538%
11	6.905	660	666	677	rBV	324935	493890	8.80%	2.063%
12	7.087	691	697	709	rBV	334748	517901	9.23%	2.163%
13	7.558	770	777	789	rBV	323471	523882	9.34%	2.188%
14	8.275	893	899	909	rBV2	230746	367156	6.55%	1.534%
15	8.716	966	974	992	rBV	399601	659900	11.76%	2.756%
16	9.122	1038	1043	1049	rVB	8964	13775	0.25%	0.058%
17	9.434	1089	1096	1104	rBV	310819	518187	9.24%	2.164%
18	9.969	1179	1187	1199	rBV	400756	685630	12.22%	2.864%
19	10.340	1242	1250	1259	rBV	411853	673034	12.00%	2.811%
20	10.440	1262	1267	1272	rBV4	5831	11117	0.20%	0.046%
21	10.499	1272	1277	1288	rVV	47569	93384	1.66%	0.390%
22	11.622	1463	1468	1473	rVB2	10346	16813	0.30%	0.070%
23	11.952	1518	1524	1532	rBV4	7175	15233	0.27%	0.064%
24	13.651	1807	1813	1827	rBV	749158	1040607	18.55%	4.346%
25	13.916	1851	1858	1867	rBV	789882	1157197	20.63%	4.833%
26	14.228	1904	1911	1920	rBV	552764	781707	13.94%	3.265%
27	14.463	1946	1951	1964	rBV2	27466	71559	1.28%	0.299%
28	15.234	2075	2082	2090	rBV	1030066	1409741	25.13%	5.888%
29	15.369	2098	2105	2114	rBV	376875	495986	8.84%	2.072%
30	15.475	2120	2123	2128	rVB6	5286	7808	0.14%	0.033%
31	16.481	2290	2294	2298	rVB	5121	6485	0.12%	0.027%
32	16.787	2341	2346	2351	rBV9	2480	5826	0.10%	0.024%
33	16.998	2376	2382	2393	rVV	603633	843795	15.04%	3.524%
34	17.098	2393	2399	2413	rBV	1121568	1564271	27.89%	6.534%
35	17.563	2475	2478	2482	rBV4	4779	6966	0.12%	0.029%
36	17.692	2496	2500	2506	rBV7	5302	8128	0.14%	0.034%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081822\
 Data File : BP011490.D
 Acq On : 18 Aug 2022 19:49
 Operator : CG/JU
 Sample : N4221-18
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0KP0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP081622.M
 Title : SVOA CALIBRATION

37	17.916	2534	2538	2543	rBV5	12175	19038	0.34%	0.080%
38	18.486	2633	2635	2642	rVB8	5082	6330	0.11%	0.026%
39	18.939	2708	2712	2718	rBV4	13105	18313	0.33%	0.076%
40	19.010	2720	2724	2728	rVV2	11951	17816	0.32%	0.074%
41	19.263	2765	2767	2773	rVB6	10771	14508	0.26%	0.061%
42	19.363	2778	2784	2791	rBV	1382494	1723854	30.73%	7.200%
43	20.269	2935	2938	2942	rBV3	30368	38747	0.69%	0.162%
44	21.128	3080	3084	3092	rBV	759057	938156	16.73%	3.918%
45	23.274	3443	3449	3457	rBV2	1014306	1818158	32.41%	7.594%
46	23.422	3468	3474	3482	rVB2	525916	993159	17.71%	4.148%




Sum of corrected areas: 23942288

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081822\
Data File : BP011490.D
Acq On : 18 Aug 2022 19:49
Operator : CG/JU
Sample : N4221-18
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0KP0

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP081622.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

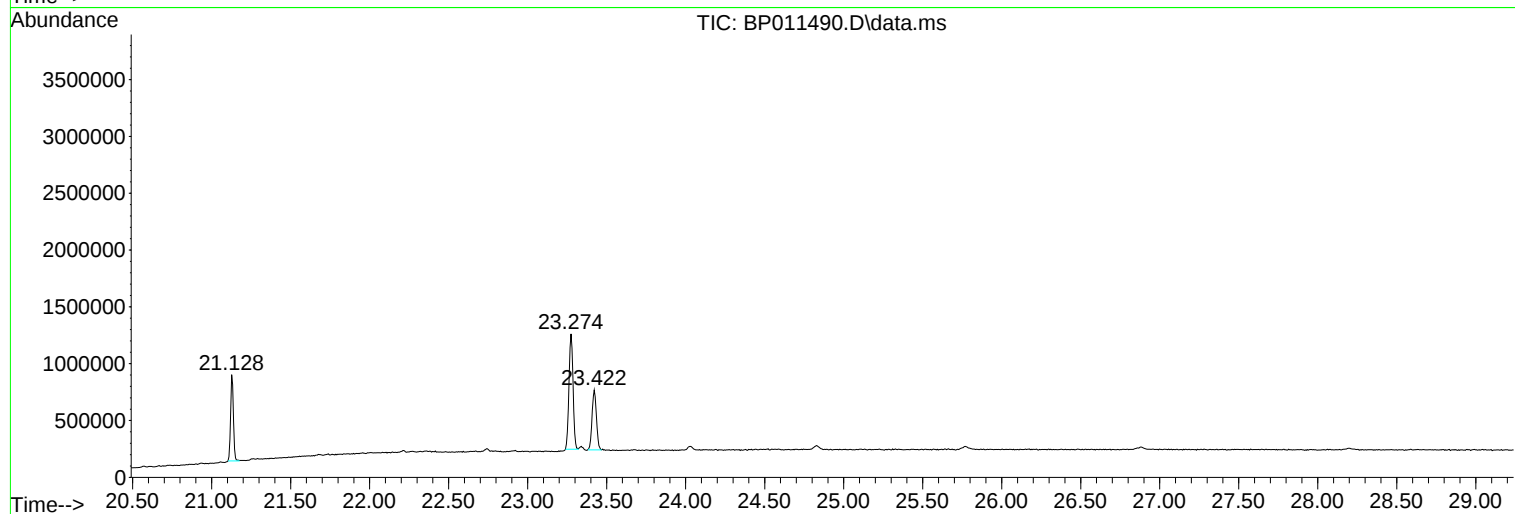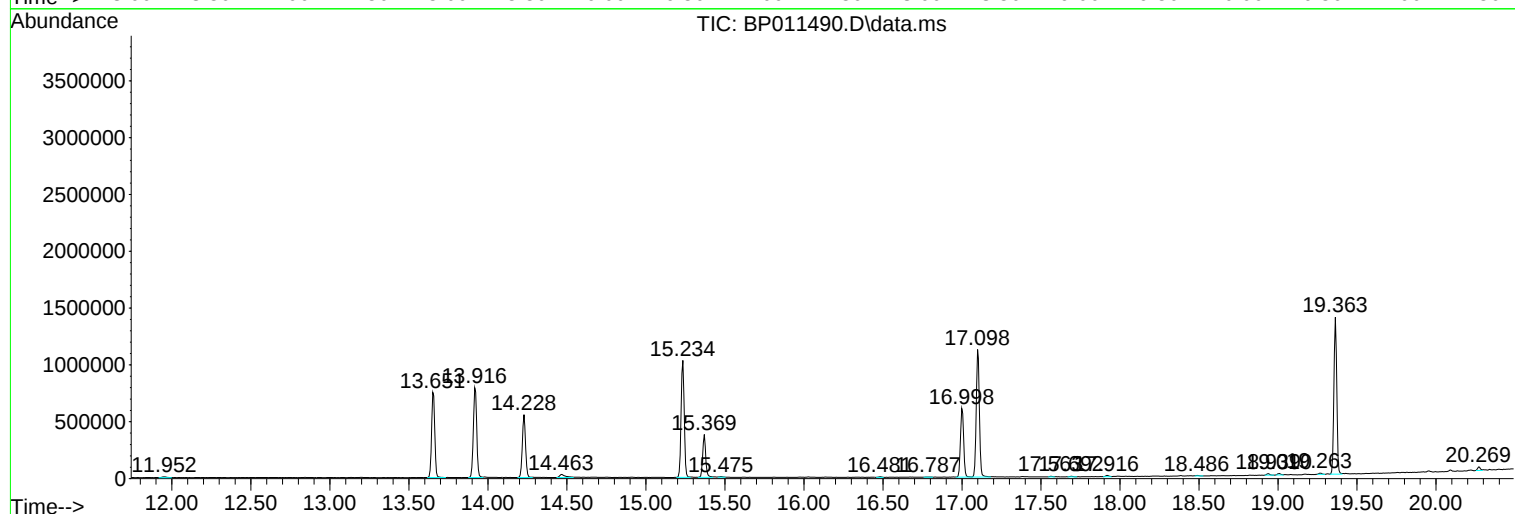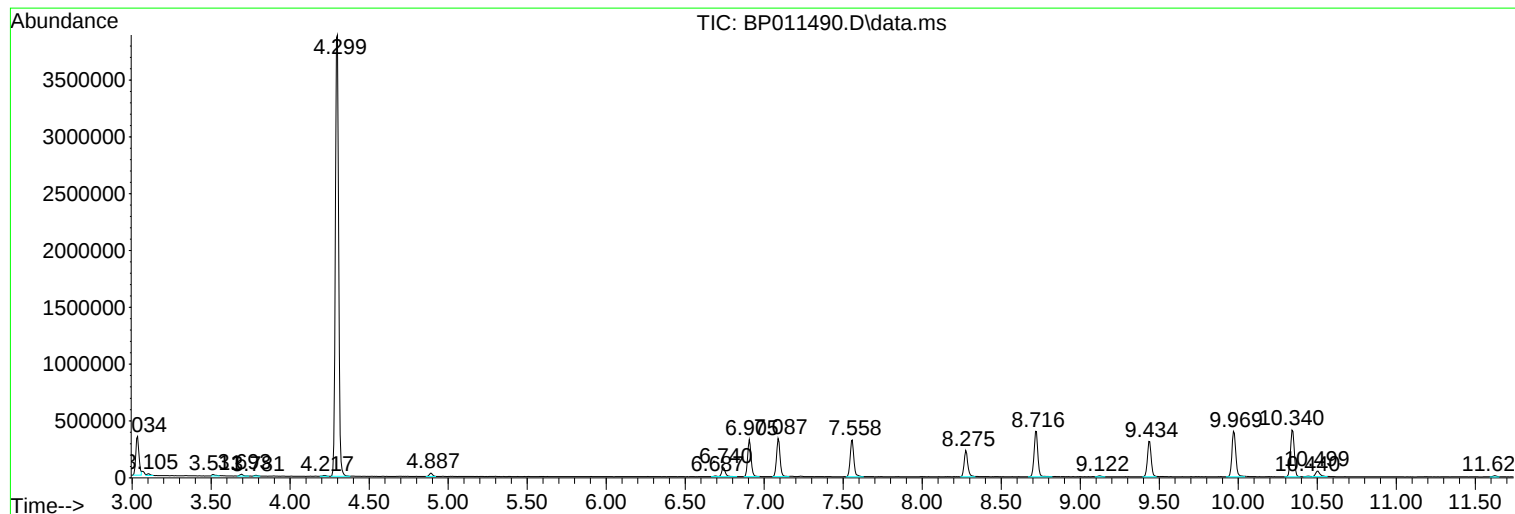

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081822\
Data File : BP011490.D
Acq On : 18 Aug 2022 19:49
Operator : CG/JU
Sample : N4221-18
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0KP0

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP081622.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081822\
Data File : BP011490.D
Acq On : 18 Aug 2022 19:49
Operator : CG/JU
Sample : N4221-18
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0KP0

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP081622.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc