

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081822\
 Data File : BP011491.D
 Acq On : 18 Aug 2022 20:23
 Operator : CG/JU
 Sample : N4221-20
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0KP6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP081622.M
 Title : SVOA CALIBRATION

Signal : TIC: BP011491.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.070	10	14	22	rVB	23272	29390	1.66%	0.160%
2	3.328	56	58	59	rBV2	2161	1863	0.11%	0.010%
3	3.487	82	85	99	rBV	83543	134433	7.61%	0.733%
4	3.693	115	120	127	rVB	17573	27320	1.55%	0.149%
5	3.781	131	135	141	rVB	11121	16006	0.91%	0.087%
6	4.152	193	198	205	rVB	29806	41323	2.34%	0.225%
7	4.217	205	209	214	rBV	5788	8103	0.46%	0.044%
8	4.293	219	222	226	rBV4	3795	4569	0.26%	0.025%
9	5.081	354	356	359	rBV4	1733	2545	0.14%	0.014%
10	5.128	361	364	369	rVB3	3813	5533	0.31%	0.030%
11	5.434	412	416	421	rBV8	1716	2924	0.17%	0.016%
12	5.511	424	429	436	rVB	7574	11764	0.67%	0.064%
13	5.628	444	449	456	rBV2	26677	42411	2.40%	0.231%
14	6.587	609	612	619	rBV8	1855	4043	0.23%	0.022%
15	6.740	623	638	646	rBV2	71338	145650	8.25%	0.794%
16	6.905	660	666	677	rBV	316765	474833	26.89%	2.590%
17	7.005	681	683	686	rBV4	1367	1868	0.11%	0.010%
18	7.087	690	697	709	rBV	315295	477551	27.04%	2.605%
19	7.258	724	726	731	rVB6	2276	3207	0.18%	0.017%
20	7.552	769	776	784	rBV	338867	540222	30.59%	2.947%
21	7.628	784	789	800	rVB	27915	47310	2.68%	0.258%
22	7.769	811	813	817	rVB5	1673	1940	0.11%	0.011%
23	7.822	819	822	823	rBV3	1691	1873	0.11%	0.010%
24	8.175	878	882	890	rVB10	3057	5983	0.34%	0.033%
25	8.275	892	899	909	rBV	198324	325274	18.42%	1.774%
26	8.387	914	918	924	rVB4	5546	9629	0.55%	0.053%
27	8.658	959	964	968	rBV	15023	23502	1.33%	0.128%
28	8.716	968	974	982	rVV	383791	620550	35.14%	3.385%
29	8.775	982	984	988	rVB5	2792	3575	0.20%	0.020%
30	8.887	997	1003	1020	rBV	135163	232782	13.18%	1.270%
31	9.116	1039	1042	1043	rBV3	1995	1999	0.11%	0.011%
32	9.434	1089	1096	1102	rBV	288058	460138	26.05%	2.510%
33	9.481	1102	1104	1112	rVB	18813	27032	1.53%	0.147%
34	9.628	1125	1129	1133	rVB6	1923	2415	0.14%	0.013%
35	9.775	1148	1154	1161	rVB6	1740	3639	0.21%	0.020%
36	9.840	1161	1165	1167	rBV5	1510	2224	0.13%	0.012%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081822\
 Data File : BP011491.D
 Acq On : 18 Aug 2022 20:23
 Operator : CG/JU
 Sample : N4221-20
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0KP6

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0.1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP081622.M
 Title : SVOA CALIBRATION

37	9.969	1179	1187	1204	rBV	387200	639285	36.20%	3.487%
38	10.116	1208	1212	1213	rVV4	1817	2160	0.12%	0.012%
39	10.140	1213	1216	1220	rVB5	2847	4065	0.23%	0.022%
40	10.216	1225	1229	1233	rBV6	2555	3311	0.19%	0.018%
41	10.269	1233	1238	1244	rBV7	5194	9436	0.53%	0.051%
42	10.340	1244	1250	1257	rVB	427167	694632	39.33%	3.789%
43	10.410	1257	1262	1268	rVB3	12109	19398	1.10%	0.106%
44	10.493	1268	1276	1292	rBV	355795	627587	35.54%	3.423%
45	10.904	1344	1346	1350	rVB4	2029	2112	0.12%	0.012%
46	10.963	1354	1356	1361	rVV6	1867	2971	0.17%	0.016%
47	11.022	1363	1366	1374	rVB8	2064	3434	0.19%	0.019%
48	11.169	1384	1391	1394	rBV7	5490	9738	0.55%	0.053%
49	11.540	1451	1454	1457	rBV4	1784	2562	0.15%	0.014%
50	11.628	1463	1469	1470	rBV3	3704	5710	0.32%	0.031%
51	11.663	1470	1475	1484	rVB	33746	61788	3.50%	0.337%
52	11.769	1491	1493	1501	rVB9	1326	2762	0.16%	0.015%
53	11.875	1507	1511	1513	rBV5	1544	2109	0.12%	0.012%
54	11.946	1519	1523	1530	rVB2	7695	13346	0.76%	0.073%
55	12.293	1580	1582	1586	rVV4	1806	2277	0.13%	0.012%
56	12.451	1608	1609	1614	rVB5	1417	1790	0.10%	0.010%
57	12.522	1614	1621	1625	rBV7	5145	9829	0.56%	0.054%
58	12.575	1625	1630	1633	rBV6	3140	5056	0.29%	0.028%
59	12.834	1667	1674	1678	rBV3	8476	12477	0.71%	0.068%
60	13.163	1721	1730	1740	rBV4	12511	31808	1.80%	0.174%
61	13.481	1778	1784	1787	rBV8	1487	2407	0.14%	0.013%
62	13.651	1807	1813	1823	rBV	697259	958217	54.26%	5.227%
63	13.916	1851	1858	1867	rBV	776749	1094773	61.99%	5.972%
64	14.228	1904	1911	1920	rBV	550889	779391	44.13%	4.251%
65	14.322	1924	1927	1932	rVB3	6985	9147	0.52%	0.050%
66	14.469	1946	1952	1964	rBV3	17684	45645	2.58%	0.249%
67	14.681	1984	1988	1992	rVB6	2747	4877	0.28%	0.027%
68	14.787	2002	2006	2009	rVB5	1507	1874	0.11%	0.010%
69	14.922	2024	2029	2037	rBV	21368	35382	2.00%	0.193%
70	14.998	2037	2042	2046	rVB2	5822	8415	0.48%	0.046%
71	15.057	2047	2052	2058	rVB6	5910	12443	0.70%	0.068%
72	15.234	2075	2082	2095	rBV	951292	1340382	75.89%	7.311%
73	15.369	2099	2105	2116	rVV2	113777	187131	10.60%	1.021%
74	15.475	2120	2123	2128	rVV7	6861	15724	0.89%	0.086%
75	15.522	2128	2131	2139	rVV8	7586	12922	0.73%	0.070%
76	15.616	2143	2147	2151	rVB5	5998	8409	0.48%	0.046%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081822\
 Data File : BP011491.D
 Acq On : 18 Aug 2022 20:23
 Operator : CG/JU
 Sample : N4221-20
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0KP6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP081622.M
 Title : SVOA CALIBRATION

77	15.816	2177	2181	2184	rBV6	3048	4149	0.23%	0.023%
78	15.857	2184	2188	2193	rVB8	2912	4828	0.27%	0.026%
79	16.098	2223	2229	2232	rBV7	1829	2663	0.15%	0.015%
80	16.134	2232	2235	2242	rVV9	1905	4051	0.23%	0.022%
81	16.604	2312	2315	2319	rVB6	3579	4256	0.24%	0.023%
82	16.775	2341	2344	2353	rVB9	3377	6226	0.35%	0.034%
83	16.957	2369	2375	2376	rBV5	2936	4996	0.28%	0.027%
84	16.998	2376	2382	2392	rVB	593530	807977	45.75%	4.407%
85	17.098	2392	2399	2413	rBV	1107919	1527395	86.48%	8.332%
86	17.216	2417	2419	2423	rVB5	4538	5330	0.30%	0.029%
87	17.310	2432	2435	2438	rBV2	3346	3104	0.18%	0.017%
88	17.686	2494	2499	2505	rBV	223827	272642	15.44%	1.487%
89	17.857	2524	2528	2531	rBV5	4515	5909	0.33%	0.032%
90	17.916	2534	2538	2542	rBV7	9307	13336	0.76%	0.073%
91	17.992	2547	2551	2558	rVV2	9448	19862	1.12%	0.108%
92	18.157	2576	2579	2583	rVB5	4592	5644	0.32%	0.031%
93	18.345	2608	2611	2615	rBV6	2110	3676	0.21%	0.020%
94	18.757	2677	2681	2684	rVB6	4286	6265	0.35%	0.034%
95	18.933	2708	2711	2716	rBV2	13640	17561	0.99%	0.096%
96	19.010	2720	2724	2727	rVB2	11691	15127	0.86%	0.083%
97	19.363	2778	2784	2793	rBV	1274587	1619666	91.71%	8.835%
98	21.127	3079	3084	3090	rBV	718513	867901	49.14%	4.734%
99	23.274	3442	3449	3456	rBV	956641	1766105	100.00%	9.634%
100	23.421	3468	3474	3481	rVB2	479600	911652	51.62%	4.973%




Sum of corrected areas: 18332526

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081822\
Data File : BP011491.D
Acq On : 18 Aug 2022 20:23
Operator : CG/JU
Sample : N4221-20
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0KP6

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP081622.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

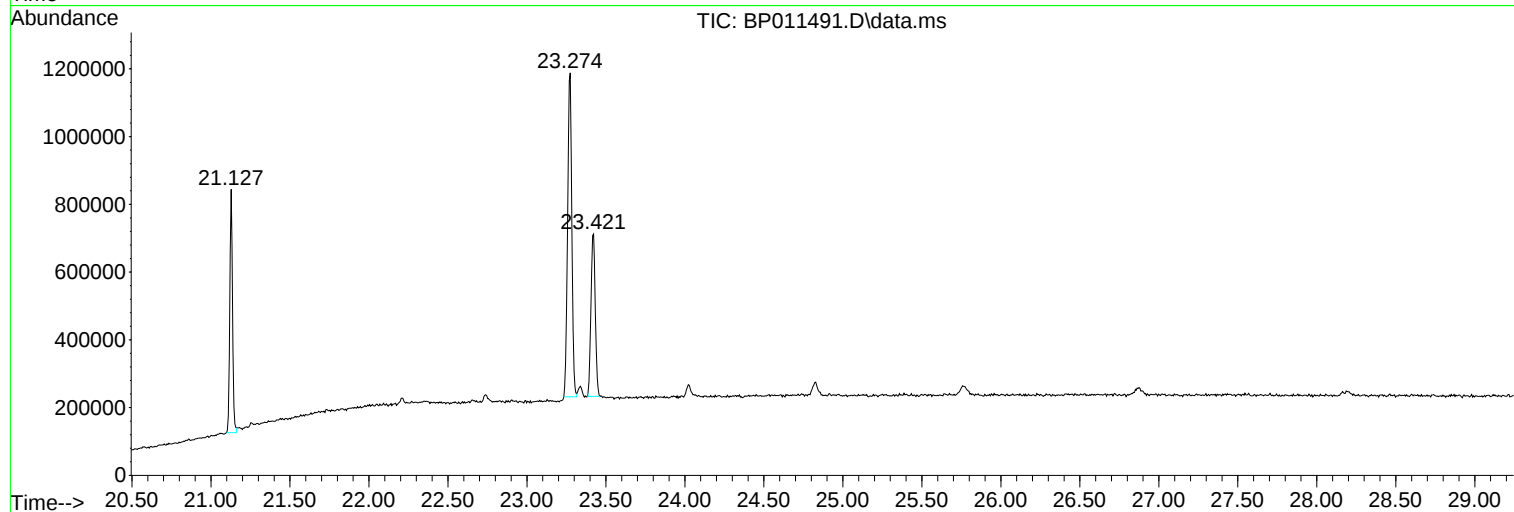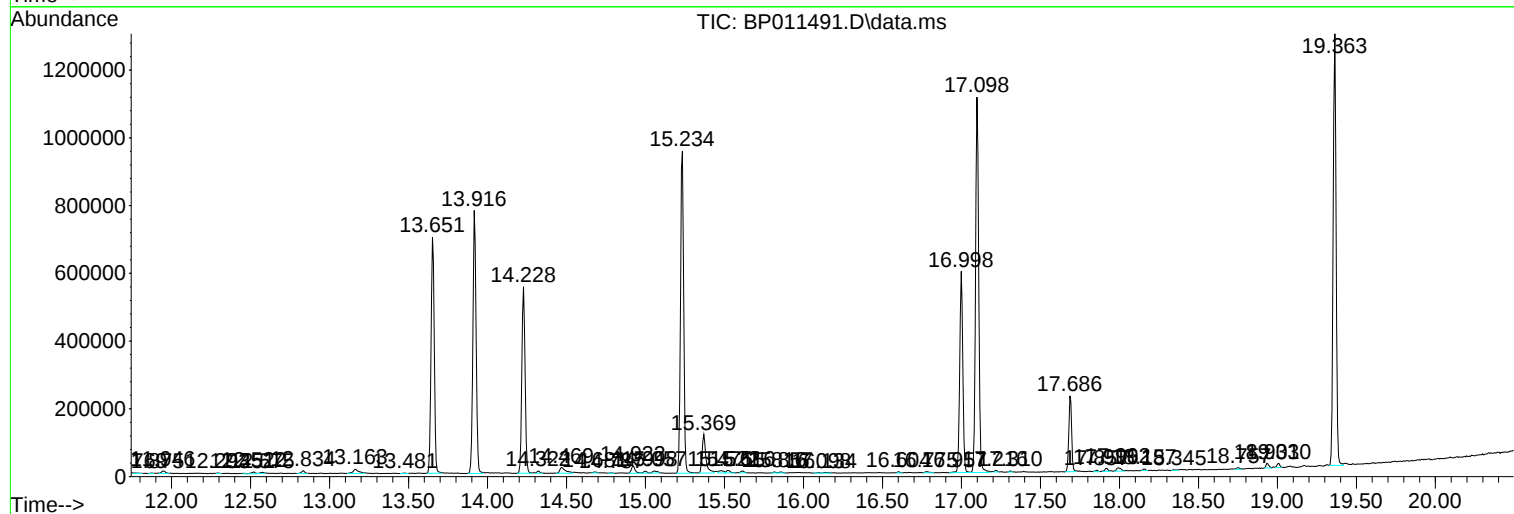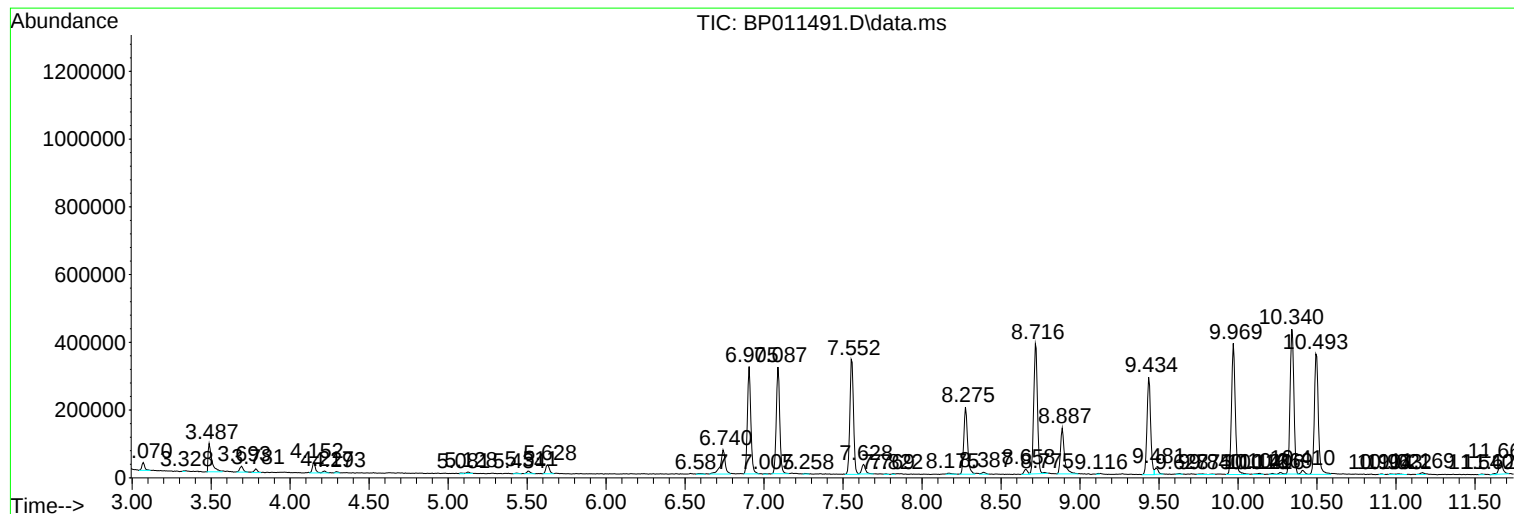

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081822\
Data File : BP011491.D
Acq On : 18 Aug 2022 20:23
Operator : CG/JU
Sample : N4221-20
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0KP6










Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP081622.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Ethanol, 2-(hexyloxy)- Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
8.887	8.62 ng/ul	232782	1,4-Dichlorobenzene-d4	7.558

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Ethanol, 2-(hexyloxy)-	146	C8H18O2	000112-25-4	78
2			Ethanol, 2-(hexyloxy)-	146	C8H18O2	000112-25-4	72
3			Ethanol, 2-(hexyloxy)-	146	C8H18O2	000112-25-4	40
4			1-Chloro-3-(hexyloxy)-2-propanol	194	C9H19ClO2	016224-24-1	32
5			Piperazine, 1-nitroso-	115	C4H9N3O	005632-47-3	27

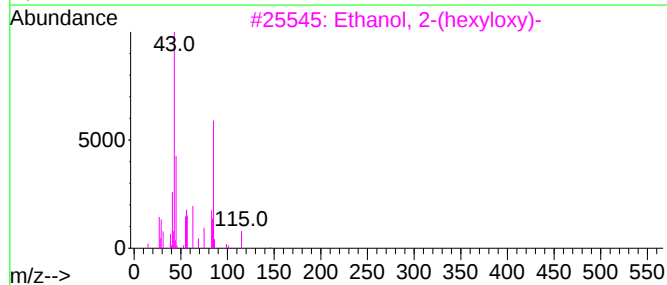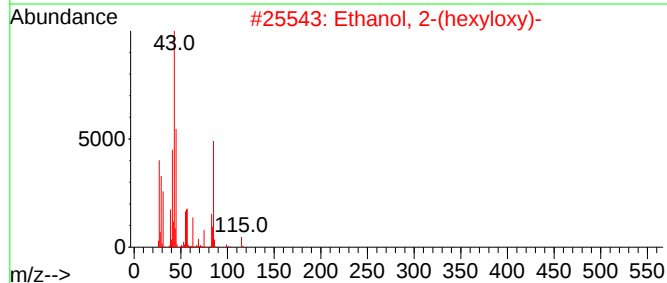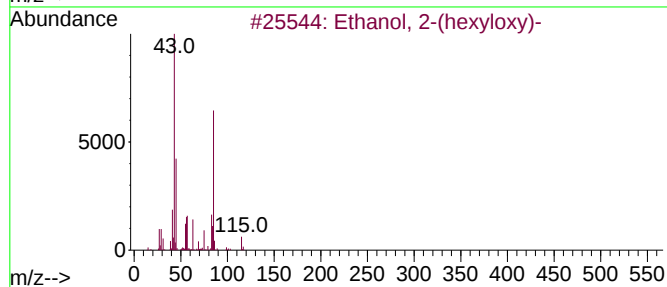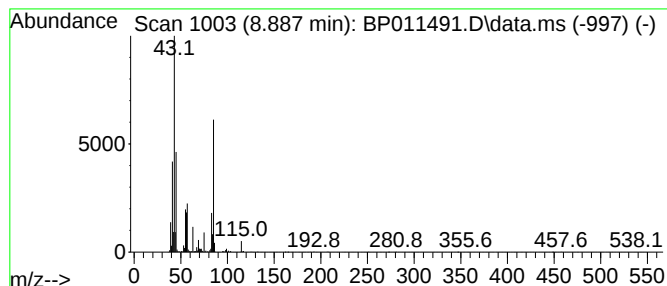

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081822\
Data File : BP011491.D
Acq On : 18 Aug 2022 20:23
Operator : CG/JU
Sample : N4221-20
Misc :
ALS Vial : 16 Sample Multiplier: 1










Instrument :
BNA_P
ClientSampleId :
C0KP6

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP081622.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 2 7,9-Di-tert-butyl-1-oxaspiro... Concentration Rank 2

R.T.	EstConc	Area	Relative to ISTD	R.T.	
17.686	6.75 ng/ul	272642	Phenanthrene-d10	16.998	
Hit# of 5	Tentative ID	MW	MolForm	CAS#	Qual
1	7,9-Di-tert-butyl-1-oxaspiro(4,5...	276	C17H24O3	082304-66-3	99
2	7,9-Di-tert-butyl-1-oxaspiro(4,5...	276	C17H24O3	082304-66-3	83
3	7,9-Di-tert-butyl-1-oxaspiro(4,5...	276	C17H24O3	082304-66-3	68
4	1-(3-Amino-4,6-dimethylthieno[2,...	220	C11H12N2OS	052505-42-7	45
5	(1R,3aR,5aR,9aS)-1,4,4,7-Tetrame...	220	C15H24O	104188-25-2	42

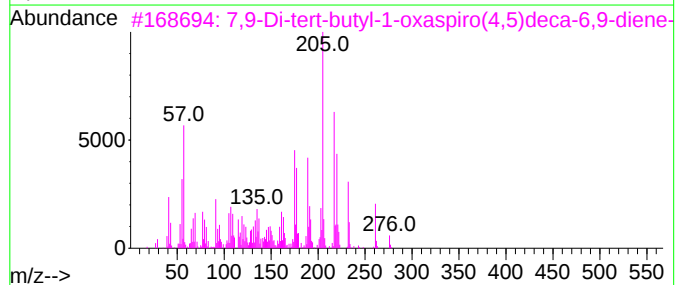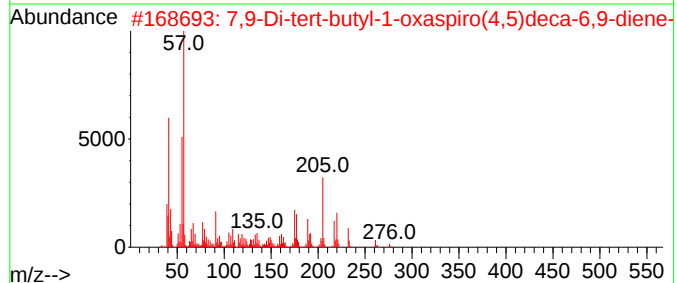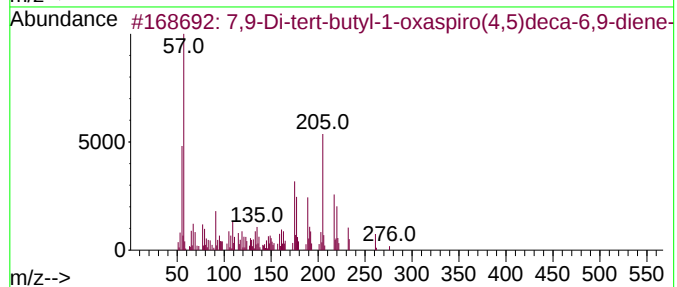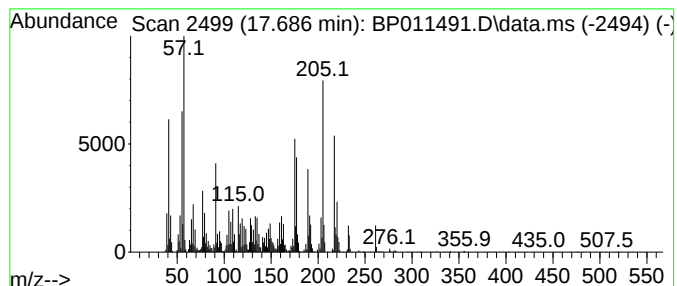

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081822\
Data File : BP011491.D
Acq On : 18 Aug 2022 20:23
Operator : CG/JU
Sample : N4221-20
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0KP6

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP081622.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Ethanol, 2-(hex...	8.887	8.6	ng/ul	232782	1	7.558	540222	20.0
7,9-Di-tert-but...	17.686	6.8	ng/ul	272642	4	16.998	807977	20.0