

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081822\
 Data File : BP011495.D
 Acq On : 18 Aug 2022 23:15
 Operator : CG/JU
 Sample : PB147098BL
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK098

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP081622.M
 Title : SVOA CALIBRATION

Signal : TIC: BP011495.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.069	10	14	24	rVB	36442	48233	2.82%	0.212%
2	3.475	80	83	102	rBV	406147	624505	36.55%	2.750%
3	3.781	132	135	143	rVB2	10547	15824	0.93%	0.070%
4	6.740	631	638	650	rBV	468923	708694	41.47%	3.120%
5	6.905	660	666	677	rVB	347579	520667	30.47%	2.292%
6	7.087	690	697	708	rBV	479855	719531	42.11%	3.168%
7	7.552	768	776	790	rBV	443231	706330	41.34%	3.110%
8	8.275	892	899	912	rBV	519967	829609	48.55%	3.653%
9	8.716	966	974	988	rBV	427700	692477	40.53%	3.049%
10	9.434	1089	1096	1107	rBV	357810	578827	33.87%	2.548%
11	9.969	1180	1187	1198	rBV	488474	800362	46.84%	3.524%
12	10.340	1243	1250	1265	rVB	588432	944655	55.28%	4.159%
13	10.493	1269	1276	1297	rVV	460810	817907	47.87%	3.601%
14	10.622	1297	1298	1303	rVB4	2312	2017	0.12%	0.009%
15	11.181	1390	1393	1400	rBV9	1062	1775	0.10%	0.008%
16	11.951	1518	1524	1532	rBV4	6829	12103	0.71%	0.053%
17	12.945	1689	1693	1697	rVB7	1411	2052	0.12%	0.009%
18	13.198	1730	1736	1738	rBV7	2062	2734	0.16%	0.012%
19	13.651	1806	1813	1825	rBV	831819	1099044	64.32%	4.839%
20	13.769	1830	1833	1838	rVB6	1390	2234	0.13%	0.010%
21	13.916	1851	1858	1871	rBV	866578	1210433	70.84%	5.329%
22	14.092	1885	1888	1893	rVB7	1282	1807	0.11%	0.008%
23	14.228	1904	1911	1921	rBV	787149	1099371	64.34%	4.840%
24	14.363	1930	1934	1937	rBV6	1008	1905	0.11%	0.008%
25	14.457	1941	1950	1967	rBV	309376	547532	32.04%	2.411%
26	14.675	1985	1987	1992	rVB6	1883	2352	0.14%	0.010%
27	15.228	2075	2081	2094	rBV	1011999	1456887	85.26%	6.414%
28	15.369	2098	2105	2117	rBV	371051	528394	30.92%	2.326%
29	15.475	2120	2123	2128	rVB5	5277	7077	0.41%	0.031%
30	15.581	2136	2141	2143	rBV6	1476	2059	0.12%	0.009%
31	15.804	2175	2179	2181	rBV5	1735	2195	0.13%	0.010%
32	16.028	2213	2217	2219	rVB5	1480	1859	0.11%	0.008%
33	16.675	2322	2327	2330	rBV7	1758	3160	0.18%	0.014%
34	16.780	2340	2345	2353	rVB8	3859	7183	0.42%	0.032%
35	16.998	2376	2382	2393	rBV	891936	1203730	70.44%	5.300%
36	17.098	2393	2399	2409	rBV	1183933	1566561	91.68%	6.897%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081822\
Data File : BP011495.D
Acq On : 18 Aug 2022 23:15
Operator : CG/JU
Sample : PB147098BL
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK098

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP081622.M
Title : SVOA CALIBRATION

37	17.298	2431	2433	2438	rBV6	1090	1775	0.10%	0.008%
38	17.686	2496	2499	2508	rBV6	1741	3885	0.23%	0.017%
39	18.310	2603	2605	2608	rVB3	1592	1881	0.11%	0.008%
40	18.933	2708	2711	2717	rVB3	11849	14426	0.84%	0.064%
41	19.004	2719	2723	2727	rBV2	13527	19799	1.16%	0.087%
42	19.363	2778	2784	2792	rBV	1284920	1655985	96.91%	7.291%
43	21.127	3079	3084	3093	rBV	1016103	1248896	73.09%	5.499%
44	23.274	3442	3449	3456	rBV	922309	1708759	100.00%	7.523%
45	23.421	3468	3474	3483	rVB2	685571	1285496	75.23%	5.660%




Sum of corrected areas: 22712987

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081822\
Data File : BP011495.D
Acq On : 18 Aug 2022 23:15
Operator : CG/JU
Sample : PB147098BL
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK098

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP081622.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

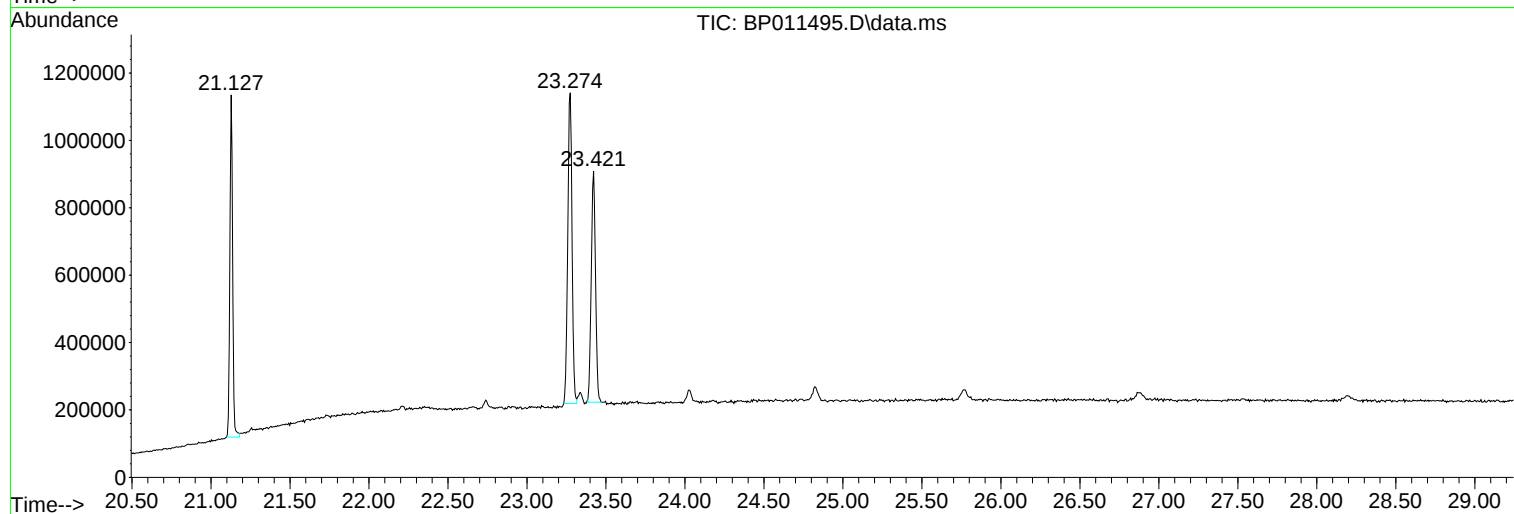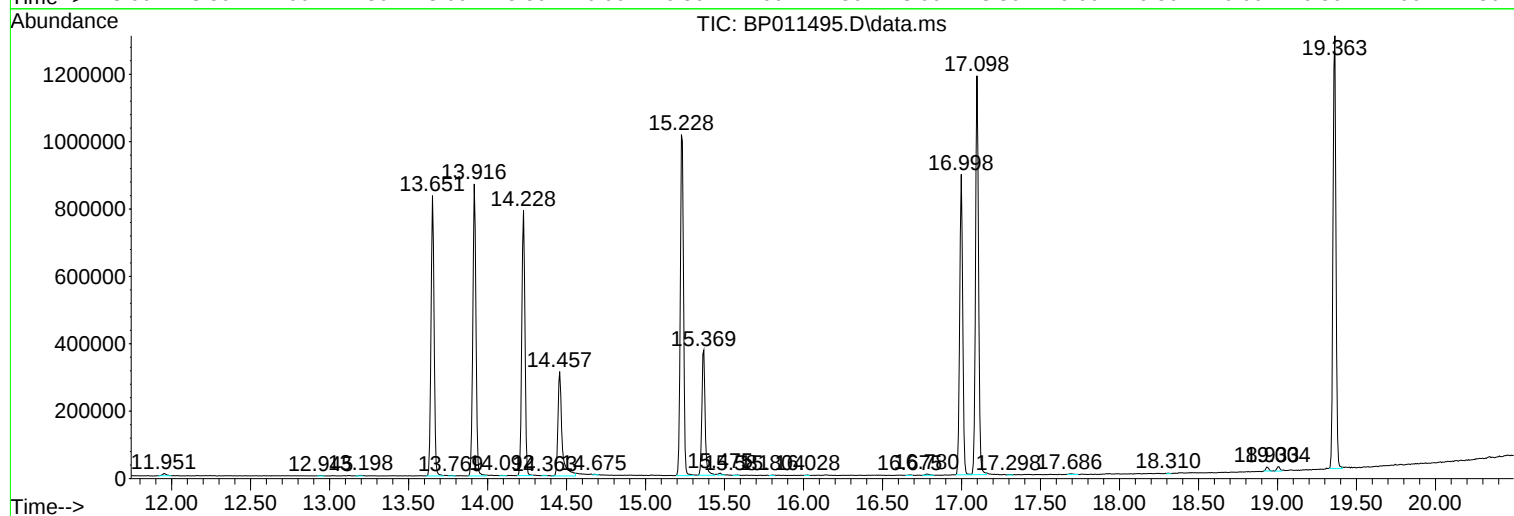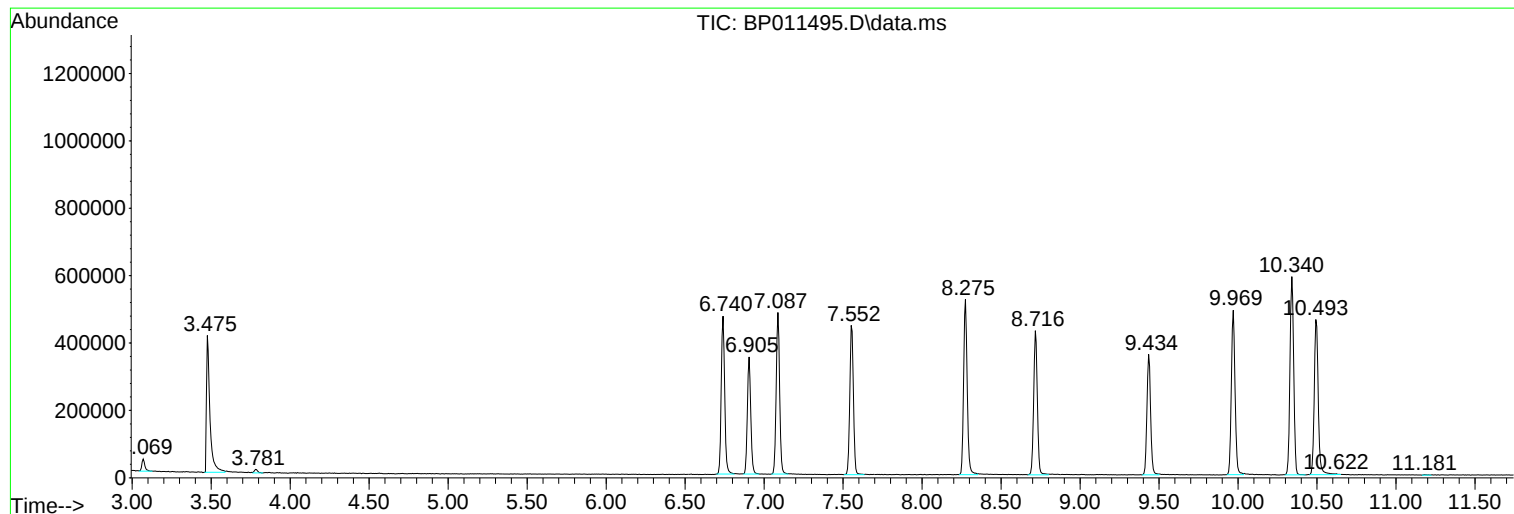

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081822\
Data File : BP011495.D
Acq On : 18 Aug 2022 23:15
Operator : CG/JU
Sample : PB147098BL
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK098

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP081622.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081822\
Data File : BP011495.D
Acq On : 18 Aug 2022 23:15
Operator : CG/JU
Sample : PB147098BL
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK098

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP081622.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc