

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081825\
 Data File : BP025458.D
 Acq On : 18 Aug 2025 12:47
 Operator : CG/JU
 Sample : Q2864-01
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 LAW-25-122-126

Quant Time: Aug 18 13:09:23 2025
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP081425.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Aug 14 18:14:31 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.784	152	128442	20.000	ng	-0.01
21) Naphthalene-d8	10.555	136	492363	20.000	ng	0.00
39) Acenaphthene-d10	14.401	164	296040	20.000	ng	0.00
64) Phenanthrene-d10	17.195	188	610617	20.000	ng	0.00
76) Chrysene-d12	21.625	240	702047	20.000	ng	-0.02
86) Perylene-d12	24.989	264	838587	20.000	ng	-0.04
System Monitoring Compounds						
5) 2-Fluorophenol	5.408	112	472023	61.030	ng	0.00
7) Phenol-d6	6.961	99	370036	37.317	ng	0.00
23) Nitrobenzene-d5	8.925	82	815714	83.807	ng	-0.01
42) 2,4,6-Tribromophenol	15.907	330	530008	133.010	ng	0.00
45) 2-Fluorobiphenyl	13.013	172	1726000	79.682	ng	0.00
79) Terphenyl-d14	19.919	244	2831902	73.801	ng	0.00
Target Compounds						
80) Butylbenzylphthalate	20.642	149	249604	12.070	ng	Qvalue 98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081825\
Data File : BP025458.D
Acq On : 18 Aug 2025 12:47
Operator : CG/JU
Sample : Q2864-01
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
LAW-25-122-126

Quant Time: Aug 18 13:09:23 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP081425.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Aug 14 18:14:31 2025
Response via : Initial Calibration




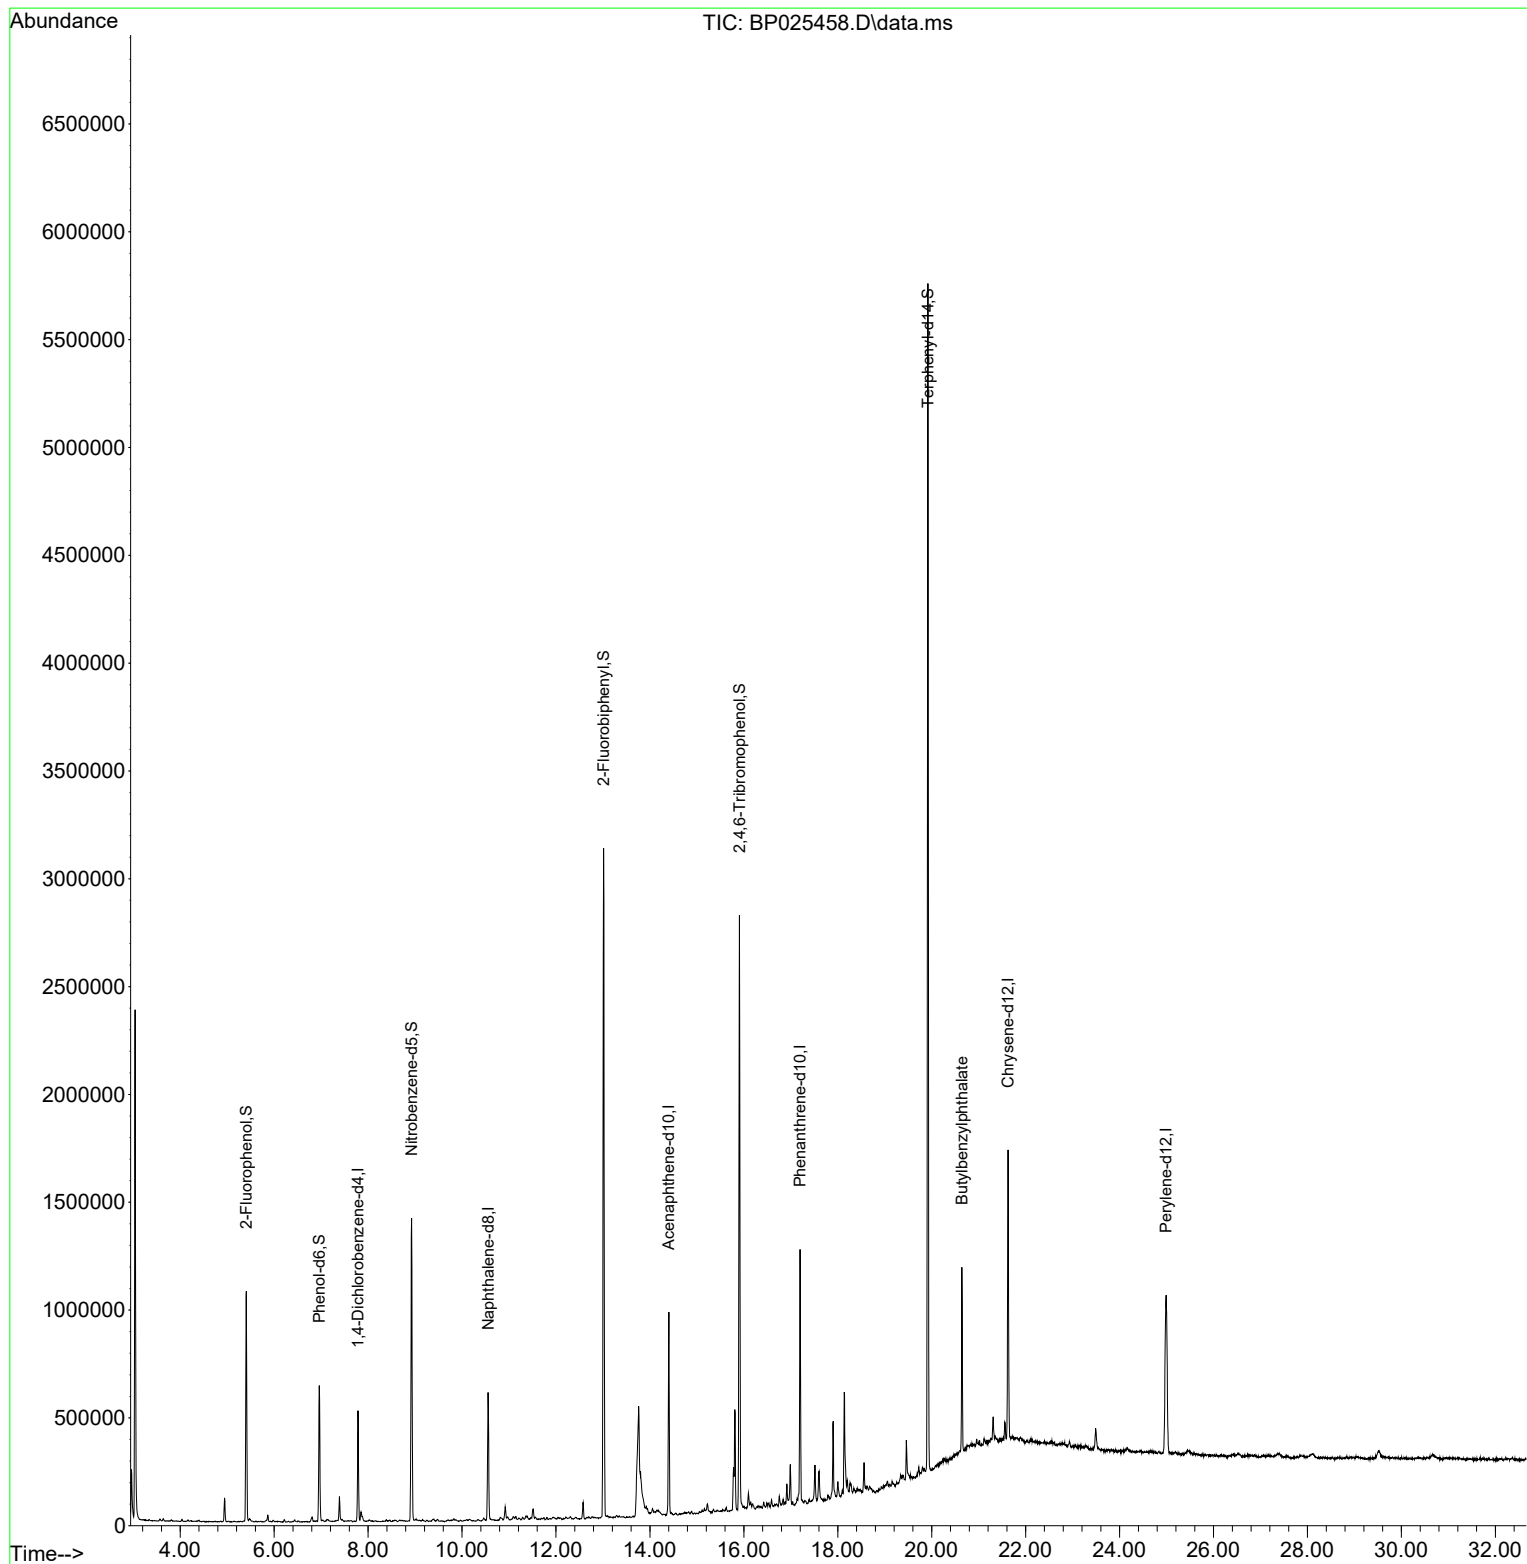




#1
 1,4-Dichlorobenzene-d4
 Concen: 20.000 ng
 RT: 7.784 min Scan# 81
 Delta R.T. -0.012 min
 Lab File: BP025458.D
 Acq: 18 Aug 2025 12:47




Instrument :
 BNA_P
 ClientSampleId :
 LAW-25-122-126


Tgt Ion:152 Resp: 128442
 Ion Ratio Lower Upper
 152 100
 150 157.2 125.9 188.9
 115 61.6 48.5 72.7

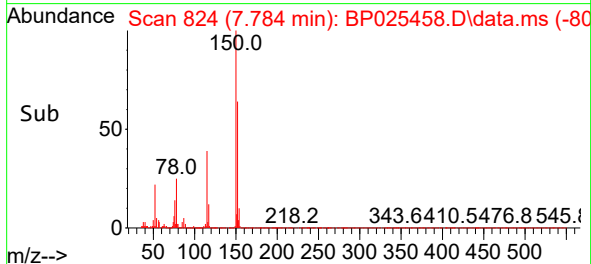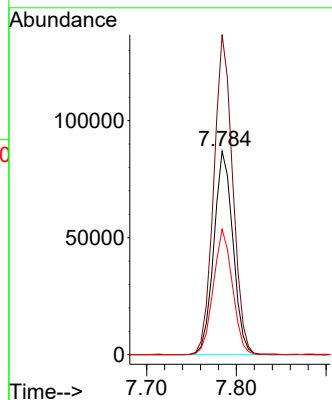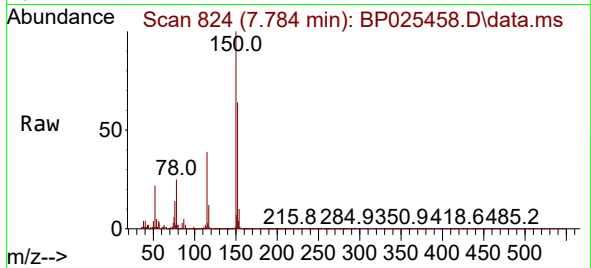

#5
 2-Fluorophenol
 Concen: 61.030 ng
 RT: 5.408 min Scan# 420
 Delta R.T. 0.000 min
 Lab File: BP025458.D
 Acq: 18 Aug 2025 12:47

Tgt Ion:112 Resp: 472023
 Ion Ratio Lower Upper
 112 100
 64 56.3 43.8 65.8
 63 30.1 22.7 34.1


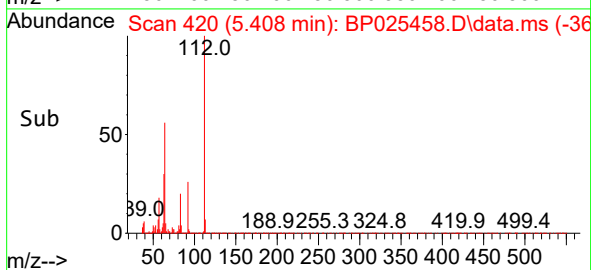
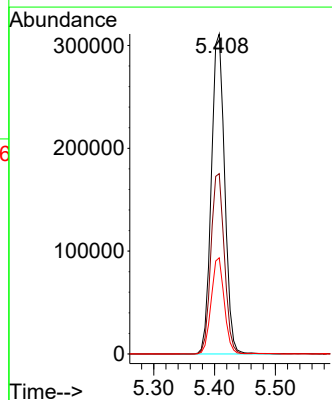
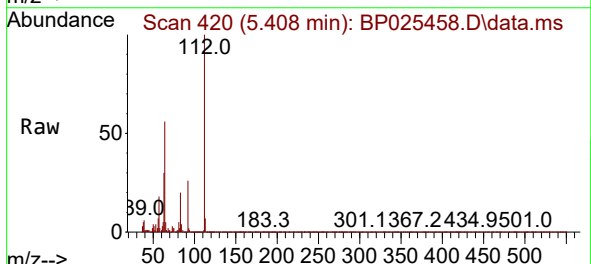




#7
Phenol-d6
Concen: 37.317 ng
RT: 6.961 min Scan# 61
Delta R.T. -0.006 min
Lab File: BP025458.D
Acq: 18 Aug 2025 12:47




Instrument :
BNA_P
ClientSampleId :
LAW-25-122-126


Tgt Ion: 99 Resp: 370036
Ion Ratio Lower Upper
99 100
42 17.7 13.7 20.5
71 33.9 28.2 42.4

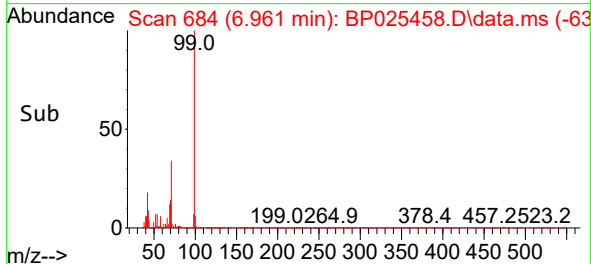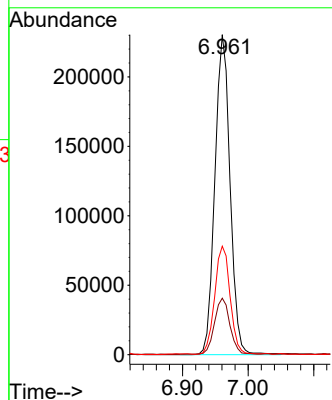

#21
Naphthalene-d8
Concen: 20.000 ng
RT: 10.555 min Scan# 1295
Delta R.T. -0.006 min
Lab File: BP025458.D
Acq: 18 Aug 2025 12:47

Tgt Ion:136 Resp: 492363
Ion Ratio Lower Upper
136 100
137 11.3 9.2 13.8
54 8.1 6.0 9.0
68 5.4 4.3 6.5


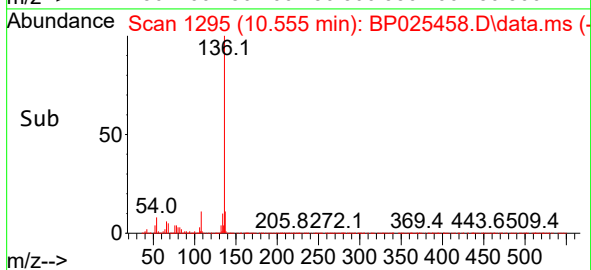
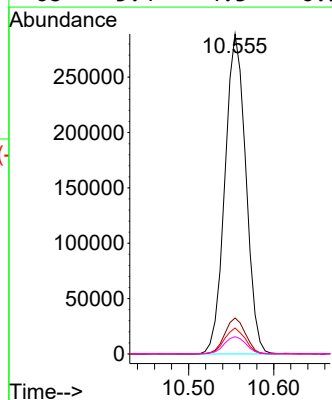
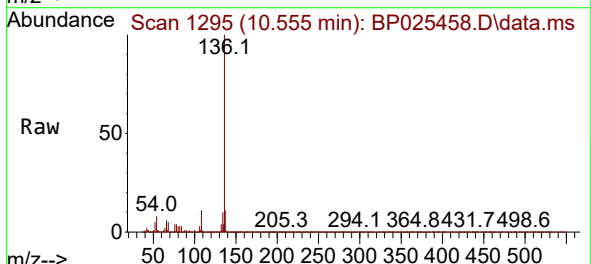




#23
Nitrobenzene-d5
Concen: 83.807 ng
RT: 8.925 min Scan# 1018
Delta R.T. -0.012 min
Lab File: BP025458.D
Acq: 18 Aug 2025 12:47




Instrument :
BNA_P
ClientSampleId :
LAW-25-122-126


Tgt Ion: 82 Resp: 815714
Ion Ratio Lower Upper
82 100
128 45.4 37.7 56.5
54 51.1 39.8 59.6

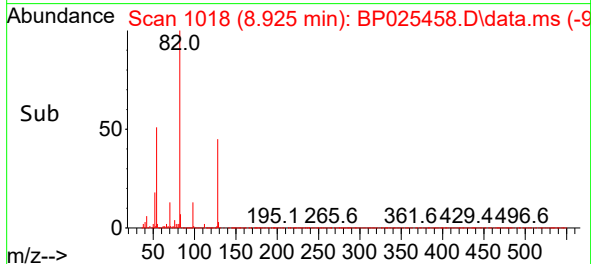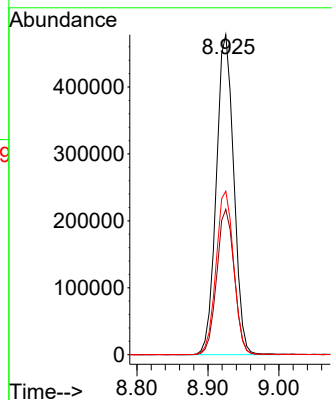

#39
Acenaphthene-d10
Concen: 20.000 ng
RT: 14.401 min Scan# 1949
Delta R.T. -0.006 min
Lab File: BP025458.D
Acq: 18 Aug 2025 12:47

Tgt Ion:164 Resp: 296040
Ion Ratio Lower Upper
164 100
162 100.6 81.0 121.6
160 44.6 35.4 53.2


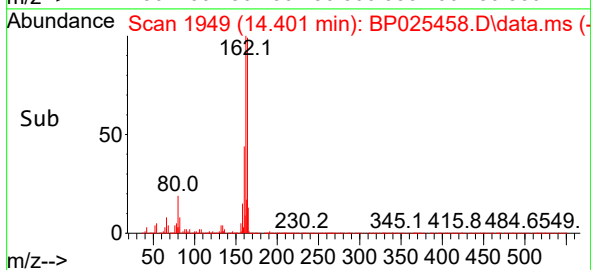
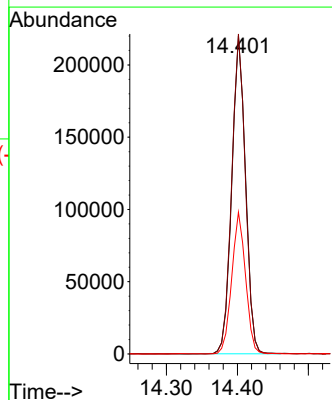
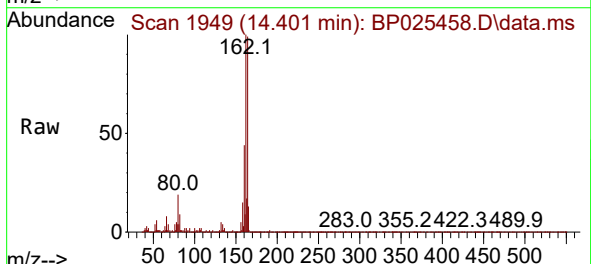




#42
2,4,6-Tribromophenol
Concen: 133.010 ng
RT: 15.907 min Scan# 21
Delta R.T. -0.006 min
Lab File: BP025458.D
Acq: 18 Aug 2025 12:47




Instrument :
BNA_P
ClientSampleId :
LAW-25-122-126


Tgt Ion	330	Resp	530008
Ion Ratio	Lower	Upper	
330	100		
332	97.2	77.3	115.9
141	36.3	26.6	39.8

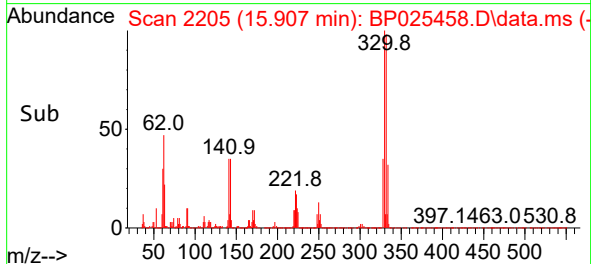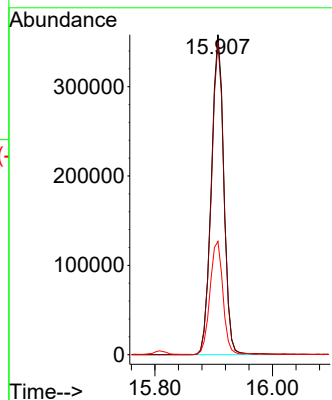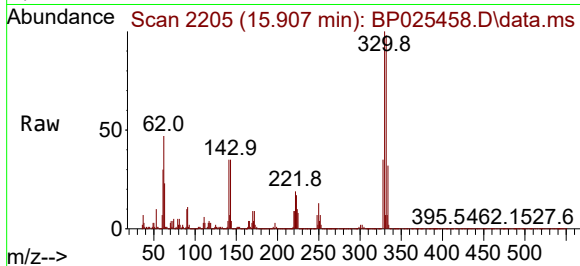

#45
2-Fluorobiphenyl
Concen: 79.682 ng
RT: 13.013 min Scan# 1713
Delta R.T. -0.006 min
Lab File: BP025458.D
Acq: 18 Aug 2025 12:47

Tgt Ion	172	Resp	1726000
Ion Ratio	Lower	Upper	
172	100		
171	34.8	28.1	42.1
170	23.5	18.6	28.0

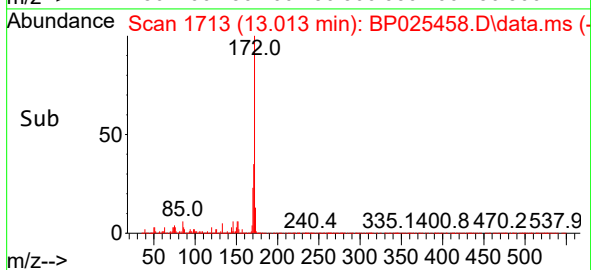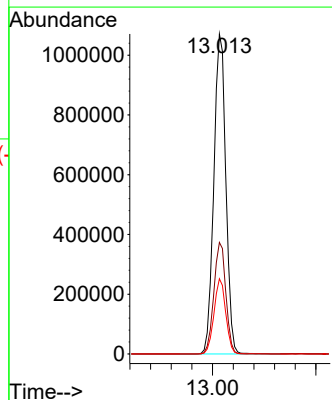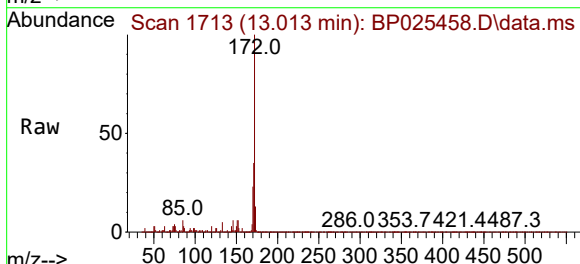

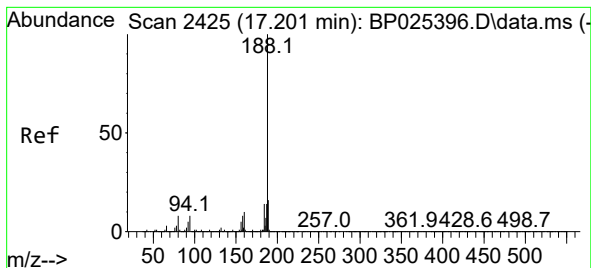

#64

Phenanthrene-d10

Concen: 20.000 ng

RT: 17.195 min Scan# 24

Delta R.T. -0.006 min

Lab File: BP025458.D

Acq: 18 Aug 2025 12:47

Instrument :

BNA_P

ClientSampleId :

LAW-25-122-126





Tgt Ion:188 Resp: 610617

Ion Ratio Lower Upper

188 100

94 8.8 6.6 10.0

80 9.9 6.7 10.1

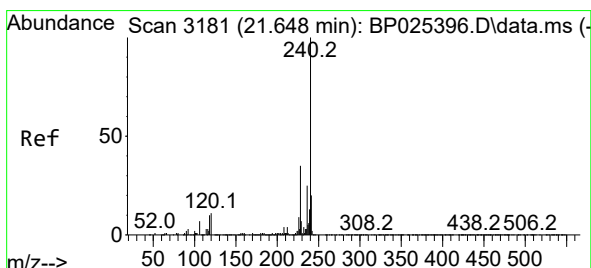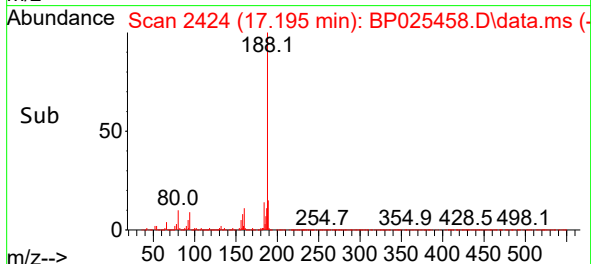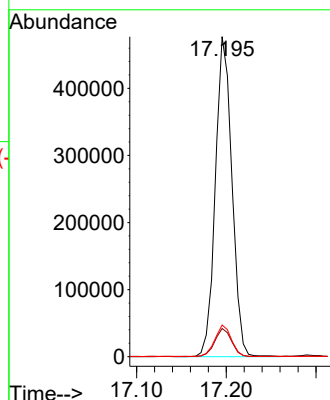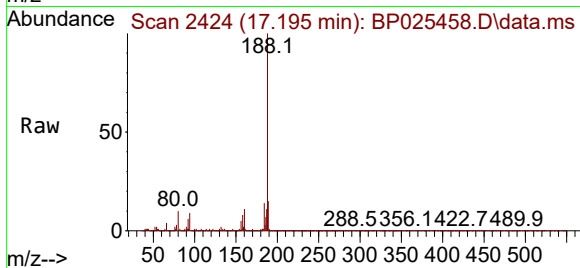

#76

Chrysene-d12

Concen: 20.000 ng

RT: 21.625 min Scan# 3177

Delta R.T. -0.023 min

Lab File: BP025458.D

Acq: 18 Aug 2025 12:47




Tgt Ion:240 Resp: 702047


Ion Ratio Lower Upper

240 100

120 10.6 8.9 13.3

236 25.5 19.8 29.8

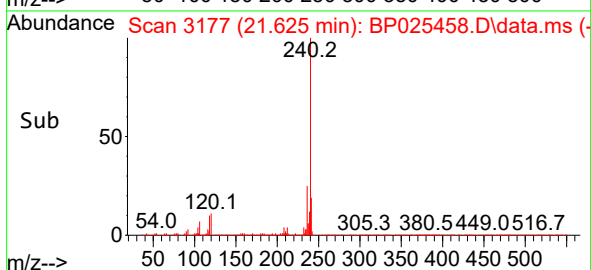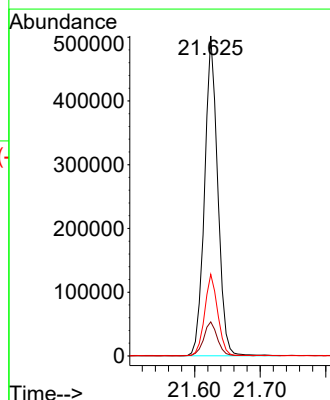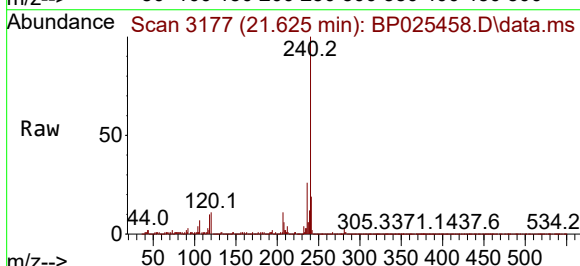

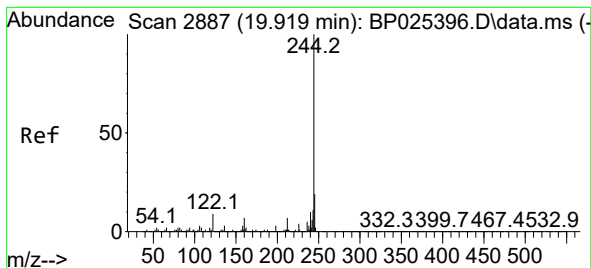

#79

Terphenyl-d14

Concen: 73.801 ng

RT: 19.919 min Scan# 2

Delta R.T. 0.000 min

Lab File: BP025458.D

Acq: 18 Aug 2025 12:47

Instrument :

BNA_P

ClientSampleId :

LAW-25-122-126





Tgt Ion:244 Resp: 2831902

Ion Ratio Lower Upper

244 100

212 7.5 5.8 8.6

122 10.2 7.4 11.2

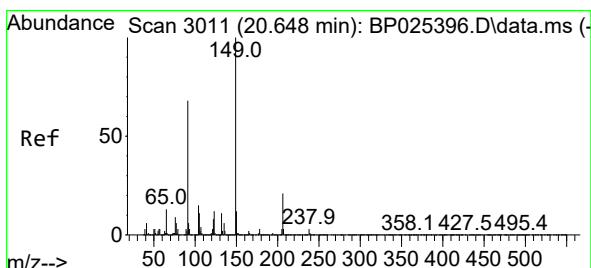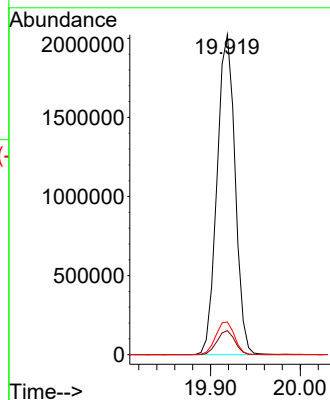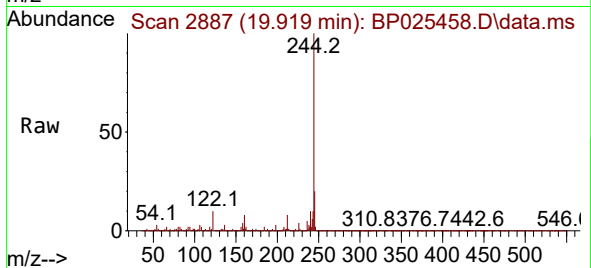

#80

Butylbenzylphthalate

Concen: 12.070 ng

RT: 20.642 min Scan# 3010

Delta R.T. -0.006 min

Lab File: BP025458.D

Acq: 18 Aug 2025 12:47




Tgt Ion:149 Resp: 249604


Ion Ratio Lower Upper

149 100

91 68.9 54.2 81.2

206 19.7 16.6 24.8

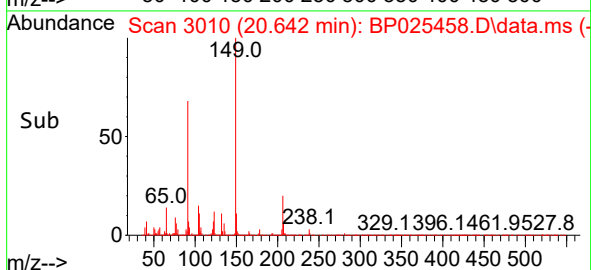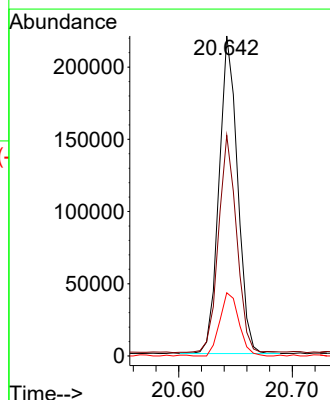

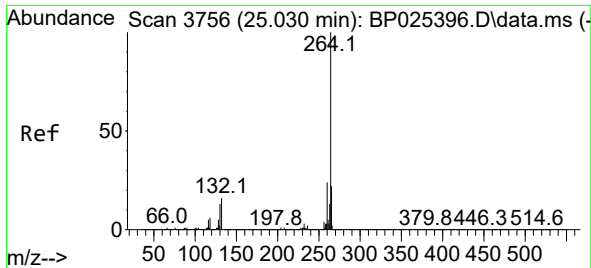

#86
Perylene-d12
Concen: 20.000 ng
RT: 24.989 min Scan# 31
Delta R.T. -0.041 min
Lab File: BP025458.D
Acq: 18 Aug 2025 12:47

Instrument :
BNA_P
ClientSampleId :
LAW-25-122-126

Tgt Ion:264 Resp: 838587

Ion	Ratio	Lower	Upper
264	100		
260	24.2	19.3	28.9
265	22.4	17.4	26.0

