
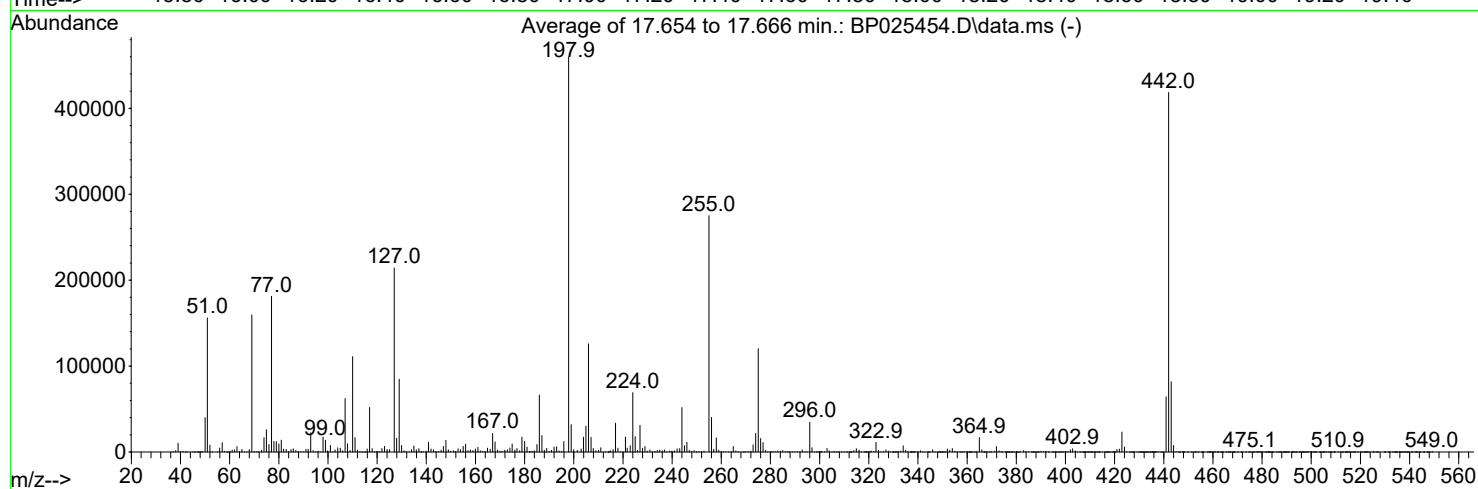


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081825\
Data File : BP025454.D
Acq On : 18 Aug 2025 08:34
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP081425.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Thu Aug 14 18:14:31 2025

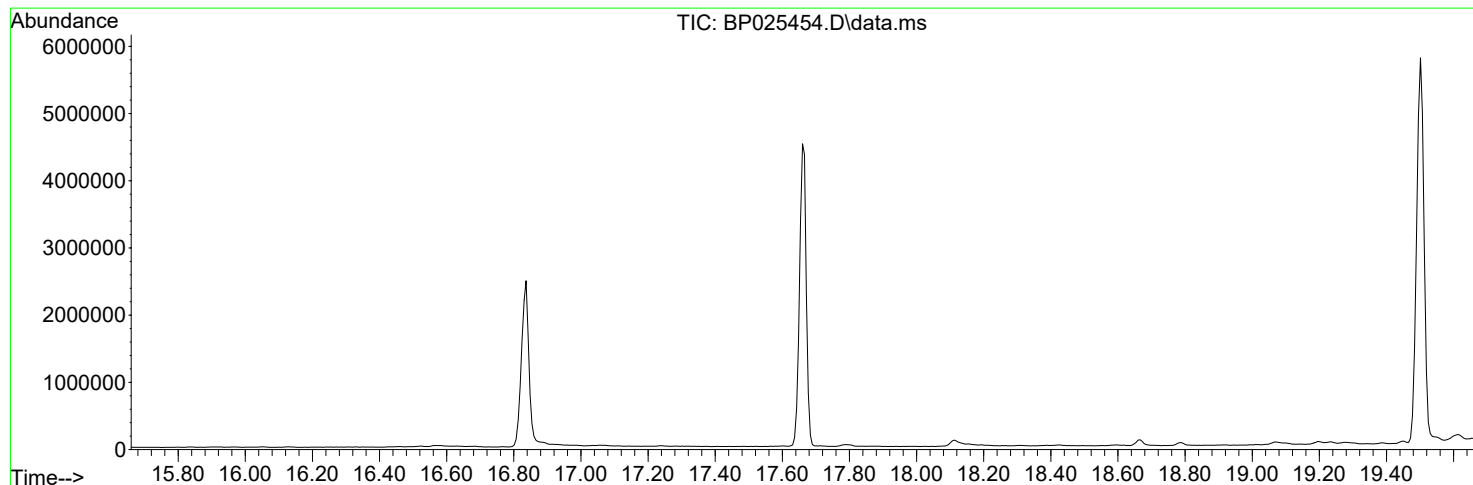

AutoFind: Scans 2502, 2503, 2504; Background Corrected with Scan 2495

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
68	69	0.00	2	1.8	2890	PASS
69	69	100	100	100.0	159655	PASS
70	69	0.00	2	0.4	697	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	459535	PASS
199	198	5	9	6.9	31889	PASS
365	198	1	100	3.6	16720	PASS
441	443	0.01	150	78.6	64292	PASS
442	442	100	100	100.0	418539	PASS
443	442	15	24	19.5	81824	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
8/18/2025	BNA_P	<u>BP025454.D</u>
Compound Name	Response	Retention Time
DDT	1608093	20.795
DDD	147444	20.342
DDE	16114	19.807
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
163558	1771651	9.23

Instrument :
BNA_P
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081825\
Data File : BP025454.D
Acq On : 18 Aug 2025 08:34
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: Aug 18 12:36:51 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP081425.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Aug 14 18:14:31 2025
Response via : Initial Calibration

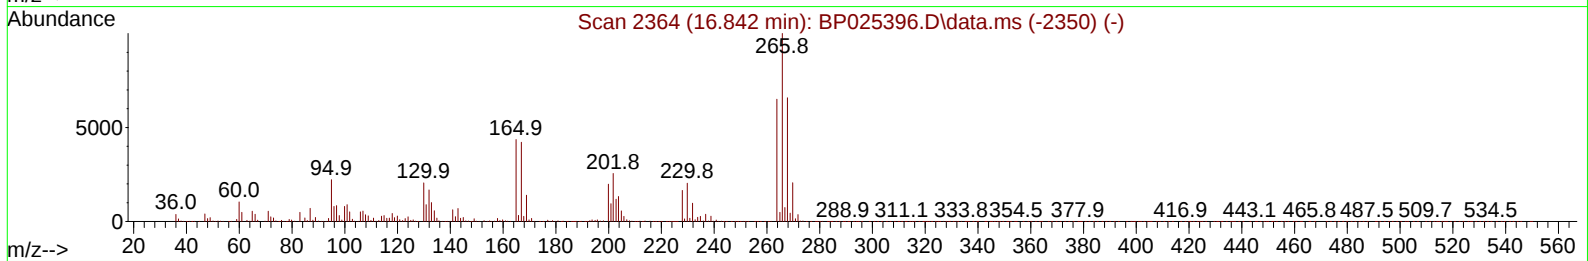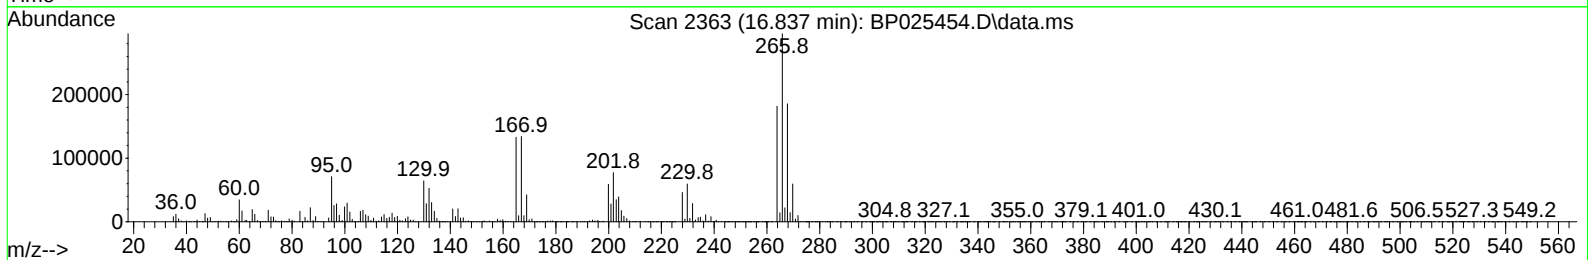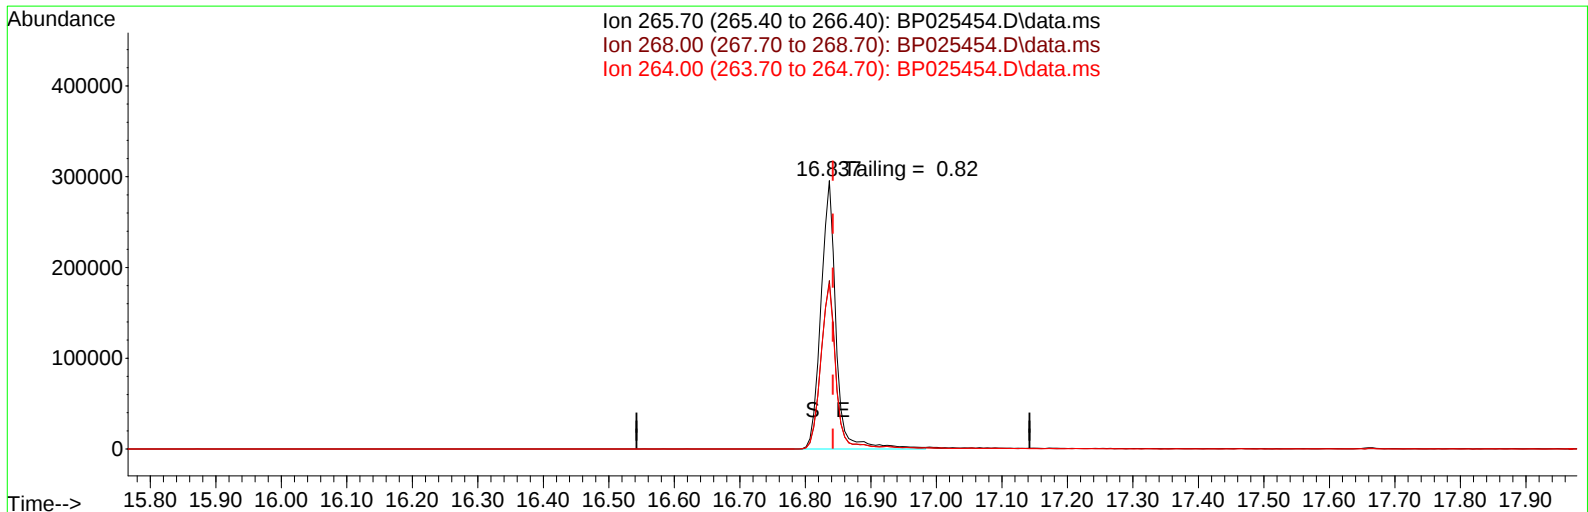

TIC: BP025454.D\data.ms

(70) Pentachlorophenol (C)

16.837min (-0.006) 1000078.55 ng




response 474864

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	65.80	62.75
264.00	65.00	61.47
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081825\
Data File : BP025454.D
Acq On : 18 Aug 2025 08:34
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: Aug 18 12:36:51 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP081425.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Aug 14 18:14:31 2025
Response via : Initial Calibration

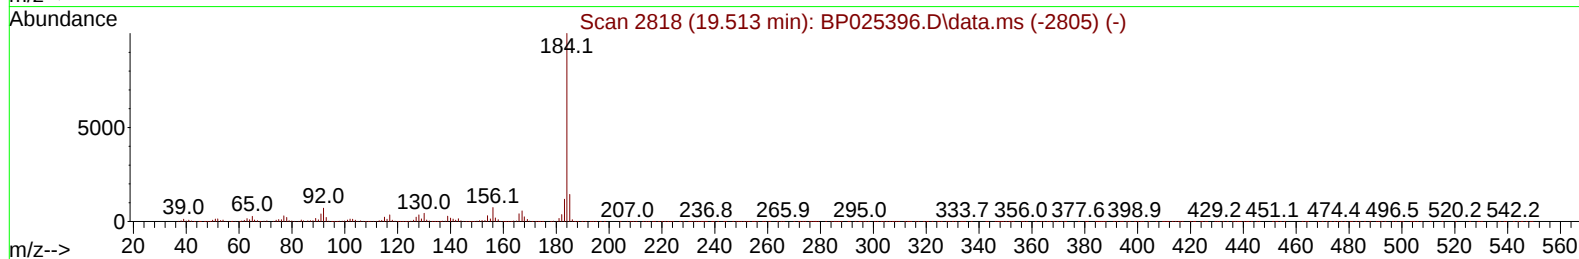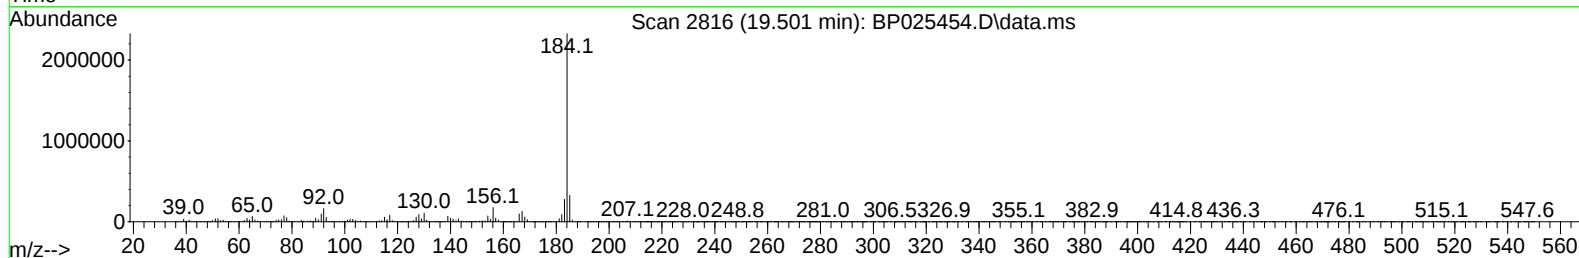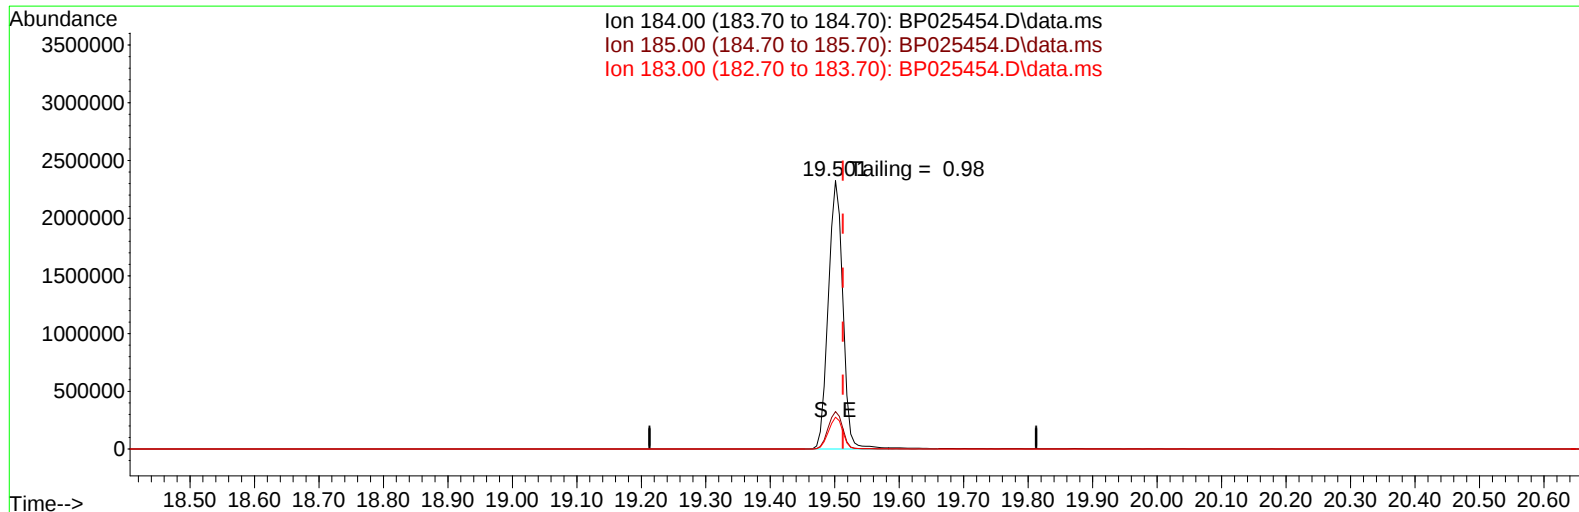

TIC: BP025454.D\data.ms

(77) Benzidine

19.501min (-0.012) 945.06 ng

response 3654054

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.40	13.95
183.00	11.80	11.91
0.00	0.00	0.00