
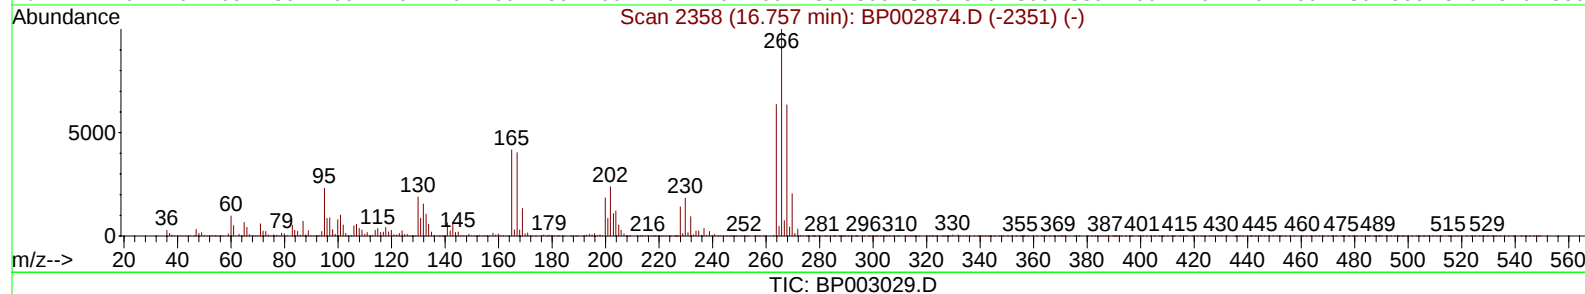
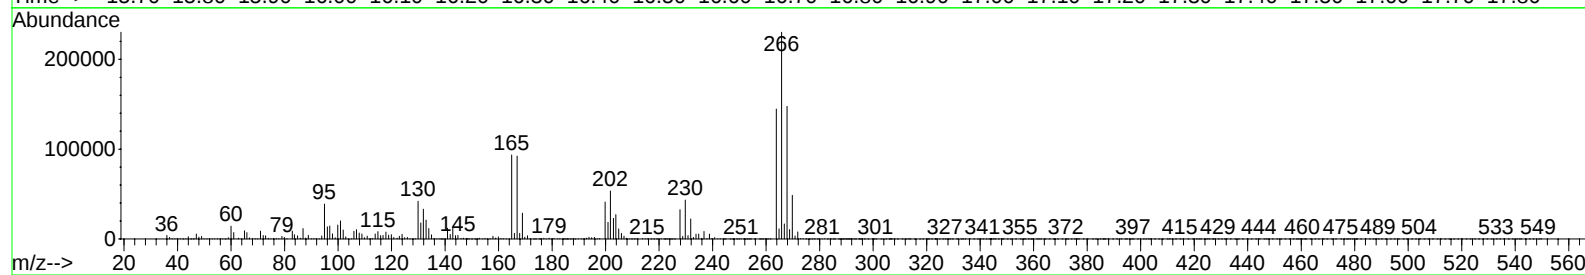


Data Path : Z:\SVOASRV\HPCHEM1\BNA P\DATA\BP081920\
 Data File : BP003029.D
 Acq On : 19 Aug 2020 09:05
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 19 18:36:04 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA P\METHODS\8270-BP073020.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Aug 17 14:07:35 2020
 Response via : Initial Calibration

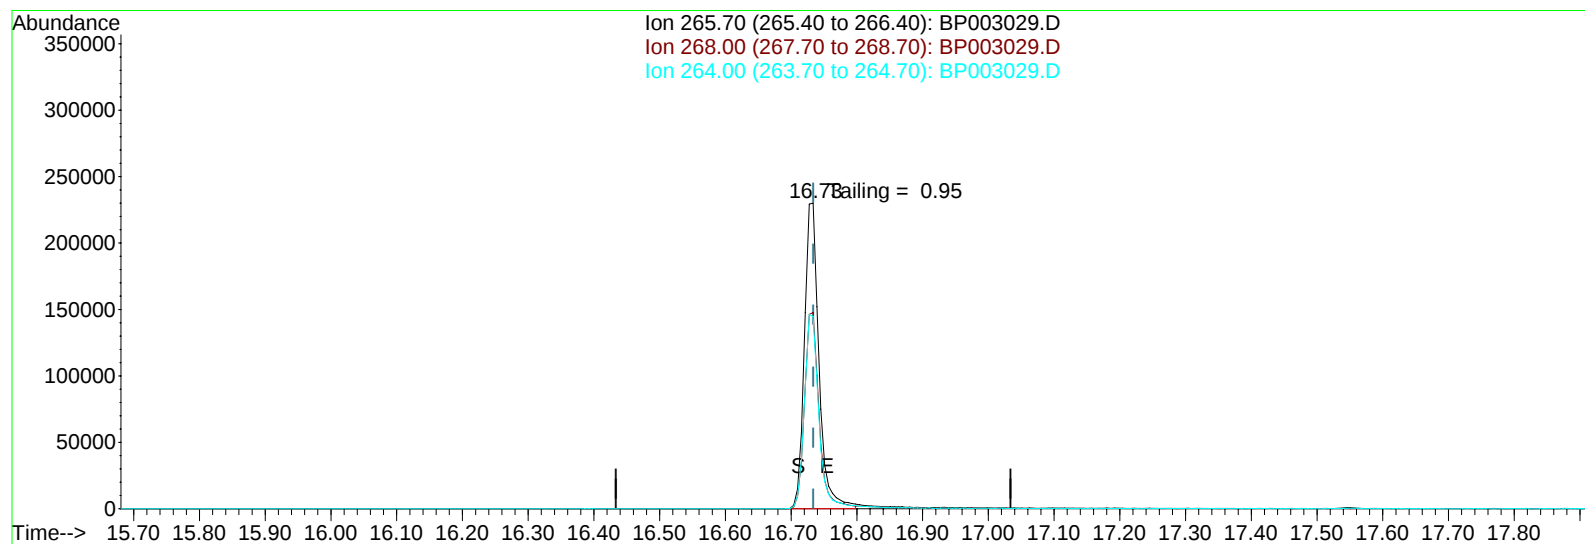

(70) Pentachlorophenol (C)




16.733min (-0.000) 29025.54ng

response 364511

Ion	Exp%	Act%
265.70	100	100
268.00	63.60	64.15
264.00	63.00	62.88
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA P\DATA\BP081920\
 Data File : BP003029.D
 Acq On : 19 Aug 2020 09:05
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 19 18:36:04 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA P\METHODS\8270-BP073020.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Aug 17 14:07:35 2020
 Response via : Initial Calibration

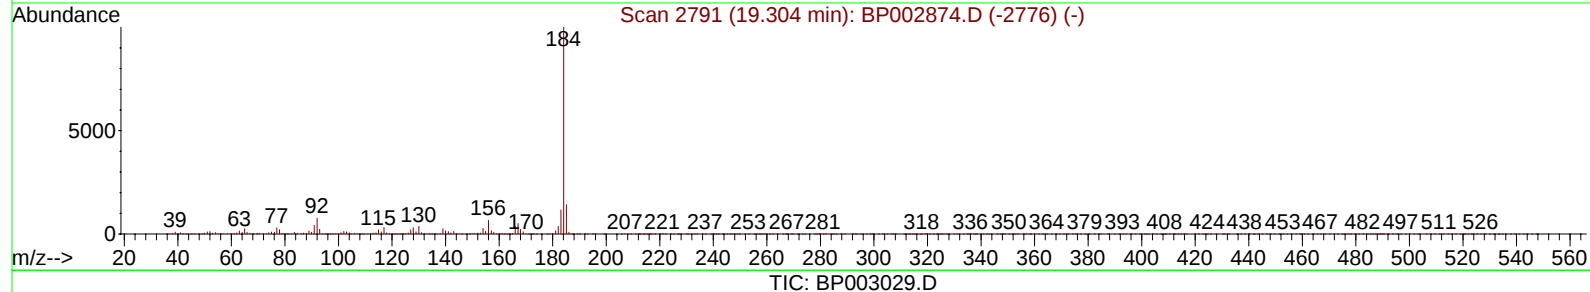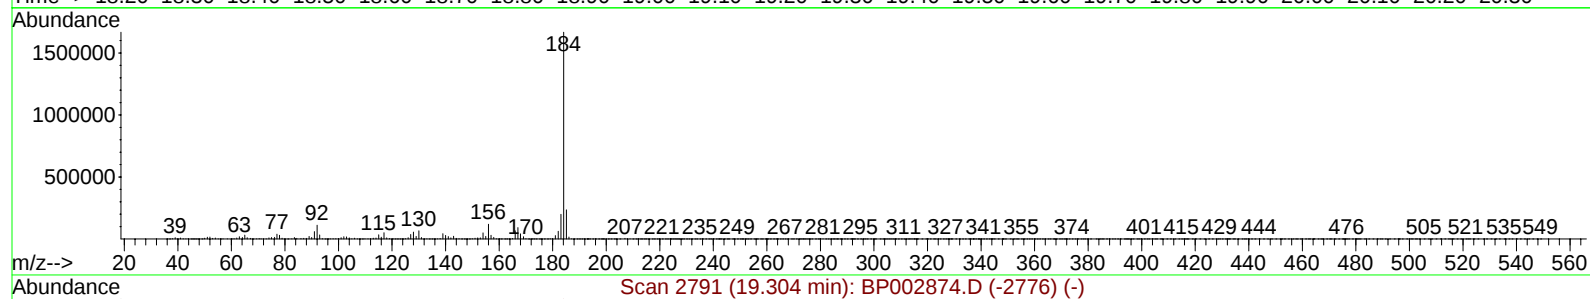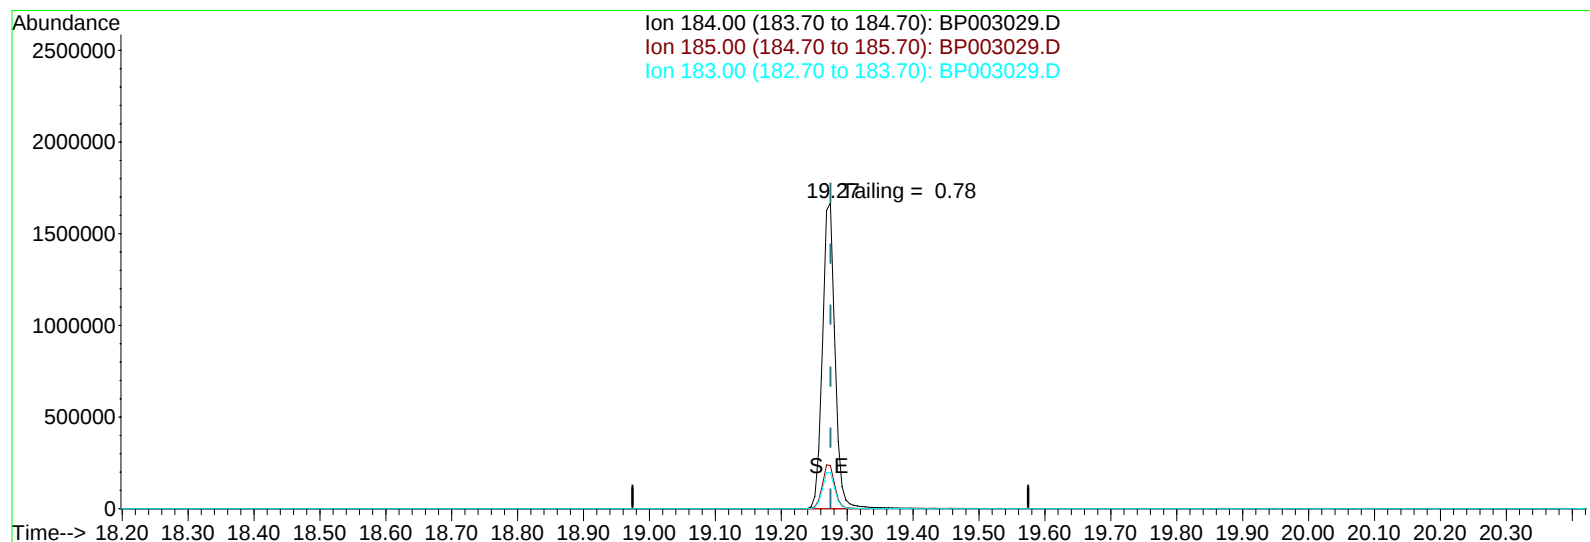

(77) Benzidine

19.274min (-0.000) 19877.89ng

response 2215468

Ion	Exp%	Act%
184.00	100	100
185.00	14.40	14.12
183.00	11.70	11.95
0.00	0.00	0.00