
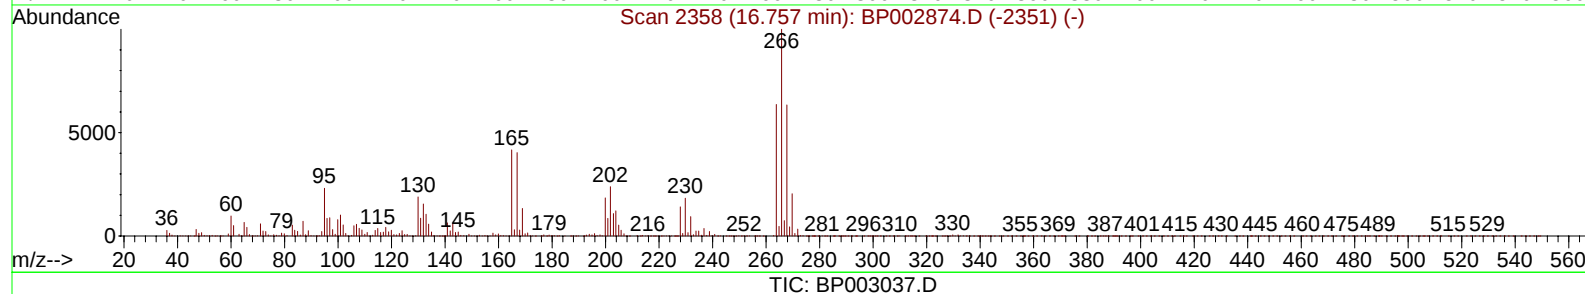
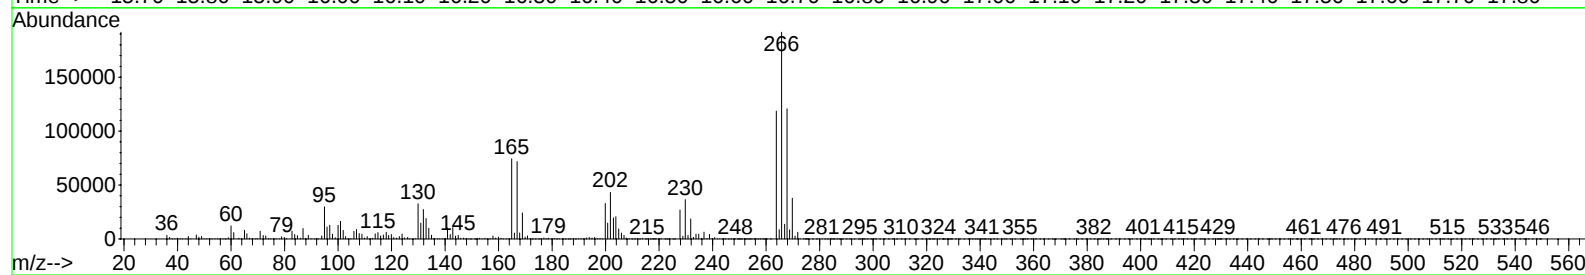


Data Path : Z:\SVOASRV\HPCHEM1\BNA P\DATA\BP081920\
Data File : BP003037.D
Acq On : 19 Aug 2020 17:13
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 19 18:38:01 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA P\METHODS\8270-BP073020.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Aug 17 14:07:35 2020
Response via : Initial Calibration

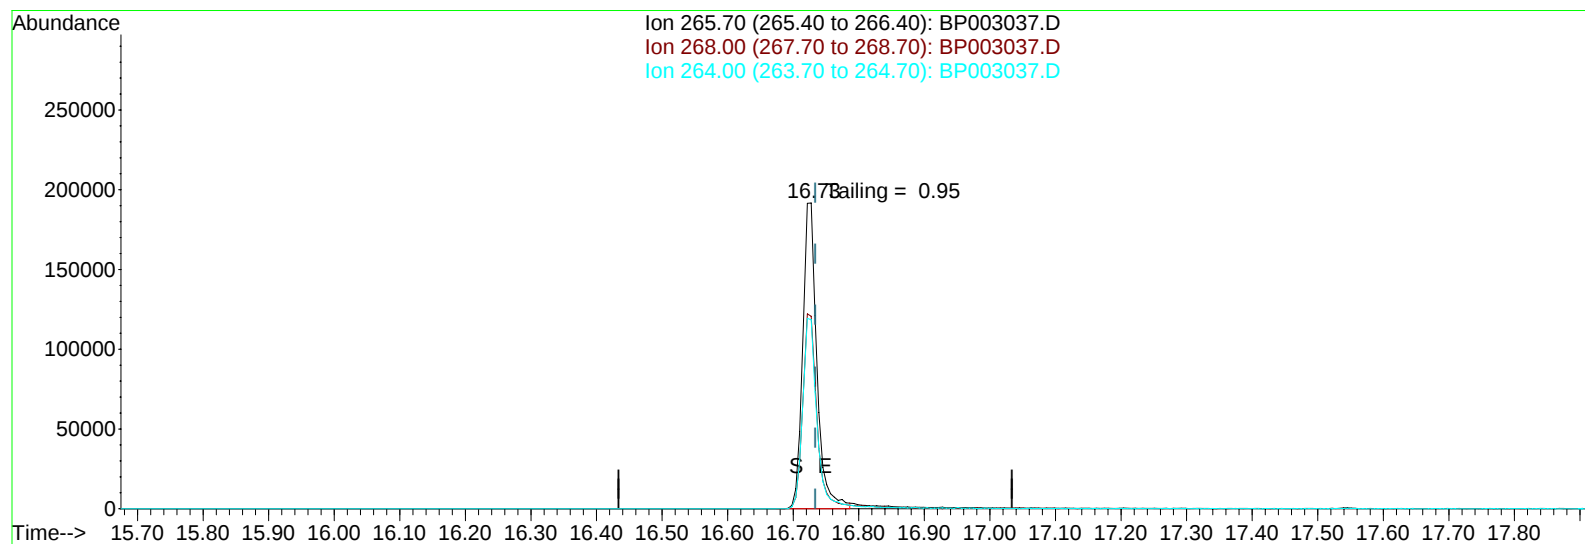

(70) Pentachlorophenol (C)




16.728min (-0.006) 39024.28ng

response 300995

Ion	Exp%	Act%
265.70	100	100
268.00	63.60	62.98
264.00	63.00	61.83
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA P\DATA\BP081920\
 Data File : BP003037.D
 Acq On : 19 Aug 2020 17:13
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 19 18:38:01 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA P\METHODS\8270-BP073020.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Aug 17 14:07:35 2020
 Response via : Initial Calibration

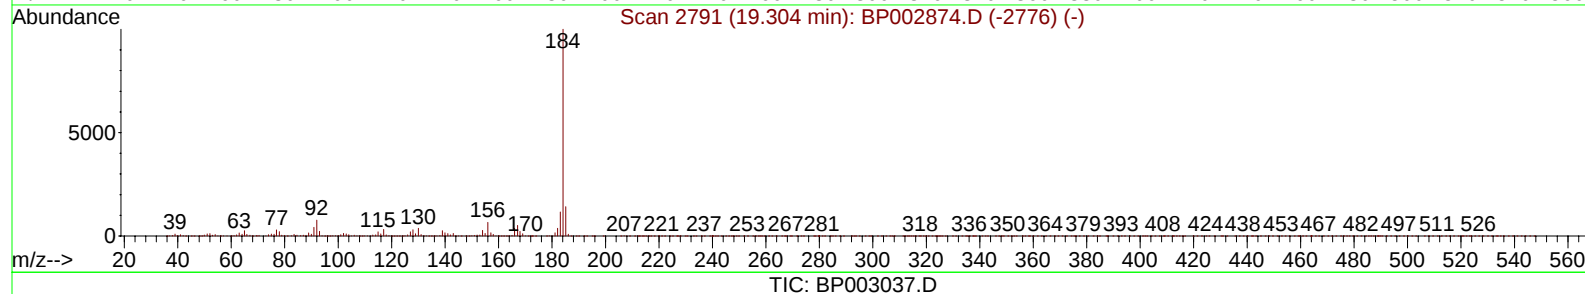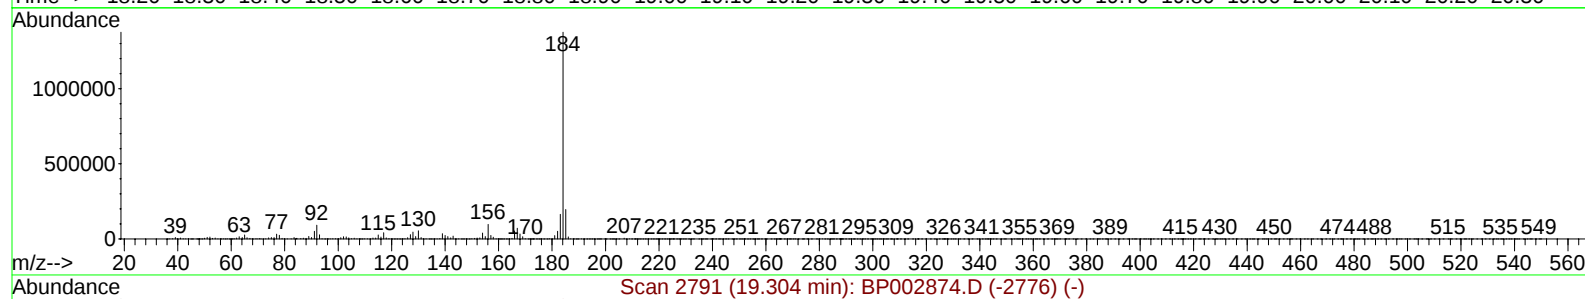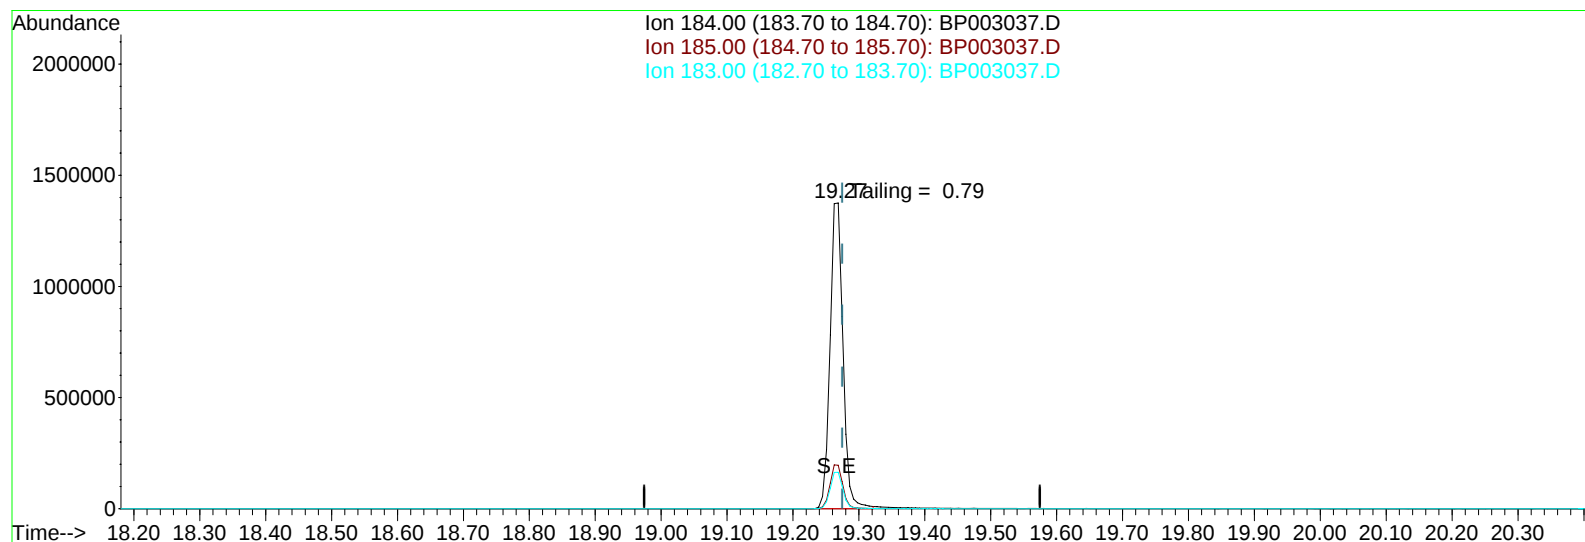

(77) Benzidine

19.269min (-0.006) 13803.93ng

response 1892083

Ion	Exp%	Act%
184.00	100	100
185.00	14.40	14.24
183.00	11.70	11.92
0.00	0.00	0.00