

Data Path : Z:\SVOASRV\HPCHEM1\BNA P\DATA\BP081920\
 Data File : BP003035.D
 Acq On : 19 Aug 2020 13:10
 Operator : CG/JU
 Sample : PB131036BL
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 PB131036BL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0
 Filtering: 5
 Min Area: 3 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP073020.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.963	8	13	20	rVB	148432	178366	1.36%	0.270%
2	5.293	402	409	423	rBV	4246719	6102048	46.52%	9.242%
3	6.863	667	676	693	rBV	3530039	5789876	44.14%	8.769%
4	7.687	806	816	824	rBV	1113710	1799391	13.72%	2.725%
5	8.828	1002	1010	1022	rBV	2492201	4150764	31.65%	6.287%
6	10.463	1280	1288	1302	rBV	1296946	2192967	16.72%	3.322%
7	12.945	1702	1710	1731	rBV	7040005	10760570	82.04%	16.298%
8	14.322	1936	1944	1963	rBV2	2062780	3213187	24.50%	4.867%
9	15.816	2190	2198	2221	rBV	4140095	6130840	46.74%	9.286%
10	17.074	2405	2412	2425	rBV	2247989	3259252	24.85%	4.937%
11	19.651	2844	2850	2863	rBV	10620837	13115794	100.00%	19.866%
12	20.857	3050	3055	3060	rBV	76510	134219	1.02%	0.203%
13	20.910	3060	3064	3068	rVV	112816	163664	1.25%	0.248%
14	20.957	3068	3072	3081	rVV	240333	323116	2.46%	0.489%
15	21.163	3102	3107	3119	rBV	3244801	4177019	31.85%	6.327%
16	23.409	3482	3489	3503	rVB2	2361343	4531880	34.55%	6.864%




Sum of corrected areas: 66022953

Data Path : Z:\SVOASRV\HPCHEM1\BNA P\DATA\BP081920\
Data File : BP003035.D
Acq On : 19 Aug 2020 13:10
Operator : CG/JU
Sample : PB131036BL
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB131036BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA P\METHODS\8270-BP073020.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

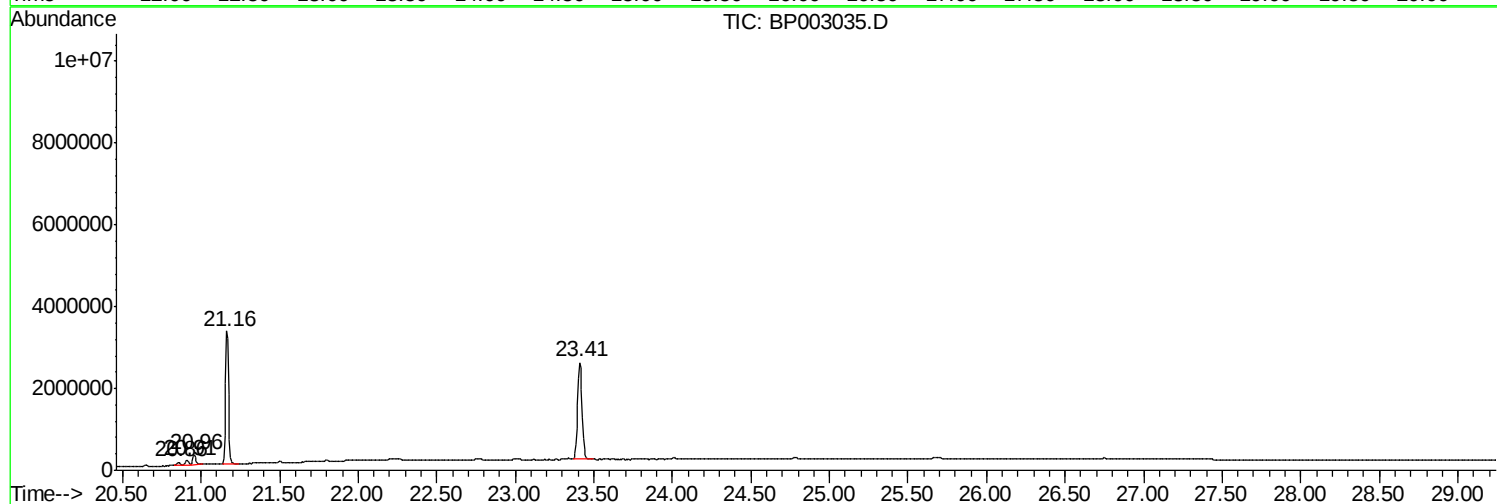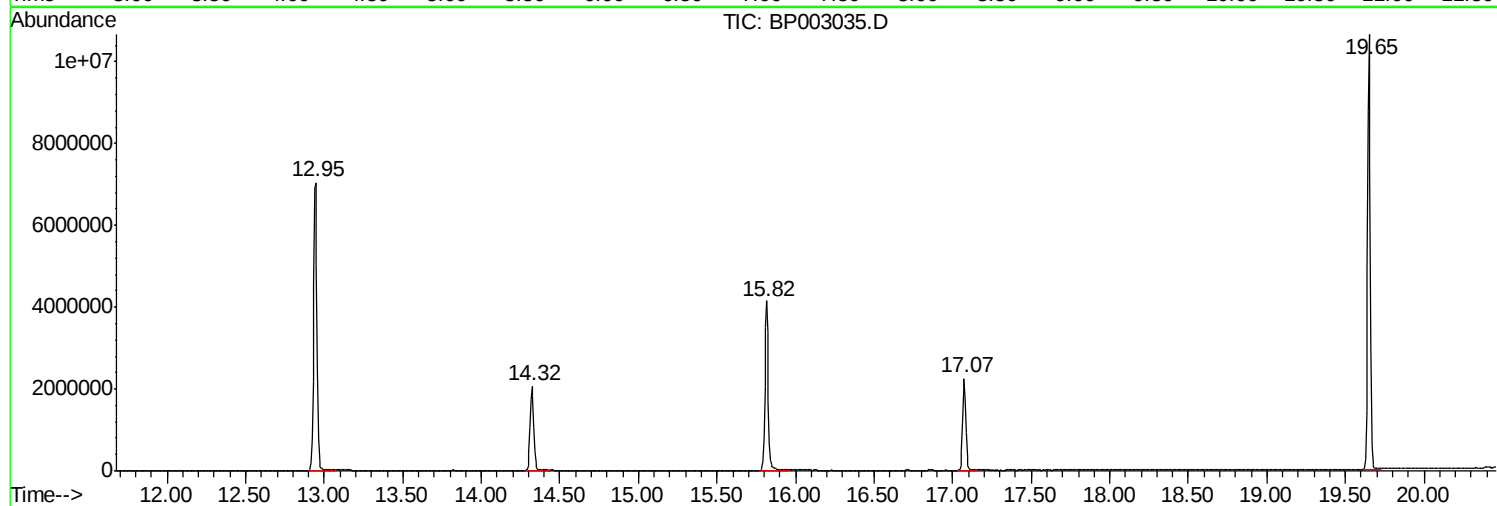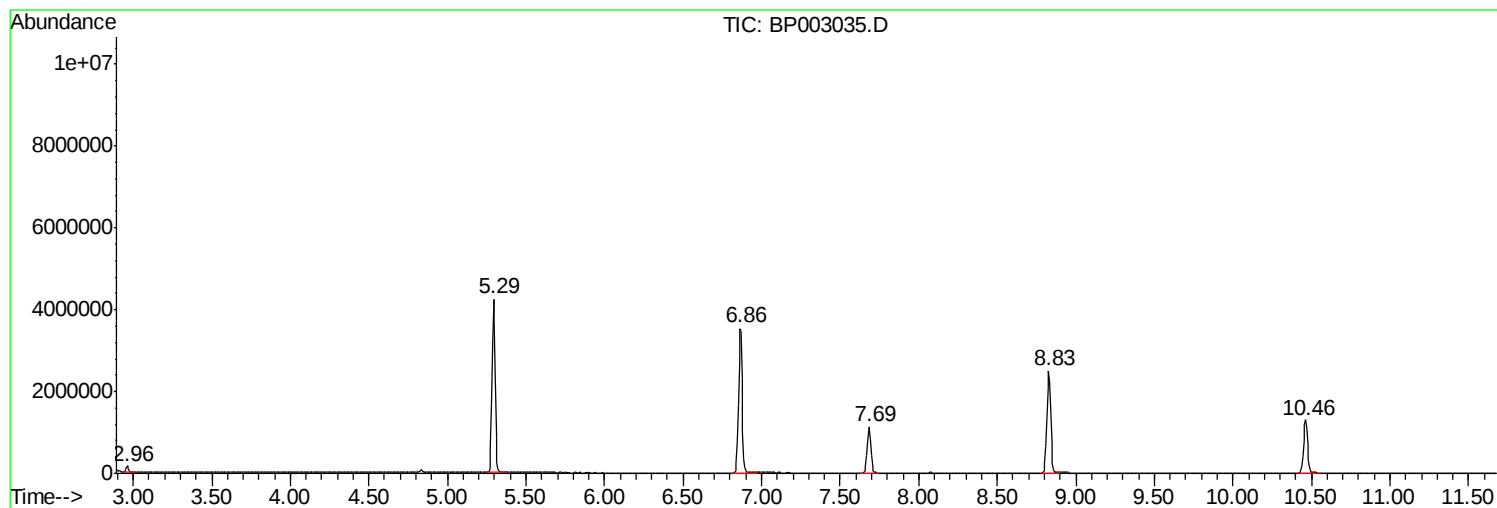

Data Path : Z:\SVOASRV\HPCHEM1\BNA_P\DATA\BP081920\
Data File : BP003035.D
Acq On : 19 Aug 2020 13:10
Operator : CG/JU
Sample : PB131036BL
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB131036BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP073020.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\SVOASRV\HPCHEM1\BNA_P\DATA\BP081920\
Data File : BP003035.D
Acq On : 19 Aug 2020 13:10
Operator : CG/JU
Sample : PB131036BL
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB131036BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP073020.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc