


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081920\
 Data File : BP003029.D
 Acq On : 19 Aug 2020 09:05
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP073020.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Aug 17 14:07:35 2020

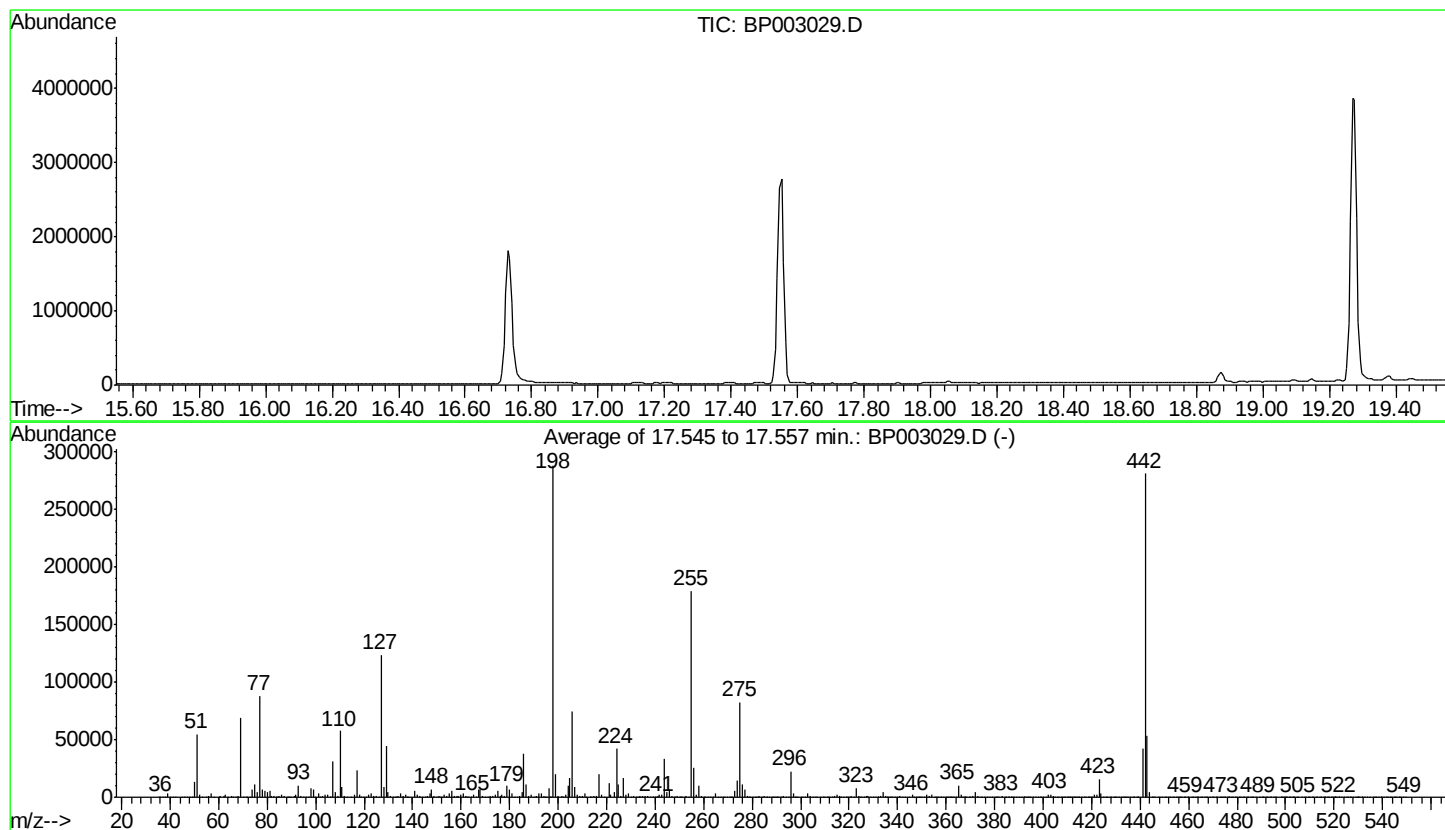

AutoFind: Scans 2492, 2493, 2494; Background Corrected with Scan 2481

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	18.9	54474	PASS
68	69	0.00	2	1.6	1125	PASS
69	198	0.00	100	23.8	68539	PASS
70	69	0.00	2	0.6	405	PASS
127	198	10	80	43.0	123551	PASS
197	198	0.00	2	0.2	542	PASS
198	198	100	100	100.0	287616	PASS
199	198	5	9	6.8	19478	PASS
275	198	10	60	28.7	82426	PASS
365	198	1	100	3.7	10568	PASS
441	198	0.01	100	14.6	41937	PASS
442	198	50	100	97.8	281173	PASS
443	442	15	24	18.8	52938	PASS