


Data Path : Z:\SVOASRV\HPCHEM1\BNA_P\DATA\BP081920\
 Data File : BP003037.D
 Acq On : 19 Aug 2020 17:13
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP073020.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Aug 17 14:07:35 2020

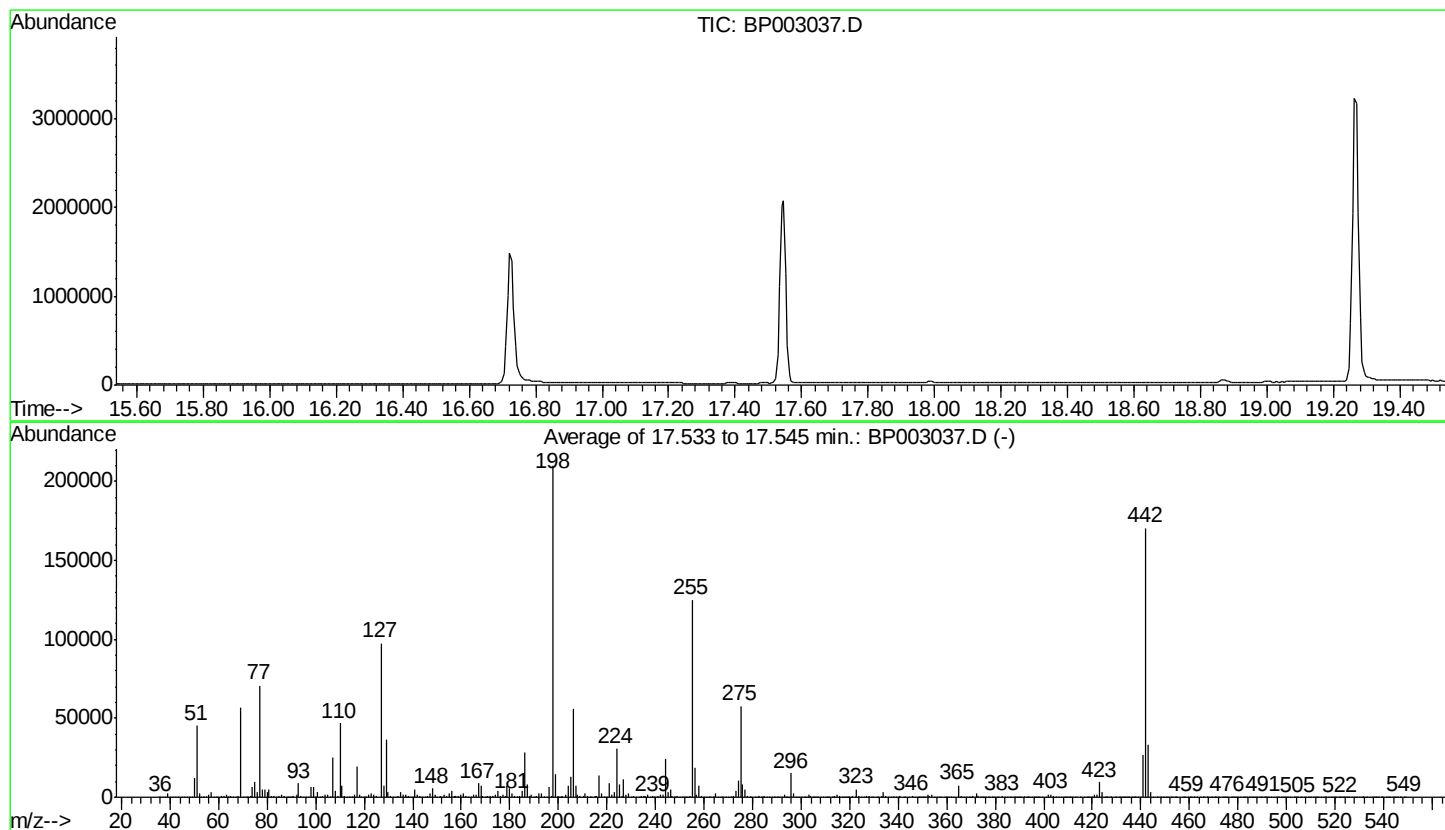

AutoFind: Scans 2490, 2491, 2492; Background Corrected with Scan 2482

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	21.6	45395	PASS
68	69	0.00	2	1.8	1009	PASS
69	198	0.00	100	27.2	57187	PASS
70	69	0.00	2	0.4	231	PASS
127	198	10	80	46.4	97554	PASS
197	198	0.00	2	0.2	521	PASS
198	198	100	100	100.0	210048	PASS
199	198	5	9	7.0	14744	PASS
275	198	10	60	27.6	57917	PASS
365	198	1	100	3.5	7324	PASS
441	198	0.01	100	12.6	26391	PASS
442	198	50	100	81.2	170528	PASS
443	442	15	24	19.5	33258	PASS