
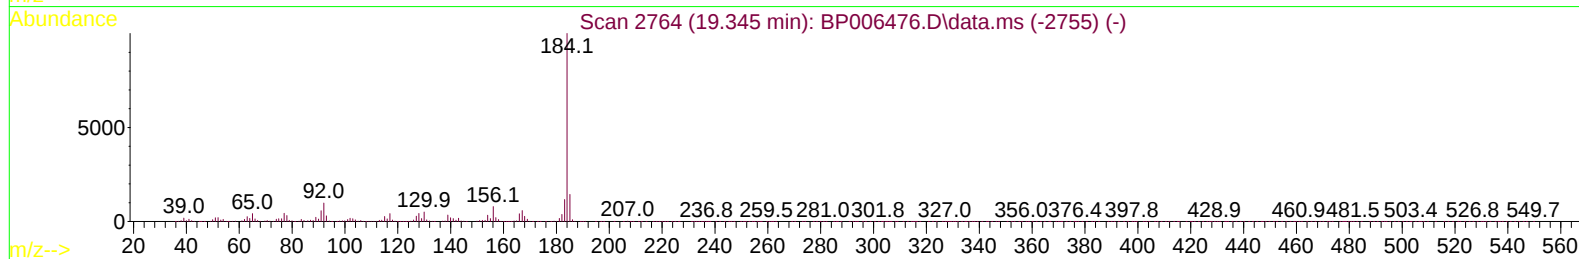
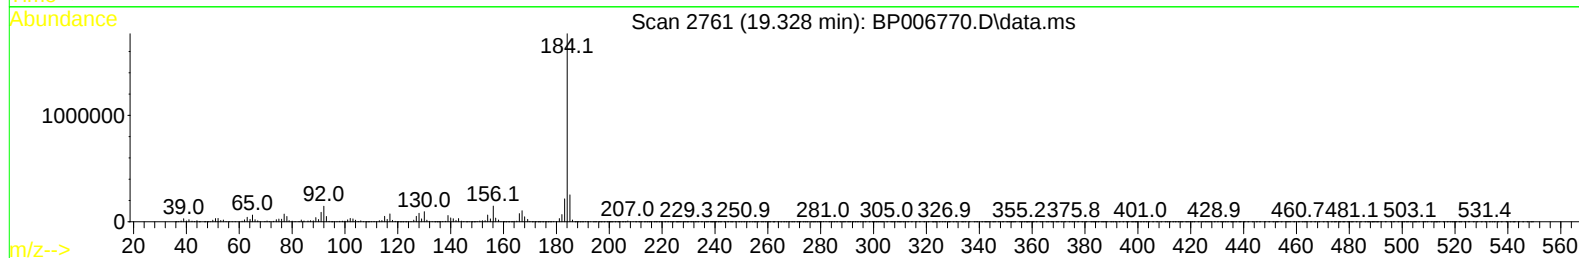


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081921\
Data File : BP006770.D
Acq On : 19 Aug 2021 08:38
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 19 11:03:18 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP080321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Aug 16 18:17:59 2021
Response via : Initial Calibration

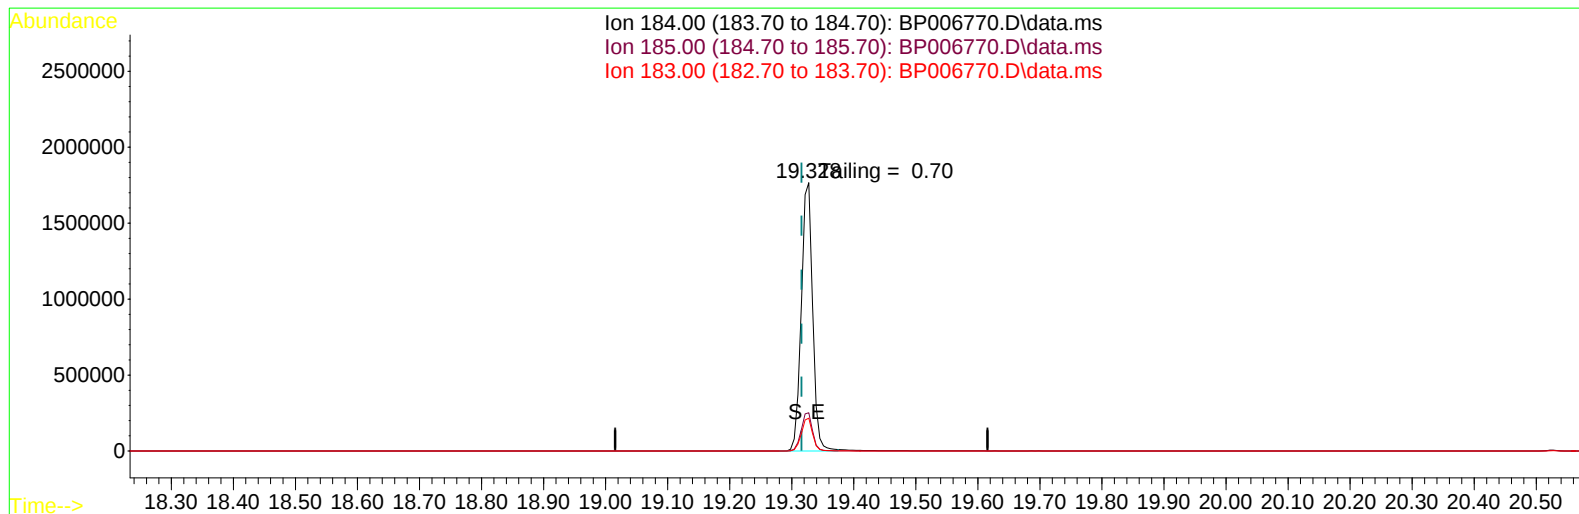




TIC: BP006770.D\data.ms

(77) Benzidine**19.328min (+ 0.012) 9850.40 ng****response 2277565**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.70	14.28
183.00	11.90	12.21
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081921\
Data File : BP006770.D
Acq On : 19 Aug 2021 08:38
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 19 11:03:18 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP080321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Aug 16 18:17:59 2021
Response via : Initial Calibration

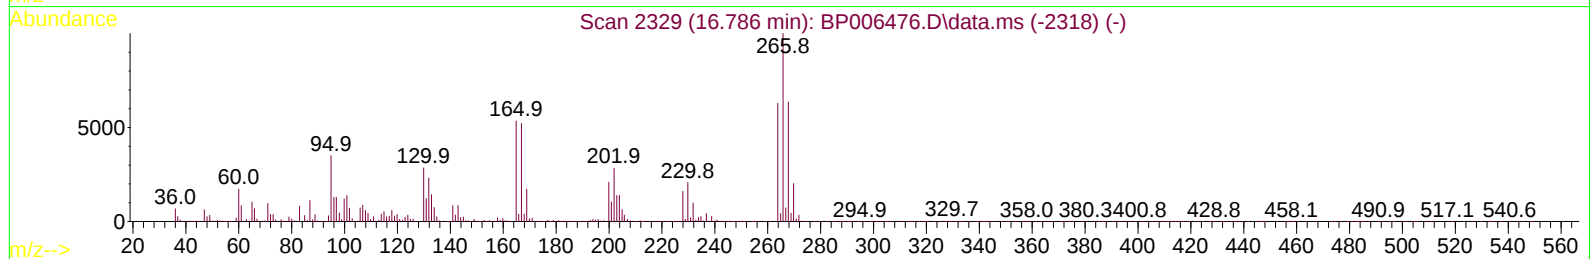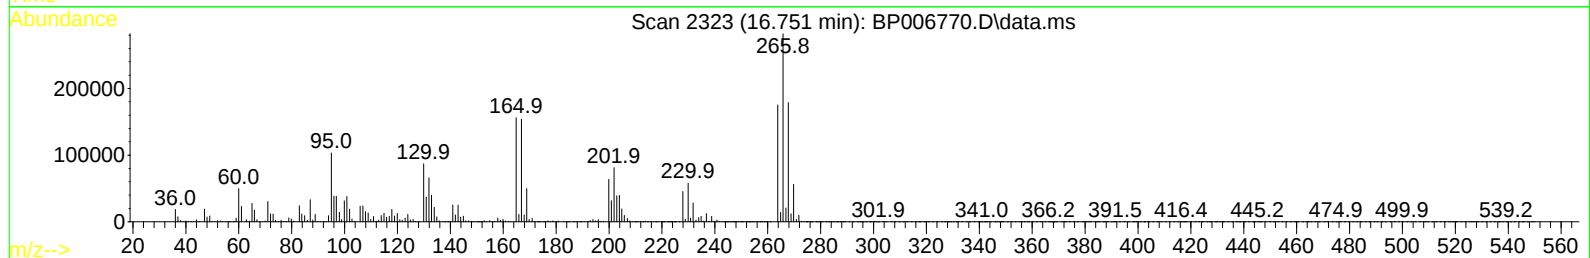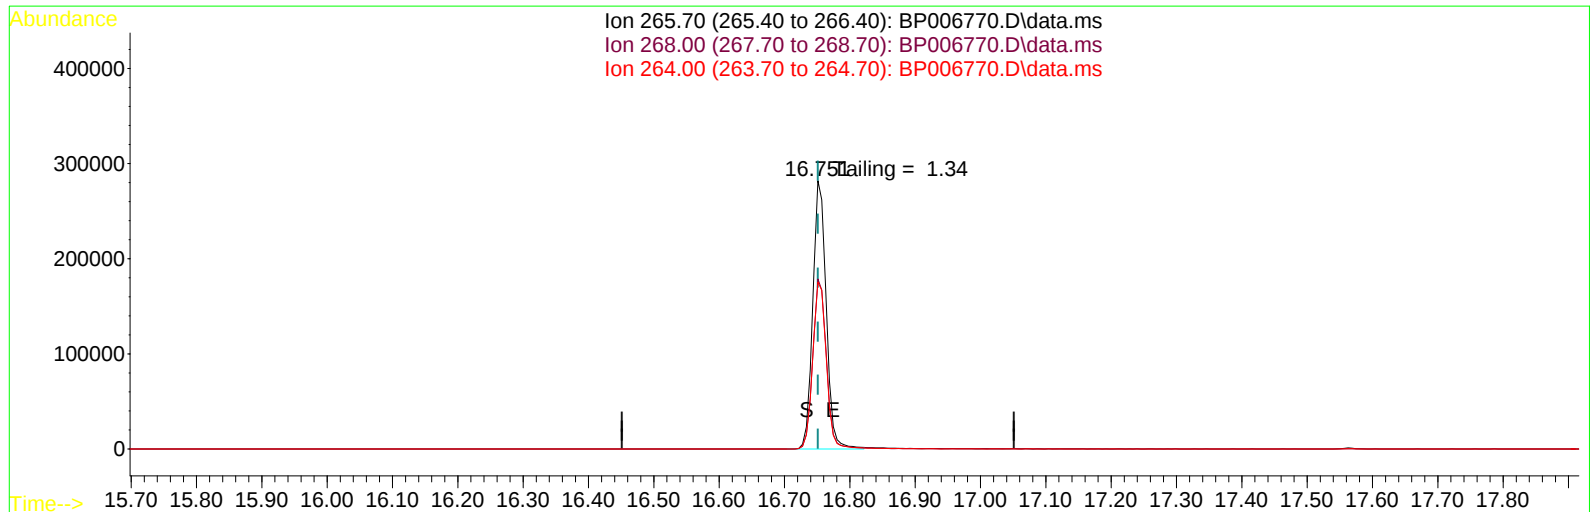

TIC: BP006770.D\data.ms

(70) Pentachlorophenol (C)

16.751min (+ 0.000) 23434.57 ng

response 407821

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.50	63.38
264.00	62.90	62.16
0.00	0.00	0.00