

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081921\
 Data File : BP006777.D
 Acq On : 19 Aug 2021 12:55
 Operator : CG/JU
 Sample : M3434-07
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SWCS-11-1015

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP080321.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BP006777.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.299	370	376	387	rVB	2149185	2976294	48.88%	3.794%
2	6.881	639	645	656	rVB	1881351	2983212	48.99%	3.803%
3	7.693	777	783	791	rVB	590939	942216	15.47%	1.201%
4	8.858	974	981	988	rBV	1239132	2000130	32.85%	2.550%
5	10.281	1217	1223	1230	rBV2	71267	122781	2.02%	0.157%
6	10.481	1250	1257	1265	rBV	815686	1309131	21.50%	1.669%
7	12.963	1672	1679	1687	rBV	2851049	4034255	66.26%	5.143%
8	14.340	1907	1913	1923	rBV	1119845	1594126	26.18%	2.032%
9	14.781	1984	1988	1994	rVB3	52225	73189	1.20%	0.093%
10	14.922	2007	2012	2020	rVB3	42327	77114	1.27%	0.098%
11	15.163	2046	2053	2063	rBV6	27380	95545	1.57%	0.122%
12	15.687	2126	2142	2154	rVB	147715	619352	10.17%	0.790%
13	15.840	2158	2168	2178	rBV	2212699	3258390	53.51%	4.154%
14	16.145	2216	2220	2231	rVB3	60283	109953	1.81%	0.140%
15	16.510	2275	2282	2292	rBV6	112812	290748	4.78%	0.371%
16	17.098	2376	2382	2389	rBV	1332598	1888103	31.01%	2.407%
17	18.016	2532	2538	2555	rBV	1558046	2391559	39.28%	3.049%
18	18.286	2574	2584	2585	rBV2	520208	1023352	16.81%	1.305%
19	18.334	2587	2592	2616	rVB3	1047430	4317181	70.90%	5.504%
20	18.745	2659	2662	2670	rVB2	70627	110468	1.81%	0.141%
21	19.116	2721	2725	2726	rBV2	78387	95355	1.57%	0.122%
22	19.139	2726	2729	2733	rVV5	67553	121360	1.99%	0.155%
23	19.257	2745	2749	2766	rVB	1044514	1544754	25.37%	1.969%
24	19.686	2816	2822	2827	rVB	4893599	5945838	97.65%	7.580%
25	20.045	2868	2883	2899	rBV2	1324850	5241700	86.09%	6.682%
26	20.945	3032	3036	3042	rBV2	305242	478109	7.85%	0.610%
27	20.998	3042	3045	3050	rVB	444601	518341	8.51%	0.661%
28	21.092	3051	3061	3068	rBV	1847217	5171931	84.94%	6.593%
29	21.175	3069	3075	3077	rVV	1127206	2010859	33.03%	2.564%
30	21.210	3077	3081	3089	rVB	2044214	2929308	48.11%	3.734%
31	21.322	3094	3100	3107	rVB4	756844	1598559	26.25%	2.038%
32	21.698	3160	3164	3169	rVB3	304280	512018	8.41%	0.653%
33	21.786	3173	3179	3194	rVB4	820365	2230038	36.62%	2.843%
34	21.986	3204	3213	3224	rVB	1698695	4358788	71.59%	5.557%
35	23.010	3379	3387	3397	rVB	1090149	3179636	52.22%	4.054%
36	23.521	3468	3474	3490	rVB2	1250405	2585178	42.46%	3.296%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081921\
Data File : BP006777.D
Acq On : 19 Aug 2021 12:55
Operator : CG/JU
Sample : M3434-07
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SWCS-11-1015

Integration Parameters: rteint.p
Integrator: RTE
Smoothing : ON Filtering: 5
Sampling : 1 Min Area: 3 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP080321.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

37	23.845	3521	3529	3549	rVB3	1758985	6088856	100.00%	7.762%
38	24.563	3642	3651	3662	rVB	1099395	3613314	59.34%	4.606%




Sum of corrected areas: 78441041

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081921\
Data File : BP006777.D
Acq On : 19 Aug 2021 12:55
Operator : CG/JU
Sample : M3434-07
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SWCS-11-1015

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP080321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

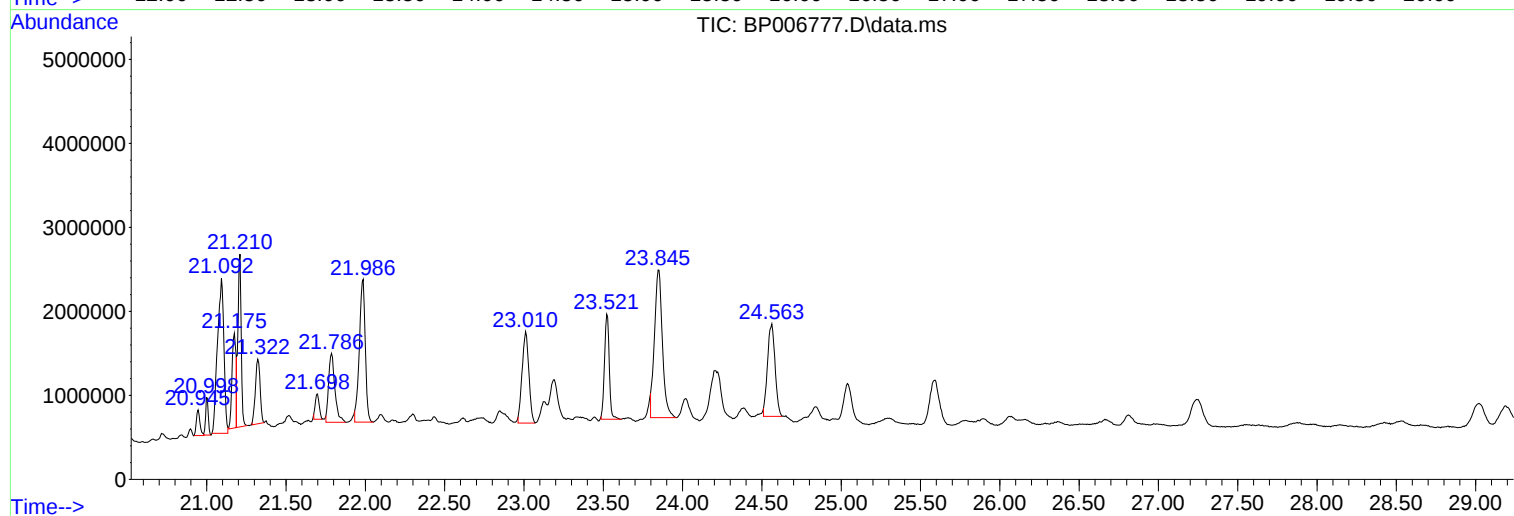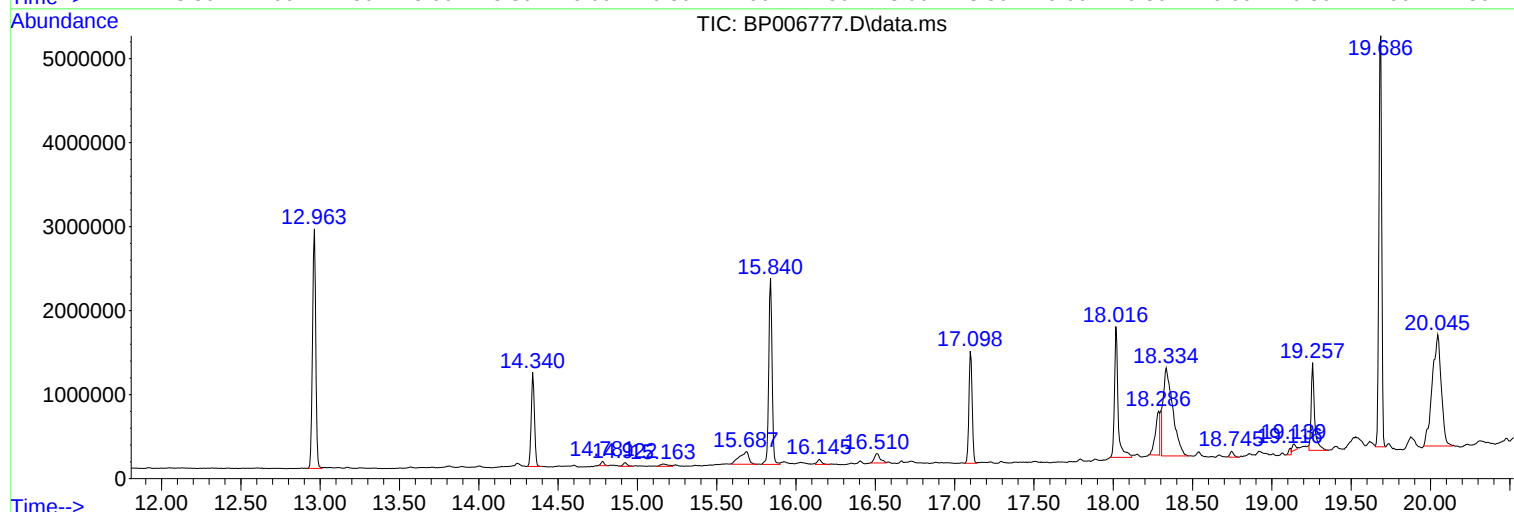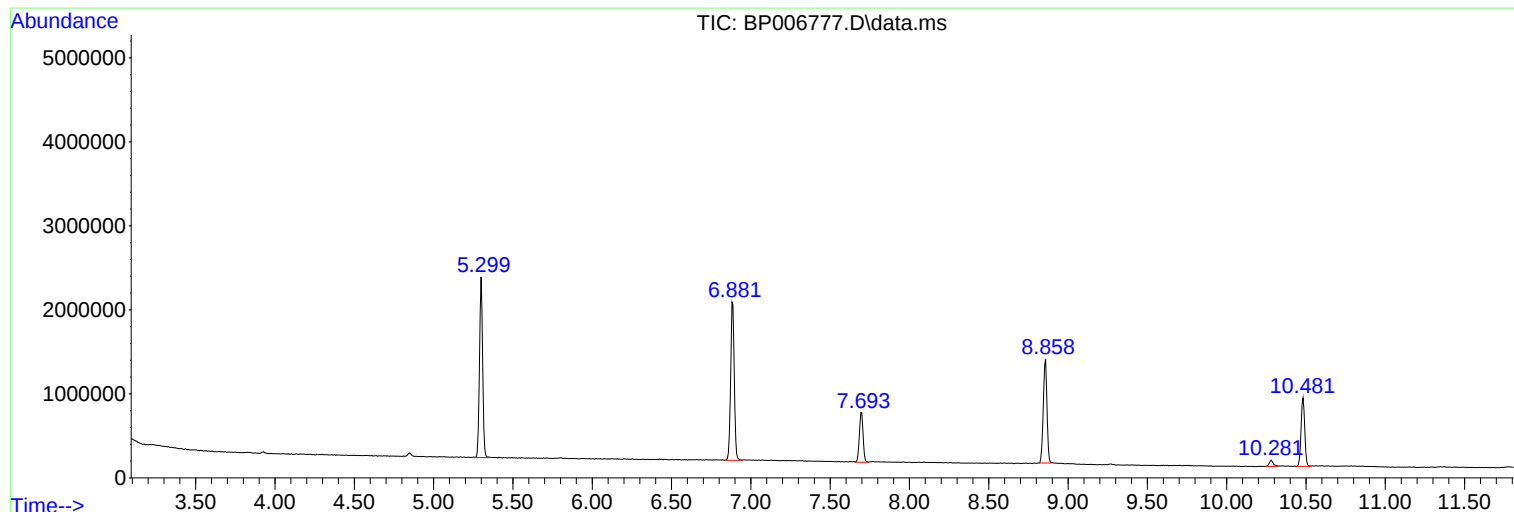

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081921\
Data File : BP006777.D
Acq On : 19 Aug 2021 12:55
Operator : CG/JU
Sample : M3434-07
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SWCS-11-1015

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP080321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081921\
Data File : BP006777.D
Acq On : 19 Aug 2021 12:55
Operator : CG/JU
Sample : M3434-07
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SWCS-11-1015

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP080321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------