

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081921\
 Data File : BP006781.D
 Acq On : 19 Aug 2021 15:11
 Operator : CG/JU
 Sample : M3434-11
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SWCS-12-0205

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP080321.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BP006781.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	4.846	296	299	307	rVB	116649	159370	3.34%	0.515%
2	5.299	370	376	386	rVB	2163596	3054600	63.99%	9.878%
3	6.881	639	645	657	rVB	1971669	3045213	63.79%	9.848%
4	7.693	778	783	792	rVB	679643	1069641	22.41%	3.459%
5	8.857	974	981	993	rVB	1279596	2115981	44.32%	6.843%
6	10.281	1217	1223	1234	rBV	62987	135414	2.84%	0.438%
7	10.481	1250	1257	1271	rVB	882339	1453525	30.45%	4.701%
8	12.963	1670	1679	1691	rBV	2687682	4056325	84.97%	13.118%
9	14.339	1906	1913	1928	rBV	1093139	1613873	33.81%	5.219%
10	15.834	2157	2167	2191	rBV	1732426	2746090	57.52%	8.880%
11	17.098	2375	2382	2395	rBV	1174344	1672008	35.02%	5.407%
12	18.010	2532	2537	2551	rBV	310087	502778	10.53%	1.626%
13	19.251	2744	2748	2758	rBV	205099	309399	6.48%	1.001%
14	19.680	2816	2821	2827	rBV	3851549	4773903	100.00%	15.438%
15	20.939	3031	3035	3043	rBV2	183187	318924	6.68%	1.031%
16	21.210	3076	3081	3089	rBV	1335120	1763104	36.93%	5.702%
17	23.521	3468	3474	3485	rVB2	1102292	2132612	44.67%	6.897%




Sum of corrected areas: 30922760

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081921\
Data File : BP006781.D
Acq On : 19 Aug 2021 15:11
Operator : CG/JU
Sample : M3434-11
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SWCS-12-0205

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP080321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

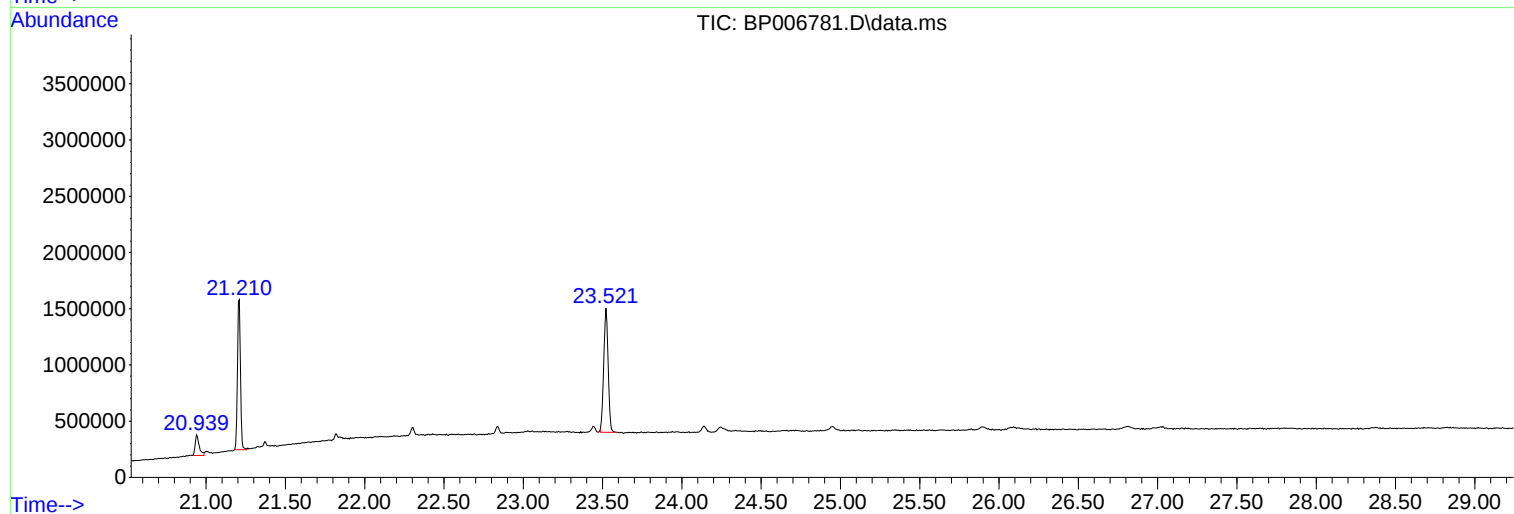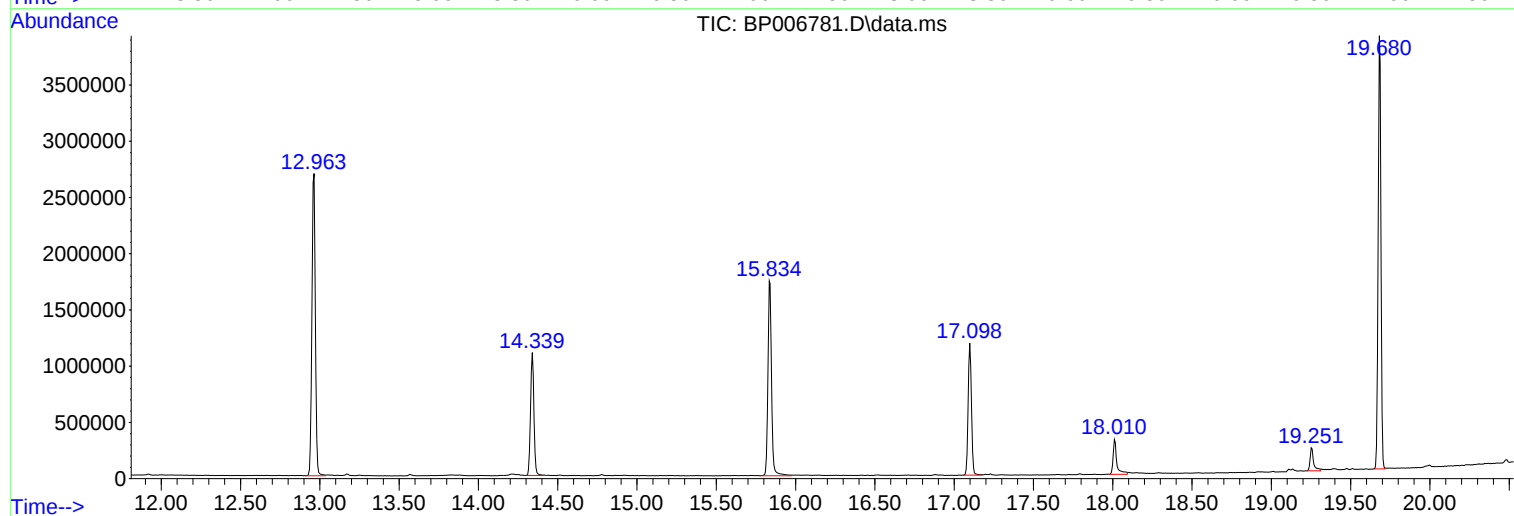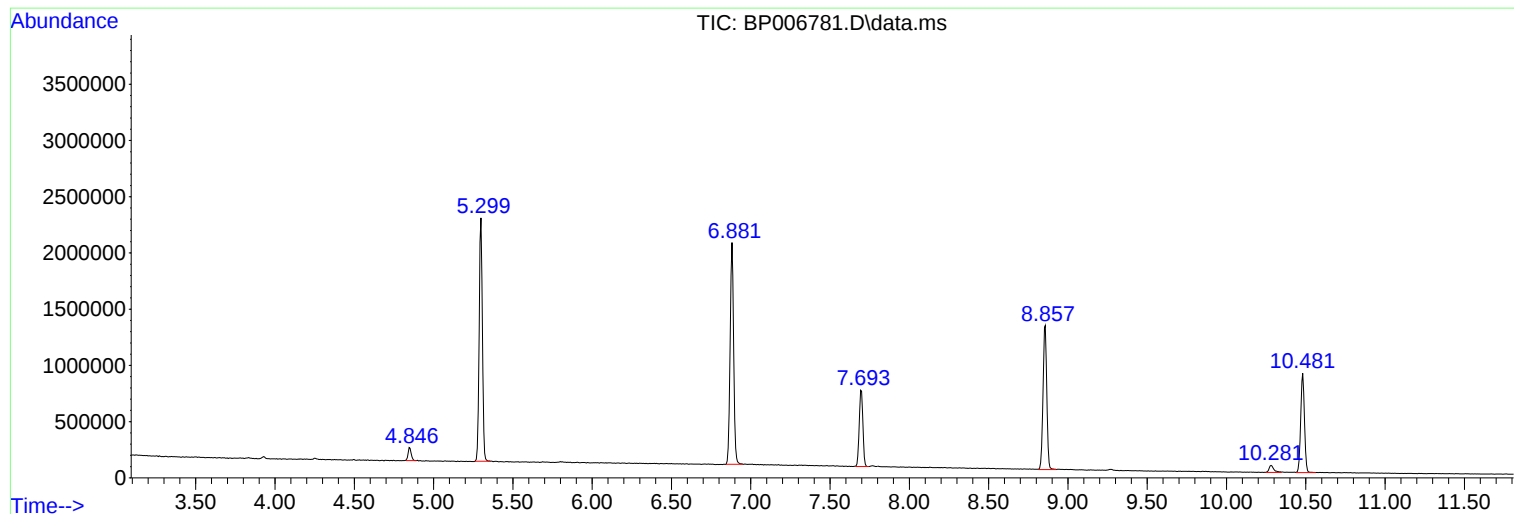

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081921\
Data File : BP006781.D
Acq On : 19 Aug 2021 15:11
Operator : CG/JU
Sample : M3434-11
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SWCS-12-0205

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP080321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081921\
Data File : BP006781.D
Acq On : 19 Aug 2021 15:11
Operator : CG/JU
Sample : M3434-11
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SWCS-12-0205

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP080321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc