

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081921\
 Data File : BP006782.D
 Acq On : 19 Aug 2021 15:45
 Operator : CG/JU
 Sample : M3434-15
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SWCS-12-1015

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP080321.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BP006782.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	4.852	297	300	307	rVB	79378	103878	1.69%	0.269%
2	5.299	370	376	386	rVB	3167912	4371889	71.17%	11.316%
3	6.881	638	645	659	rVB	2775914	4341346	70.67%	11.236%
4	7.693	777	783	791	rBV	731454	1150362	18.73%	2.977%
5	8.857	974	981	989	rVB	1833232	2970373	48.35%	7.688%
6	10.281	1217	1223	1233	rBV	103439	206501	3.36%	0.534%
7	10.481	1250	1257	1264	rBV	955811	1559935	25.39%	4.037%
8	12.963	1670	1679	1694	rBV	3832603	5726527	93.22%	14.822%
9	14.339	1906	1913	1925	rBV	1227039	1777456	28.94%	4.600%
10	15.839	2157	2168	2186	rBV	2598936	3965451	64.55%	10.264%
11	17.098	2375	2382	2395	rBV	1316190	1859762	30.28%	4.814%
12	18.010	2532	2537	2547	rBV	190707	286000	4.66%	0.740%
13	19.251	2744	2748	2757	rBV	122175	177372	2.89%	0.459%
14	19.680	2816	2821	2829	rBV	5436338	6142895	100.00%	15.899%
15	20.939	3031	3035	3041	rBV	163257	237587	3.87%	0.615%
16	21.204	3075	3080	3086	rBV2	1333141	1688458	27.49%	4.370%
17	21.368	3106	3108	3113	rVB2	59767	61429	1.00%	0.159%
18	23.515	3467	3473	3484	rVB2	1026608	2008992	32.70%	5.200%




Sum of corrected areas: 38636213

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081921\
Data File : BP006782.D
Acq On : 19 Aug 2021 15:45
Operator : CG/JU
Sample : M3434-15
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SWCS-12-1015

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP080321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

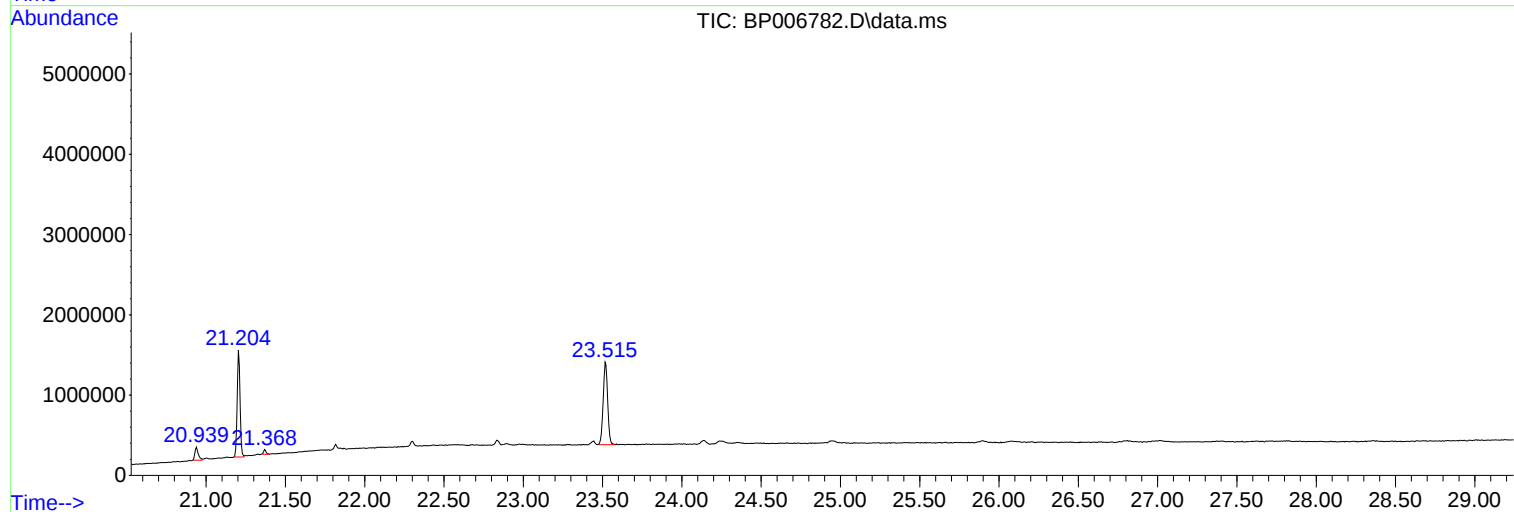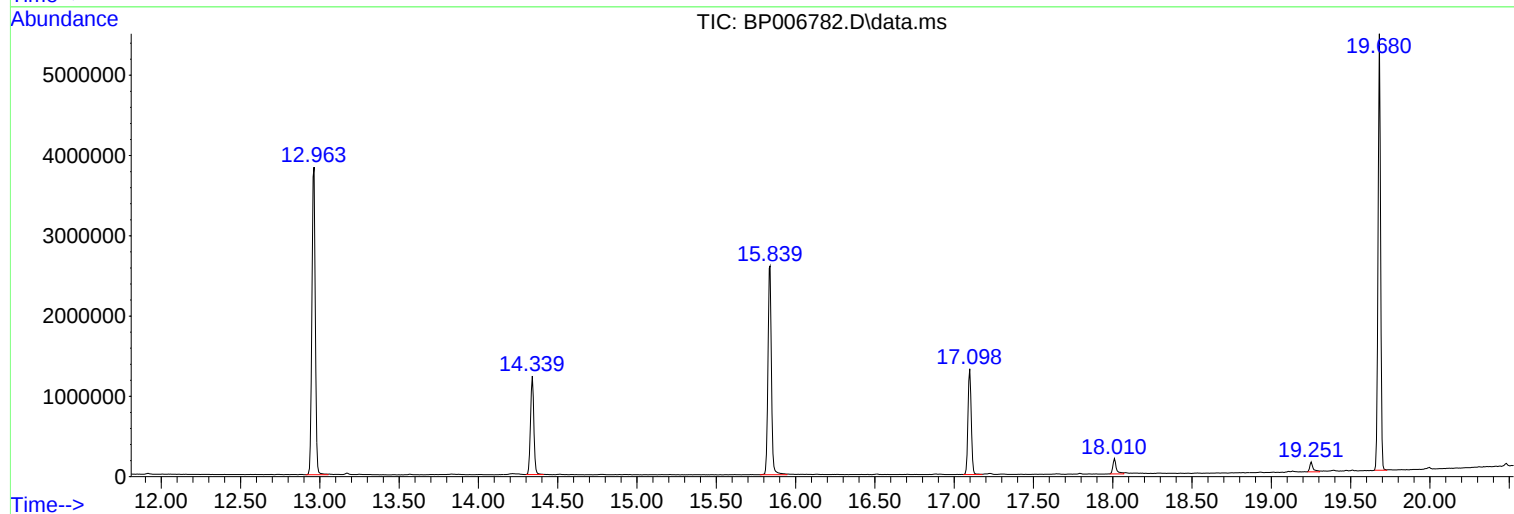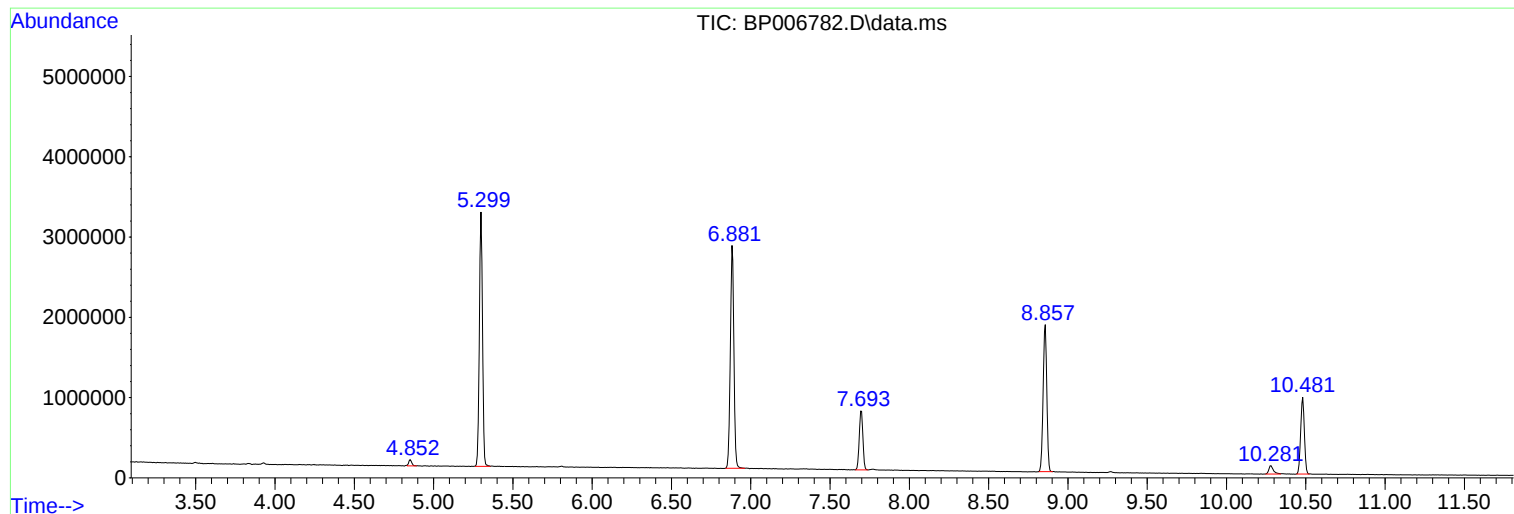

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081921\
Data File : BP006782.D
Acq On : 19 Aug 2021 15:45
Operator : CG/JU
Sample : M3434-15
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SWCS-12-1015

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP080321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081921\
Data File : BP006782.D
Acq On : 19 Aug 2021 15:45
Operator : CG/JU
Sample : M3434-15
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SWCS-12-1015

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP080321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
