

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081921\
 Data File : BP006786.D
 Acq On : 19 Aug 2021 18:03
 Operator : CG/JU
 Sample : M3397-18
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SWCS-06-0510

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP080321.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BP006786.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	4.846	295	299	306	rVB	108030	151223	2.94%	0.462%
2	5.299	370	376	391	rVB	1998508	2856594	55.56%	8.733%
3	6.881	638	645	657	rVB	1888017	2864146	55.71%	8.756%
4	7.693	777	783	791	rVB	589645	909567	17.69%	2.781%
5	8.852	973	980	988	rBV	1207492	1965042	38.22%	6.008%
6	10.281	1218	1223	1235	rVB2	43946	94552	1.84%	0.289%
7	10.475	1249	1256	1263	rBV	740371	1242237	24.16%	3.798%
8	12.957	1669	1678	1693	rBV	2519536	3671065	71.40%	11.223%
9	14.340	1904	1913	1921	rBV	943201	1494518	29.07%	4.569%
10	15.834	2159	2167	2188	rBV	1964906	2934081	57.07%	8.970%
11	17.092	2375	2381	2386	rBV	1202310	1727959	33.61%	5.283%
12	17.140	2386	2389	2395	rVB	116762	164231	3.19%	0.502%
13	18.004	2532	2536	2546	rVB2	162089	240888	4.69%	0.736%
14	18.157	2557	2562	2566	rBV2	37332	66194	1.29%	0.202%
15	19.116	2720	2725	2733	rBV	395169	546590	10.63%	1.671%
16	19.251	2744	2748	2754	rBV2	88019	142937	2.78%	0.437%
17	19.469	2777	2785	2790	rBV	356991	534763	10.40%	1.635%
18	19.681	2815	2821	2830	rVB	4204886	5141394	100.00%	15.718%
19	20.933	3030	3034	3040	rBV3	228980	365942	7.12%	1.119%
20	21.204	3073	3080	3084	rBV	1736511	2450540	47.66%	7.492%
21	21.239	3084	3086	3093	rVB	199034	231325	4.50%	0.707%
22	21.816	3181	3184	3186	rBV	87325	102820	2.00%	0.314%
23	22.822	3349	3355	3365	rBV3	207484	633605	12.32%	1.937%
24	23.510	3466	3472	3480	rBV2	1092555	2177086	42.34%	6.656%




Sum of corrected areas: 32709299

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081921\
Data File : BP006786.D
Acq On : 19 Aug 2021 18:03
Operator : CG/JU
Sample : M3397-18
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SWCS-06-0510

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP080321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

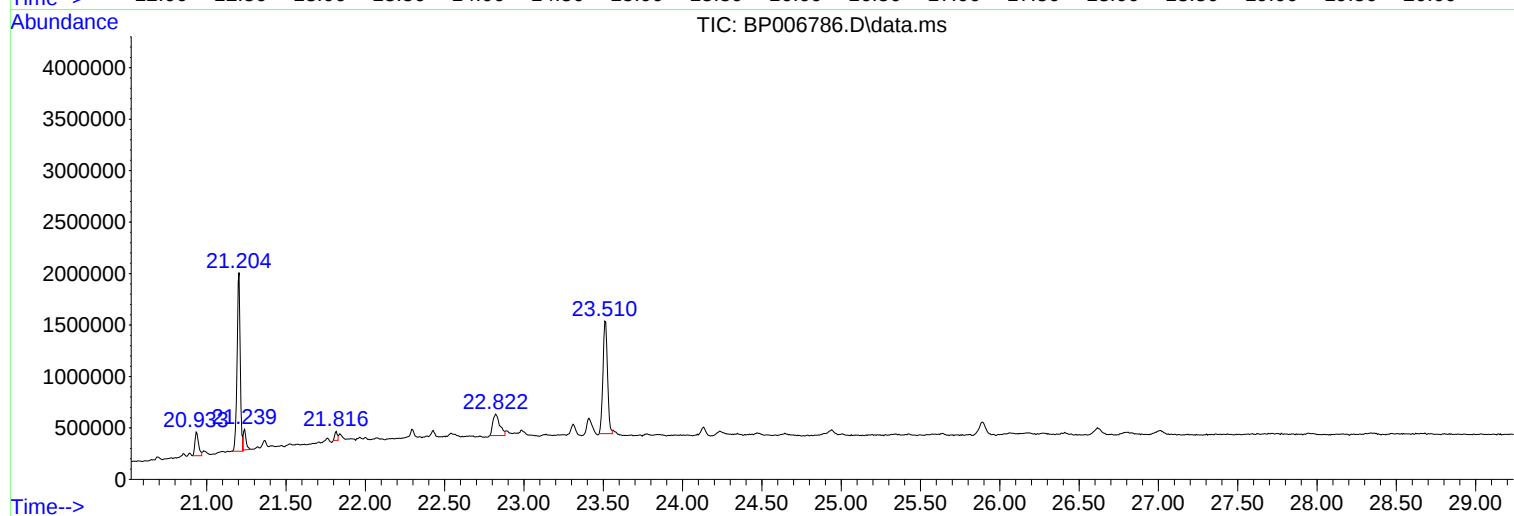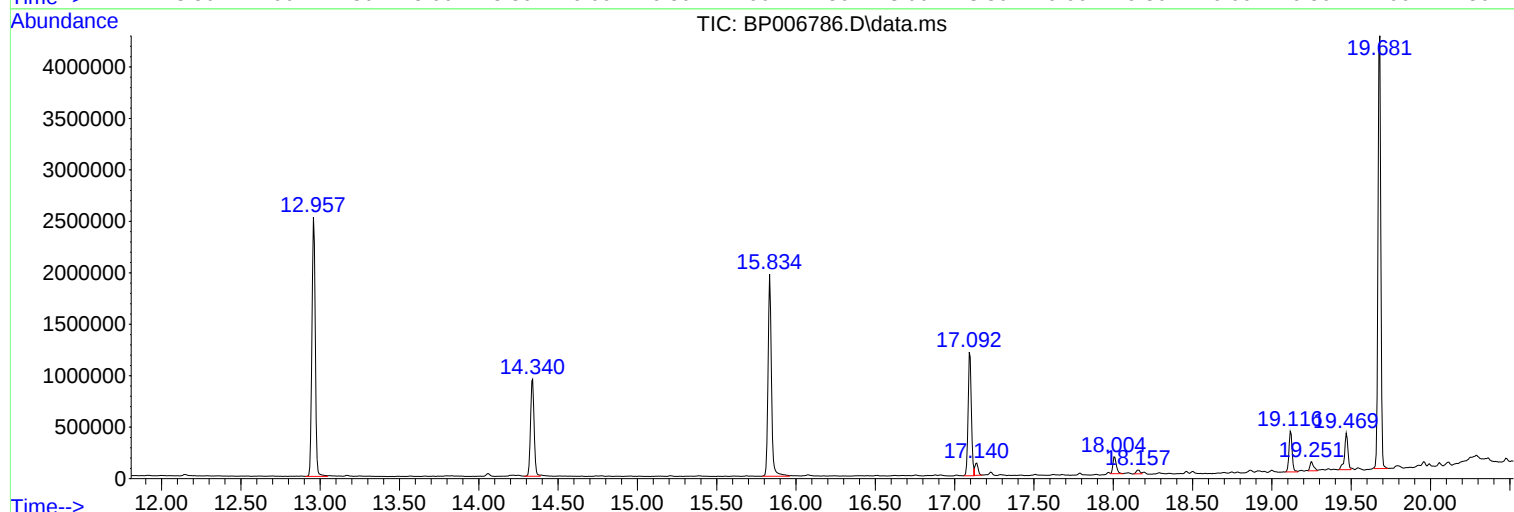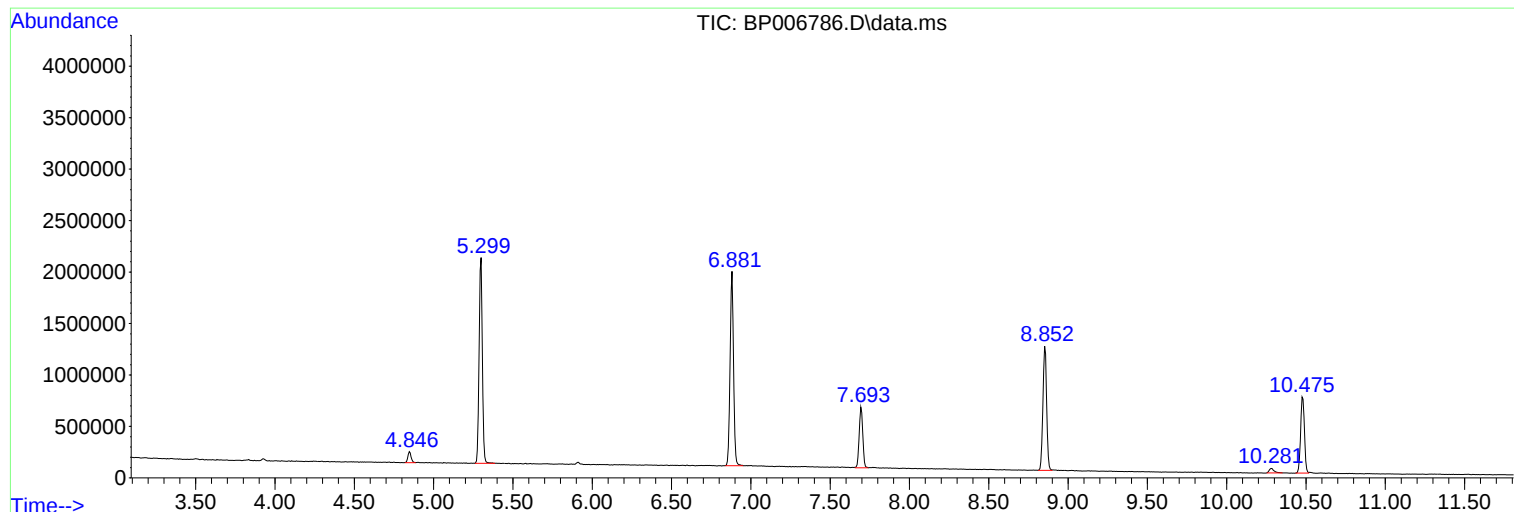

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081921\
Data File : BP006786.D
Acq On : 19 Aug 2021 18:03
Operator : CG/JU
Sample : M3397-18
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SWCS-06-0510

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP080321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081921\
Data File : BP006786.D
Acq On : 19 Aug 2021 18:03
Operator : CG/JU
Sample : M3397-18
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SWCS-06-0510

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP080321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
