


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081921\
 Data File : BP006770.D
 Acq On : 19 Aug 2021 08:38
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP080321.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Aug 20 11:25:25 2021

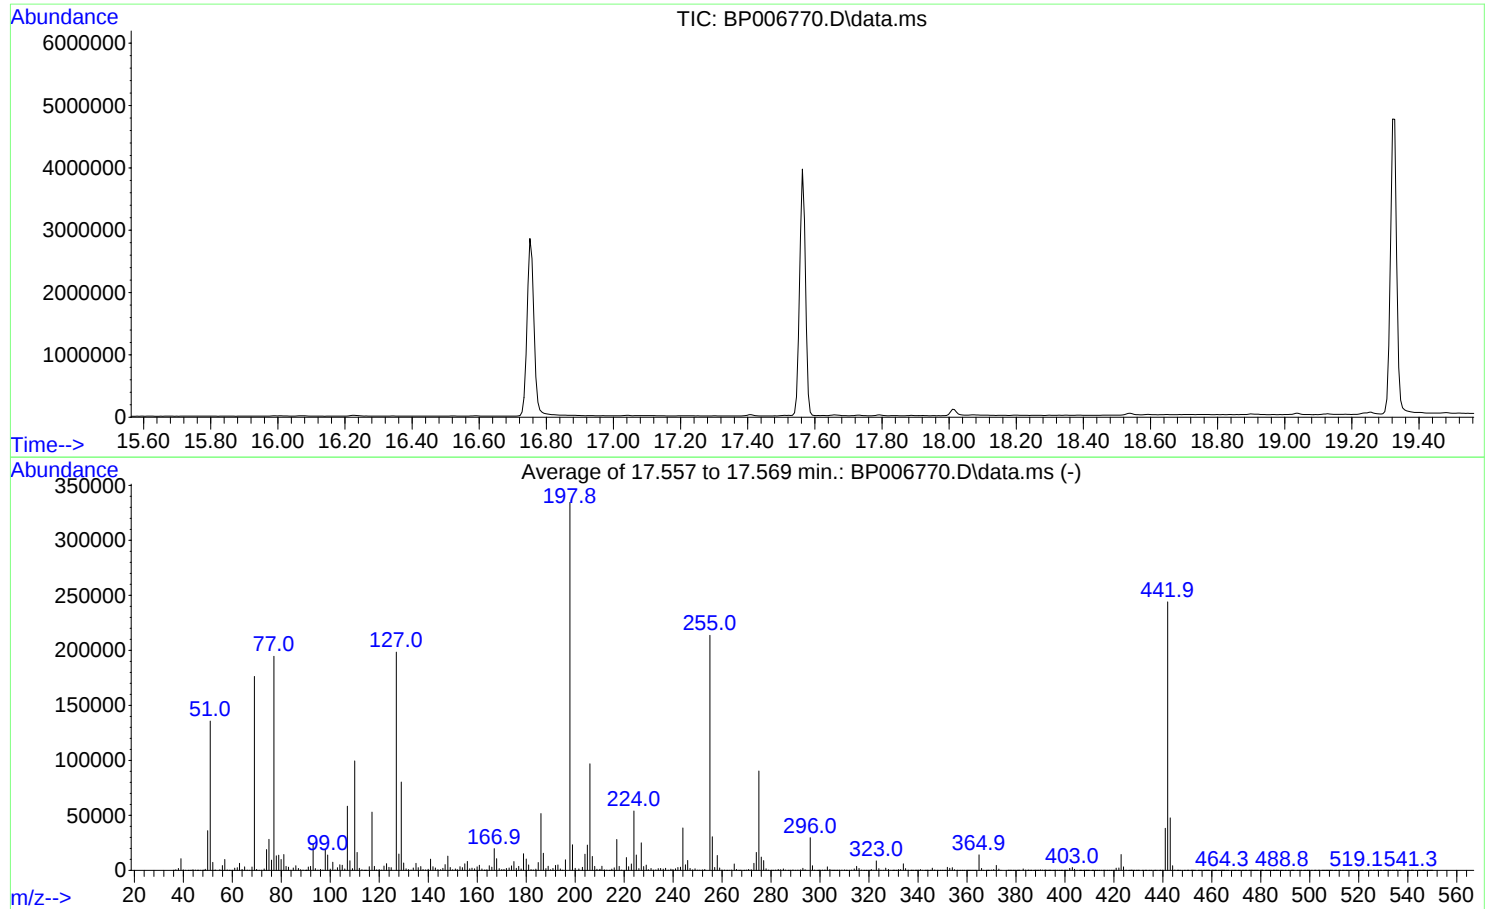




AutoFind: Scans 2460, 2461, 2462; Background Corrected with Scan 2448

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	40.6	135725	PASS
68	69	0.00	2	1.8	3127	PASS
69	198	0.00	100	52.7	176271	PASS
70	69	0.00	2	0.5	866	PASS
127	198	10	80	59.3	198408	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	334400	PASS
199	198	5	9	7.0	23317	PASS
275	198	10	60	27.0	90404	PASS
365	198	1	100	4.2	14114	PASS
441	198	0.01	100	11.5	38331	PASS
442	442	100	100	100.0	244151	PASS
443	442	15	24	19.6	47755	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081921\
Data File : BP006770.D
Acq On : 19 Aug 2021 08:38
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: Aug 19 11:03:18 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP080321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Aug 16 18:17:59 2021
Response via : Initial Calibration

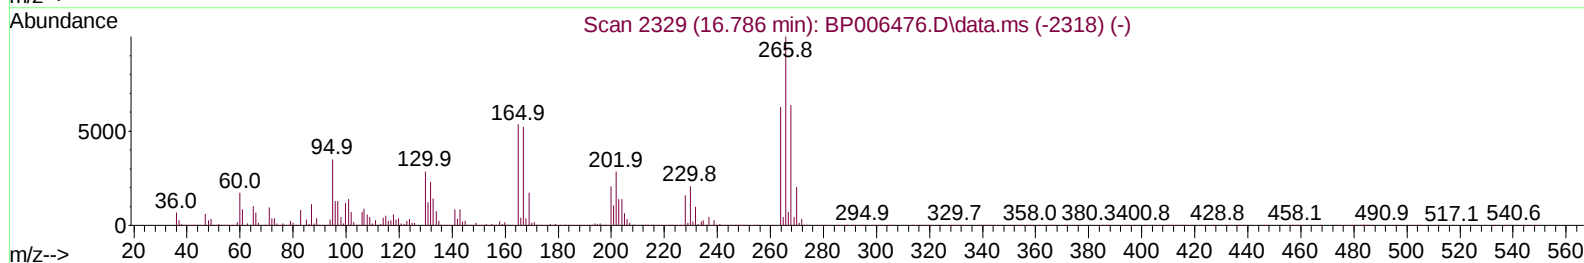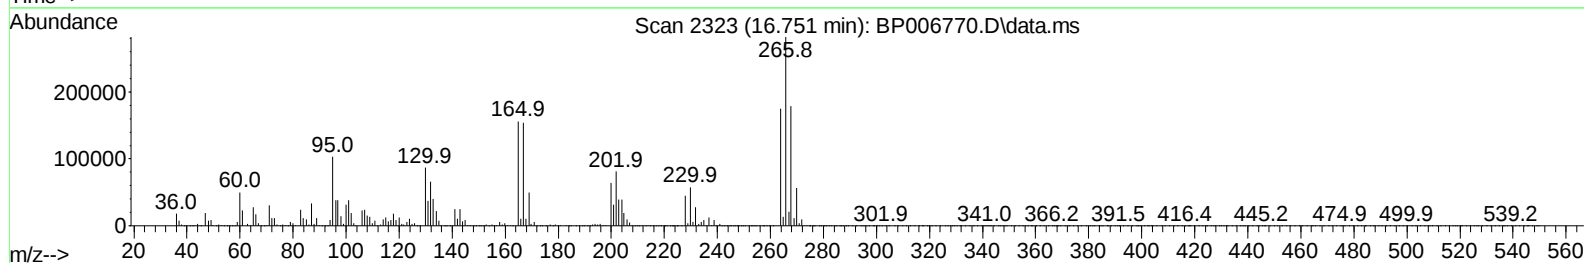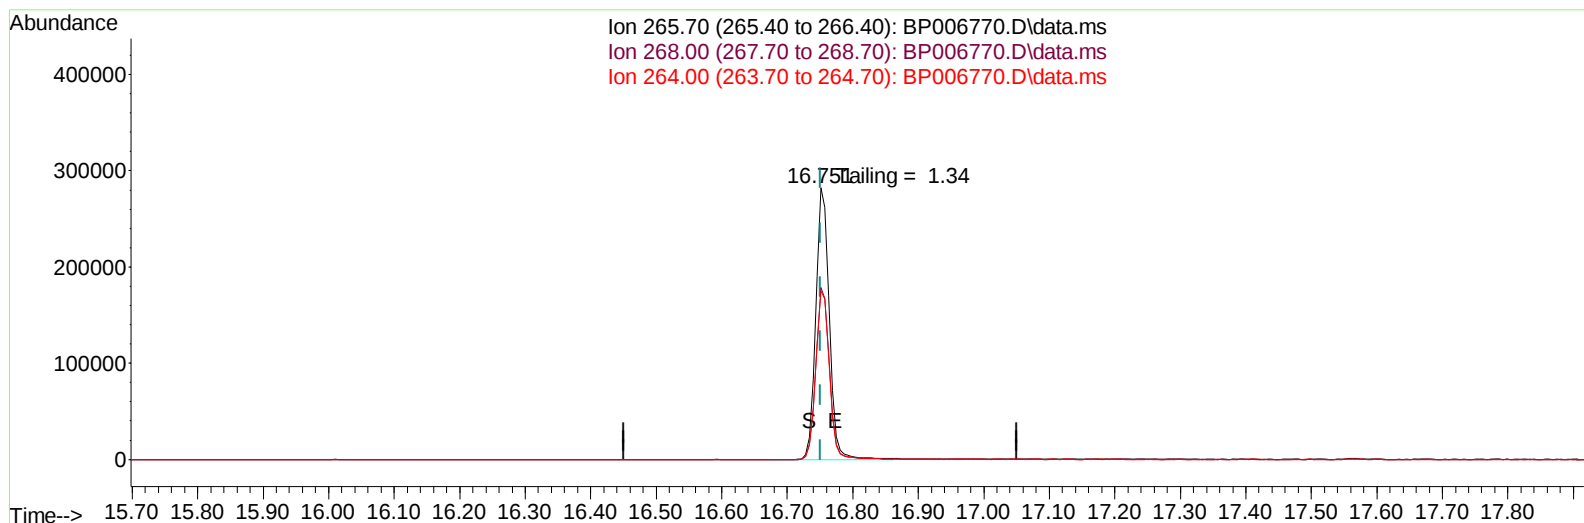

TIC: BP006770.D\data.ms

(70) Pentachlorophenol (C)

16.751min (+ 0.000) 23434.57 ng




response 407821

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.50	63.38
264.00	62.90	62.16
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081921\
 Data File : BP006770.D
 Acq On : 19 Aug 2021 08:38
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Quant Time: Aug 19 11:03:18 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP080321.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Aug 16 18:17:59 2021
 Response via : Initial Calibration

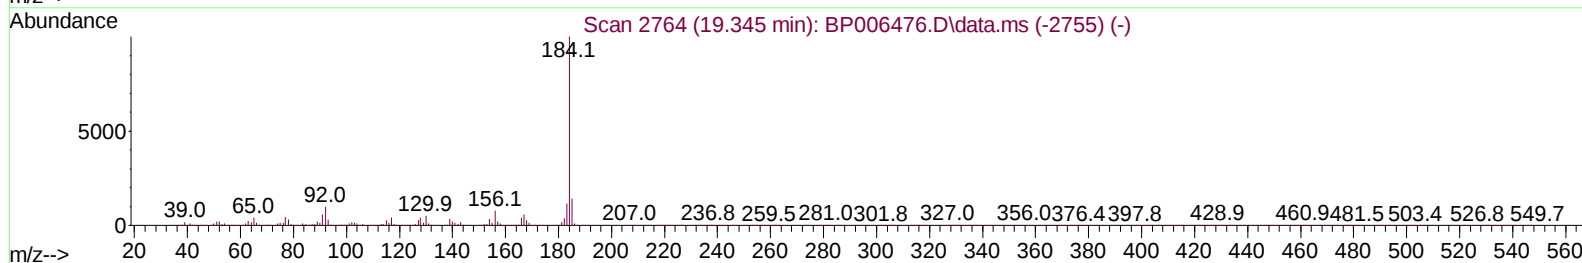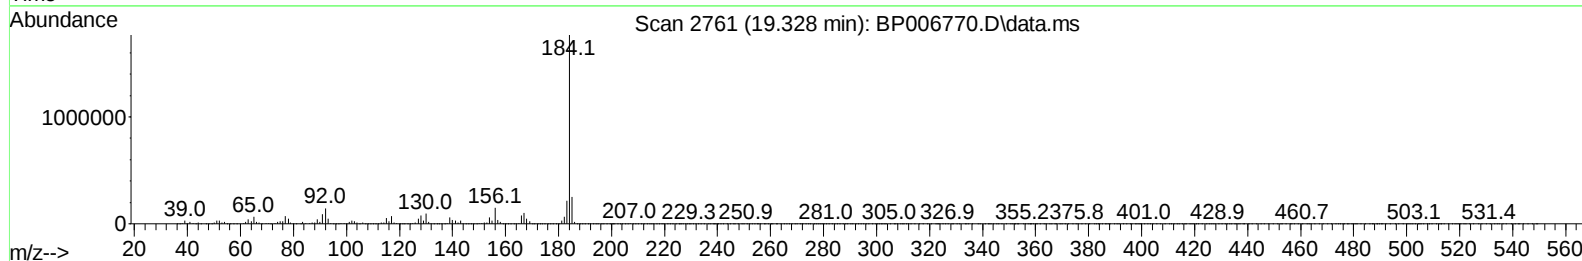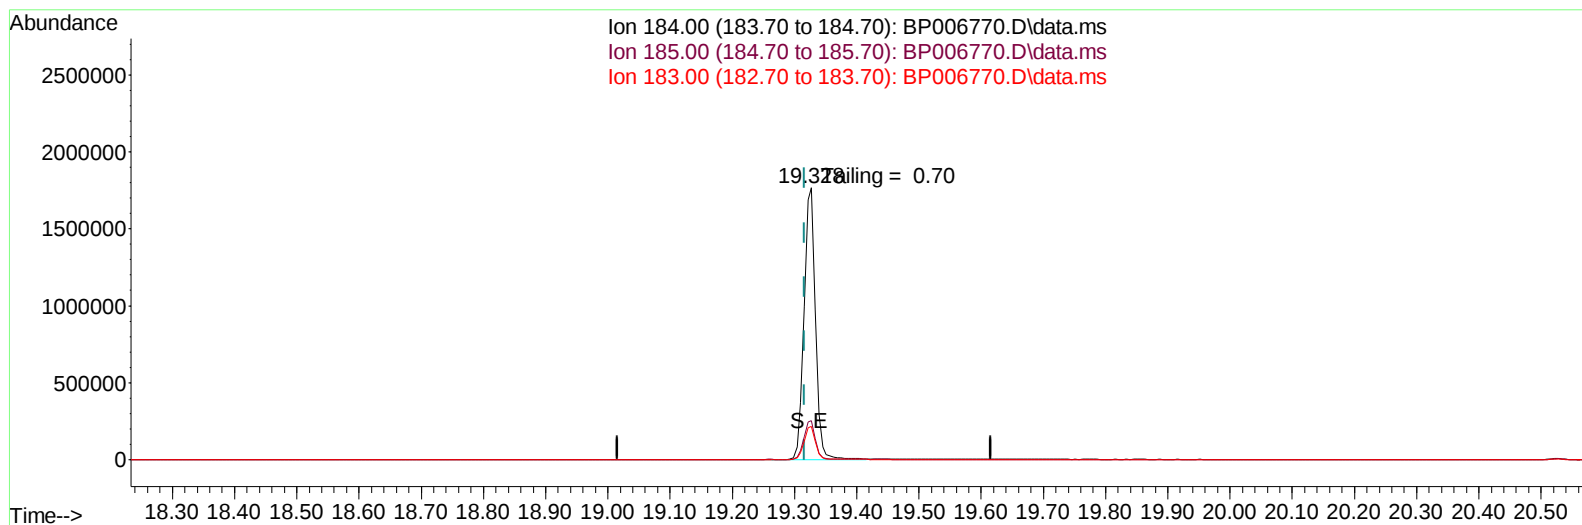

TIC: BP006770.D\data.ms

(77) Benzidine

19.328min (+ 0.012) 9850.40 ng

response 2277565

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.70	14.28
183.00	11.90	12.21
0.00	0.00	0.00

DDT Breakdown

Instrument :
BNA_P
ClientSampleId :
DFTPP

Date	Instrument Name	DFTPP Data File
8/19/2021	BNA_P	BP006770.D
Compound Name	Response	Retention Time
DDT	1134219	20.52
DDD	17030	20.09
DDE	2105	19.59
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
19135	1153354	1.66

Instrument :
BNA_P
ClientSampleId :
DFTPP