

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081922\
 Data File : BP011520.D
 Acq On : 19 Aug 2022 22:59
 Operator : CG/JU
 Sample : N4221-13DL 10X
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :

Quant Time: Aug 20 04:42:26 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP081622.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Aug 17 01:58:37 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.552	152	107803	20.000	ng/u1	0.00
20) Naphthalene-d8	10.340	136	449804	20.000	ng/u1	-0.01
38) Acenaphthene-d10	14.228	164	254044	20.000	ng/u1	0.00
64) Phenanthrene-d10	16.998	188	498189	20.000	ng/u1	0.00
79) Chrysene-d12	21.121	240	484210	20.000	ng/u1	-0.01
88) Perylene-d12	23.410	264	516603	20.000	ng/u1	-0.02
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.028	96	30823	8.873	ng/uL	-0.04
4) Pyridine-d5	3.487	84	384	0.043	ng/u1	0.00
7) Phenol-d5	6.746	99	4396	0.444	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	6.905	67	15151	2.354	ng/u1	0.00
11) 2-Chlorophenol-d4	7.087	132	13669	1.876	ng/u1	0.00
15) 4-Methylphenol-d8	8.281	113	6559	0.827	ng/u1	0.00
21) Nitrobenzene-d5	8.722	128	7122	2.199	ng/u1	0.00
24) 2-Nitrophenol-d4	9.440	143	6544	1.986	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	9.975	165	10871	1.787	ng/u1	0.00
31) 4-Chloroaniline-d4	10.504	131	10688	1.055	ng/u1	0.00
46) Dimethylphthalate-d6	13.651	166	47278	2.631	ng/u1	0.00
49) Acenaphthylene-d8	13.916	160	46164	2.312	ng/u1	0.00
54) 4-Nitrophenol-d4	14.545	143	184	0.053	ng/u1	0.08
60) Fluorene-d10	15.228	176	38462	2.544	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.369	200	3791	1.408	ng/u1	0.00
73) Anthracene-d10	17.098	188	66065	2.994	ng/u1	0.00
81) Pyrene-d10	19.357	212	71481	2.918	ng/u1	0.00
92) Benzo(a)pyrene-d12	23.262	264	70849	2.819	ng/u1	-0.02
Target Compounds						
2) 1,4-Dioxane	3.105	88	39249	10.835	ng/uL	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081922\
Data File : BP011520.D
Acq On : 19 Aug 2022 22:59
Operator : CG/JU
Sample : N4221-13DL 10X
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :


Quant Time: Aug 20 04:42:26 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP081622.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Aug 17 01:58:37 2022
Response via : Initial Calibration

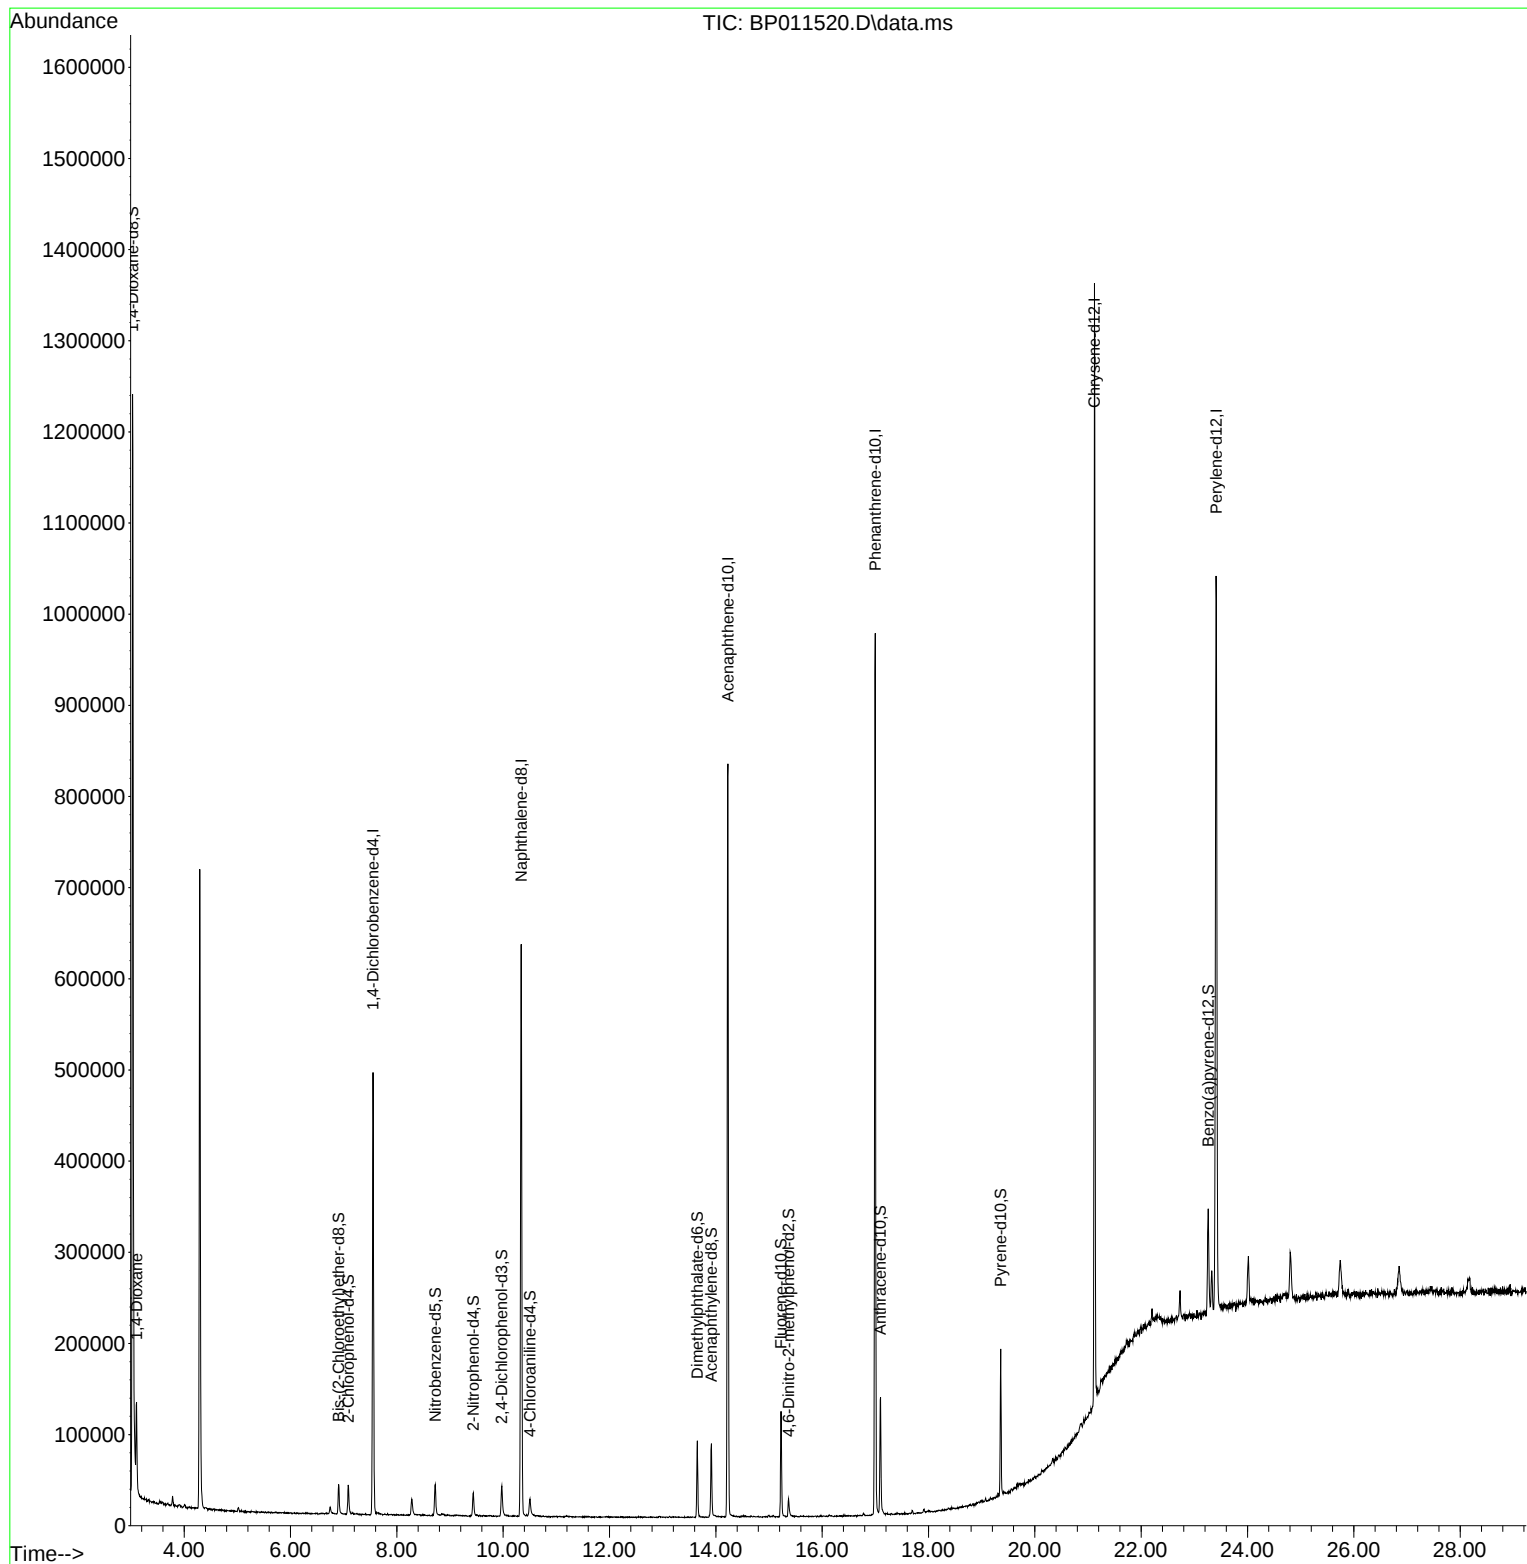

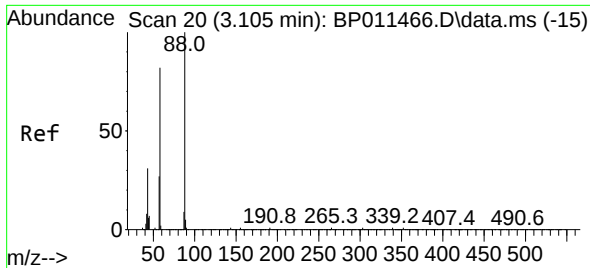

#2
 1,4-Dioxane
 Concen: 10.835 ng/uL
 RT: 3.105 min Scan# 20
 Delta R.T. -0.000 min
 Lab File: BP011520.D
 Acq: 19 Aug 2022 22:59

Instrument :
 BNA_P
 ClientSampleId :

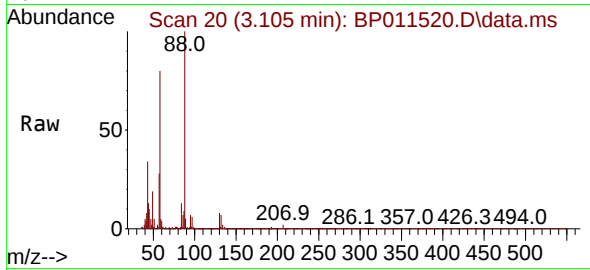

Tgt Ion: 88 Resp: 39249
 Ion Ratio Lower Upper
 88 100
 43 33.6 29.0 43.4
 58 79.6 64.7 97.1

