

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081922\
 Data File : BP011500.D
 Acq On : 19 Aug 2022 10:06
 Operator : CG/JU
 Sample : PB147110BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK110

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP081622.M
 Title : SVOA CALIBRATION

Signal : TIC: BP011500.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.070	11	14	20	rVB	38266	44418	2.75%	0.221%
2	3.476	81	83	100	rBV	403657	594990	36.85%	2.960%
3	3.781	132	135	138	rBV2	6485	8063	0.50%	0.040%
4	4.334	227	229	233	rVB5	2357	2548	0.16%	0.013%
5	4.370	233	235	238	rBV4	1434	1810	0.11%	0.009%
6	5.117	360	362	365	rVB4	1711	1735	0.11%	0.009%
7	6.740	631	638	656	rBV	424271	666756	41.29%	3.317%
8	6.905	660	666	677	rVB	321145	487752	30.21%	2.426%
9	7.087	690	697	707	rBV	442185	673512	41.71%	3.350%
10	7.469	760	762	765	rBV3	1304	1855	0.11%	0.009%
11	7.552	770	776	789	rVV	370326	581721	36.03%	2.894%
12	8.275	892	899	916	rBV	486871	772943	47.87%	3.845%
13	8.528	940	942	945	rVB3	1385	1746	0.11%	0.009%
14	8.716	967	974	989	rBV	397173	639518	39.61%	3.181%
15	8.911	1005	1007	1010	rVB4	1506	1656	0.10%	0.008%
16	9.434	1088	1096	1110	rBV	318992	521459	32.29%	2.594%
17	9.969	1180	1187	1197	rBV	448823	720859	44.64%	3.586%
18	10.340	1242	1250	1259	rBV	469945	767001	47.50%	3.815%
19	10.493	1267	1276	1299	rBV	410992	752655	46.61%	3.744%
20	11.469	1437	1442	1446	rBV7	1101	1915	0.12%	0.010%
21	11.769	1490	1493	1495	rVB4	1439	1654	0.10%	0.008%
22	11.952	1517	1524	1534	rBV4	5587	13020	0.81%	0.065%
23	13.193	1731	1735	1737	rBV4	1802	2037	0.13%	0.010%
24	13.246	1741	1744	1748	rVB6	1215	1989	0.12%	0.010%
25	13.651	1806	1813	1827	rBV	690671	960140	59.46%	4.776%
26	13.916	1851	1858	1874	rBV	757585	1090540	67.54%	5.425%
27	14.228	1903	1911	1920	rBV	617109	863642	53.49%	4.296%
28	14.457	1944	1950	1970	rBV	247063	463761	28.72%	2.307%
29	15.234	2075	2082	2092	rBV	923566	1296430	80.29%	6.449%
30	15.369	2098	2105	2118	rBV	317565	441674	27.35%	2.197%
31	15.475	2118	2123	2128	rVB7	4469	8096	0.50%	0.040%
32	15.810	2177	2180	2183	rVB5	1873	1858	0.12%	0.009%
33	16.016	2212	2215	2219	rVB5	1146	1770	0.11%	0.009%
34	16.145	2233	2237	2241	rBV7	1706	2991	0.19%	0.015%
35	16.681	2323	2328	2332	rBV8	1315	2198	0.14%	0.011%
36	16.781	2342	2345	2348	rBV5	1744	1942	0.12%	0.010%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081922\
 Data File : BP011500.D
 Acq On : 19 Aug 2022 10:06
 Operator : CG/JU
 Sample : PB147110BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK110

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP081622.M
 Title : SVOA CALIBRATION

37	16.998	2376	2382	2392	rBV	695535	956553	59.24%	4.758%
38	17.098	2393	2399	2416	rVB	989790	1396901	86.51%	6.948%
39	17.398	2445	2450	2452	rBV6	1426	2443	0.15%	0.012%
40	17.692	2496	2500	2507	rBV9	2135	5935	0.37%	0.030%
41	17.781	2513	2515	2520	rBV6	1054	1658	0.10%	0.008%
42	18.939	2708	2712	2717	rBV2	11230	14345	0.89%	0.071%
43	19.010	2720	2724	2728	rVV2	10936	14512	0.90%	0.072%
44	19.363	2778	2784	2792	rBV	1196651	1533917	95.00%	7.630%
45	21.133	3080	3085	3091	rBV	823880	1034952	64.10%	5.148%
46	23.274	3443	3449	3458	rBV2	868353	1614679	100.00%	8.032%
47	23.427	3468	3475	3487	rVB2	579467	1129085	69.93%	5.616%




Sum of corrected areas: 20103634

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081922\
Data File : BP011500.D
Acq On : 19 Aug 2022 10:06
Operator : CG/JU
Sample : PB147110BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK110

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP081622.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

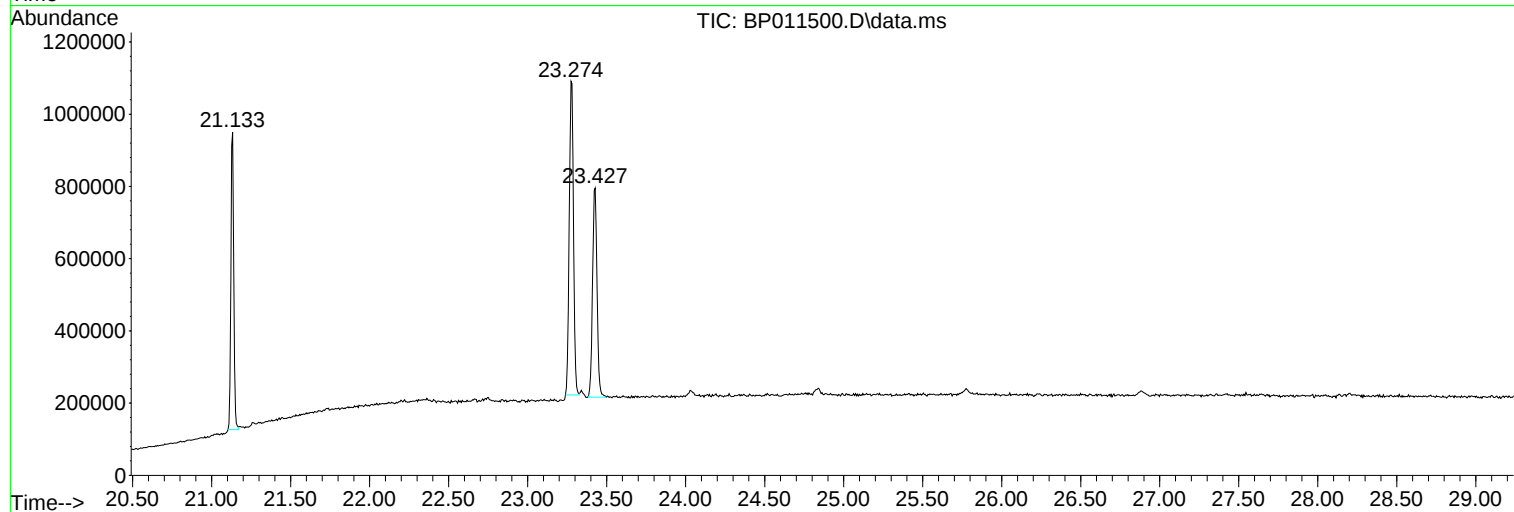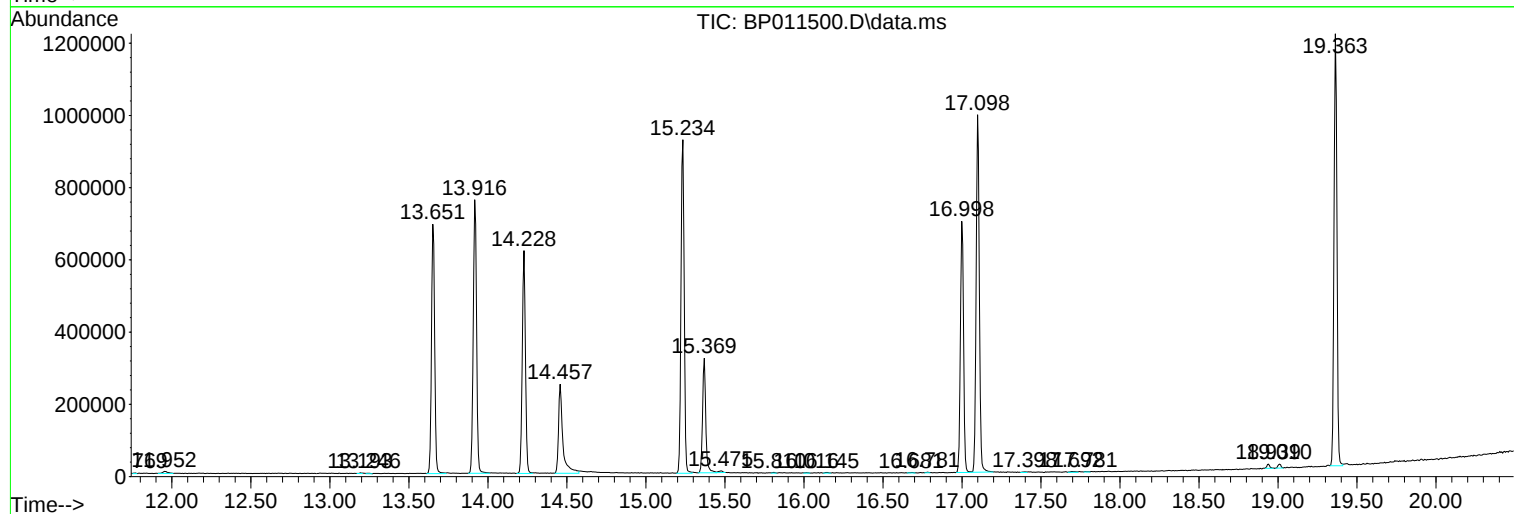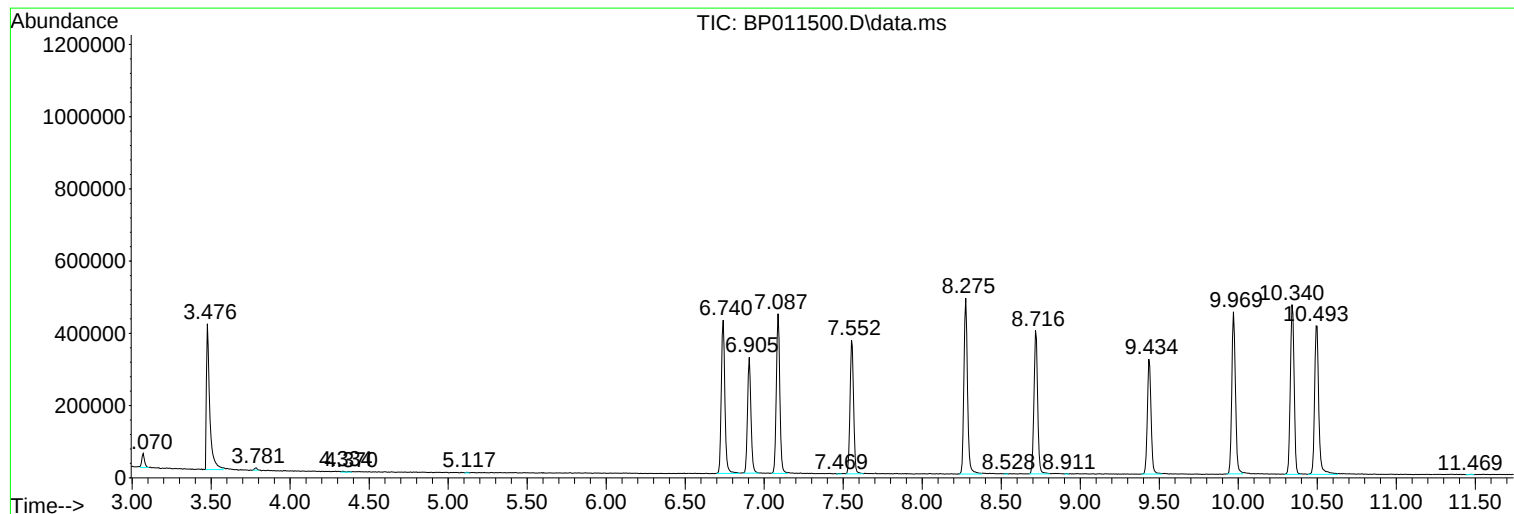

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081922\
Data File : BP011500.D
Acq On : 19 Aug 2022 10:06
Operator : CG/JU
Sample : PB147110BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK110

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP081622.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081922\
Data File : BP011500.D
Acq On : 19 Aug 2022 10:06
Operator : CG/JU
Sample : PB147110BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK110

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP081622.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------