

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081922\
 Data File : BP011510.D
 Acq On : 19 Aug 2022 16:37
 Operator : CG/JU
 Sample : N4221-08
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0KQ0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP081622.M
 Title : SVOA CALIBRATION

Signal : TIC: BP011510.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.070	11	14	24	rVB	28757	39382	2.33%	0.182%
2	3.352	60	62	71	rVB	15496	24054	1.42%	0.111%
3	3.487	82	85	104	rVB	150244	233053	13.77%	1.074%
4	3.693	117	120	125	rVB	7782	10213	0.60%	0.047%
5	3.781	132	135	142	rVB2	9584	14605	0.86%	0.067%
6	4.152	196	198	201	rBV3	2973	3160	0.19%	0.015%
7	4.858	315	318	320	rBV4	1860	2046	0.12%	0.009%
8	5.222	377	380	383	rBV5	1328	1960	0.12%	0.009%
9	5.299	391	393	396	rVB4	2075	2383	0.14%	0.011%
10	5.340	396	400	402	rBV5	1638	2674	0.16%	0.012%
11	5.652	450	453	456	rVB5	1567	1957	0.12%	0.009%
12	5.975	504	508	510	rBV4	1856	2232	0.13%	0.010%
13	6.240	549	553	555	rVB5	1611	2190	0.13%	0.010%
14	6.369	573	575	578	rBV4	1430	1969	0.12%	0.009%
15	6.746	633	639	649	rBV	358283	578725	34.19%	2.668%
16	6.905	659	666	677	rBV	280037	427317	25.25%	1.970%
17	6.999	679	682	686	rVV2	3851	5264	0.31%	0.024%
18	7.087	691	697	705	rBV	365943	573938	33.91%	2.646%
19	7.269	726	728	732	rVB5	1557	1913	0.11%	0.009%
20	7.558	770	777	786	rBV	426887	659616	38.97%	3.041%
21	7.634	786	790	795	rVV5	4205	8758	0.52%	0.040%
22	7.681	797	798	803	rVB5	2111	2819	0.17%	0.013%
23	7.922	837	839	842	rVB4	1514	1750	0.10%	0.008%
24	8.281	891	900	916	rBV	432969	727189	42.96%	3.352%
25	8.722	966	975	984	rBV	358101	572457	33.82%	2.639%
26	8.852	993	997	1001	rBV6	3302	5615	0.33%	0.026%
27	8.893	1001	1004	1007	rVB5	2601	3313	0.20%	0.015%
28	8.952	1012	1014	1020	rVB7	1218	2144	0.13%	0.010%
29	9.122	1040	1043	1047	rVB6	3870	5673	0.34%	0.026%
30	9.187	1052	1054	1059	rVB6	1447	2442	0.14%	0.011%
31	9.240	1059	1063	1066	rBV6	1617	2430	0.14%	0.011%
32	9.440	1089	1097	1107	rBV	289545	482731	28.52%	2.225%
33	9.605	1121	1125	1128	rBV6	1580	2523	0.15%	0.012%
34	9.675	1134	1137	1140	rBV5	1415	1853	0.11%	0.009%
35	9.975	1181	1188	1203	rBV	412710	700431	41.38%	3.229%
36	10.346	1241	1251	1259	rBV	548591	904884	53.46%	4.171%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081922\
 Data File : BP011510.D
 Acq On : 19 Aug 2022 16:37
 Operator : CG/JU
 Sample : N4221-08
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0KQ0

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0.1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP081622.M
 Title : SVOA CALIBRATION

37	10.499	1265	1277	1293	rBV	398929	711164	42.02%	3.278%
38	10.846	1331	1336	1342	rBV8	4160	9204	0.54%	0.042%
39	10.922	1346	1349	1352	rVB5	1458	1726	0.10%	0.008%
40	11.169	1389	1391	1394	rBV3	1941	2344	0.14%	0.011%
41	11.622	1461	1468	1470	rBV7	2372	4003	0.24%	0.018%
42	11.951	1517	1524	1530	rBV4	8258	15895	0.94%	0.073%
43	12.575	1626	1630	1635	rBV8	1921	3020	0.18%	0.014%
44	12.834	1668	1674	1676	rBV7	2221	3685	0.22%	0.017%
45	13.057	1707	1712	1717	rVB5	2839	5099	0.30%	0.024%
46	13.128	1722	1724	1729	rVV6	2017	3065	0.18%	0.014%
47	13.198	1729	1736	1742	rVB6	2867	6942	0.41%	0.032%
48	13.469	1779	1782	1784	rBV4	1652	2217	0.13%	0.010%
49	13.657	1807	1814	1823	rBV	755302	1032307	60.99%	4.759%
50	13.763	1830	1832	1838	rVB7	1714	2105	0.12%	0.010%
51	13.857	1842	1848	1849	rBV6	1369	2185	0.13%	0.010%
52	13.922	1849	1859	1870	rBV	830124	1200641	70.94%	5.535%
53	14.004	1870	1873	1878	rVB7	1837	3660	0.22%	0.017%
54	14.140	1893	1896	1902	rVB8	3068	4312	0.25%	0.020%
55	14.228	1904	1911	1930	rVB	728848	1098909	64.92%	5.066%
56	14.404	1938	1941	1945	rBV6	1936	2373	0.14%	0.011%
57	14.463	1945	1951	1967	rBV	275705	500928	29.60%	2.309%
58	14.675	1984	1987	1995	rVB7	6937	11500	0.68%	0.053%
59	15.004	2039	2043	2047	rVV6	3022	4535	0.27%	0.021%
60	15.051	2047	2051	2054	rVV4	3033	4625	0.27%	0.021%
61	15.104	2057	2060	2065	rVB6	3814	5288	0.31%	0.024%
62	15.234	2075	2082	2094	rBV	1025532	1451217	85.74%	6.690%
63	15.369	2099	2105	2116	rVV	264964	383015	22.63%	1.766%
64	15.475	2119	2123	2130	rVB10	5840	11740	0.69%	0.054%
65	15.810	2178	2180	2182	rBV3	2470	1893	0.11%	0.009%
66	15.975	2204	2208	2213	rVB6	4861	7994	0.47%	0.037%
67	16.145	2232	2237	2243	rBV10	2963	7011	0.41%	0.032%
68	16.410	2277	2282	2284	rBV5	1545	2314	0.14%	0.011%
69	16.539	2300	2304	2305	rBV4	1757	2152	0.13%	0.010%
70	16.781	2341	2345	2350	rBV7	4750	7705	0.46%	0.036%
71	16.892	2359	2364	2369	rBV3	10166	15927	0.94%	0.073%
72	16.945	2371	2373	2376	rVV4	2445	2265	0.13%	0.010%
73	17.004	2376	2383	2393	rVV	866860	1208621	71.41%	5.572%
74	17.104	2393	2400	2413	rVV	1089111	1555540	91.90%	7.171%
75	17.222	2415	2420	2425	rVB8	15412	23312	1.38%	0.107%
76	17.281	2427	2430	2432	rBV4	2836	3713	0.22%	0.017%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081922\
 Data File : BP011510.D
 Acq On : 19 Aug 2022 16:37
 Operator : CG/JU
 Sample : N4221-08
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0KQ0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP081622.M
 Title : SVOA CALIBRATION

77	17.310	2433	2435	2438	rVB4	3076	3334	0.20%	0.015%
78	17.704	2497	2502	2509	rVB	37022	45999	2.72%	0.212%
79	17.922	2534	2539	2547	rBV2	34038	54218	3.20%	0.250%
80	18.333	2607	2609	2612	rVB3	5408	4897	0.29%	0.023%
81	18.939	2709	2712	2715	rVB4	13361	16228	0.96%	0.075%
82	19.004	2721	2723	2729	rVB	12421	16449	0.97%	0.076%
83	19.363	2779	2784	2793	rBV	1301890	1692584	100.00%	7.803%
84	20.869	3035	3040	3048	rBV	189170	349726	20.66%	1.612%
85	21.133	3080	3085	3090	rBV	1011185	1252417	73.99%	5.773%
86	23.280	3443	3450	3457	rBV2	901338	1670866	98.72%	7.702%
87	23.427	3469	3475	3483	rVB2	659980	1244142	73.51%	5.735%




Sum of corrected areas: 21692674

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081922\
Data File : BP011510.D
Acq On : 19 Aug 2022 16:37
Operator : CG/JU
Sample : N4221-08
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0KQ0

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP081622.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

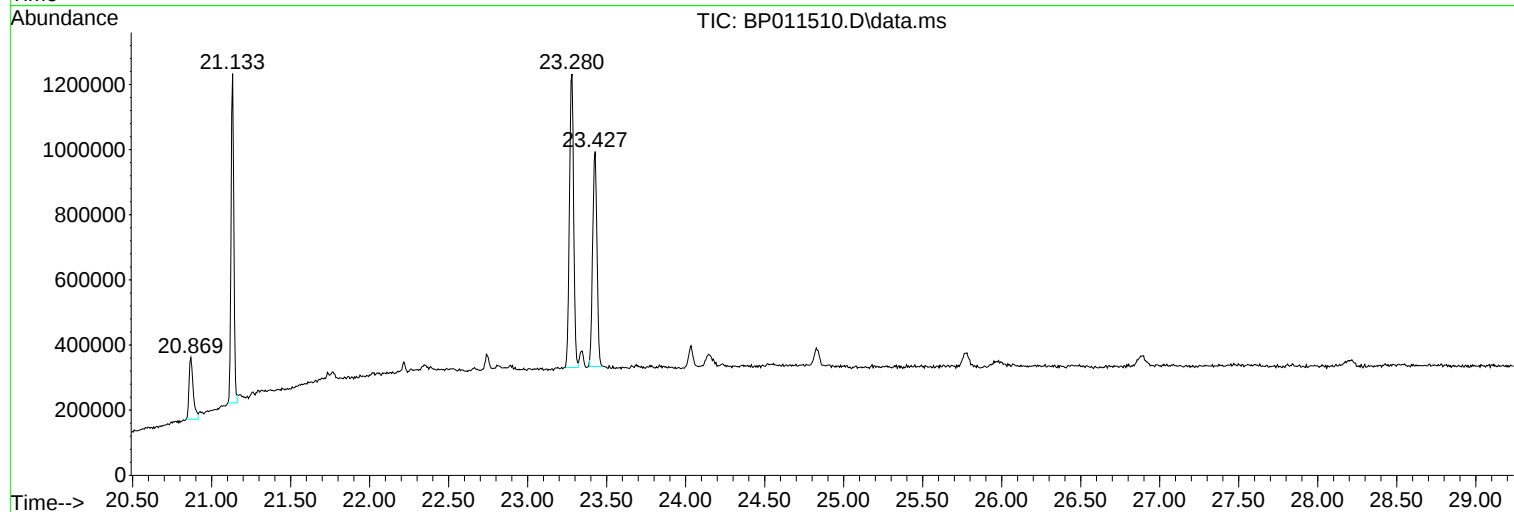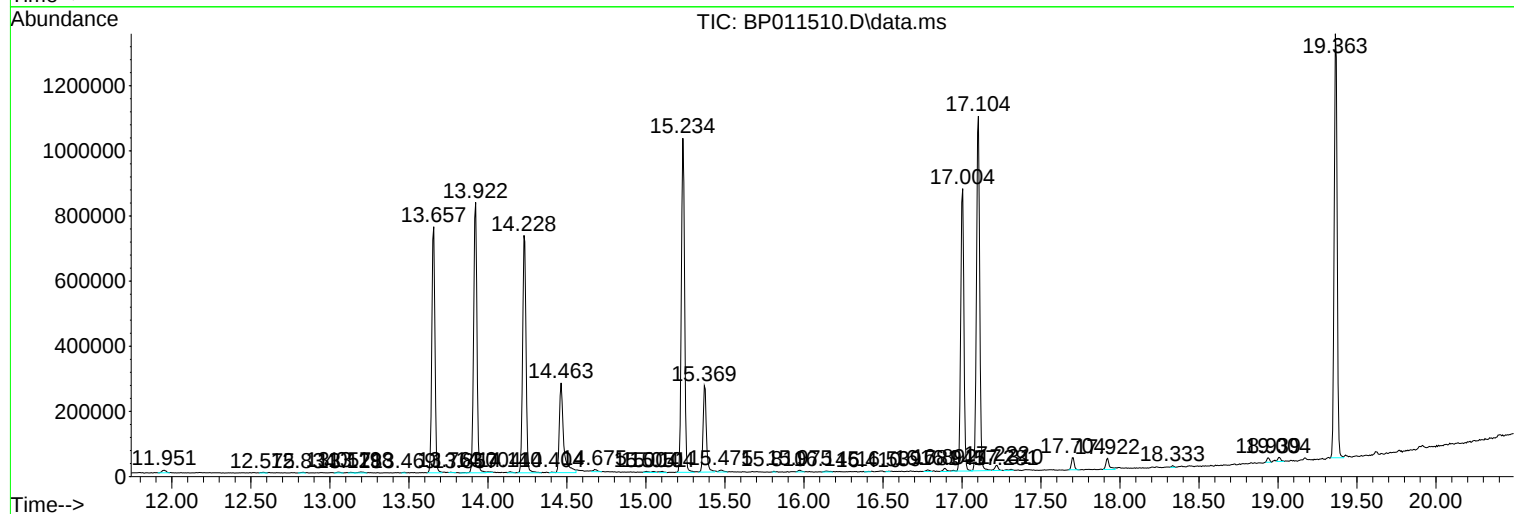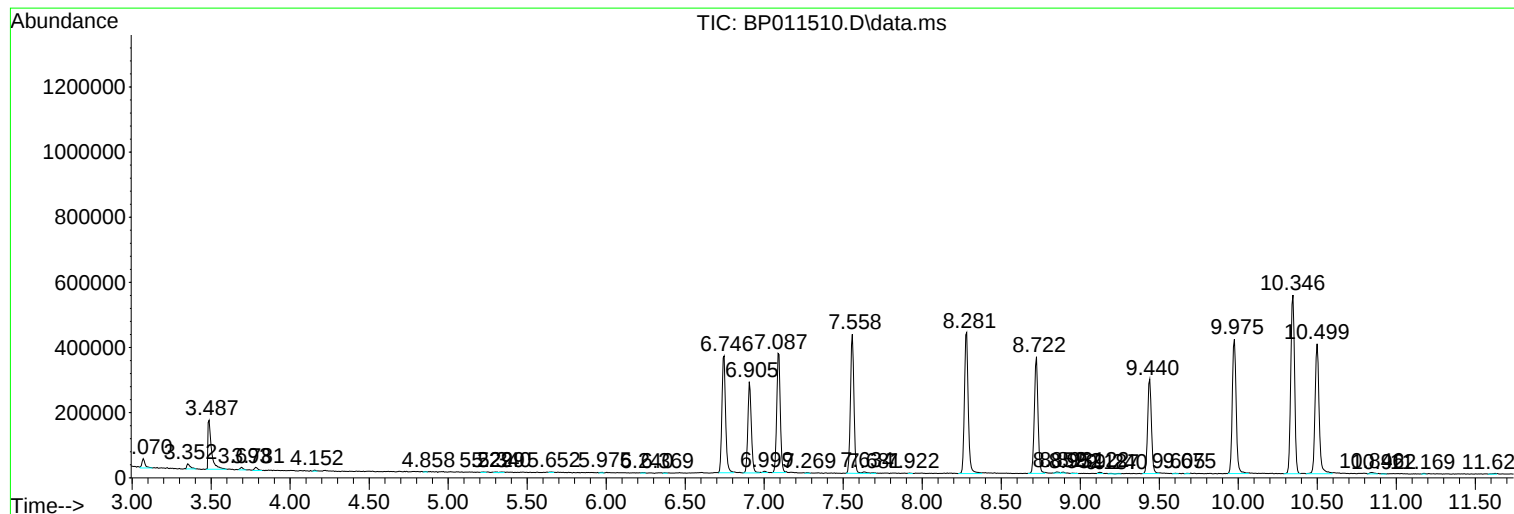

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081922\
Data File : BP011510.D
Acq On : 19 Aug 2022 16:37
Operator : CG/JU
Sample : N4221-08
Misc :
ALS Vial : 13 Sample Multiplier: 1










Instrument :
BNA_P
ClientSampleId :
C0KQ0

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP081622.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 (DEL) Alkane: Straight-Chai... Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD		R.T.	
20.869	5.58 ng/ul	349726	Chrysene-d12		21.133	
Hit# of 5	Tentative ID		MW	MolForm	CAS#	Qual
1	1-Tricosene		322	C23H46	018835-32-0	98
2	1-Nonadecene		266	C19H38	018435-45-5	96
3	1-Hexacosene		364	C26H52	018835-33-1	94
4	Heptacos-1-ene		378	C27H54	015306-27-1	94
5	1-Heneicosanol		312	C21H44O	015594-90-8	94

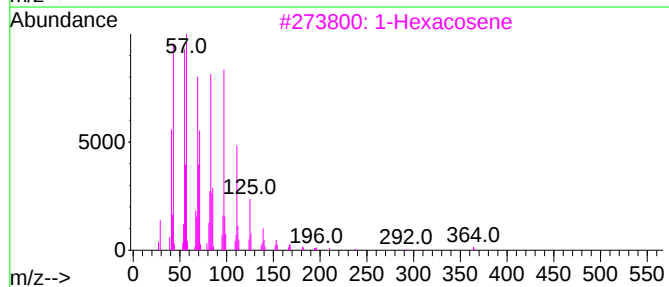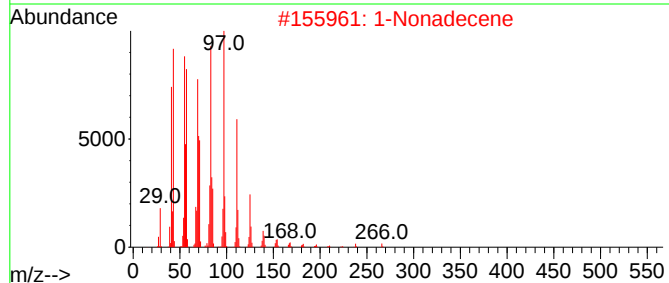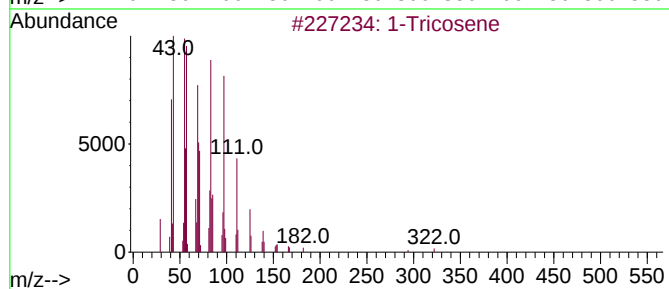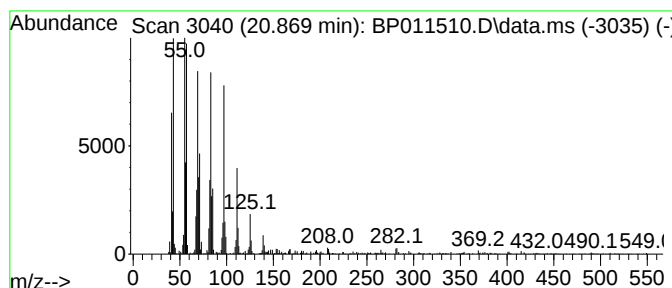

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081922\
Data File : BP011510.D
Acq On : 19 Aug 2022 16:37
Operator : CG/JU
Sample : N4221-08
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0KQ0

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP081622.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
(DEL) Alkane: S...	20.869	5.6	ng/u1	349726	5	21.133	1252420	20.0