

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081922\
 Data File : BP011511.D
 Acq On : 19 Aug 2022 17:12
 Operator : CG/JU
 Sample : N4221-04
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0KP5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP081622.M
 Title : SVOA CALIBRATION

Signal : TIC: BP011511.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.069	11	14	25	rVB	27099	37654	2.37%	0.179%
2	3.352	59	62	73	rVB	15898	26725	1.68%	0.127%
3	3.487	82	85	100	rBV	123338	190292	11.97%	0.905%
4	3.693	117	120	125	rVB	9050	12171	0.77%	0.058%
5	3.781	132	135	142	rVB2	11075	16255	1.02%	0.077%
6	4.222	206	210	214	rVB7	3118	5704	0.36%	0.027%
7	4.293	220	222	225	rBV4	1980	2227	0.14%	0.011%
8	4.764	300	302	305	rBV4	1409	1935	0.12%	0.009%
9	5.440	414	417	420	rVB5	1221	1726	0.11%	0.008%
10	5.640	448	451	455	rBV6	1219	2094	0.13%	0.010%
11	5.681	455	458	462	rVB5	1772	2260	0.14%	0.011%
12	6.052	519	521	525	rBV5	1652	1622	0.10%	0.008%
13	6.699	627	631	632	rBV4	1568	1860	0.12%	0.009%
14	6.740	632	638	650	rBV	370319	597168	37.57%	2.840%
15	6.905	660	666	674	rBV	287521	433880	27.30%	2.064%
16	6.999	678	682	690	rVB3	2737	6619	0.42%	0.031%
17	7.087	690	697	710	rBV	390560	607509	38.22%	2.890%
18	7.181	710	713	717	rVB6	2130	2734	0.17%	0.013%
19	7.557	770	777	786	rBV	453520	703609	44.26%	3.347%
20	7.634	786	790	795	rVV6	4063	6088	0.38%	0.029%
21	7.687	798	799	803	rBV4	1691	2476	0.16%	0.012%
22	8.063	860	863	866	rBV5	1034	1676	0.11%	0.008%
23	8.275	892	899	913	rBV	443579	712776	44.84%	3.390%
24	8.722	967	975	987	rBV	355872	583417	36.70%	2.775%
25	8.846	994	996	999	rBV4	1654	2430	0.15%	0.012%
26	8.893	1001	1004	1010	rVB8	3423	4905	0.31%	0.023%
27	9.116	1038	1042	1049	rBV6	3369	5537	0.35%	0.026%
28	9.434	1086	1096	1105	rBV	290369	487807	30.69%	2.320%
29	9.969	1180	1187	1200	rBV	399459	694627	43.70%	3.304%
30	10.340	1243	1250	1258	rBV	558955	940730	59.18%	4.475%
31	10.499	1265	1277	1293	rBV	378748	677375	42.61%	3.222%
32	10.851	1334	1337	1340	rVB5	1877	2408	0.15%	0.011%
33	11.181	1388	1393	1394	rBV5	1770	2359	0.15%	0.011%
34	11.404	1426	1431	1433	rBV6	1068	1740	0.11%	0.008%
35	11.616	1464	1467	1474	rVB6	2348	4028	0.25%	0.019%
36	11.916	1515	1518	1519	rBV3	2167	2072	0.13%	0.010%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081922\
 Data File : BP011511.D
 Acq On : 19 Aug 2022 17:12
 Operator : CG/JU
 Sample : N4221-04
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0KP5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP081622.M
 Title : SVOA CALIBRATION

37	11.951	1519	1524	1536	rVB3	8027	16876	1.06%	0.080%
38	12.163	1556	1560	1561	rBV4	1598	1811	0.11%	0.009%
39	12.428	1602	1605	1609	rVB5	1323	2100	0.13%	0.010%
40	12.575	1627	1630	1634	rVB6	1992	2305	0.15%	0.011%
41	12.757	1658	1661	1664	rBV5	1568	2272	0.14%	0.011%
42	12.834	1667	1674	1678	rVV9	1820	3964	0.25%	0.019%
43	13.022	1700	1706	1709	rBV8	1238	2479	0.16%	0.012%
44	13.057	1709	1712	1715	rVB4	2494	2694	0.17%	0.013%
45	13.198	1731	1736	1740	rVB8	2666	3956	0.25%	0.019%
46	13.475	1777	1783	1786	rVB8	1575	2403	0.15%	0.011%
47	13.651	1807	1813	1826	rBV	705720	935539	58.85%	4.450%
48	13.916	1850	1858	1873	rBV	770287	1104861	69.51%	5.255%
49	14.151	1894	1898	1904	rVB8	3178	6033	0.38%	0.029%
50	14.228	1904	1911	1920	rBV	748866	1080087	67.95%	5.137%
51	14.292	1920	1922	1927	rVB4	2704	3226	0.20%	0.015%
52	14.410	1940	1942	1945	rBV4	1430	1606	0.10%	0.008%
53	14.463	1945	1951	1969	rBV	232973	442868	27.86%	2.107%
54	14.598	1972	1974	1977	rVB4	2008	2111	0.13%	0.010%
55	14.675	1984	1987	1992	rVB5	5276	8302	0.52%	0.039%
56	15.039	2047	2049	2053	rBV4	2813	3798	0.24%	0.018%
57	15.098	2055	2059	2064	rVB8	2979	5169	0.33%	0.025%
58	15.234	2075	2082	2091	rBV	946398	1322927	83.23%	6.292%
59	15.369	2099	2105	2117	rBV	278537	383713	24.14%	1.825%
60	15.475	2119	2123	2133	rVB9	6470	12852	0.81%	0.061%
61	15.610	2143	2146	2148	rBV4	1373	1837	0.12%	0.009%
62	15.669	2152	2156	2160	rVB7	1440	2239	0.14%	0.011%
63	15.798	2176	2178	2182	rBV4	1655	2656	0.17%	0.013%
64	15.963	2197	2206	2213	rBV	23229	39808	2.50%	0.189%
65	16.028	2213	2217	2225	rVB	2495	5885	0.37%	0.028%
66	16.134	2230	2235	2236	rBV5	3198	3813	0.24%	0.018%
67	16.363	2271	2274	2278	rBV5	978	2033	0.13%	0.010%
68	16.781	2340	2345	2351	rBV10	3140	7602	0.48%	0.036%
69	16.886	2359	2363	2366	rBV6	3137	5453	0.34%	0.026%
70	16.939	2371	2372	2375	rVV3	2273	2269	0.14%	0.011%
71	16.998	2375	2382	2392	rVV	902741	1229236	77.33%	5.847%
72	17.098	2392	2399	2415	rVV	1061286	1418219	89.22%	6.746%
73	17.216	2415	2419	2425	rVB7	9905	15738	0.99%	0.075%
74	17.698	2497	2501	2505	rBV3	11247	15928	1.00%	0.076%
75	17.863	2527	2529	2532	rBV4	2038	1844	0.12%	0.009%
76	17.916	2534	2538	2543	rBV3	25397	33314	2.10%	0.158%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081922\
 Data File : BP011511.D
 Acq On : 19 Aug 2022 17:12
 Operator : CG/JU
 Sample : N4221-04
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0KP5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP081622.M
 Title : SVOA CALIBRATION

77	18.198	2584	2586	2588	rBV3	2819	2993	0.19%	0.014%
78	18.439	2625	2627	2629	rBV3	2991	2780	0.17%	0.013%
79	18.933	2708	2711	2715	rVB2	11108	14107	0.89%	0.067%
80	19.004	2719	2723	2726	rBV	13816	17585	1.11%	0.084%
81	19.363	2778	2784	2791	rBV	1240887	1589566	100.00%	7.561%
82	20.863	3035	3039	3046	rBV2	102178	180857	11.38%	0.860%
83	21.127	3079	3084	3092	rBV	1114602	1358302	85.45%	6.461%
84	23.268	3442	3448	3456	rBV2	850164	1572346	98.92%	7.479%
85	23.415	3467	3473	3482	rVB2	713569	1357018	85.37%	6.455%




Sum of corrected areas: 21023875

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081922\
Data File : BP011511.D
Acq On : 19 Aug 2022 17:12
Operator : CG/JU
Sample : N4221-04
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0KP5

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP081622.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

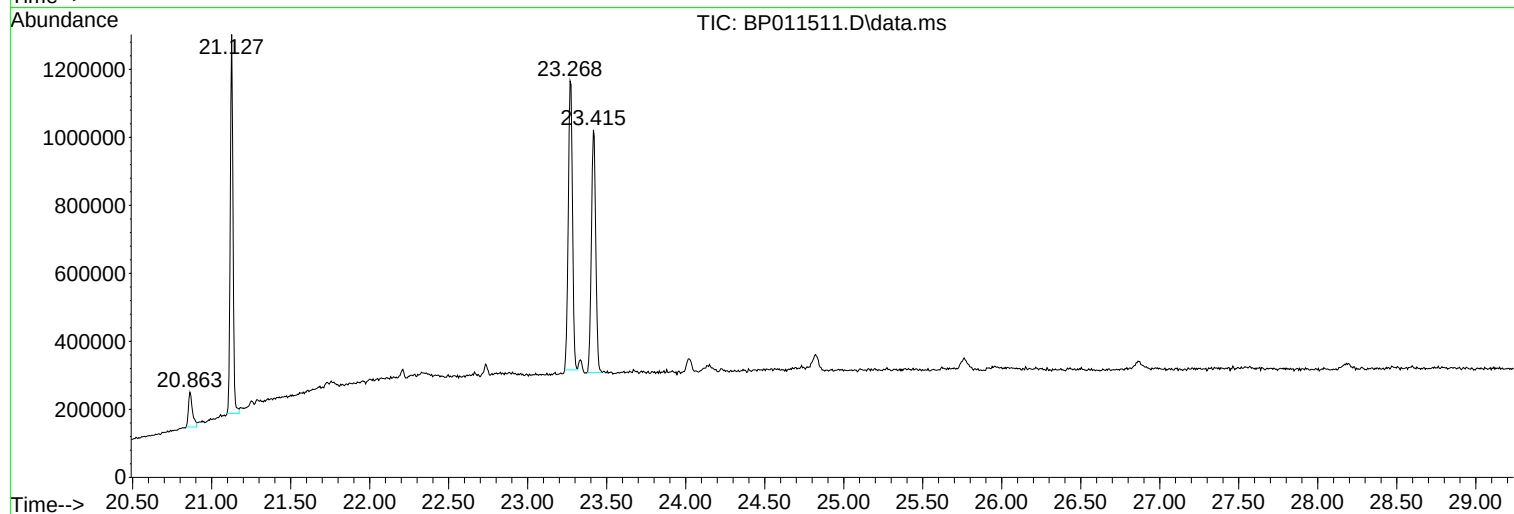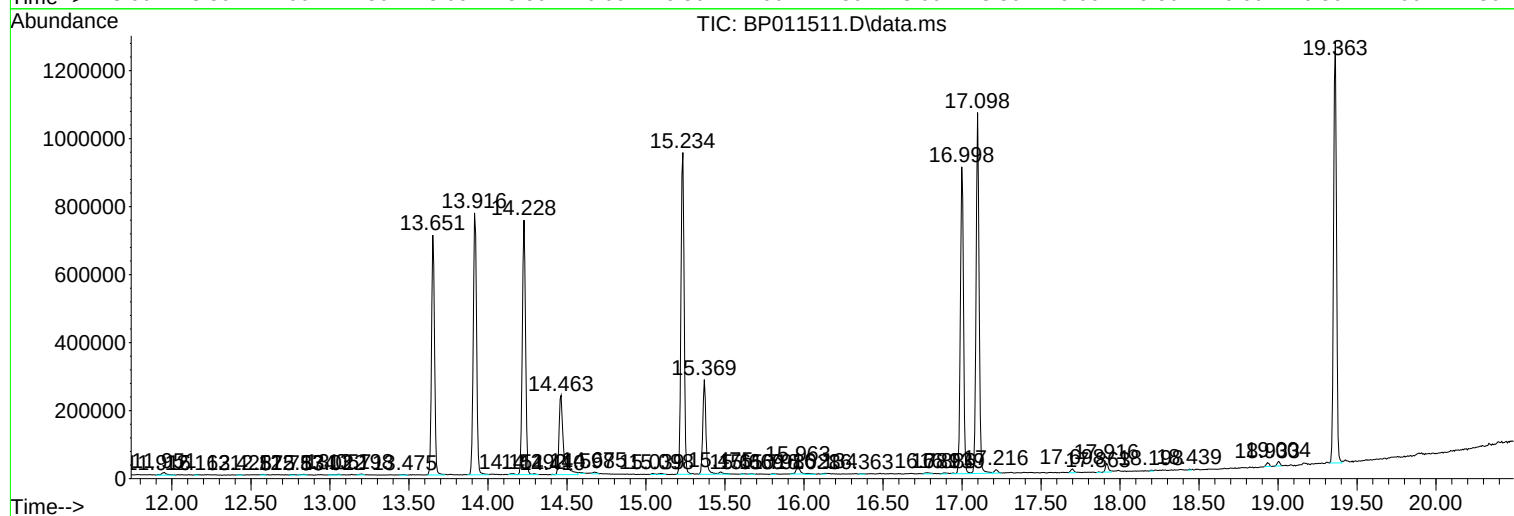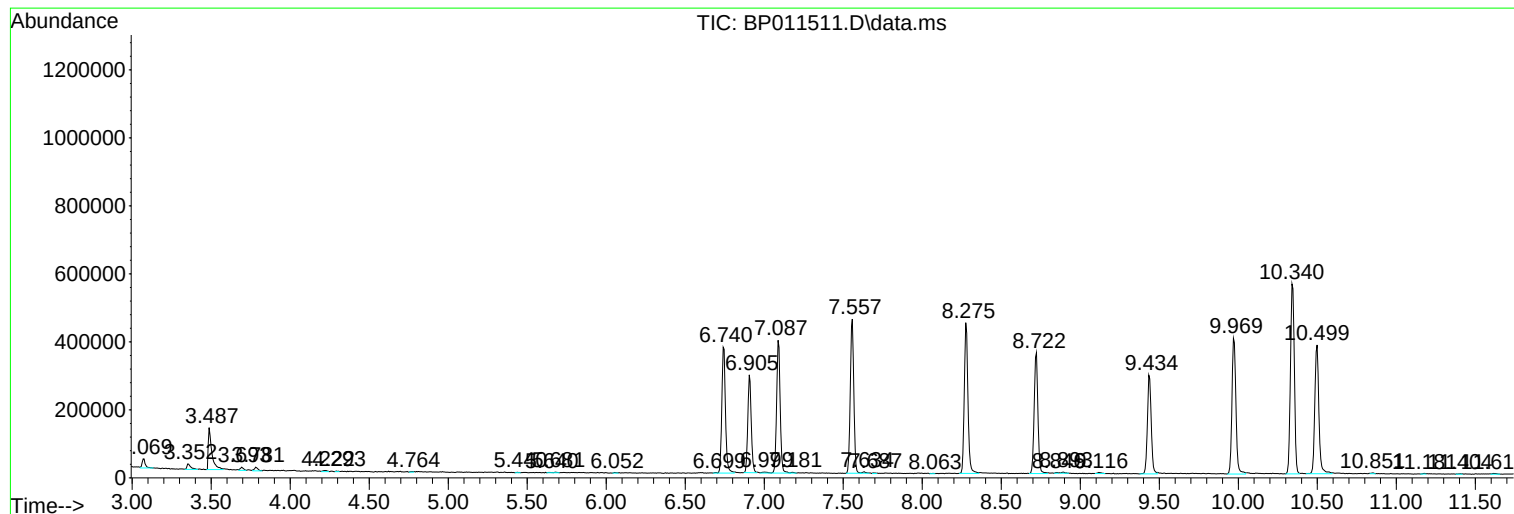

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081922\
Data File : BP011511.D
Acq On : 19 Aug 2022 17:12
Operator : CG/JU
Sample : N4221-04
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0KP5










Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP081622.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 (DEL) Alkane: Straight-Chai... Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
20.863	2.66 ng/ul	180857	Chrysene-d12	21.127

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Heptacos-1-ene	378	C27H54	015306-27-1	96
2			Nonacos-1-ene	406	C29H58	018835-35-3	94
3			Trifluoroacetoxy hexadecane	338	C18H33F3O2	006222-03-3	94
4			Trichloroacetic acid, hexadecyl ...	386	C18H33Cl3O2	074339-54-1	93
5			Trichloroacetic acid, pentadecyl...	372	C17H31Cl3O2	074339-53-0	93

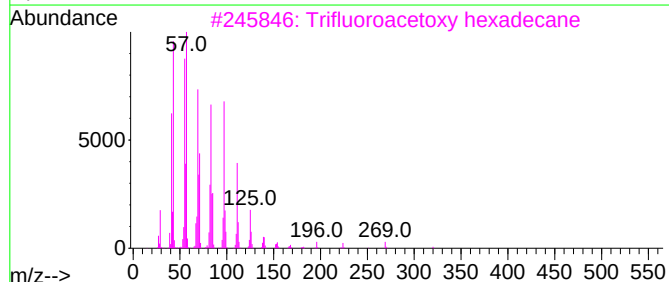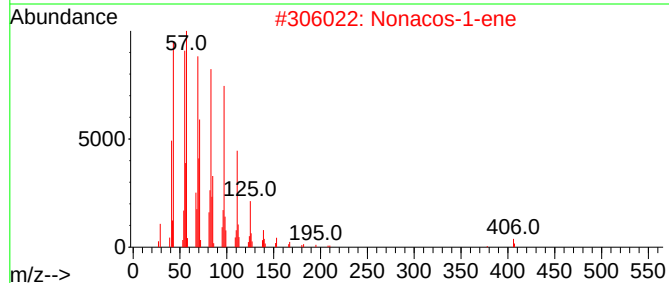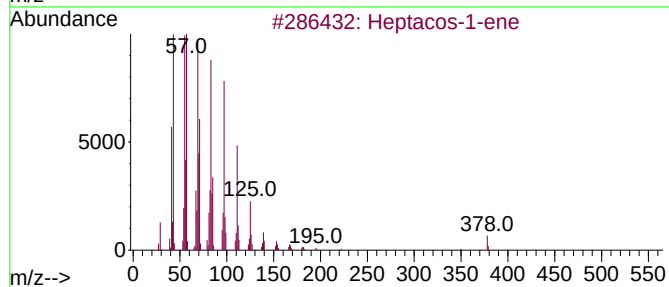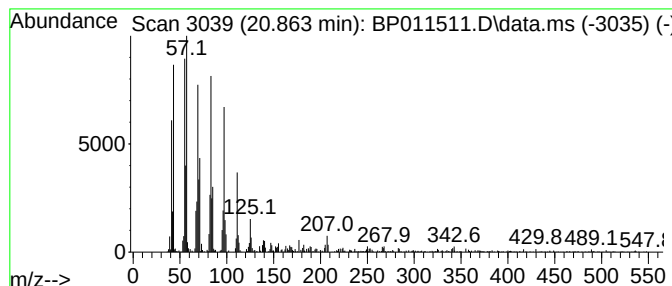

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081922\
Data File : BP011511.D
Acq On : 19 Aug 2022 17:12
Operator : CG/JU
Sample : N4221-04
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0KP5

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP081622.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
(DEL) Alkane: S...	20.863	2.7	ng/u1	180857	5	21.127	1358300	20.0