

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081922\
 Data File : BP011515.D
 Acq On : 19 Aug 2022 20:06
 Operator : CG/JU
 Sample : PB147110BL
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK110

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP081622.M
 Title : SVOA CALIBRATION

Signal : TIC: BP011515.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.069	11	14	19	rVB	34045	38958	1.90%	0.155%
2	3.481	80	84	103	rBV	394673	600186	29.32%	2.383%
3	3.781	131	135	143	rVB	38595	53990	2.64%	0.214%
4	6.005	509	513	515	rBV5	1755	2330	0.11%	0.009%
5	6.740	631	638	653	rBV	469765	724341	35.38%	2.875%
6	6.905	660	666	675	rBV	351746	522864	25.54%	2.076%
7	7.087	691	697	709	rVB	471026	723115	35.32%	2.871%
8	7.552	769	776	788	rVB	461002	717079	35.03%	2.847%
9	8.275	890	899	913	rBV	537858	858138	41.92%	3.407%
10	8.716	965	974	986	rBV	433602	707858	34.58%	2.810%
11	9.434	1088	1096	1107	rBV	360966	596582	29.14%	2.368%
12	9.969	1177	1187	1202	rBV	503830	843534	41.20%	3.349%
13	10.340	1242	1250	1259	rBV	621473	986243	48.17%	3.915%
14	10.493	1268	1276	1295	rBV	487145	852728	41.65%	3.385%
15	11.951	1515	1524	1536	rBV4	7686	17201	0.84%	0.068%
16	13.198	1734	1736	1741	rVB6	2386	3310	0.16%	0.013%
17	13.651	1806	1813	1827	rBV	909693	1239049	60.52%	4.919%
18	13.916	1851	1858	1869	rBV	945278	1334298	65.18%	5.297%
19	14.228	1904	1911	1920	rBV	859748	1186430	57.95%	4.710%
20	14.457	1944	1950	1972	rBV	374401	662254	32.35%	2.629%
21	15.228	2075	2081	2092	rBV	1164881	1632804	79.76%	6.482%
22	15.369	2098	2105	2119	rBV	450441	628424	30.70%	2.495%
23	15.469	2119	2122	2129	rVB7	7405	12364	0.60%	0.049%
24	16.786	2341	2346	2349	rBV7	2635	5142	0.25%	0.020%
25	16.998	2376	2382	2392	rBV	986163	1357602	66.31%	5.389%
26	17.098	2392	2399	2414	rVV	1348122	1843046	90.03%	7.316%
27	17.680	2496	2498	2501	rBV4	1571	2106	0.10%	0.008%
28	17.916	2536	2538	2541	rVB4	2480	2586	0.13%	0.010%
29	17.945	2541	2543	2546	rBV4	1570	2429	0.12%	0.010%
30	18.380	2614	2617	2620	rBV5	2240	3847	0.19%	0.015%
31	18.433	2624	2626	2629	rBV4	2264	2963	0.14%	0.012%
32	18.933	2708	2711	2715	rVB3	15073	18375	0.90%	0.073%
33	19.004	2720	2723	2727	rVB2	16204	19623	0.96%	0.078%
34	19.363	2778	2784	2792	rBV	1569083	2033071	99.31%	8.071%
35	21.127	3079	3084	3089	rBV	1182829	1442940	70.48%	5.728%
36	23.268	3441	3448	3454	rBV2	1119347	2047249	100.00%	8.127%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081922\
Data File : BP011515.D
Acq On : 19 Aug 2022 20:06
Operator : CG/JU
Sample : PB147110BL
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK110

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP081622.M
Title : SVOA CALIBRATION

37	23.415	3467	3473	3484	rVB2	758044	1465315	71.57%	5.817%
----	--------	------	------	------	------	--------	---------	--------	--------




Sum of corrected areas: 25190374

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081922\
Data File : BP011515.D
Acq On : 19 Aug 2022 20:06
Operator : CG/JU
Sample : PB147110BL
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK110

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP081622.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

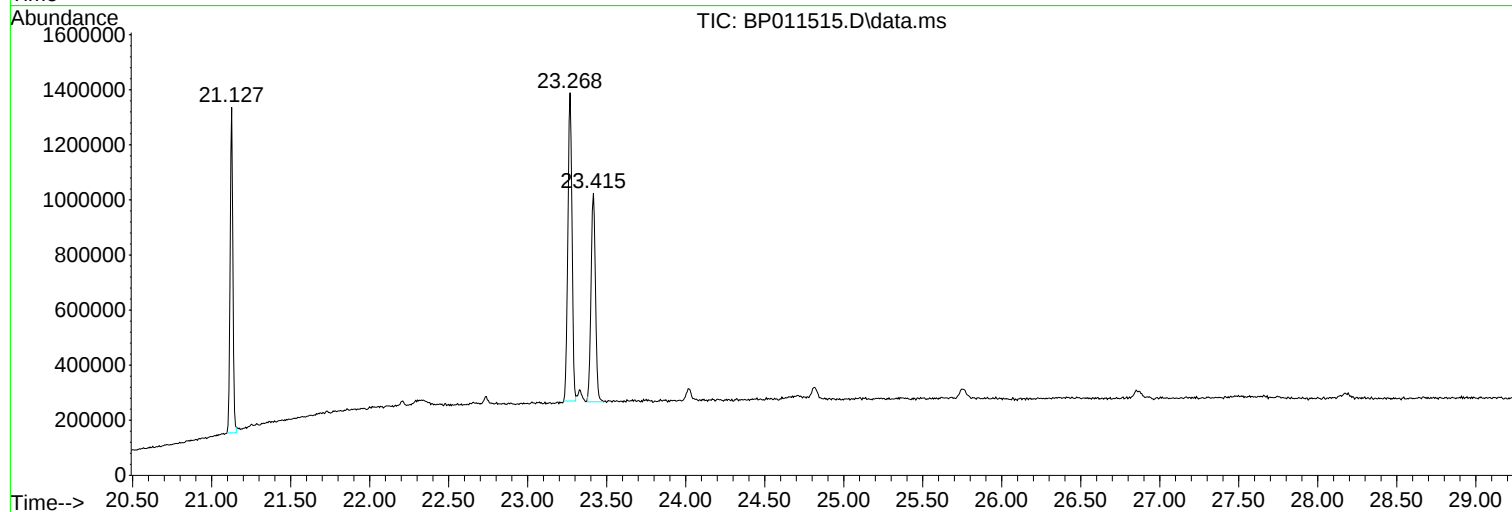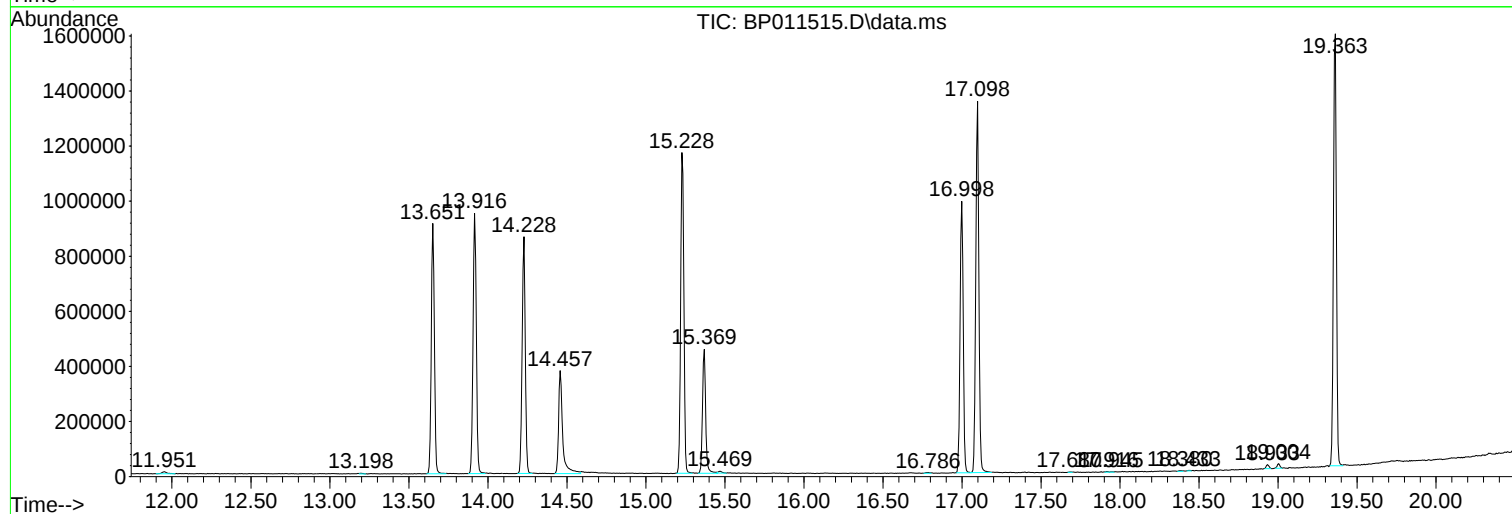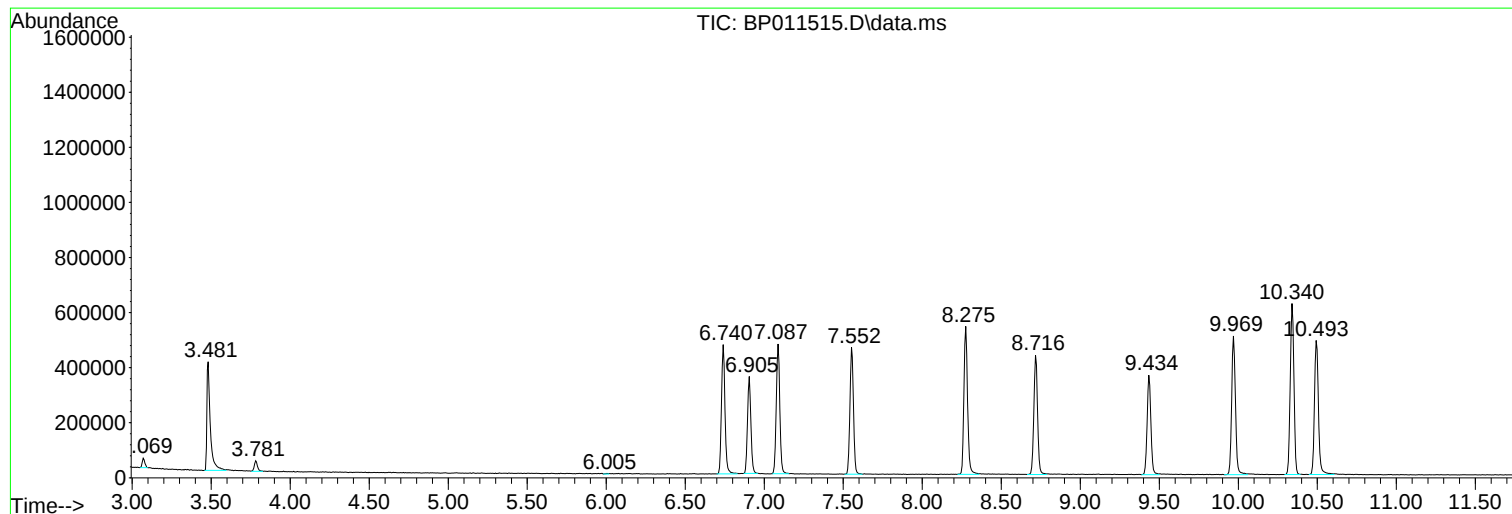

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081922\
Data File : BP011515.D
Acq On : 19 Aug 2022 20:06
Operator : CG/JU
Sample : PB147110BL
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK110

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP081622.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081922\
Data File : BP011515.D
Acq On : 19 Aug 2022 20:06
Operator : CG/JU
Sample : PB147110BL
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK110

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP081622.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc
