

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081922\
 Data File : BP011516.D
 Acq On : 19 Aug 2022 20:41
 Operator : CG/JU
 Sample : PB147151BL
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK151

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP081622.M
 Title : SVOA CALIBRATION

Signal : TIC: BP011516.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.070	10	14	22	rVB	36489	47243	2.55%	0.216%
2	3.475	80	83	100	rBV	412610	570958	30.84%	2.616%
3	3.781	130	135	141	rBV	39821	52038	2.81%	0.238%
4	4.417	242	243	248	rBV5	2015	2635	0.14%	0.012%
5	6.064	518	523	526	rBV6	1280	1909	0.10%	0.009%
6	6.740	632	638	648	rBV	435609	671952	36.29%	3.079%
7	6.905	660	666	678	rVB	331620	493963	26.68%	2.263%
8	7.087	690	697	707	rBV	455785	686512	37.08%	3.146%
9	7.552	769	776	788	rBV	470914	718440	38.81%	3.292%
10	8.275	892	899	916	rBV	486784	774853	41.85%	3.550%
11	8.716	967	974	987	rBV	393444	634995	34.30%	2.910%
12	9.205	1054	1057	1062	rBV7	1465	1952	0.11%	0.009%
13	9.434	1089	1096	1108	rBV	332190	538842	29.10%	2.469%
14	9.969	1180	1187	1204	rBV	452838	744439	40.21%	3.411%
15	10.340	1242	1250	1258	rBV	585133	932375	50.36%	4.272%
16	10.493	1266	1276	1292	rBV	433792	748174	40.41%	3.428%
17	11.951	1517	1524	1531	rBV3	5642	12043	0.65%	0.055%
18	12.893	1680	1684	1689	rBV7	949	2005	0.11%	0.009%
19	13.187	1731	1734	1740	rVB7	1517	3006	0.16%	0.014%
20	13.651	1804	1813	1824	rBV	754529	1008500	54.47%	4.621%
21	13.916	1851	1858	1870	rBV	781972	1098952	59.36%	5.035%
22	14.016	1873	1875	1880	rVB5	1538	2062	0.11%	0.009%
23	14.228	1904	1911	1919	rBV	702551	1035073	55.91%	4.743%
24	14.457	1944	1950	1967	rBV	273126	489356	26.43%	2.242%
25	15.228	2075	2081	2090	rBV	931668	1327544	71.70%	6.083%
26	15.369	2099	2105	2117	rBV	336908	476983	25.76%	2.186%
27	15.469	2119	2122	2128	rVB4	5385	8025	0.43%	0.037%
28	15.810	2177	2180	2185	rVB7	1681	2508	0.14%	0.011%
29	16.016	2211	2215	2218	rVB5	1855	2194	0.12%	0.010%
30	16.781	2341	2345	2348	rBV6	2328	3186	0.17%	0.015%
31	16.998	2375	2382	2392	rBV	821483	1129407	61.00%	5.175%
32	17.098	2392	2399	2411	rVV	1059104	1446913	78.15%	6.630%
33	17.528	2467	2472	2474	rBV6	1568	2704	0.15%	0.012%
34	18.192	2583	2585	2591	rBV7	1841	3254	0.18%	0.015%
35	18.933	2707	2711	2717	rVB4	11650	16873	0.91%	0.077%
36	19.004	2719	2723	2727	rVB2	13203	17448	0.94%	0.080%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081922\
Data File : BP011516.D
Acq On : 19 Aug 2022 20:41
Operator : CG/JU
Sample : PB147151BL
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK151

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP081622.M
Title : SVOA CALIBRATION

37	19.357	2778	2783	2790	rBV	1259104	1644894	88.85%	7.537%
38	21.127	3079	3084	3090	rBV	1001290	1269626	68.58%	5.818%
39	23.269	3441	3448	3455	rBV2	1035712	1851410	100.00%	8.483%
40	23.416	3466	3473	3481	rBV2	688279	1348934	72.86%	6.181%




Sum of corrected areas: 21824180

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081922\
Data File : BP011516.D
Acq On : 19 Aug 2022 20:41
Operator : CG/JU
Sample : PB147151BL
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK151

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP081622.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

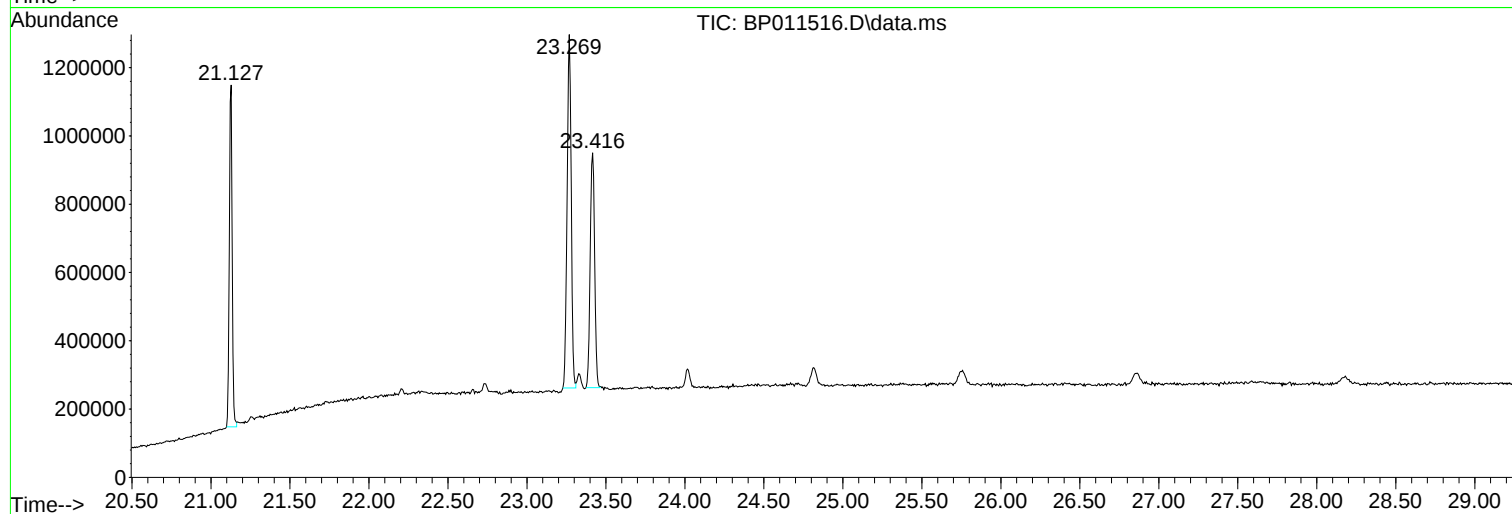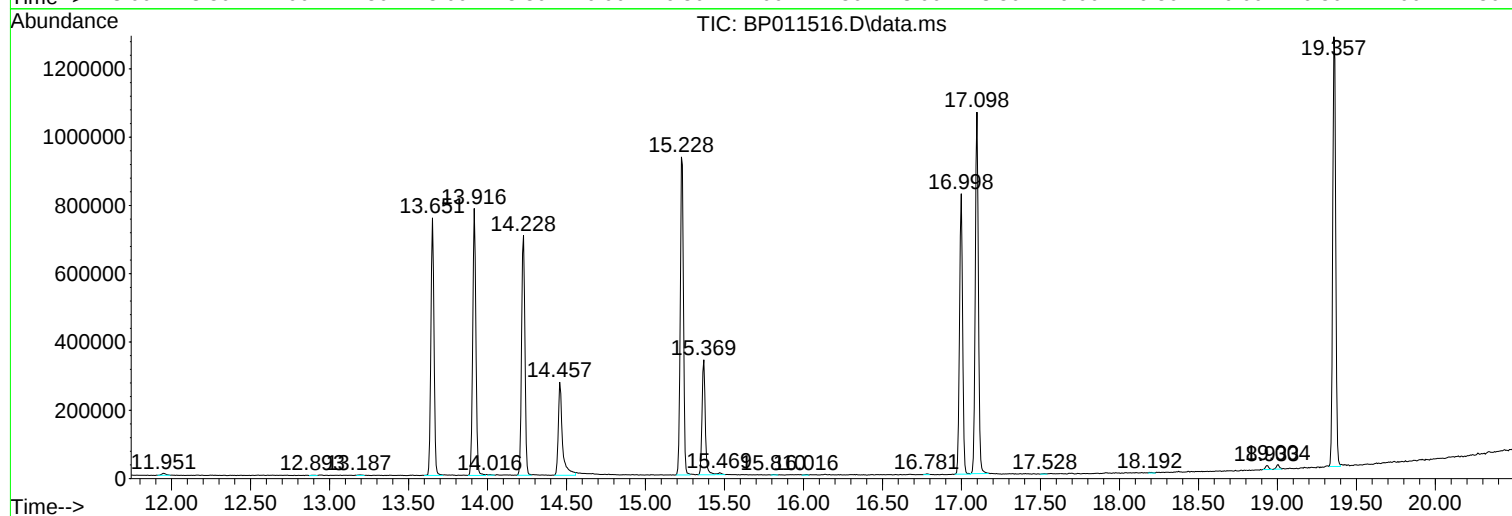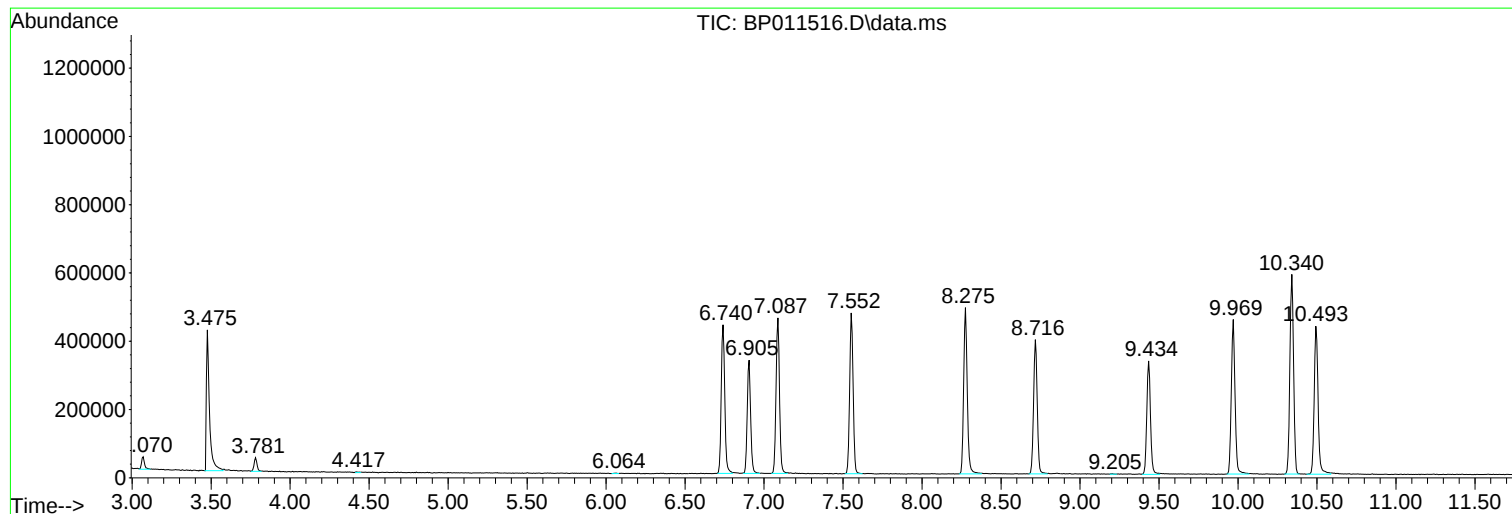

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081922\
Data File : BP011516.D
Acq On : 19 Aug 2022 20:41
Operator : CG/JU
Sample : PB147151BL
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK151

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP081622.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081922\
Data File : BP011516.D
Acq On : 19 Aug 2022 20:41
Operator : CG/JU
Sample : PB147151BL
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK151

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP081622.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc