

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081922\
 Data File : BP011520.D
 Acq On : 19 Aug 2022 22:59
 Operator : CG/JU
 Sample : N4221-13DL 10X
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0KN3DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP081622.M
 Title : SVOA CALIBRATION

Signal : TIC: BP011520.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.028	3	7	17	rBV	1198291	1826097	100.00%	15.355%
2	3.105	17	20	33	rVB	104840	151933	8.32%	1.278%
3	3.781	132	135	141	rVB	11501	14895	0.82%	0.125%
4	4.293	216	222	237	rVB	701277	1014139	55.54%	8.528%
5	5.022	342	346	350	rVB4	4537	7008	0.38%	0.059%
6	6.746	634	639	645	rBV3	7248	12311	0.67%	0.104%
7	6.905	660	666	675	rBV	32820	55167	3.02%	0.464%
8	7.087	691	697	704	rBV	32264	54651	2.99%	0.460%
9	7.552	769	776	787	rBV	484793	749095	41.02%	6.299%
10	8.281	895	900	911	rVB3	17331	33722	1.85%	0.284%
11	8.722	968	975	985	rBV	34269	65619	3.59%	0.552%
12	9.440	1090	1097	1104	rVV2	25452	45765	2.51%	0.385%
13	9.975	1181	1188	1197	rBV	33461	65262	3.57%	0.549%
14	10.340	1242	1250	1263	rBV	627674	1025410	56.15%	8.622%
15	10.504	1270	1278	1289	rBV2	18853	43438	2.38%	0.365%
16	13.128	1720	1724	1729	rBV8	1495	2269	0.12%	0.019%
17	13.651	1807	1813	1819	rBV	84326	120283	6.59%	1.011%
18	13.916	1849	1858	1865	rBV2	80765	132598	7.26%	1.115%
19	14.228	1904	1911	1921	rBV	825933	1227837	67.24%	10.325%
20	14.992	2037	2041	2042	rBV4	2107	2620	0.14%	0.022%
21	15.081	2052	2056	2059	rVB5	1832	2520	0.14%	0.021%
22	15.228	2074	2081	2090	rBV	116187	169577	9.29%	1.426%
23	15.369	2101	2105	2113	rBV3	19271	31691	1.74%	0.266%
24	16.133	2230	2235	2236	rBV5	2089	2656	0.15%	0.022%
25	16.628	2317	2319	2323	rVB5	1509	2023	0.11%	0.017%
26	16.780	2340	2345	2349	rBV8	2807	4661	0.26%	0.039%
27	16.998	2375	2382	2393	rBV	966473	1385749	75.89%	11.652%
28	17.098	2393	2399	2411	rVV2	128362	194542	10.65%	1.636%
29	17.298	2431	2433	2439	rBV6	1742	2774	0.15%	0.023%
30	17.692	2497	2500	2504	rVB6	3731	5145	0.28%	0.043%
31	17.916	2534	2538	2543	rBV7	3587	4893	0.27%	0.041%
32	19.304	2772	2774	2777	rBV4	4607	5259	0.29%	0.044%
33	19.357	2778	2783	2791	rVV	161366	212904	11.66%	1.790%
34	21.121	3078	3083	3089	rBV	1231949	1505657	82.45%	12.661%
35	23.263	3443	3447	3453	rVB	107243	178785	9.79%	1.503%
36	23.410	3466	3472	3485	rVB2	802554	1533364	83.97%	12.894%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081922\
Data File : BP011520.D
Acq On : 19 Aug 2022 22:59
Operator : CG/JU
Sample : N4221-13DL 10X
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0KN3DL

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP081622.M
Title : SVOA CALIBRATION




Sum of corrected areas: 11892319

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081922\
Data File : BP011520.D
Acq On : 19 Aug 2022 22:59
Operator : CG/JU
Sample : N4221-13DL 10X
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0KN3DL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP081622.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

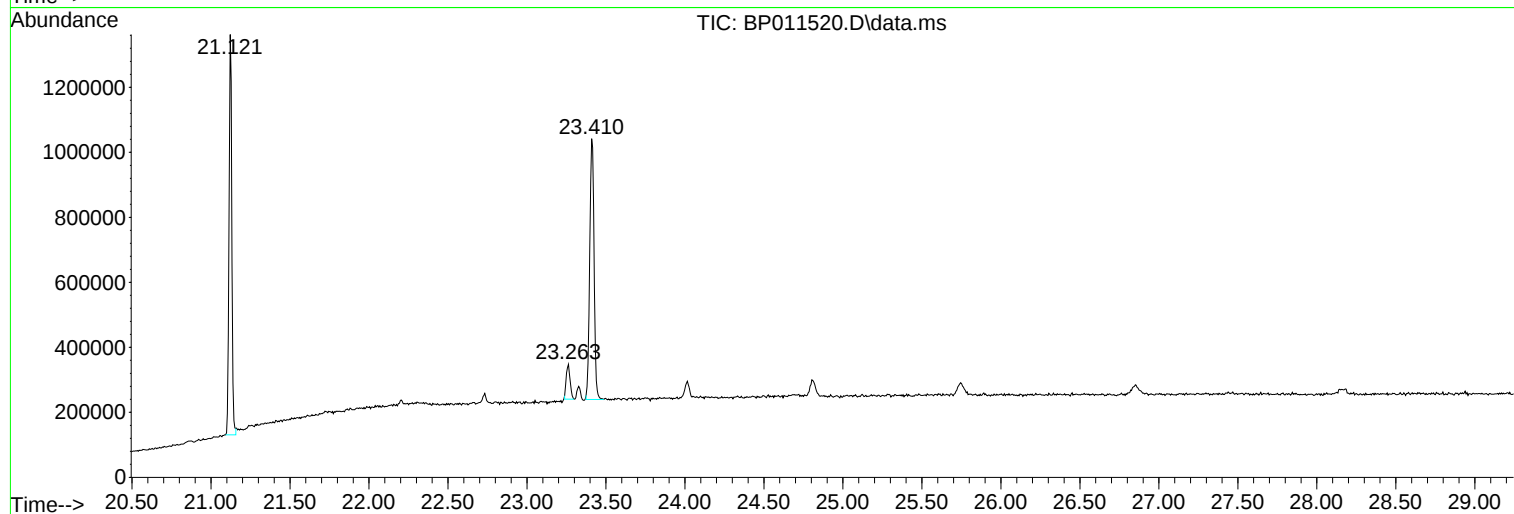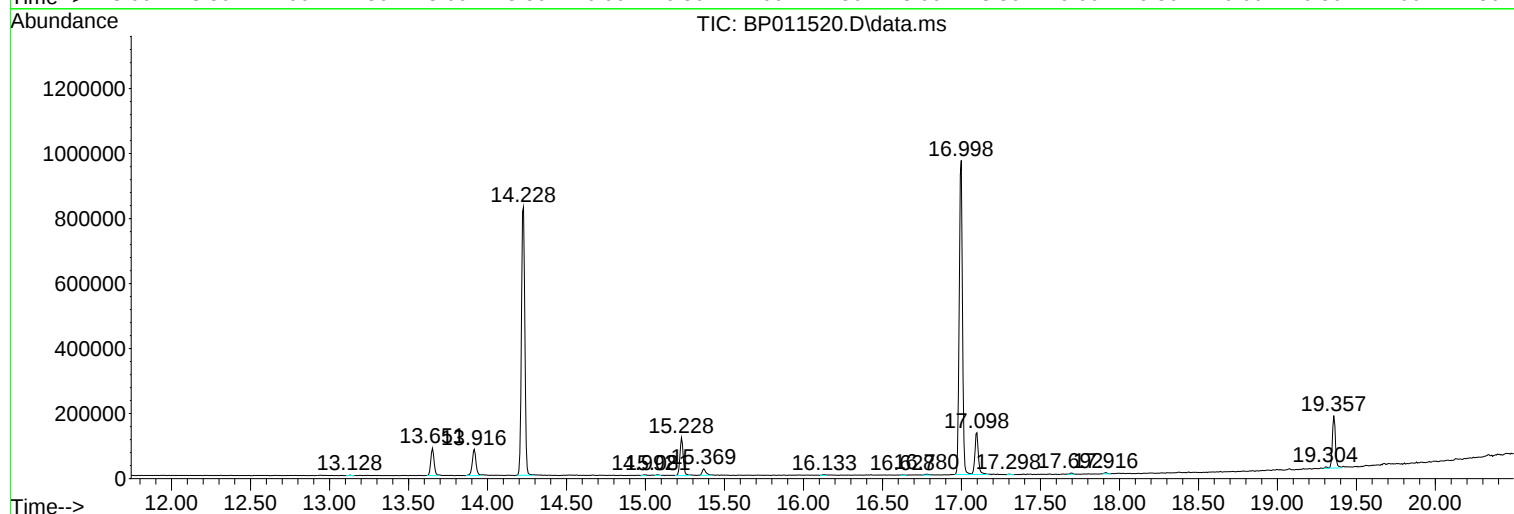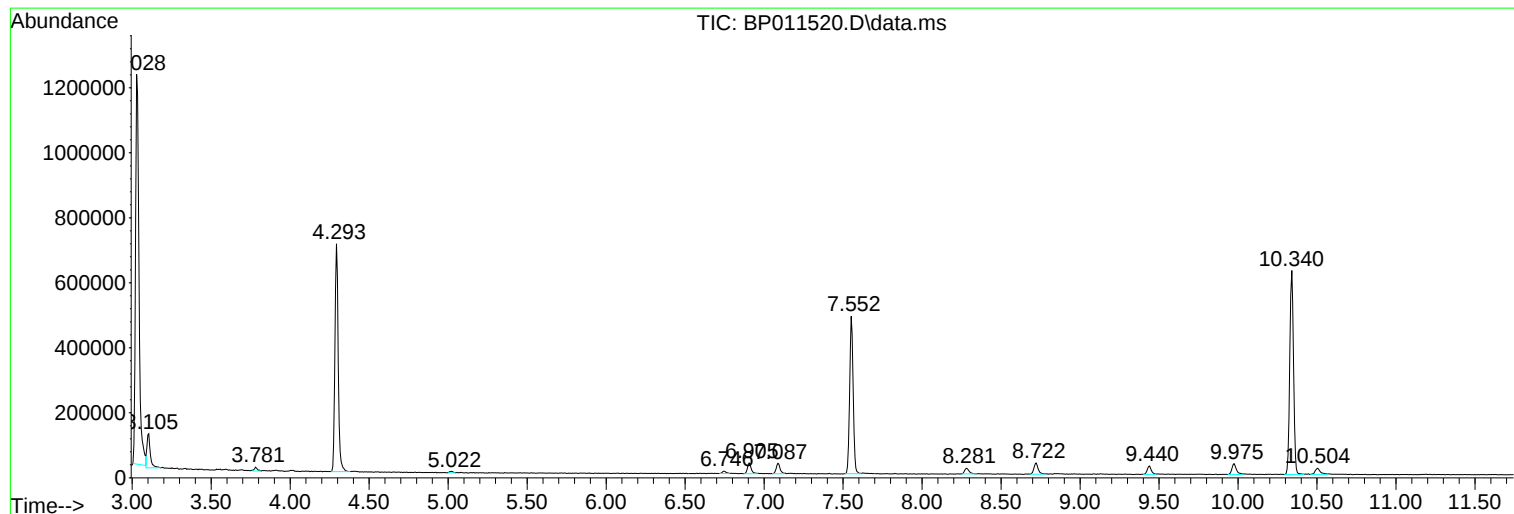

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081922\
Data File : BP011520.D
Acq On : 19 Aug 2022 22:59
Operator : CG/JU
Sample : N4221-13DL 10X
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0KN3DL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP081622.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081922\
Data File : BP011520.D
Acq On : 19 Aug 2022 22:59
Operator : CG/JU
Sample : N4221-13DL 10X
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0KN3DL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP081622.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc