

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081922\
 Data File : BP011521.D
 Acq On : 19 Aug 2022 23:33
 Operator : CG/JU
 Sample : N4221-14DL 5X
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0KN6DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP081622.M
 Title : SVOA CALIBRATION

Signal : TIC: BP011521.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.028	3	7	16	rBV	1232805	1666050	61.95%	11.563%
2	3.099	16	19	25	rVB	181558	206013	7.66%	1.430%
3	3.511	88	89	96	rBV4	5777	8779	0.33%	0.061%
4	3.693	116	120	124	rVB5	4522	6221	0.23%	0.043%
5	3.781	131	135	138	rBV2	11352	14324	0.53%	0.099%
6	3.905	153	156	161	rVB3	5517	7269	0.27%	0.050%
7	4.293	215	222	235	rBV	1987998	2689253	100.00%	18.664%
8	4.393	237	239	245	rVB7	3749	5026	0.19%	0.035%
9	4.740	294	298	304	rVB9	1895	4093	0.15%	0.028%
10	5.016	341	345	351	rVB	26321	36723	1.37%	0.255%
11	6.740	633	638	648	rBV2	14039	27664	1.03%	0.192%
12	6.905	660	666	676	rBV	62420	100204	3.73%	0.695%
13	7.087	690	697	707	rBV	62240	100312	3.73%	0.696%
14	7.552	768	776	785	rBV	477616	739313	27.49%	5.131%
15	8.275	892	899	908	rBV2	36044	71393	2.65%	0.495%
16	8.716	967	974	983	rBV	67197	122676	4.56%	0.851%
17	9.434	1090	1096	1104	rBV2	50016	89093	3.31%	0.618%
18	9.969	1178	1187	1199	rBV	65334	129197	4.80%	0.897%
19	10.340	1240	1250	1260	rBV	601552	982665	36.54%	6.820%
20	10.499	1270	1277	1290	rBV	46760	91927	3.42%	0.638%
21	13.069	1708	1714	1718	rBV8	4207	7430	0.28%	0.052%
22	13.651	1807	1813	1820	rBV	150328	211251	7.86%	1.466%
23	13.875	1845	1851	1853	rBV3	26346	47395	1.76%	0.329%
24	13.916	1853	1858	1873	rVB	157199	251011	9.33%	1.742%
25	14.222	1904	1910	1920	rBV	774033	1137122	42.28%	7.892%
26	14.481	1951	1954	1956	rBV4	2785	3207	0.12%	0.022%
27	15.081	2053	2056	2062	rVB7	1865	2755	0.10%	0.019%
28	15.228	2073	2081	2091	rBV	214599	301768	11.22%	2.094%
29	15.363	2099	2104	2115	rBV	43619	72626	2.70%	0.504%
30	16.134	2230	2235	2239	rBV8	2373	4260	0.16%	0.030%
31	16.781	2340	2345	2348	rBV6	3875	5686	0.21%	0.039%
32	16.998	2375	2382	2388	rVV	899145	1274651	47.40%	8.847%
33	17.092	2392	2398	2413	rVB	227140	346592	12.89%	2.405%
34	17.698	2495	2501	2507	rVB	3742	6403	0.24%	0.044%
35	17.910	2532	2537	2541	rBV7	4330	7267	0.27%	0.050%
36	17.992	2546	2551	2552	rBV5	2714	3527	0.13%	0.024%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081922\
 Data File : BP011521.D
 Acq On : 19 Aug 2022 23:33
 Operator : CG/JU
 Sample : N4221-14DL 5X
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0KN6DL

Integration Parameters: LSCINT.P
 Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0.1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP081622.M
 Title : SVOA CALIBRATION

37	18.380	2613	2617	2618	rBV4	3762	3633	0.14%	0.025%
38	18.528	2640	2642	2647	rBV4	2337	3309	0.12%	0.023%
39	19.357	2778	2783	2791	rBV	299590	381255	14.18%	2.646%
40	21.122	3078	3083	3089	rBV	1155660	1411725	52.50%	9.798%
41	23.263	3442	3447	3454	rVB3	208039	363223	13.51%	2.521%
42	23.410	3466	3472	3482	rVB2	755559	1464133	54.44%	10.162%




Sum of corrected areas: 14408424

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081922\
Data File : BP011521.D
Acq On : 19 Aug 2022 23:33
Operator : CG/JU
Sample : N4221-14DL 5X
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0KN6DL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP081622.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

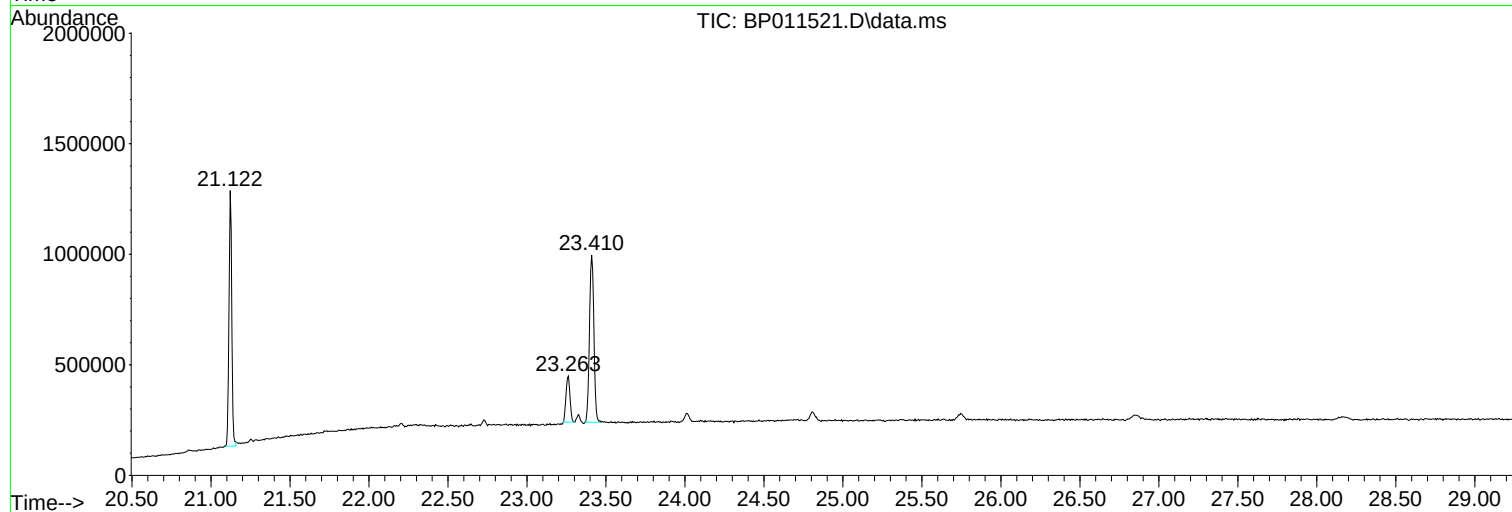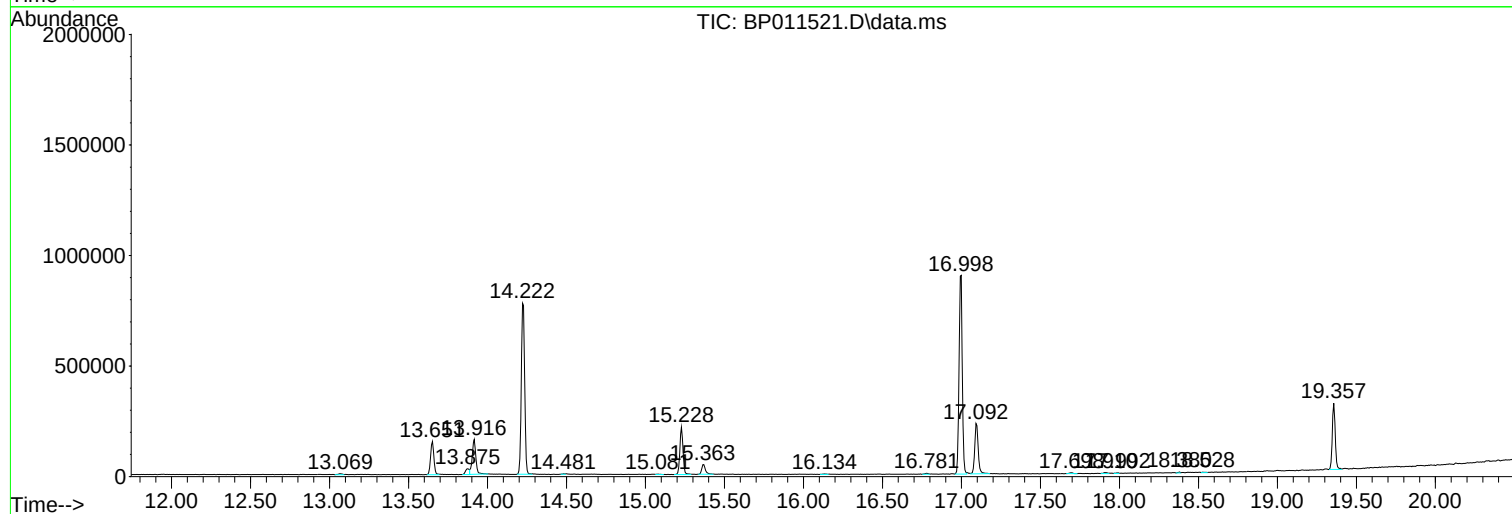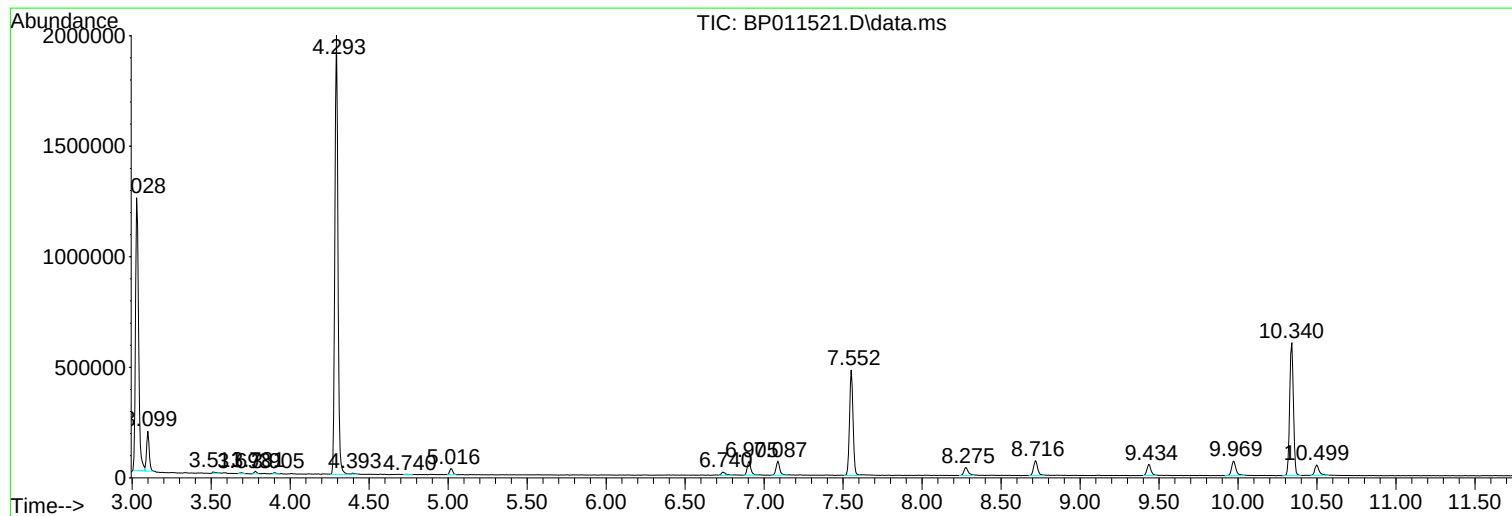

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081922\
Data File : BP011521.D
Acq On : 19 Aug 2022 23:33
Operator : CG/JU
Sample : N4221-14DL 5X
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0KN6DL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP081622.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081922\
Data File : BP011521.D
Acq On : 19 Aug 2022 23:33
Operator : CG/JU
Sample : N4221-14DL 5X
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0KN6DL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP081622.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc