

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081922\
 Data File : BP011522.D
 Acq On : 20 Aug 2022 00:08
 Operator : CG/JU
 Sample : N4221-15DL 5X
 Misc :
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0KN7DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP081622.M
 Title : SVOA CALIBRATION

Signal : TIC: BP011522.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.029	3	7	15	rBV	1204498	1436758	50.15%	10.268%
2	3.099	15	19	31	rVB	166811	215920	7.54%	1.543%
3	3.499	86	87	95	rBV	13556	19729	0.69%	0.141%
4	3.687	117	119	125	rVB5	5715	6925	0.24%	0.049%
5	3.781	130	135	139	rBV2	11194	15319	0.53%	0.109%
6	3.905	152	156	160	rVB4	5219	7259	0.25%	0.052%
7	4.011	172	174	177	rVB4	4099	4123	0.14%	0.029%
8	4.293	216	222	236	rVV	2089876	2864903	100.00%	20.475%
9	4.399	236	240	246	rVB8	3799	7563	0.26%	0.054%
10	5.017	341	345	353	rVB	29316	41699	1.46%	0.298%
11	6.740	632	638	647	rBV	14374	25584	0.89%	0.183%
12	6.905	660	666	674	rBV	58946	95651	3.34%	0.684%
13	7.087	691	697	706	rBV	58957	99265	3.46%	0.709%
14	7.228	718	721	726	rVB7	2891	4639	0.16%	0.033%
15	7.552	769	776	790	rBV	456171	709780	24.78%	5.073%
16	8.275	893	899	909	rBV2	36204	72313	2.52%	0.517%
17	8.716	967	974	984	rBV	66691	115979	4.05%	0.829%
18	9.434	1091	1096	1103	rBV	47535	81620	2.85%	0.583%
19	9.969	1180	1187	1198	rBV2	64148	123862	4.32%	0.885%
20	10.340	1242	1250	1261	rBV	588622	958449	33.45%	6.850%
21	10.499	1270	1277	1289	rBV	55661	105814	3.69%	0.756%
22	13.063	1707	1713	1718	rVB10	3629	6120	0.21%	0.044%
23	13.652	1806	1813	1821	rBV	150535	218840	7.64%	1.564%
24	13.875	1843	1851	1853	rBV2	27368	47866	1.67%	0.342%
25	13.910	1853	1857	1872	rVB	145069	242888	8.48%	1.736%
26	14.222	1903	1910	1919	rBV	770154	1123765	39.23%	8.031%
27	14.487	1948	1955	1961	rBV10	3458	8462	0.30%	0.060%
28	15.228	2075	2081	2090	rBV	213473	305371	10.66%	2.182%
29	15.363	2100	2104	2112	rBV2	42923	69254	2.42%	0.495%
30	16.775	2340	2344	2349	rBV7	2839	5510	0.19%	0.039%
31	16.998	2375	2382	2393	rBV	864472	1245814	43.49%	8.904%
32	17.092	2393	2398	2413	rVB	237033	341191	11.91%	2.438%
33	17.910	2533	2537	2541	rBV6	4238	5834	0.20%	0.042%
34	18.816	2689	2691	2695	rBV5	2688	3459	0.12%	0.025%
35	18.998	2719	2722	2725	rBV4	4636	6195	0.22%	0.044%
36	19.357	2778	2783	2790	rBV	285858	366335	12.79%	2.618%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081922\
Data File : BP011522.D
Acq On : 20 Aug 2022 00:08
Operator : CG/JU
Sample : N4221-15DL 5X
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0KN7DL

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP081622.M
Title : SVOA CALIBRATION

37	21.122	3078	3083	3089	rBV	1085829	1311316	45.77%	9.372%
38	23.263	3442	3447	3454	rVB2	187814	334878	11.69%	2.393%
39	23.410	3466	3472	3480	rVB2	712348	1335980	46.63%	9.548%




Sum of corrected areas: 13992232

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081922\
Data File : BP011522.D
Acq On : 20 Aug 2022 00:08
Operator : CG/JU
Sample : N4221-15DL 5X
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0KN7DL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP081622.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

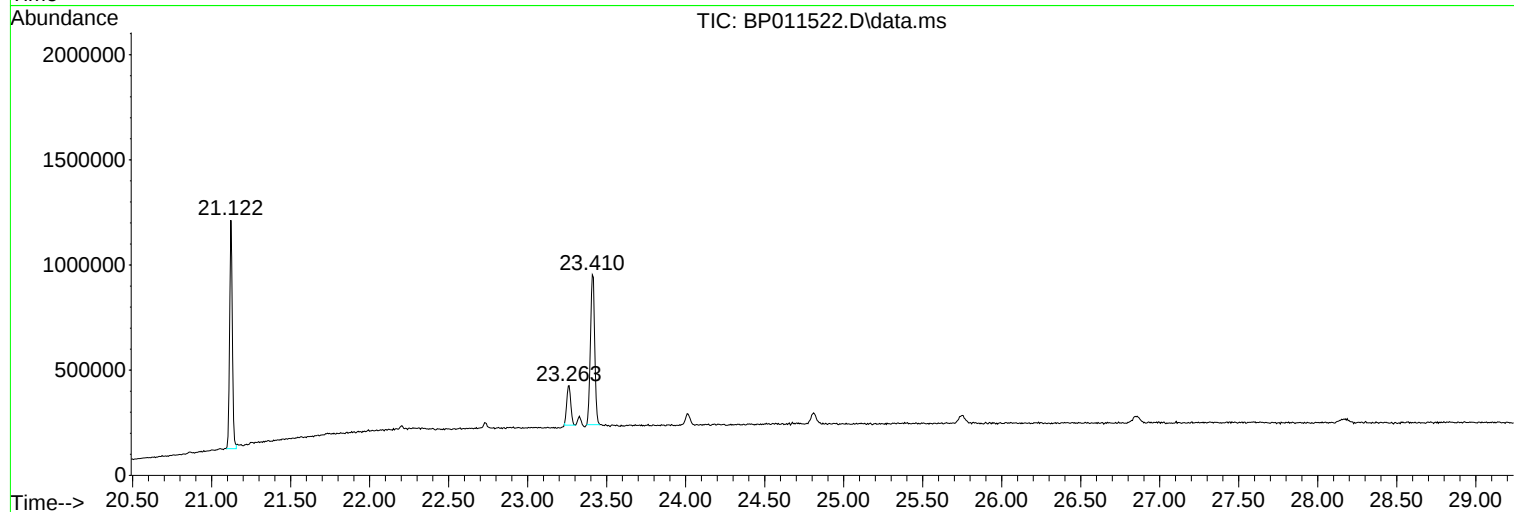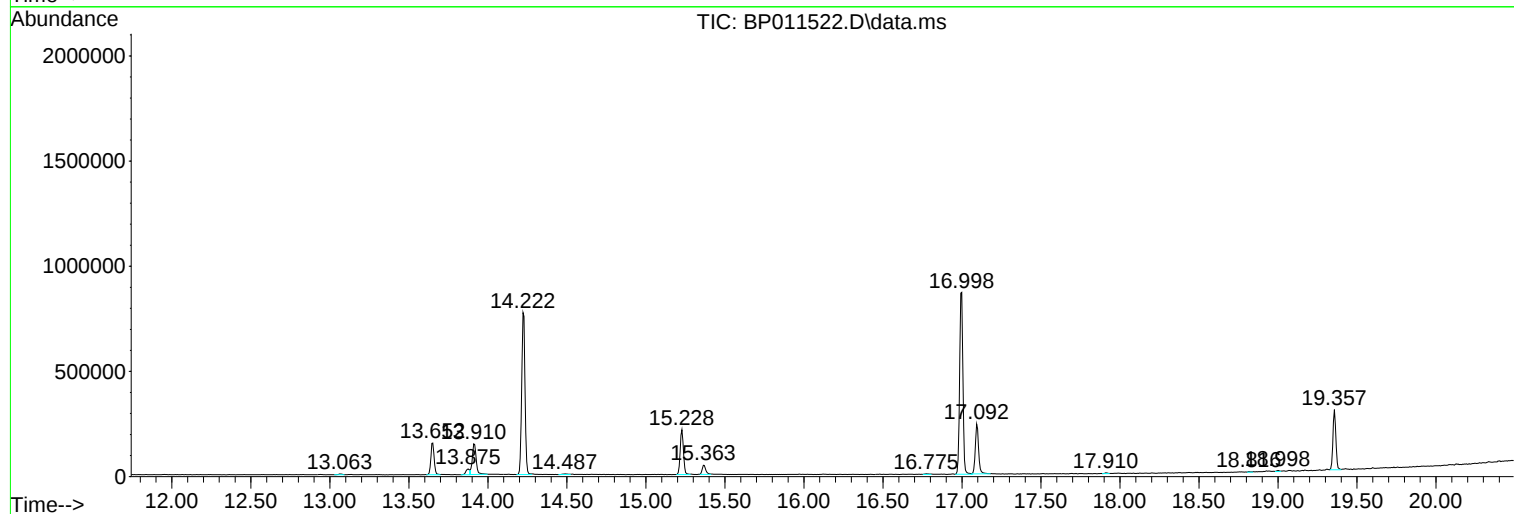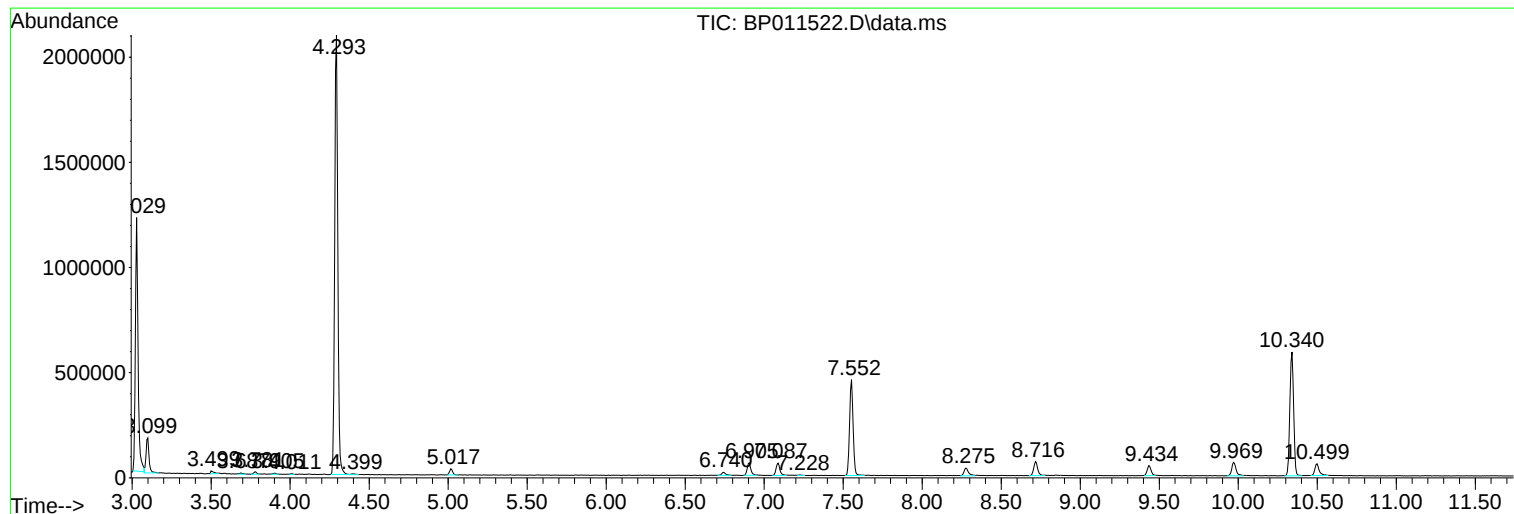

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081922\
Data File : BP011522.D
Acq On : 20 Aug 2022 00:08
Operator : CG/JU
Sample : N4221-15DL 5X
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0KN7DL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP081622.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081922\
Data File : BP011522.D
Acq On : 20 Aug 2022 00:08
Operator : CG/JU
Sample : N4221-15DL 5X
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0KN7DL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP081622.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc