

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081922\
 Data File : BP011523.D
 Acq On : 20 Aug 2022 00:42
 Operator : CG/JU
 Sample : N4210-05DL 5X
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BGC48DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP081622.M
 Title : SVOA CALIBRATION

Signal : TIC: BP011523.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.069	12	14	19	rVB2	7335	8842	0.34%	0.063%
2	3.493	84	86	97	rVV	24142	37755	1.46%	0.267%
3	3.581	97	101	106	rVB3	7704	10343	0.40%	0.073%
4	3.687	115	119	124	rVB3	8600	12629	0.49%	0.089%
5	3.781	129	135	140	rBV	30153	39043	1.51%	0.276%
6	4.005	168	173	178	rBV3	12023	18975	0.73%	0.134%
7	4.211	207	208	215	rVB7	3821	5698	0.22%	0.040%
8	4.416	239	243	245	rBV2	7760	9836	0.38%	0.070%
9	5.211	372	378	386	rBV3	6059	13623	0.53%	0.096%
10	5.569	435	439	447	rVB7	8783	15017	0.58%	0.106%
11	6.640	617	621	625	rVV6	3395	5596	0.22%	0.040%
12	6.687	625	629	631	rVV5	3401	5679	0.22%	0.040%
13	6.740	633	638	651	rVB	69129	117780	4.54%	0.834%
14	6.905	660	666	677	rVB	58047	93570	3.61%	0.662%
15	7.087	690	697	707	rBV	72839	119077	4.59%	0.843%
16	7.169	707	711	714	rBV4	7633	12700	0.49%	0.090%
17	7.552	767	776	787	rBV	414138	639053	24.65%	4.524%
18	8.093	860	868	872	rBV9	2589	5323	0.21%	0.038%
19	8.275	893	899	909	rBV	64062	113288	4.37%	0.802%
20	8.716	967	974	980	rVV	65726	110683	4.27%	0.783%
21	8.775	980	984	992	rVB2	12582	20605	0.79%	0.146%
22	8.846	992	996	1000	rBV6	3910	6922	0.27%	0.049%
23	9.434	1090	1096	1105	rBV2	48810	91284	3.52%	0.646%
24	9.969	1180	1187	1200	rBV	69954	131226	5.06%	0.929%
25	10.340	1242	1250	1256	rBV	526591	865488	33.39%	6.126%
26	10.381	1256	1257	1266	rVB	11044	16867	0.65%	0.119%
27	10.499	1270	1277	1296	rVB	43985	94232	3.64%	0.667%
28	11.263	1401	1407	1413	rBV10	2384	5892	0.23%	0.042%
29	11.369	1418	1425	1433	rBV3	7438	13402	0.52%	0.095%
30	11.781	1489	1495	1504	rVB	16389	24942	0.96%	0.177%
31	12.022	1530	1536	1541	rVB	14082	23373	0.90%	0.165%
32	12.157	1554	1559	1561	rBV6	2960	5359	0.21%	0.038%
33	12.240	1567	1573	1581	rVB2	12025	19909	0.77%	0.141%
34	12.610	1634	1636	1646	rVB9	3176	6988	0.27%	0.049%
35	12.751	1656	1660	1665	rBV4	6513	10094	0.39%	0.071%
36	12.904	1682	1686	1694	rBV6	7342	14087	0.54%	0.100%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081922\
 Data File : BP011523.D
 Acq On : 20 Aug 2022 00:42
 Operator : CG/JU
 Sample : N4210-05DL 5X
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BGC48DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP081622.M
 Title : SVOA CALIBRATION

37	13.045	1704	1710	1715	rBV2	20605	28645	1.11%	0.203%
38	13.134	1720	1725	1732	rVB10	2673	5458	0.21%	0.039%
39	13.387	1761	1768	1769	rBV6	6344	10611	0.41%	0.075%
40	13.398	1769	1770	1774	rVV3	5510	5364	0.21%	0.038%
41	13.540	1789	1794	1799	rVV3	9755	16997	0.66%	0.120%
42	13.592	1799	1803	1806	rVV4	8660	11833	0.46%	0.084%
43	13.651	1807	1813	1818	rVV	135876	193670	7.47%	1.371%
44	13.710	1818	1823	1827	rVB4	10831	17367	0.67%	0.123%
45	13.775	1827	1834	1838	rBV7	7527	13019	0.50%	0.092%
46	13.916	1851	1858	1868	rBV	138037	223816	8.63%	1.584%
47	14.134	1889	1895	1901	rBV	19196	27963	1.08%	0.198%
48	14.222	1901	1910	1918	rBV	684493	1002609	38.68%	7.097%
49	14.292	1918	1922	1926	rVB5	5884	9644	0.37%	0.068%
50	14.469	1943	1952	1960	rBV5	16606	43165	1.67%	0.306%
51	14.634	1975	1980	1984	rBV3	9133	12880	0.50%	0.091%
52	14.710	1990	1993	1997	rVB6	5293	7548	0.29%	0.053%
53	14.757	1997	2001	2008	rVV6	5301	8049	0.31%	0.057%
54	14.851	2011	2017	2022	rBV9	4851	10421	0.40%	0.074%
55	14.904	2022	2026	2030	rVB5	5348	6251	0.24%	0.044%
56	15.016	2038	2045	2049	rBV9	5367	12469	0.48%	0.088%
57	15.098	2055	2059	2062	rBV2	15048	17340	0.67%	0.123%
58	15.228	2075	2081	2087	rBV	206362	281283	10.85%	1.991%
59	15.275	2087	2089	2094	rVB5	12004	15705	0.61%	0.111%
60	15.369	2100	2105	2115	rVB3	31959	54092	2.09%	0.383%
61	15.504	2123	2128	2135	rVB6	8787	16181	0.62%	0.115%
62	15.581	2138	2141	2149	rVB4	6256	11089	0.43%	0.078%
63	15.728	2161	2166	2174	rVB8	7000	14212	0.55%	0.101%
64	15.969	2199	2207	2208	rBV2	23051	29661	1.14%	0.210%
65	16.139	2233	2236	2241	rVB7	4325	6987	0.27%	0.049%
66	16.528	2299	2302	2307	rBV7	5466	10748	0.41%	0.076%
67	16.651	2319	2323	2329	rBV7	6938	12276	0.47%	0.087%
68	16.728	2332	2336	2339	rVV4	5891	8887	0.34%	0.063%
69	16.769	2339	2343	2347	rVV3	19446	27001	1.04%	0.191%
70	16.816	2347	2351	2358	rVB6	10457	20579	0.79%	0.146%
71	16.992	2375	2381	2386	rBV	794913	1143078	44.10%	8.091%
72	17.033	2386	2388	2393	rVB	110857	139519	5.38%	0.988%
73	17.092	2393	2398	2403	rBV2	211587	305039	11.77%	2.159%
74	17.186	2412	2414	2420	rVB7	5081	9601	0.37%	0.068%
75	17.310	2433	2435	2441	rVB7	5990	9457	0.36%	0.067%
76	17.416	2449	2453	2459	rBV3	11307	18473	0.71%	0.131%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081922\
 Data File : BP011523.D
 Acq On : 20 Aug 2022 00:42
 Operator : CG/JU
 Sample : N4210-05DL 5X
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BGC48DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP081622.M
 Title : SVOA CALIBRATION

77	17.516	2466	2470	2475	rBV3	16985	22366	0.86%	0.158%
78	17.692	2496	2500	2504	rBV2	19437	23069	0.89%	0.163%
79	17.875	2524	2531	2534	rBV4	19567	44573	1.72%	0.316%
80	17.916	2534	2538	2546	rVV2	56201	92649	3.57%	0.656%
81	17.986	2546	2550	2555	rVV2	15637	31637	1.22%	0.224%
82	18.063	2558	2563	2567	rVV2	31193	54156	2.09%	0.383%
83	18.098	2567	2569	2574	rVB	16831	19085	0.74%	0.135%
84	18.198	2582	2586	2590	rBV2	18466	25937	1.00%	0.184%
85	18.375	2612	2616	2619	rBV2	13706	17376	0.67%	0.123%
86	18.416	2619	2623	2626	rBV4	10159	13493	0.52%	0.096%
87	18.775	2680	2684	2688	rBV4	14719	25680	0.99%	0.182%
88	18.816	2688	2691	2693	rBV2	19991	23528	0.91%	0.167%
89	18.839	2693	2695	2698	rVB3	19468	18624	0.72%	0.132%
90	18.975	2715	2718	2721	rBV3	15025	18952	0.73%	0.134%
91	19.027	2723	2727	2732	rVV	267314	338067	13.04%	2.393%
92	19.357	2778	2783	2785	rBV	318992	422331	16.29%	2.990%
93	19.380	2785	2787	2792	rVB	227269	278307	10.74%	1.970%
94	19.904	2874	2876	2879	rBV2	19814	19102	0.74%	0.135%
95	20.851	3034	3037	3043	rBV6	64319	111278	4.29%	0.788%
96	21.051	3067	3071	3077	rBV	2524318	2591994	100.00%	18.348%
97	21.121	3077	3083	3087	rVV	1172804	1597533	61.63%	11.308%
98	21.157	3087	3089	3097	rVB	134554	165885	6.40%	1.174%
99	23.257	3443	3446	3451	rVB2	158622	236764	9.13%	1.676%
100	23.410	3466	3472	3478	rVB2	737035	1370416	52.87%	9.701%



Sum of corrected areas: 14126969

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081922\
Data File : BP011523.D
Acq On : 20 Aug 2022 00:42
Operator : CG/JU
Sample : N4210-05DL 5X
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BGC48DL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP081622.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

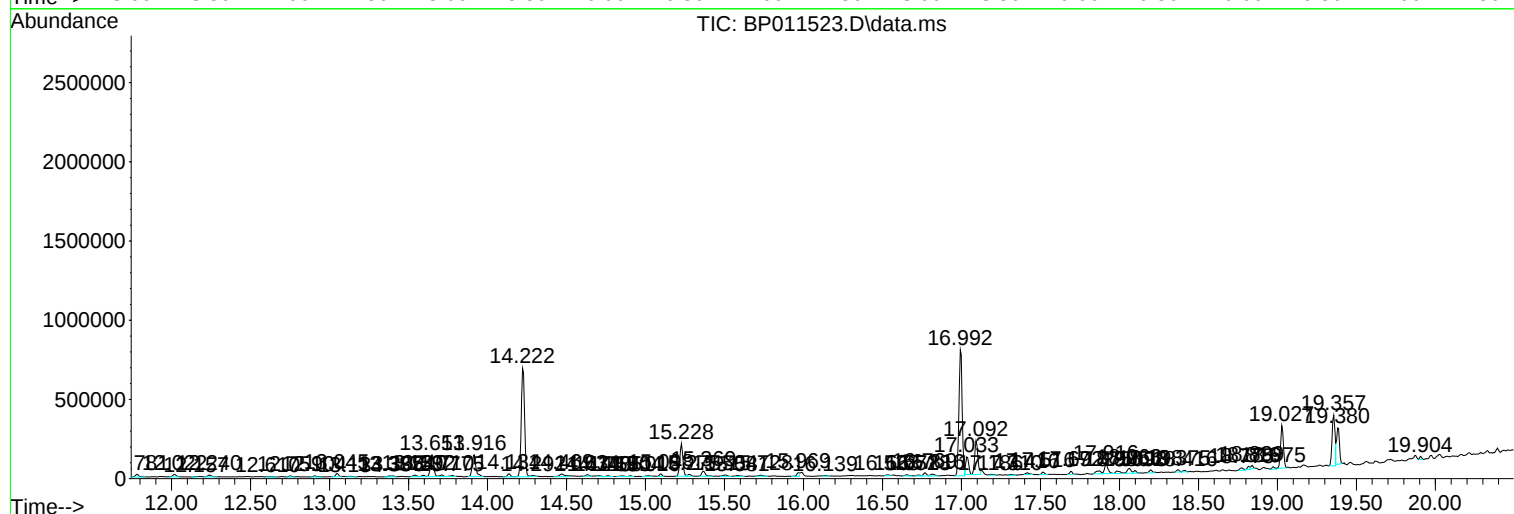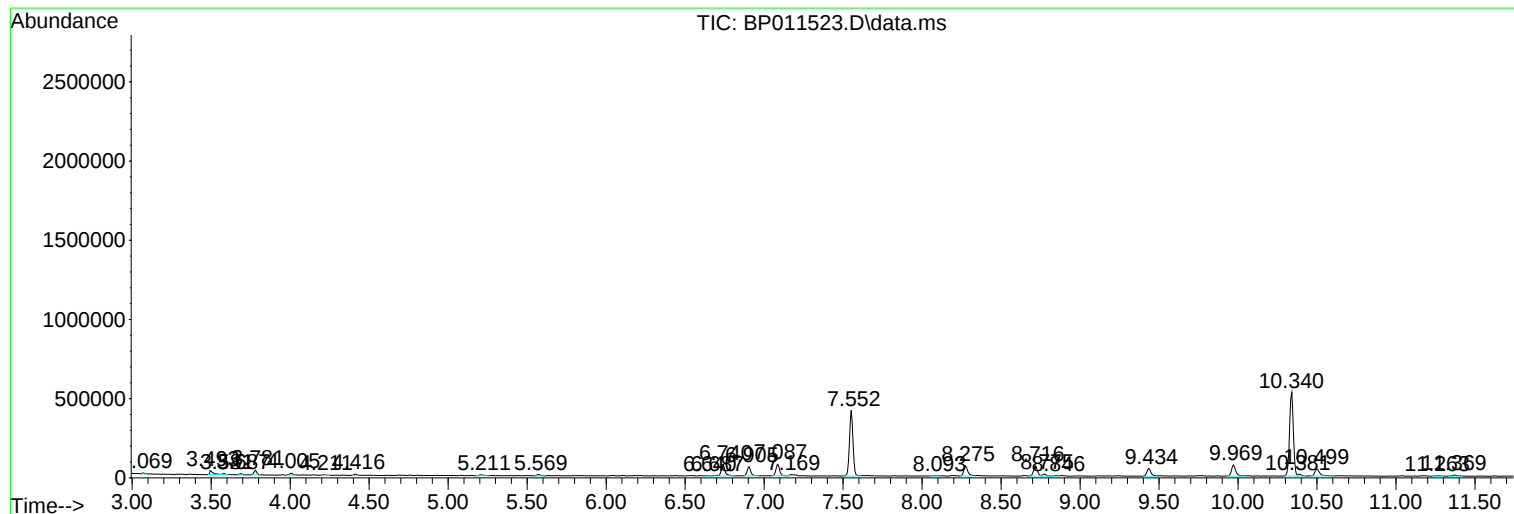

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081922\
Data File : BP011523.D
Acq On : 20 Aug 2022 00:42
Operator : CG/JU
Sample : N4210-05DL 5X
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BGC48DL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP081622.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081922\
Data File : BP011523.D
Acq On : 20 Aug 2022 00:42
Operator : CG/JU
Sample : N4210-05DL 5X
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BGC48DL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP081622.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc