

Data Path : Z:\svoasrv\HPCHEM1\BNA\_P\Data\BP081924\  
 Data File : BP021555.D  
 Acq On : 19 Aug 2024 15:58  
 Operator : RC/JU  
 Sample : P3519-05RE  
 Misc :  
 ALS Vial : 8 Sample Multiplier: 1

Instrument :  
 BNA\_P  
 ClientSampleId :  
 OU4-TS-18-080724RE

Quant Time: Aug 19 16:28:20 2024  
 Quant Method : Z:\svoasrv\HPCHEM1\BNA\_P\Methods\8270E-BP081324.M  
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 QLast Update : Wed Aug 14 00:00:30 2024  
 Response via : Initial Calibration


| Compound                      | R.T.   | QIon | Response | Conc      | Units | Dev(Min) |
|-------------------------------|--------|------|----------|-----------|-------|----------|
| -----                         |        |      |          |           |       |          |
| Internal Standards            |        |      |          |           |       |          |
| 1) 1,4-Dichlorobenzene-d4     | 7.805  | 152  | 357349   | 20.000    | ng    | 0.00     |
| 21) Naphthalene-d8            | 10.593 | 136  | 1505906  | 20.000    | ng    | 0.00     |
| 39) Acenaphthene-d10          | 14.457 | 164  | 1003830  | 20.000    | ng    | 0.00     |
| 64) Phenanthrene-d10          | 17.263 | 188  | 2190569  | 20.000    | ng    | 0.01     |
| 76) Chrysene-d12              | 21.716 | 240  | 1987317  | 20.000    | ng    | 0.02     |
| 86) Perylene-d12              | 25.151 | 264  | 2340650  | 20.000    | ng    | 0.05     |
|                               |        |      |          |           |       |          |
| System Monitoring Compounds   |        |      |          |           |       |          |
| 5) 2-Fluorophenol             | 5.399  | 112  | 1940274  | 80.623    | ng    | 0.00     |
| 7) Phenol-d6                  | 6.969  | 99   | 2798387  | 79.710    | ng    | 0.00     |
| 23) Nitrobenzene-d5           | 8.951  | 82   | 1666092  | 57.105    | ng    | 0.00     |
| 42) 2,4,6-Tribromophenol      | 15.969 | 330  | 988797   | 88.505    | ng    | 0.00     |
| 45) 2-Fluorobiphenyl          | 13.063 | 172  | 2732964  | 41.550    | ng    | 0.00     |
| 79) Terphenyl-d14             | 19.980 | 244  | 4182899  | 40.890    | ng    | 0.00     |
|                               |        |      |          |           |       |          |
| Target Compounds              |        |      |          |           |       | Qvalue   |
| 26) 2-Nitrophenol             | 9.710  | 139  | 28       | Below Cal | #     | 1        |
| 32) Benzoic acid              | 9.816  | 122  | 1698     | 3.534     | ng    | 87       |
| 48) 2-Nitroaniline            | 13.510 | 65   | 376      | 5.169     | ng    | # 59     |
| 51) 2,6-Dinitrotoluene        | 14.051 | 165  | 272      | 4.004     | ng    | # 65     |
| 53) 3-Nitroaniline            | 14.357 | 138  | 104      | 3.976     | ng    | # 1      |
| 54) 2,4-Dinitrophenol         | 14.551 | 184  | 222      | 2.520     | ng    | # 1      |
| 56) 4-Nitrophenol             | 14.786 | 139  | 404      | 5.112     | ng    | 87       |
| 57) 2,4-Dinitrotoluene        | 14.798 | 165  | 212      | 5.033     | ng    | # 22     |
| 62) 4-Nitroaniline            | 15.539 | 138  | 200      | 2.948     | ng    | # 43     |
| 65) 4,6-Dinitro-2-methylph... | 15.610 | 198  | 97       | 4.625     | ng    | # 1      |
| 71) Phenanthrene              | 17.316 | 178  | 527596   | 5.008     | ng    | 98       |
| 75) Fluoranthene              | 19.380 | 202  | 1280639  | 9.907     | ng    | 99       |
| 77) Benzidine                 | 19.592 | 184  | 567      | 4.582     | ng    | # 1      |
| 78) Pyrene                    | 19.757 | 202  | 1106481  | 8.518     | ng    | 99       |
| 80) Butylbenzylphthalate      | 20.721 | 149  | 7584     | 3.745     | ng    | # 29     |
| 81) Benzo(a)anthracene        | 21.698 | 228  | 595334   | 4.772     | ng    | 97       |
| 83) Chrysene                  | 21.763 | 228  | 592448   | 5.030     | ng    | 97       |
| 85) Di-n-octyl phthalate      | 22.957 | 149  | 946      | 4.843     | ng    | # 70     |
| 87) Indeno(1,2,3-cd)pyrene    | 29.045 | 276  | 425573   | 2.805     | ng    | 99       |
| 88) Benzo(b)fluoranthene      | 24.068 | 252  | 830030   | 6.174     | ng    | # 95     |
| 89) Benzo(k)fluoranthene      | 24.068 | 252  | 830030   | 6.330     | ng    | # 94     |
| 90) Benzo(a)pyrene            | 24.986 | 252  | 578881   | 4.962     | ng    | # 97     |
| 92) Benzo(g,h,i)perylene      | 30.244 | 276  | 398070   | 3.150     | ng    | 97       |
| -----                         |        |      |          |           |       |          |


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA\_P\Data\BP081924\  
Data File : BP021555.D  
Acq On : 19 Aug 2024 15:58  
Operator : RC/JU  
Sample : P3519-05RE  
Misc :  
ALS Vial : 8 Sample Multiplier: 1

Instrument :  
BNA\_P  
ClientSampleId :  
OU4-TS-18-080724RE

Quant Time: Aug 19 16:28:20 2024  
Quant Method : Z:\svoasrv\HPCHEM1\BNA\_P\Methods\8270E-BP081324.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Wed Aug 14 00:00:30 2024  
Response via : Initial Calibration



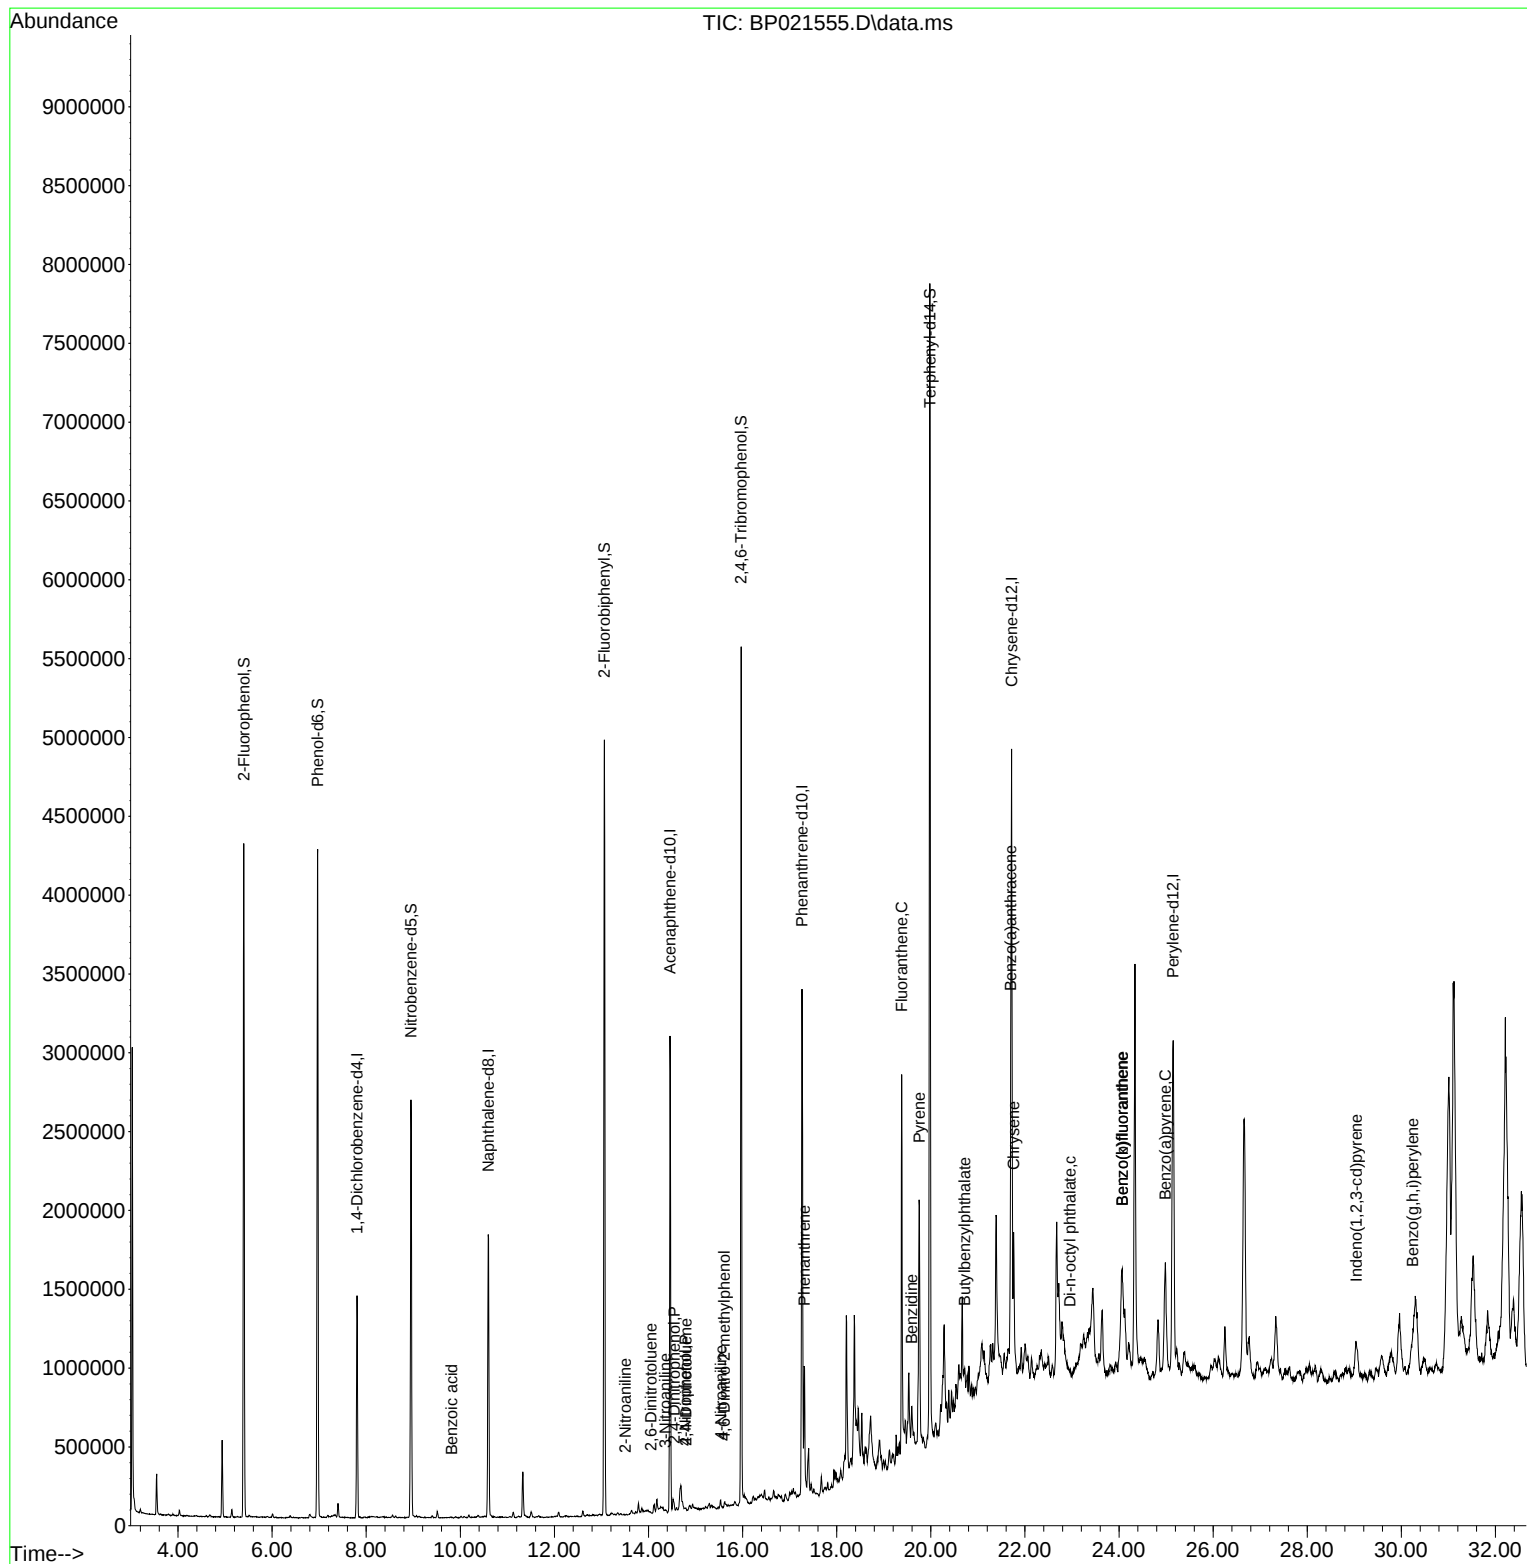




#1  
1,4-Dichlorobenzene-d4  
Concen: 20.000 ng  
RT: 7.805 min Scan# 81  
Delta R.T. -0.006 min  
Lab File: BP021555.D  
Acq: 19 Aug 2024 15:58




Instrument :  
BNA\_P  
ClientSampleId :  
OU4-TS-18-080724RE

Tgt Ion:152 Resp: 357349  
Ion Ratio Lower Upper  
152 100  
150 159.6 122.4 183.6  
115 68.8 54.7 82.1

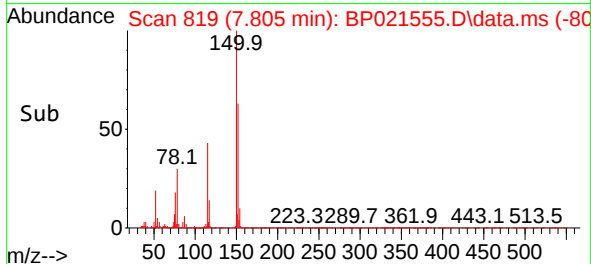

#5  
2-Fluorophenol  
Concen: 80.623 ng  
RT: 5.399 min Scan# 410  
Delta R.T. 0.006 min  
Lab File: BP021555.D  
Acq: 19 Aug 2024 15:58

Tgt Ion:112 Resp: 1940274  
Ion Ratio Lower Upper  
112 100  
64 54.8 49.0 73.6  
63 27.6 24.6 36.8

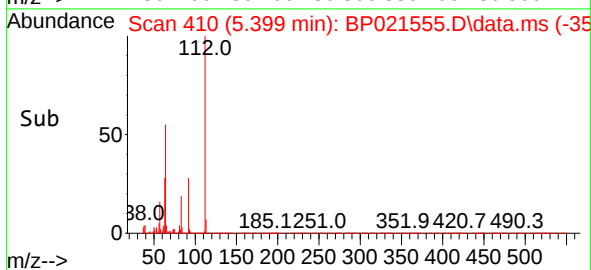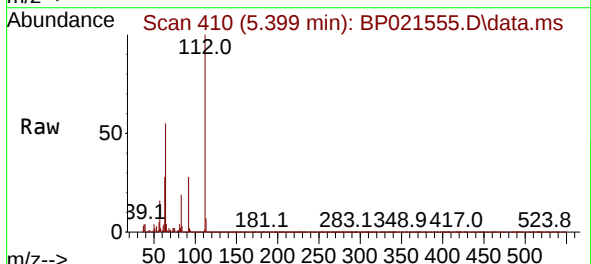







#7  
Phenol-d6  
Concen: 79.710 ng  
RT: 6.969 min Scan# 61  
Delta R.T. 0.006 min  
Lab File: BP021555.D  
Acq: 19 Aug 2024 15:58

Instrument :  
BNA\_P  
ClientSampleId :  
OU4-TS-18-080724RE

Tgt Ion: 99 Resp: 2798387




| Ion | Ratio | Lower | Upper |
|-----|-------|-------|-------|
| 99  | 100   |       |       |
| 42  | 12.2  | 10.2  | 15.4  |
| 71  | 30.2  | 25.8  | 38.8  |

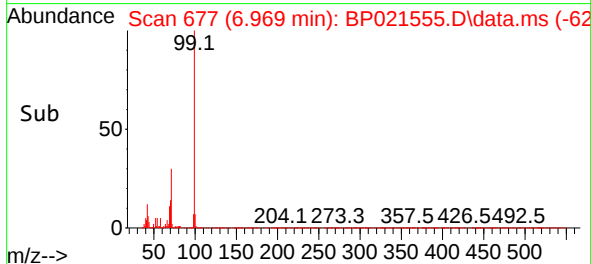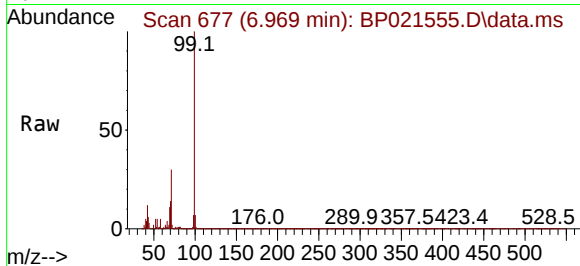


#21  
Naphthalene-d8  
Concen: 20.000 ng  
RT: 10.593 min Scan# 1293  
Delta R.T. -0.006 min  
Lab File: BP021555.D  
Acq: 19 Aug 2024 15:58

Tgt Ion:136 Resp: 1505906

| Ion | Ratio | Lower | Upper |
|-----|-------|-------|-------|
| 136 | 100   |       |       |
| 137 | 10.9  | 8.8   | 13.2  |
| 54  | 7.8   | 6.3   | 9.5   |
| 68  | 7.0   | 6.8   | 10.2  |


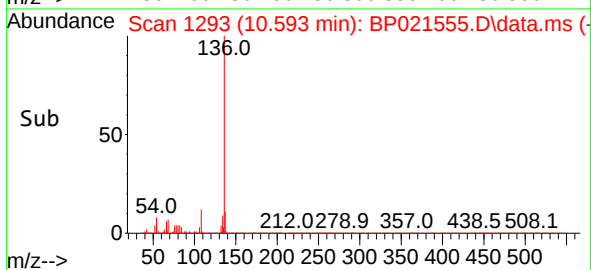

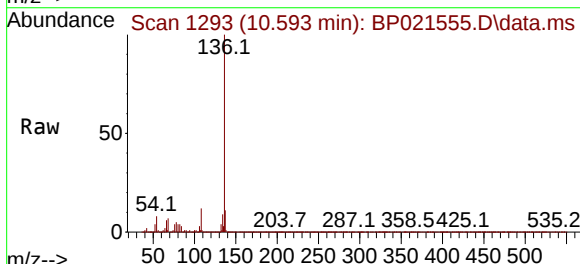


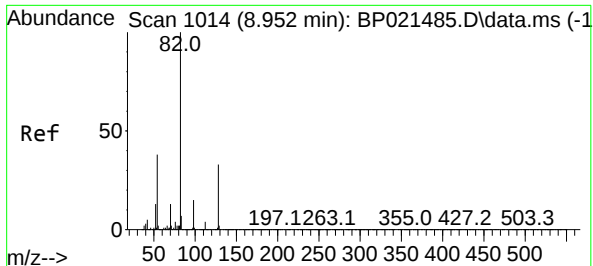

#23  
Nitrobenzene-d5  
Concen: 57.105 ng  
RT: 8.951 min Scan# 1014  
Delta R.T. -0.000 min  
Lab File: BP021555.D  
Acq: 19 Aug 2024 15:58




Instrument :  
BNA\_P  
ClientSampleId :  
OU4-TS-18-080724RE


Tgt Ion: 82 Resp: 1666092  
Ion Ratio Lower Upper  
82 100  
128 36.6 26.5 39.7  
54 38.6 30.3 45.5

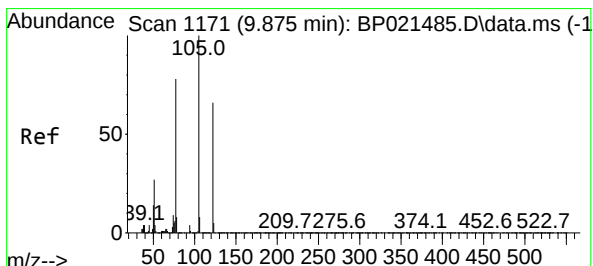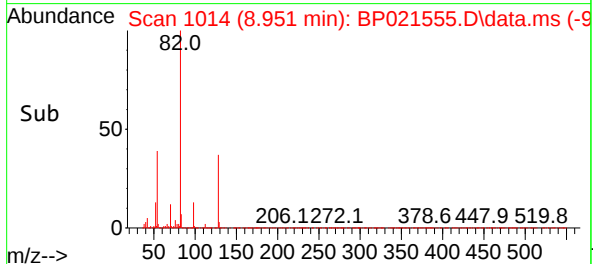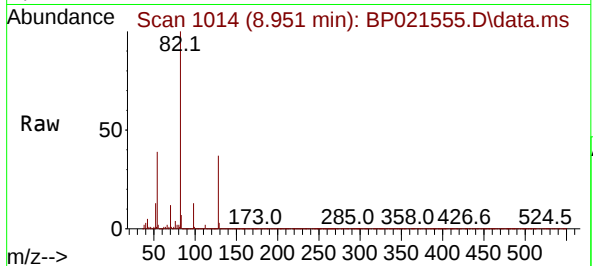

#32  
Benzoic acid  
Concen: 3.534 ng  
RT: 9.816 min Scan# 1161  
Delta R.T. -0.059 min  
Lab File: BP021555.D  
Acq: 19 Aug 2024 15:58

Tgt Ion: 122 Resp: 1698  
Ion Ratio Lower Upper  
122 100  
105 133.5 124.6 164.6  
77 135.9 96.2 136.2


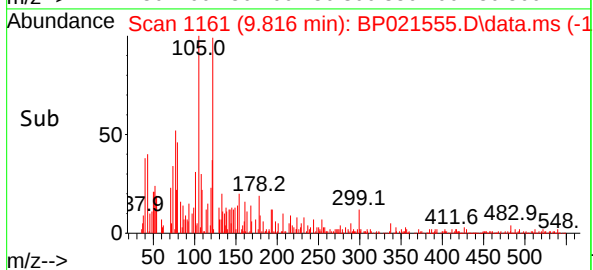

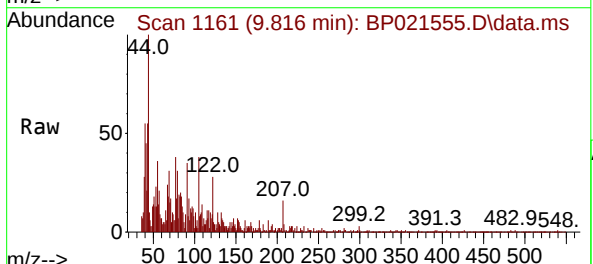


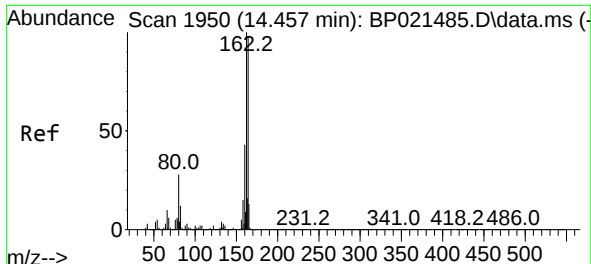

#39  
Acenaphthene-d10  
Concen: 20.000 ng  
RT: 14.457 min Scan# 1950  
Delta R.T. -0.000 min  
Lab File: BP021555.D  
Acq: 19 Aug 2024 15:58




Instrument :  
BNA\_P  
ClientSampleId :  
OU4-TS-18-080724RE


Tgt Ion:164 Resp: 1003830  
Ion Ratio Lower Upper  
164 100  
162 101.4 81.5 122.3  
160 43.9 35.2 52.8

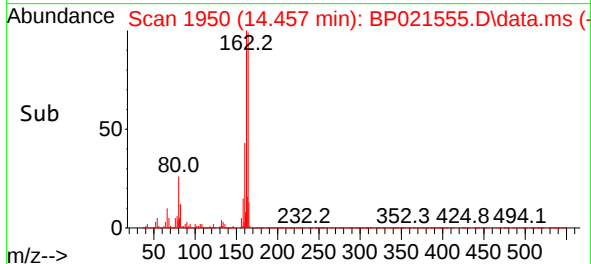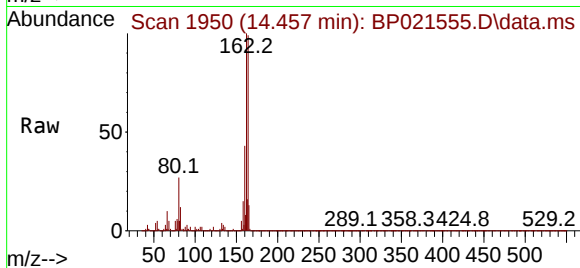

#42  
2,4,6-Tribromophenol  
Concen: 88.505 ng  
RT: 15.969 min Scan# 2207  
Delta R.T. -0.000 min  
Lab File: BP021555.D  
Acq: 19 Aug 2024 15:58

Tgt Ion:330 Resp: 988797  
Ion Ratio Lower Upper  
330 100  
332 97.7 77.4 116.0  
141 30.7 24.5 36.7

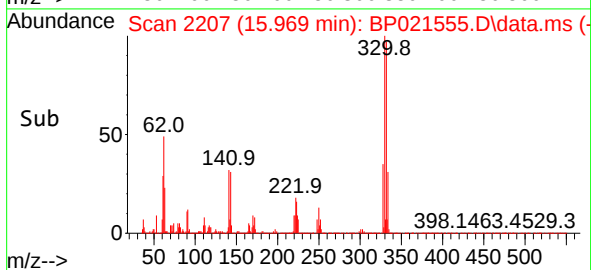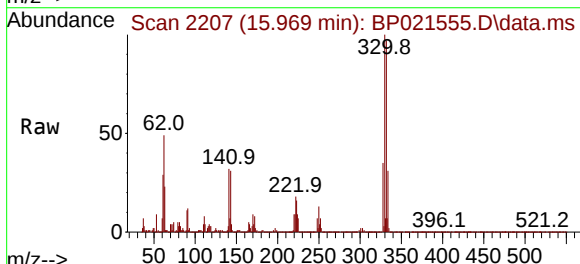



#45

2-Fluorobiphenyl

Concen: 41.550 ng

RT: 13.063 min Scan# 1713

Delta R.T. -0.000 min

Lab File: BP021555.D

Acq: 19 Aug 2024 15:58

Instrument :

BNA\_P

ClientSampleId :

OU4-TS-18-080724RE





Tgt Ion:172 Resp: 2732964

Ion Ratio Lower Upper

172 100

171 35.0 28.2 42.4

170 23.0 18.4 27.6



#48

2-Nitroaniline

Concen: 5.169 ng

RT: 13.510 min Scan# 1789

Delta R.T. 0.006 min

Lab File: BP021555.D

Acq: 19 Aug 2024 15:58




Tgt Ion: 65 Resp: 376


Ion Ratio Lower Upper

65 100

92 55.9 58.1 87.1#

138 29.0 65.5 98.3#


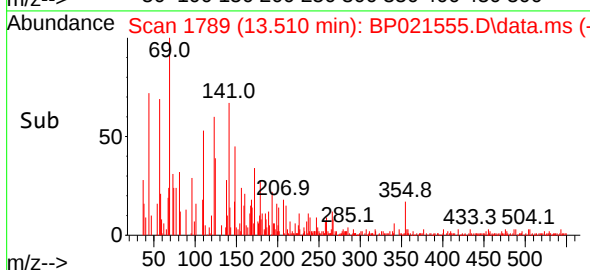






#51  
2,6-Dinitrotoluene  
Concen: 4.004 ng  
RT: 14.051 min Scan# 1881  
Delta R.T. 0.029 min  
Lab File: BP021555.D  
Acq: 19 Aug 2024 15:58




Instrument :  
BNA\_P  
ClientSampleId :  
OU4-TS-18-080724RE


Tgt Ion:165 Resp: 272  
Ion Ratio Lower Upper  
165 100  
63 108.2 51.5 77.3#  
89 58.9 57.8 86.8

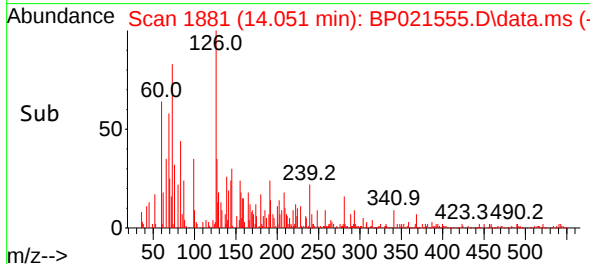

#53  
3-Nitroaniline  
Concen: 3.976 ng  
RT: 14.357 min Scan# 1933  
Delta R.T. 0.006 min  
Lab File: BP021555.D  
Acq: 19 Aug 2024 15:58

Tgt Ion:138 Resp: 104  
Ion Ratio Lower Upper  
138 100  
108 191.4 16.2 24.4#  
92 276.1 122.2 183.4#

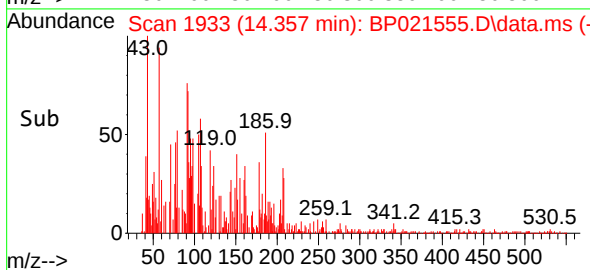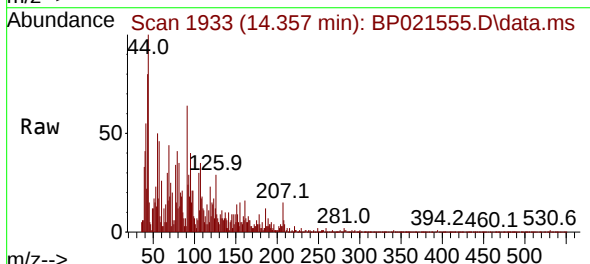



#54

2,4-Dinitrophenol

Concen: 2.520 ng

RT: 14.551 min Scan# 1966

Delta R.T. 0.000 min

Lab File: BP021555.D

Acq: 19 Aug 2024 15:58

Instrument :

BNA\_P

ClientSampleId :

OU4-TS-18-080724RE





Tgt Ion:184 Resp: 222

Ion Ratio Lower Upper

184 100

63 247.0 64.9 97.3#

154 210.7 52.1 78.1#



#56

4-Nitrophenol

Concen: 5.112 ng

RT: 14.786 min Scan# 2006

Delta R.T. 0.135 min

Lab File: BP021555.D

Acq: 19 Aug 2024 15:58




Tgt Ion:139 Resp: 404


Ion Ratio Lower Upper

139 100

109 100.0 70.2 110.2

65 106.0 101.8 141.8


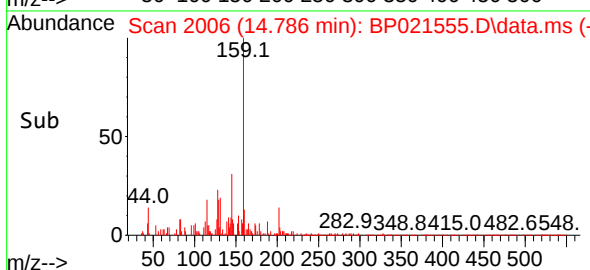






#57  
2,4-Dinitrotoluene  
Concen: 5.033 ng  
RT: 14.798 min Scan# 2010  
Delta R.T. -0.012 min  
Lab File: BP021555.D  
Acq: 19 Aug 2024 15:58




Instrument :  
BNA\_P  
ClientSampleId :  
OU4-TS-18-080724RE


Tgt Ion:165 Resp: 212  
Ion Ratio Lower Upper  
165 100  
63 127.2 42.5 63.7#  
89 33.9 77.1 115.7#  
182 25.3 2.0 3.0#

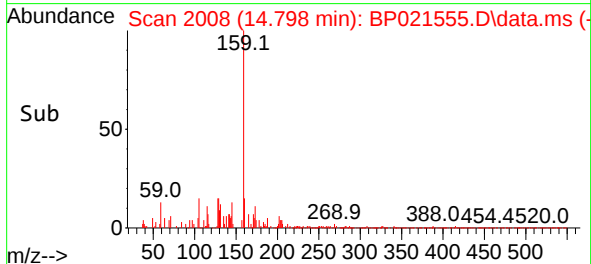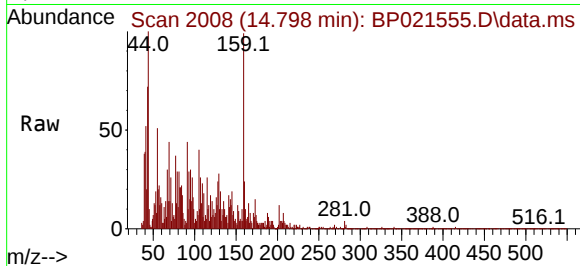

#62  
4-Nitroaniline  
Concen: 2.948 ng  
RT: 15.539 min Scan# 2134  
Delta R.T. 0.011 min  
Lab File: BP021555.D  
Acq: 19 Aug 2024 15:58

Tgt Ion:138 Resp: 200  
Ion Ratio Lower Upper  
138 100  
92 137.6 46.4 86.4#  
108 125.7 73.2 113.2#

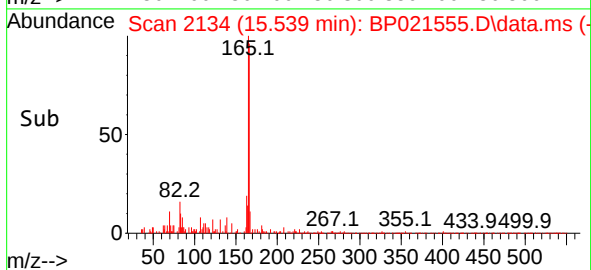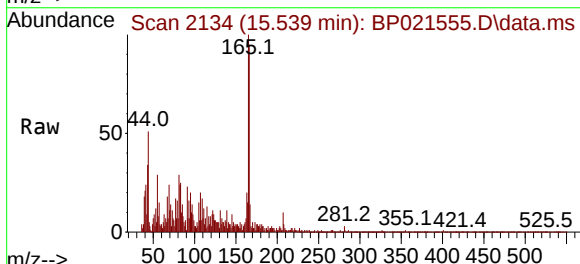



#64

Phenanthrene-d10

Concen: 20.000 ng

RT: 17.263 min Scan# 2425

Delta R.T. 0.012 min

Lab File: BP021555.D

Acq: 19 Aug 2024 15:58

Instrument :

BNA\_P

ClientSampleId :

OU4-TS-18-080724RE





Tgt Ion:188 Resp: 2190569

Ion Ratio Lower Upper

188 100

94 12.1 10.2 15.4

80 13.6 11.6 17.4

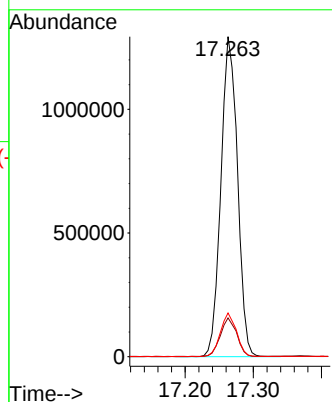

#65

4,6-Dinitro-2-methylphenol

Concen: 4.625 ng

RT: 15.610 min Scan# 2146

Delta R.T. 0.023 min

Lab File: BP021555.D

Acq: 19 Aug 2024 15:58




Tgt Ion:198 Resp: 97


Ion Ratio Lower Upper

198 100

51 574.5 21.5 61.5#

105 1659.2 32.9 72.9#

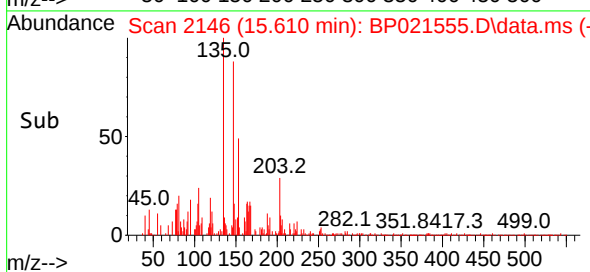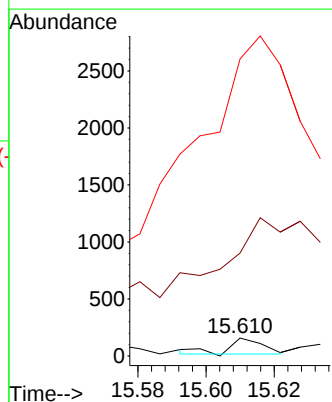



#71

Phenanthrene

Concen: 5.008 ng

RT: 17.316 min Scan# 2433

Delta R.T. 0.017 min

Lab File: BP021555.D

Acq: 19 Aug 2024 15:58

Instrument :

BNA\_P

ClientSampleId :

OU4-TS-18-080724RE





Tgt Ion:178 Resp: 527596

Ion Ratio Lower Upper

178 100

176 18.9 15.4 23.2

179 14.4 12.4 18.6

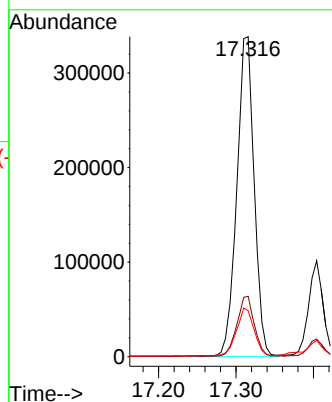

#75

Fluoranthene

Concen: 9.907 ng

RT: 19.380 min Scan# 2787

Delta R.T. -0.000 min

Lab File: BP021555.D

Acq: 19 Aug 2024 15:58




Tgt Ion:202 Resp: 1280639


Ion Ratio Lower Upper

202 100

101 14.5 0.0 34.0

203 17.1 0.0 37.5

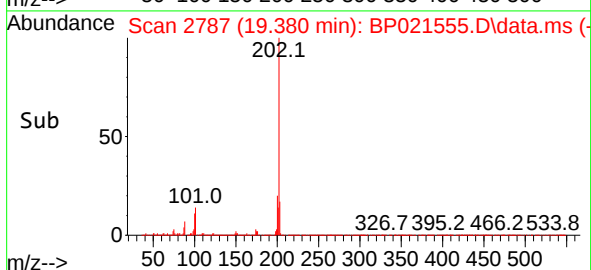



#76

Chrysene-d12

Concen: 20.000 ng

RT: 21.716 min Scan# 3184

Delta R.T. 0.017 min

Lab File: BP021555.D

Acq: 19 Aug 2024 15:58

Instrument :

BNA\_P

ClientSampleId :

OU4-TS-18-080724RE





Tgt Ion:240 Resp: 1987317

Ion Ratio Lower Upper

240 100

120 11.8 9.9 14.9

236 25.6 20.6 30.8

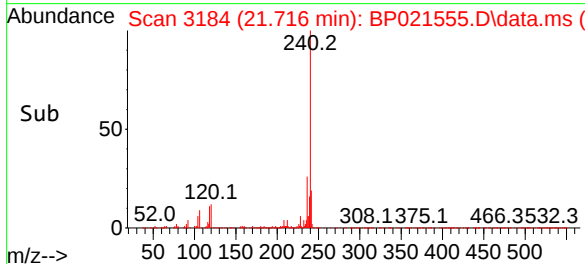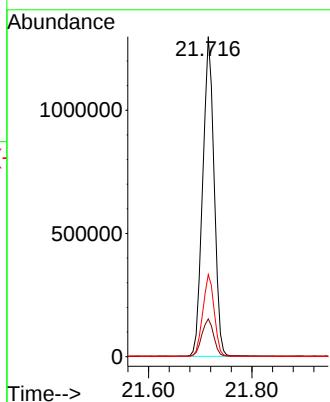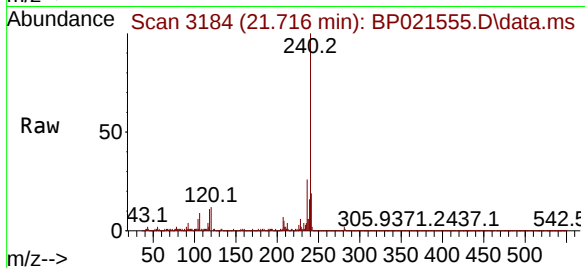

#77

Benzidine

Concen: 4.582 ng

RT: 19.592 min Scan# 2823

Delta R.T. 0.017 min

Lab File: BP021555.D

Acq: 19 Aug 2024 15:58




Tgt Ion:184 Resp: 567


Ion Ratio Lower Upper

184 100

185 197.8 11.4 17.0#

183 111.6 9.3 13.9#

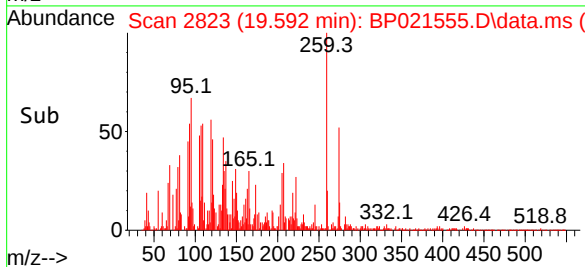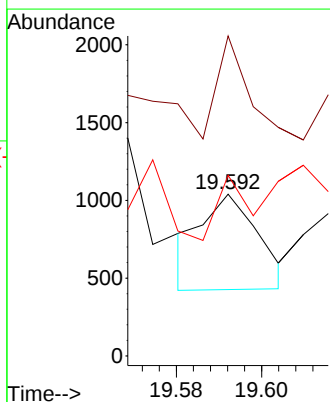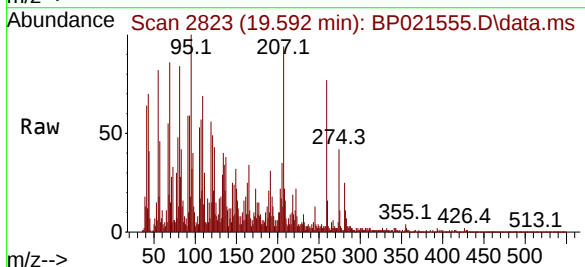



#78

Pyrene

Concen: 8.518 ng

RT: 19.757 min Scan# 2850

Delta R.T. 0.006 min

Lab File: BP021555.D

Acq: 19 Aug 2024 15:58

Instrument :

BNA\_P

ClientSampleId :

OU4-TS-18-080724RE





Tgt Ion:202 Resp: 1106481

Ion Ratio Lower Upper

202 100

200 20.3 16.7 25.1

203 18.0 14.1 21.1

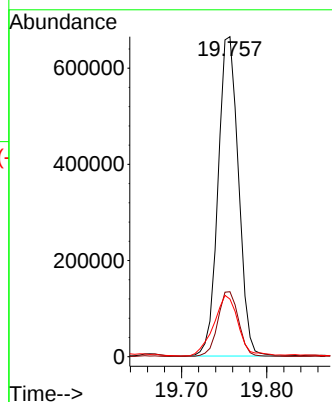

#79

Terphenyl-d14

Concen: 40.890 ng

RT: 19.980 min Scan# 2889

Delta R.T. 0.005 min

Lab File: BP021555.D

Acq: 19 Aug 2024 15:58




Tgt Ion:244 Resp: 4182899


Ion Ratio Lower Upper

244 100

212 6.7 5.6 8.4

122 11.1 9.4 14.2

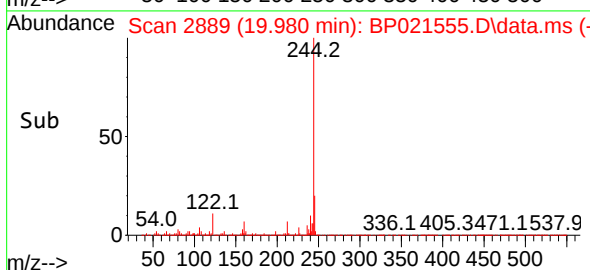



#80

Butylbenzylphthalate

Concen: 3.745 ng

RT: 20.721 min Scan# 3013

Delta R.T. 0.011 min

Lab File: BP021555.D

Acq: 19 Aug 2024 15:58

Instrument :

BNA\_P

ClientSampleId :

OU4-TS-18-080724RE





Tgt Ion:149 Resp: 7584

Ion Ratio Lower Upper

149 100

91 165.0 73.3 109.9#

206 0.0 17.1 25.7#

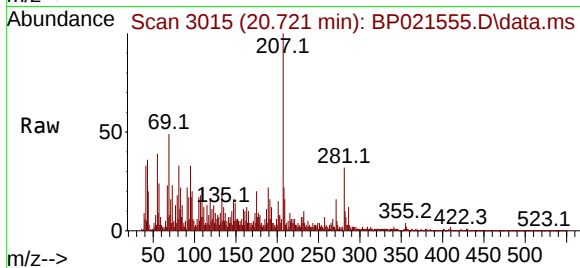

#81

Benzo(a)anthracene

Concen: 4.772 ng

RT: 21.698 min Scan# 3181

Delta R.T. 0.017 min

Lab File: BP021555.D

Acq: 19 Aug 2024 15:58




Tgt Ion:228 Resp: 595334


Ion Ratio Lower Upper

228 100

226 28.9 21.4 32.2

229 20.4 15.8 23.6


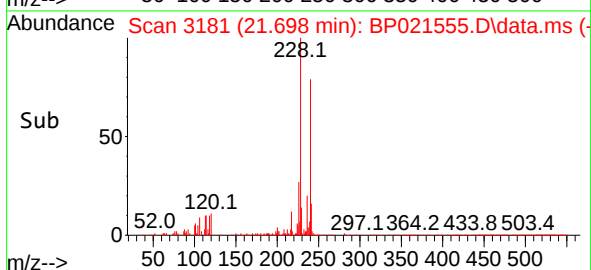

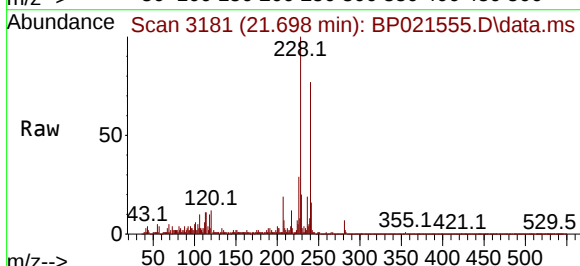




#83  
Chrysene  
Concen: 5.030 ng  
RT: 21.763 min Scan# 3192  
Delta R.T. 0.012 min  
Lab File: BP021555.D  
Acq: 19 Aug 2024 15:58




Instrument :  
BNA\_P  
ClientSampleId :  
OU4-TS-18-080724RE


Tgt Ion:228 Resp: 592448  
Ion Ratio Lower Upper  
228 100  
226 29.7 23.9 35.9  
229 22.7 15.8 23.6

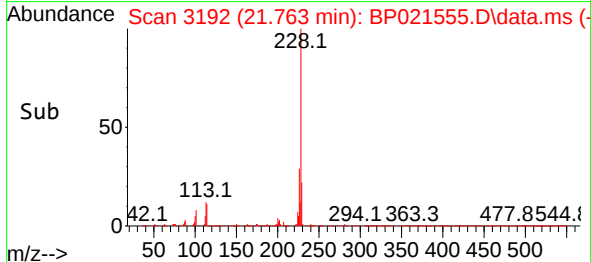

#85  
Di-n-octyl phthalate  
Concen: 4.843 ng  
RT: 22.957 min Scan# 3395  
Delta R.T. -0.006 min  
Lab File: BP021555.D  
Acq: 19 Aug 2024 15:58

Tgt Ion:149 Resp: 946  
Ion Ratio Lower Upper  
149 100  
167 22.9 1.3 1.9#  
43 0.0 7.3 10.9#

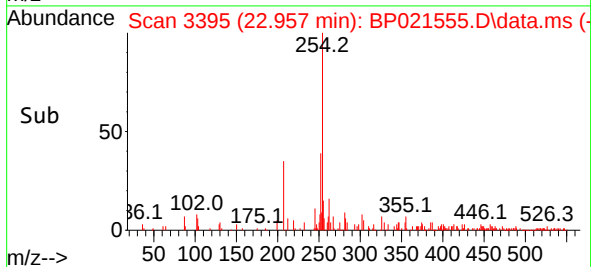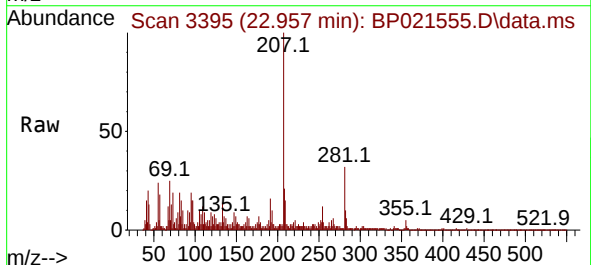



#86

Perylene-d12

Concen: 20.000 ng

RT: 25.151 min Scan# 31

Delta R.T. 0.047 min

Lab File: BP021555.D

Acq: 19 Aug 2024 15:58

Instrument :

BNA\_P

ClientSampleId :

OU4-TS-18-080724RE





Tgt Ion:264 Resp: 2340650

Ion Ratio Lower Upper

264 100

260 24.0 18.6 28.0

265 21.5 17.1 25.7

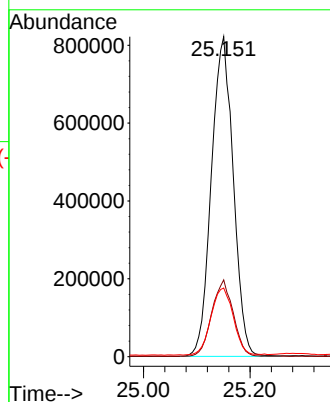

#87

Indeno(1,2,3-cd)pyrene

Concen: 2.805 ng

RT: 29.045 min Scan# 4430

Delta R.T. 0.053 min

Lab File: BP021555.D

Acq: 19 Aug 2024 15:58




Tgt Ion:276 Resp: 425573


Ion Ratio Lower Upper

276 100

138 16.7 12.8 19.2

277 20.8 16.5 24.7

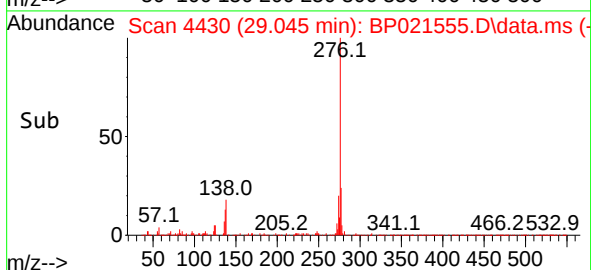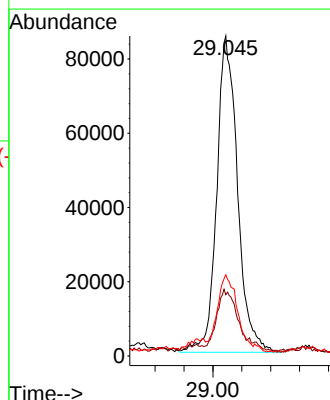



#88

Benzo(b)fluoranthene

Concen: 6.174 ng

RT: 24.068 min Scan# 3577

Delta R.T. 0.041 min

Lab File: BP021555.D

Acq: 19 Aug 2024 15:58

Instrument :

BNA\_P

ClientSampleId :

OU4-TS-18-080724RE





Tgt Ion:252 Resp: 830030

Ion Ratio Lower Upper

252 100

253 23.5 17.6 26.4

125 13.7 8.6 13.0#

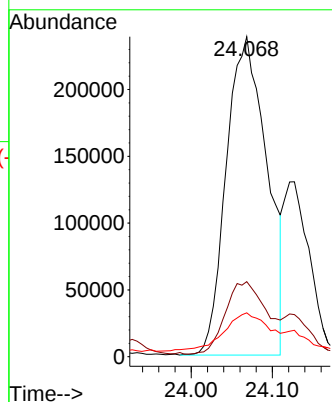

#89

Benzo(k)fluoranthene

Concen: 6.330 ng

RT: 24.068 min Scan# 3584

Delta R.T. -0.041 min

Lab File: BP021555.D

Acq: 19 Aug 2024 15:58




Tgt Ion:252 Resp: 830030


Ion Ratio Lower Upper

252 100

253 23.5 17.5 26.3

125 13.7 7.8 11.8#

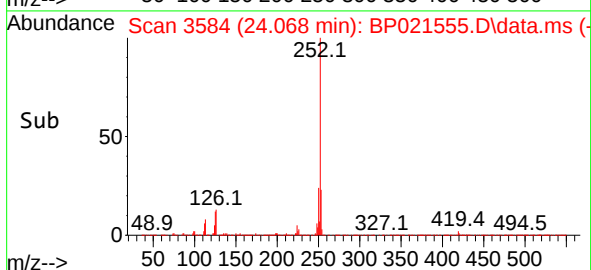



#90

Benzo(a)pyrene

Concen: 4.962 ng

RT: 24.986 min Scan# 31

Delta R.T. 0.035 min

Lab File: BP021555.D

Acq: 19 Aug 2024 15:58

Instrument :

BNA\_P

ClientSampleId :

OU4-TS-18-080724RE





Tgt Ion:252 Resp: 578881

Ion Ratio Lower Upper

252 100

253 23.0 17.7 26.5

125 13.4 8.7 13.1#

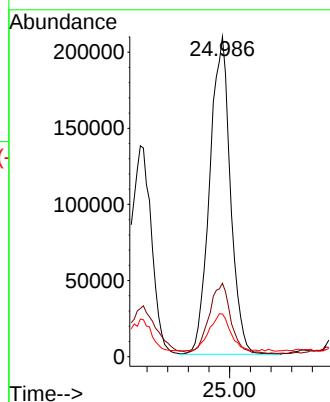

#92

Benzo(g,h,i)perylene

Concen: 3.150 ng

RT: 30.244 min Scan# 4634

Delta R.T. 0.070 min

Lab File: BP021555.D

Acq: 19 Aug 2024 15:58

Tgt Ion:276 Resp: 398070

Ion Ratio Lower Upper

276 100

277 25.1 19.0 28.6

138 22.0 16.0 24.0

